


Data Path : Z:\HPCHEM1\BNA M\DATA\BM101415\
 Data File : BM002900.D
 Acq On : 14 Oct 2015 16:01
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-ACID-BM0101315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 14 17:36:42 2015

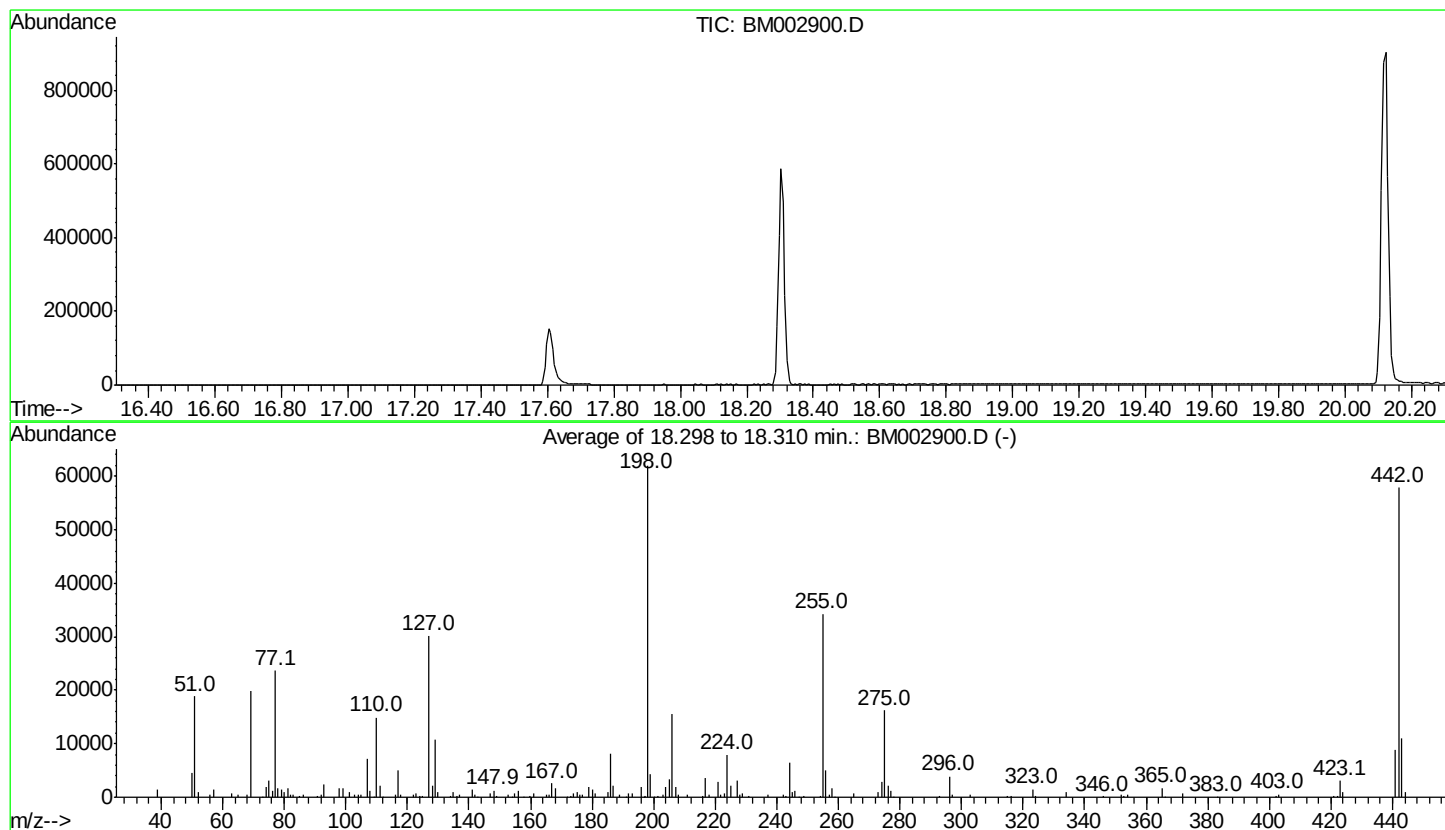

AutoFind: Scans 2586, 2587, 2588; Background Corrected with Scan 2580

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.4	18844	PASS
68	69	0.00	2	2.0	391	PASS
69	198	0.00	100	31.9	19738	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.6	30120	PASS
197	198	0.00	2	0.4	233	PASS
198	198	100	100	100.0	61912	PASS
199	198	5	9	6.9	4282	PASS
275	198	10	60	26.1	16164	PASS
365	198	1	100	2.9	1782	PASS
441	442	0.01	24	15.3	8826	PASS
442	198	50	100	93.2	57730	PASS
443	442	15	24	19.3	11114	PASS