

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101424\
 Data File : BM048072.D
 Acq On : 15 Oct 2024 22:24
 Operator : RC/JU
 Sample : P4239-08RE
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4EG7

Quant Time: Oct 15 23:04:27 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 10 05:10:14 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	207381	20.000	ng/ul	0.00
20) Naphthalene-d8	10.569	136	855615	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.416	164	530793	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.157	188	1063227	20.000	ng/ul	0.00
79) Chrysene-d12	21.386	240	993202	20.000	ng/ul	0.00
88) Perylene-d12	24.380	264	1133201	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.240	96	24646	3.841	ng/uL	0.00
4) Pyridine-d5	3.652	84	340177	18.104	ng/ul	0.00
7) Phenol-d5	6.952	99	424174	21.631	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.110	67	259848	18.674	ng/ul	0.00
11) 2-Chlorophenol-d4	7.316	132	367534	25.760	ng/ul	0.00
15) 4-Methylphenol-d8	8.493	113	345159	23.674	ng/ul	0.00
21) Nitrobenzene-d5	8.934	128	173060	25.403	ng/ul	0.00
24) 2-Nitrophenol-d4	9.657	143	196799	30.145	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.198	165	333883	25.602	ng/ul	0.00
31) 4-Chloroaniline-d4	10.710	131	464650	23.046	ng/ul	0.00
46) Dimethylphthalate-d6	13.828	166	1019521	26.493	ng/ul	0.00
49) Acenaphthylene-d8	14.110	160	1208181	26.479	ng/ul	0.00
54) 4-Nitrophenol-d4	14.633	143	123370	16.102	ng/ul	0.01
60) Fluorene-d10	15.410	176	898706	26.962	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.533	200	120525	19.371	ng/ul	0.00
73) Anthracene-d10	17.257	188	1364418	26.098	ng/ul	0.00
81) Pyrene-d10	19.545	212	1617867	28.701	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.180	264	1647933	28.028	ng/ul	0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.286	149	45475	1.159	ng/ul#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101424\
Data File : BM048072.D
Acq On : 15 Oct 2024 22:24
Operator : RC/JU
Sample : P4239-08RE
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4EG7

Quant Time: Oct 15 23:04:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 10 05:10:14 2024
Response via : Initial Calibration

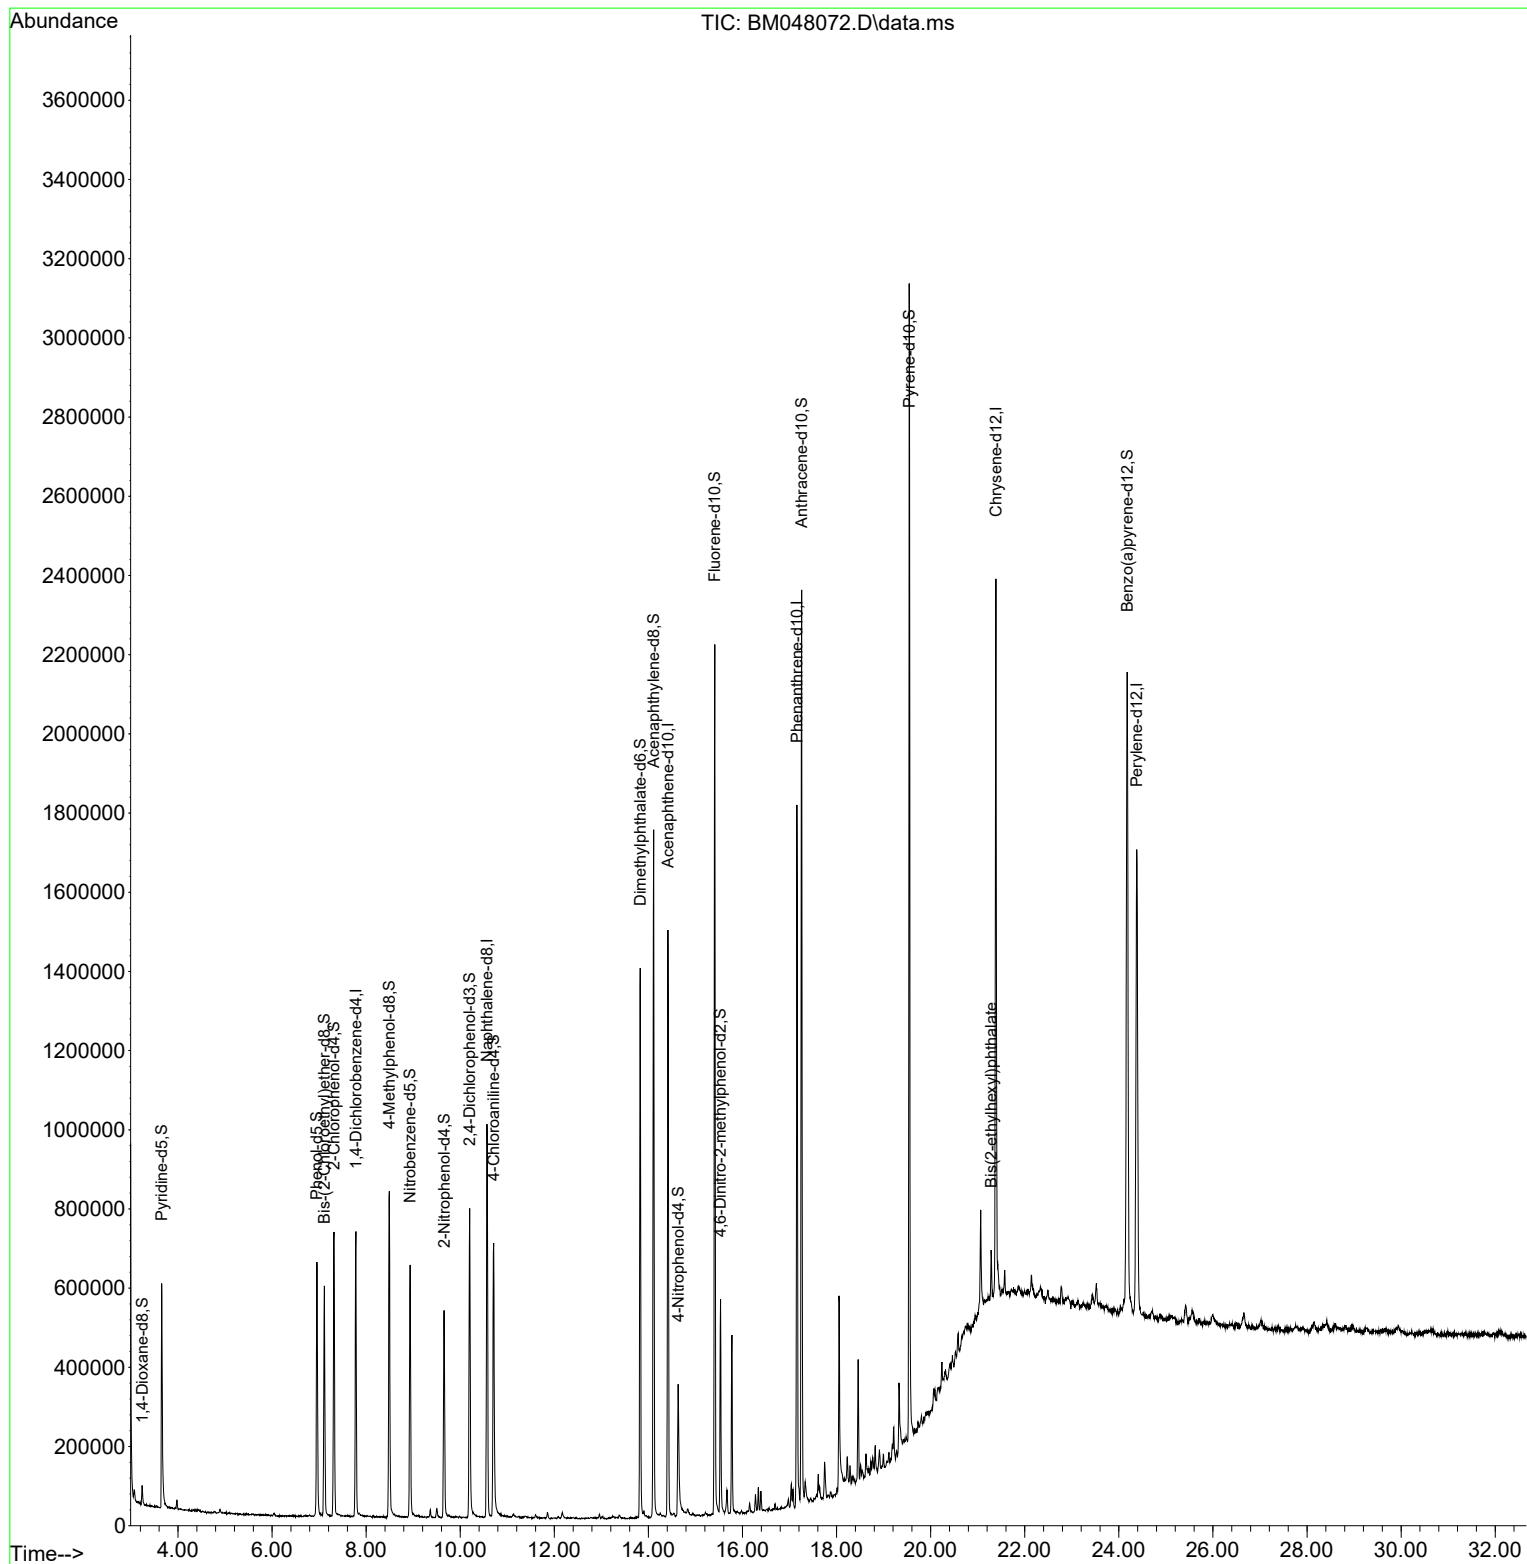

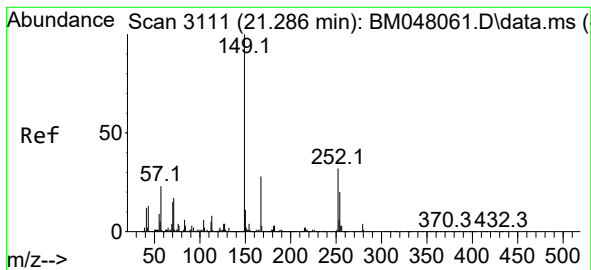

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.159 ng/ul
 RT: 21.286 min Scan# 3111
 Delta R.T. 0.000 min
 Lab File: BM048072.D
 Acq: 15 Oct 2024 22:24

Instrument :
 BNA_M
 ClientSampleId :
 A4EG7

Tgt Ion:149 Resp: 45475
 Ion Ratio Lower Upper
 149 100
 167 27.2 21.3 31.9
 279 4.1 2.7 4.1#

