

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM101424\  
 Data File : BM048067.D  
 Acq On : 15 Oct 2024 19:06  
 Operator : RC/JU  
 Sample : P4350-11  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 EOAK2

Quant Time: Oct 15 23:02:44 2024  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM092724.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Thu Oct 10 05:10:14 2024  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc   | Units  | Dev(Min) |
|-------------------------------|--------|------|----------|--------|--------|----------|
| -----                         |        |      |          |        |        |          |
| Internal Standards            |        |      |          |        |        |          |
| 1) 1,4-Dichlorobenzene-d4     | 7.781  | 152  | 276102   | 20.000 | ng/u1  | 0.00     |
| 20) Naphthalene-d8            | 10.575 | 136  | 1137657  | 20.000 | ng/u1  | # 0.00   |
| 38) Acenaphthene-d10          | 14.416 | 164  | 712849   | 20.000 | ng/u1  | 0.00     |
| 64) Phenanthrene-d10          | 17.157 | 188  | 1421906  | 20.000 | ng/u1  | 0.00     |
| 79) Chrysene-d12              | 21.386 | 240  | 1330296  | 20.000 | ng/u1  | 0.00     |
| 88) Perylene-d12              | 24.380 | 264  | 1476406  | 20.000 | ng/u1  | 0.00     |
| System Monitoring Compounds   |        |      |          |        |        |          |
| 3) 1,4-Dioxane-d8             | 3.240  | 96   | 18646    | 2.182  | ng/uL  | 0.00     |
| 4) Pyridine-d5                | 3.658  | 84   | 246997   | 9.874  | ng/u1  | 0.00     |
| 7) Phenol-d5                  | 6.957  | 99   | 332209   | 12.724 | ng/u1  | 0.00     |
| 9) Bis-(2-Chloroethyl)eth...  | 7.110  | 67   | 200297   | 10.811 | ng/u1  | 0.00     |
| 11) 2-Chlorophenol-d4         | 7.316  | 132  | 284168   | 14.960 | ng/u1  | 0.00     |
| 15) 4-Methylphenol-d8         | 8.492  | 113  | 279803   | 14.414 | ng/u1  | 0.00     |
| 21) Nitrobenzene-d5           | 8.934  | 128  | 137445   | 15.174 | ng/u1  | 0.00     |
| 24) 2-Nitrophenol-d4          | 9.657  | 143  | 155211   | 17.881 | ng/u1  | 0.00     |
| 28) 2,4-Dichlorophenol-d3     | 10.198 | 165  | 274121   | 15.808 | ng/u1  | 0.00     |
| 31) 4-Chloroaniline-d4        | 10.710 | 131  | 366932   | 13.687 | ng/u1  | 0.00     |
| 46) Dimethylphthalate-d6      | 13.827 | 166  | 899868   | 17.412 | ng/u1  | 0.00     |
| 49) Acenaphthylene-d8         | 14.110 | 160  | 1013166  | 16.534 | ng/u1  | 0.00     |
| 54) 4-Nitrophenol-d4          | 14.633 | 143  | 94007    | 9.136  | ng/u1  | 0.01     |
| 60) Fluorene-d10              | 15.410 | 176  | 775751   | 17.329 | ng/u1  | 0.00     |
| 65) 4,6-Dinitro-2-methylph... | 15.533 | 200  | 92265    | 11.088 | ng/u1  | 0.00     |
| 73) Anthracene-d10            | 17.257 | 188  | 1230735  | 17.603 | ng/u1  | 0.00     |
| 81) Pyrene-d10                | 19.545 | 212  | 1453058  | 19.246 | ng/u1  | 0.00     |
| 92) Benzo(a)pyrene-d12        | 24.174 | 264  | 1461654  | 19.081 | ng/u1  | 0.00     |
| Target Compounds              |        |      |          |        |        |          |
|                               |        |      |          |        | Qvalue |          |
| 8) Phenol                     | 6.981  | 94   | 30348    | 1.092  | ng/u1  | 97       |
| -----                         |        |      |          |        |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM101424\  
Data File : BM048067.D  
Acq On : 15 Oct 2024 19:06  
Operator : RC/JU  
Sample : P4350-11  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
EOAK2

Quant Time: Oct 15 23:02:44 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM092724.MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Thu Oct 10 05:10:14 2024  
Response via : Initial Calibration

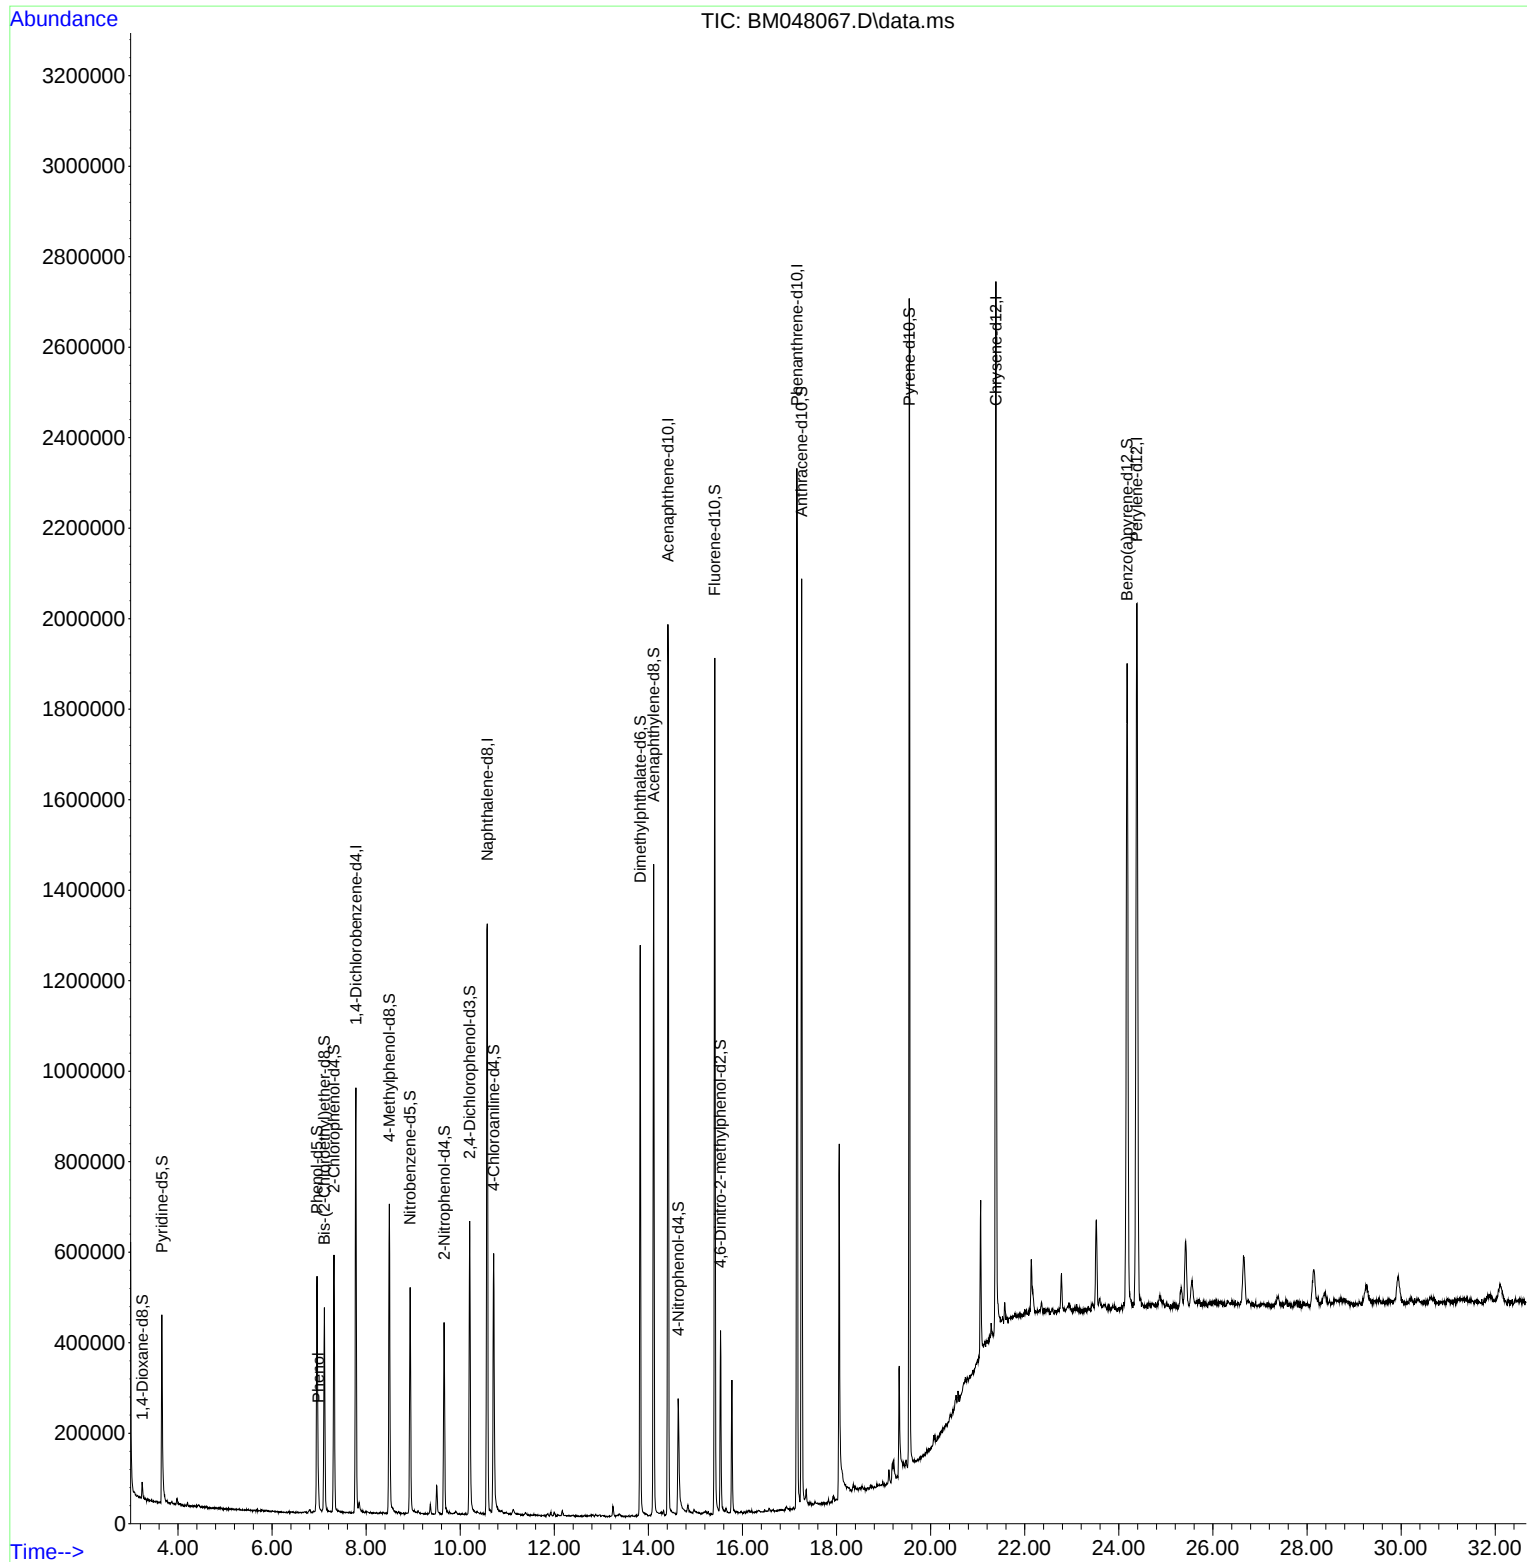

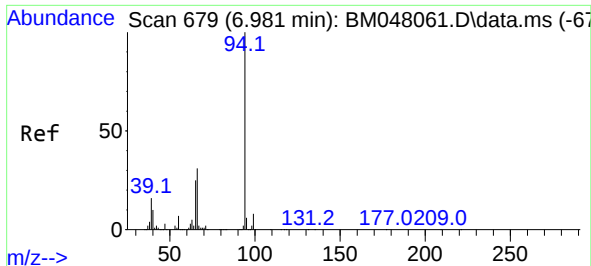

#8  
Phenol  
Concen: 1.092 ng/ul  
RT: 6.981 min Scan# 61  
Delta R.T. -0.006 min  
Lab File: BM048067.D  
Acq: 15 Oct 2024 19:06

Instrument :  
BNA\_M  
ClientSampleId :  
EOAK2

Tgt Ion: 94 Resp: 30348  
Ion Ratio Lower Upper  
94 100  
65 30.9 26.3 39.5  
66 39.5 30.5 45.7

