

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101424\
 Data File : BM048068.D
 Acq On : 15 Oct 2024 19:46
 Operator : RC/JU
 Sample : P4350-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EOAK1

Quant Time: Oct 15 23:02:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 10 05:10:14 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	256195	20.000	ng/u1	0.00
20) Naphthalene-d8	10.574	136	1039838	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.415	164	655055	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.156	188	1317515	20.000	ng/u1	0.00
79) Chrysene-d12	21.386	240	1218211	20.000	ng/u1	0.00
88) Perylene-d12	24.379	264	1370502	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.240	96	29382	3.706	ng/uL	0.00
4) Pyridine-d5	3.651	84	419934	18.091	ng/u1	0.00
7) Phenol-d5	6.957	99	532043	21.962	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.110	67	317913	18.493	ng/u1	0.00
11) 2-Chlorophenol-d4	7.316	132	449902	25.525	ng/u1	0.00
15) 4-Methylphenol-d8	8.492	113	427716	23.746	ng/u1	0.00
21) Nitrobenzene-d5	8.933	128	218249	26.361	ng/u1	0.00
24) 2-Nitrophenol-d4	9.657	143	246190	31.030	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.198	165	410047	25.872	ng/u1	0.00
31) 4-Chloroaniline-d4	10.710	131	583860	23.828	ng/u1	0.00
46) Dimethylphthalate-d6	13.827	166	1229433	25.887	ng/u1	0.00
49) Acenaphthylene-d8	14.110	160	1420113	25.220	ng/u1	0.00
54) 4-Nitrophenol-d4	14.633	143	130687	13.821	ng/u1	0.01
60) Fluorene-d10	15.409	176	1063719	25.858	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.533	200	126924	16.462	ng/u1	0.00
73) Anthracene-d10	17.256	188	1610251	24.856	ng/u1	0.00
81) Pyrene-d10	19.544	212	1895516	27.416	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.174	264	1886233	26.526	ng/u1	0.00
Target Compounds						
					Qvalue	
8) Phenol	6.981	94	44288	1.718	ng/u1	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101424\
Data File : BM048068.D
Acq On : 15 Oct 2024 19:46
Operator : RC/JU
Sample : P4350-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOAK1

Quant Time: Oct 15 23:02:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 10 05:10:14 2024
Response via : Initial Calibration

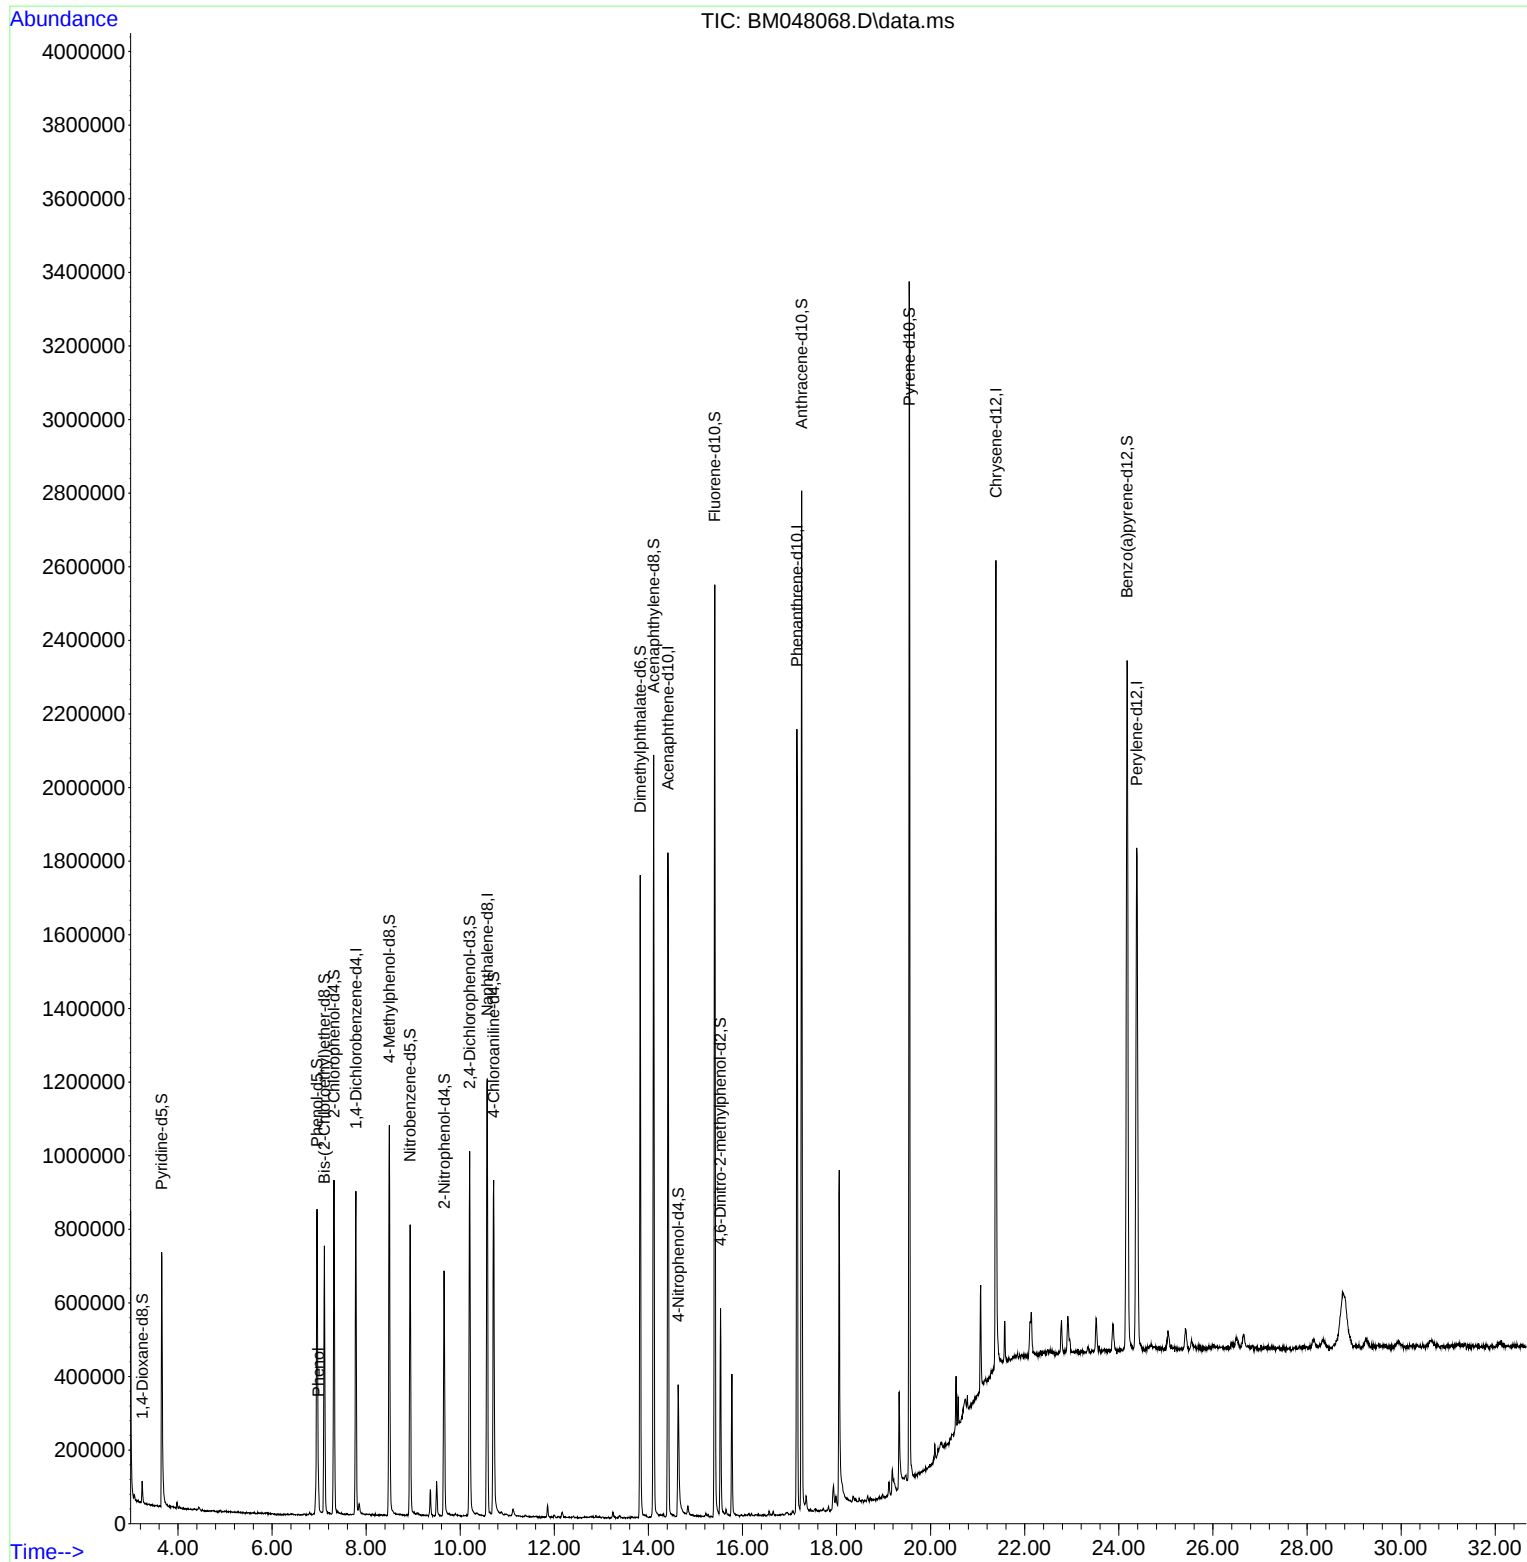

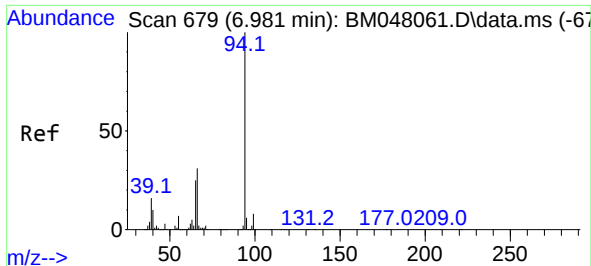

#8
Phenol
Concen: 1.718 ng/ul
RT: 6.981 min Scan# 61
Delta R.T. -0.006 min
Lab File: BM048068.D
Acq: 15 Oct 2024 19:46

Instrument :
BNA_M
ClientSampleId :
EOAK1

Tgt Ion: 94 Resp: 44288
Ion Ratio Lower Upper
94 100
65 28.6 26.3 39.5
66 36.5 30.5 45.7

