

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101424\
 Data File : BM048025.D
 Acq On : 14 Oct 2024 12:55
 Operator : RC/JU
 Sample : PB163884BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK884

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048025.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	39	43	50	rVB	56566	79138	2.16%	0.194%
2	3.652	110	113	133	rBV	606292	925003	25.21%	2.270%
3	3.981	165	169	173	rVB	24521	33946	0.93%	0.083%
4	4.152	196	198	202	rBV5	4099	4673	0.13%	0.011%
5	4.204	204	207	212	rVB7	4562	5651	0.15%	0.014%
6	4.469	250	252	256	rBV5	4338	4120	0.11%	0.010%
7	5.487	423	425	429	rBV5	2791	3882	0.11%	0.010%
8	6.951	667	674	686	rBV	620086	1033304	28.17%	2.536%
9	7.034	686	688	691	rVB4	5330	6330	0.17%	0.016%
10	7.110	691	701	712	rBV	512394	845663	23.05%	2.075%
11	7.316	727	736	750	rBV	653959	1092456	29.78%	2.681%
12	7.575	779	780	788	rVB5	3287	5047	0.14%	0.012%
13	7.781	808	815	826	rBV	739948	1204048	32.82%	2.955%
14	8.492	929	936	949	rBV	714160	1231946	33.58%	3.023%
15	8.934	1004	1011	1021	rBV	561987	949309	25.88%	2.330%
16	9.004	1021	1023	1029	rVB7	5739	8329	0.23%	0.020%
17	9.369	1078	1085	1089	rBV2	10092	19365	0.53%	0.048%
18	9.657	1126	1134	1148	rBV	455880	793867	21.64%	1.948%
19	9.857	1167	1168	1172	rBV4	3188	3811	0.10%	0.009%
20	10.198	1219	1226	1241	rBV	653545	1186565	32.34%	2.912%
21	10.575	1282	1290	1302	rVB	973249	1651443	45.02%	4.052%
22	10.710	1306	1313	1330	rBV	609056	1208584	32.94%	2.966%
23	10.992	1358	1361	1365	rVB6	2777	3893	0.11%	0.010%
24	11.057	1370	1372	1376	rBV5	3211	4007	0.11%	0.010%
25	11.857	1505	1508	1514	rBV5	9440	15441	0.42%	0.038%
26	12.180	1556	1563	1567	rBV6	7203	15141	0.41%	0.037%
27	12.263	1573	1577	1578	rVB4	3305	3894	0.11%	0.010%
28	13.827	1836	1843	1852	rBV	1206043	1716707	46.80%	4.213%
29	14.110	1884	1891	1906	rVV	1427474	2136637	58.24%	5.243%
30	14.416	1937	1943	1953	rBV	1389780	2087116	56.89%	5.122%
31	14.627	1972	1979	1992	rBV	310142	671345	18.30%	1.647%
32	15.410	2105	2112	2127	rBV	1758437	2605486	71.02%	6.394%
33	15.527	2127	2132	2142	rBV	513046	738302	20.13%	1.812%
34	15.651	2149	2153	2161	rVB8	10378	20083	0.55%	0.049%
35	15.974	2205	2208	2212	rVV5	2034	3971	0.11%	0.010%
36	16.957	2372	2375	2376	rVB3	4055	4273	0.12%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101424\
Data File : BM048025.D
Acq On : 14 Oct 2024 12:55
Operator : RC/JU
Sample : PB163884BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK884

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Title : SVOA CALIBRATION

37	17.157	2402	2409	2417	rBV	1664343	2442381	66.58%	5.993%
38	17.257	2419	2426	2439	rVV	1996717	2841466	77.46%	6.973%
39	17.557	2471	2477	2479	rBV7	3422	6240	0.17%	0.015%
40	18.057	2560	2562	2567	rVB6	4781	6320	0.17%	0.016%
41	18.662	2663	2665	2669	rBV5	4664	6443	0.18%	0.016%
42	19.109	2738	2741	2748	rVB3	22991	33627	0.92%	0.083%
43	19.186	2750	2754	2762	rVV2	22259	36419	0.99%	0.089%
44	19.545	2809	2815	2827	rBV	2520126	3409774	92.95%	8.367%
45	21.386	3122	3128	3139	rBV	1782629	2806864	76.51%	6.888%
46	24.168	3593	3601	3616	rVB	1478443	3668513	100.00%	9.002%
47	24.374	3628	3636	3648	rVB	1225771	3170477	86.42%	7.780%




Sum of corrected areas: 40751300

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101424\
Data File : BM048025.D
Acq On : 14 Oct 2024 12:55
Operator : RC/JU
Sample : PB163884BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK884

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

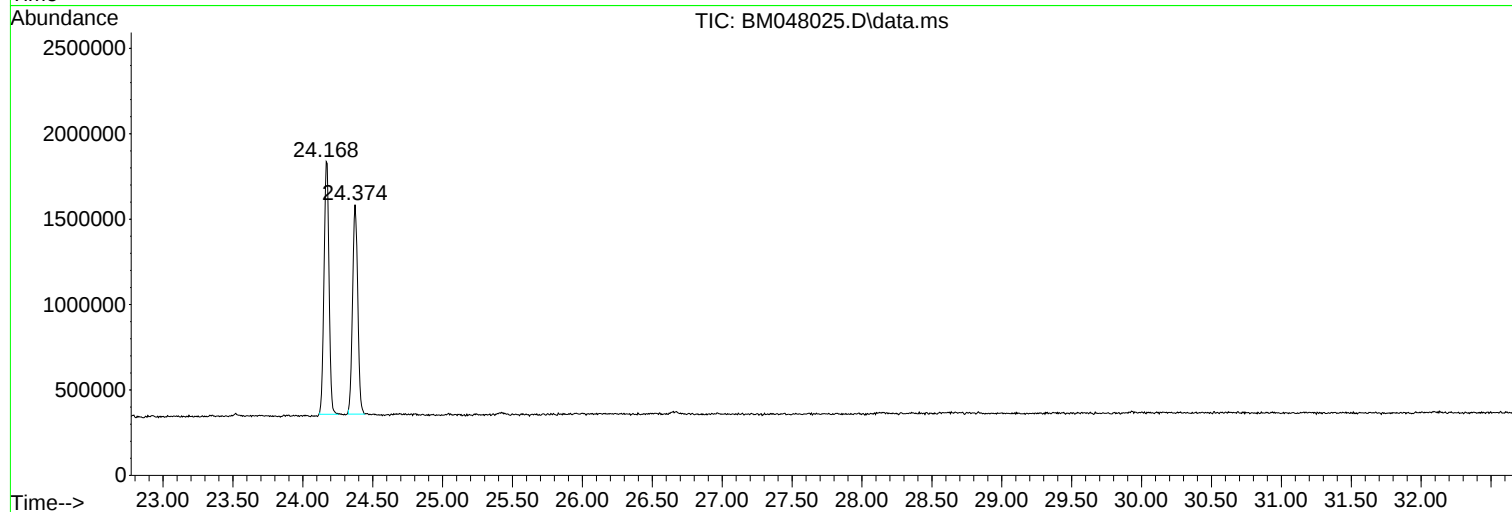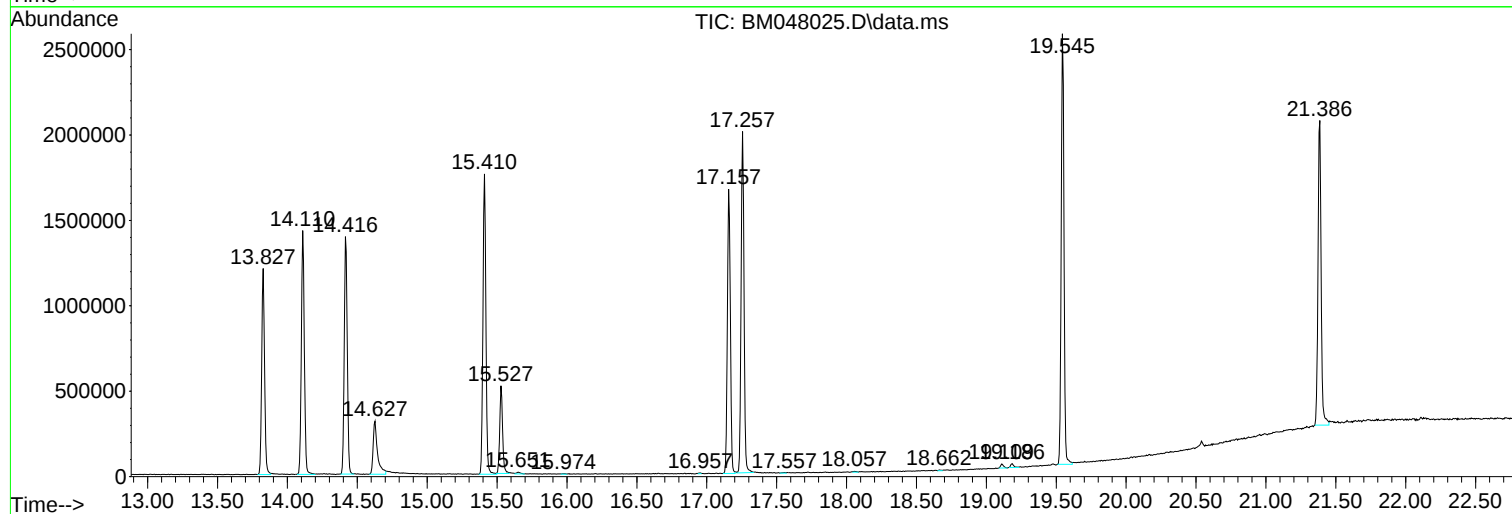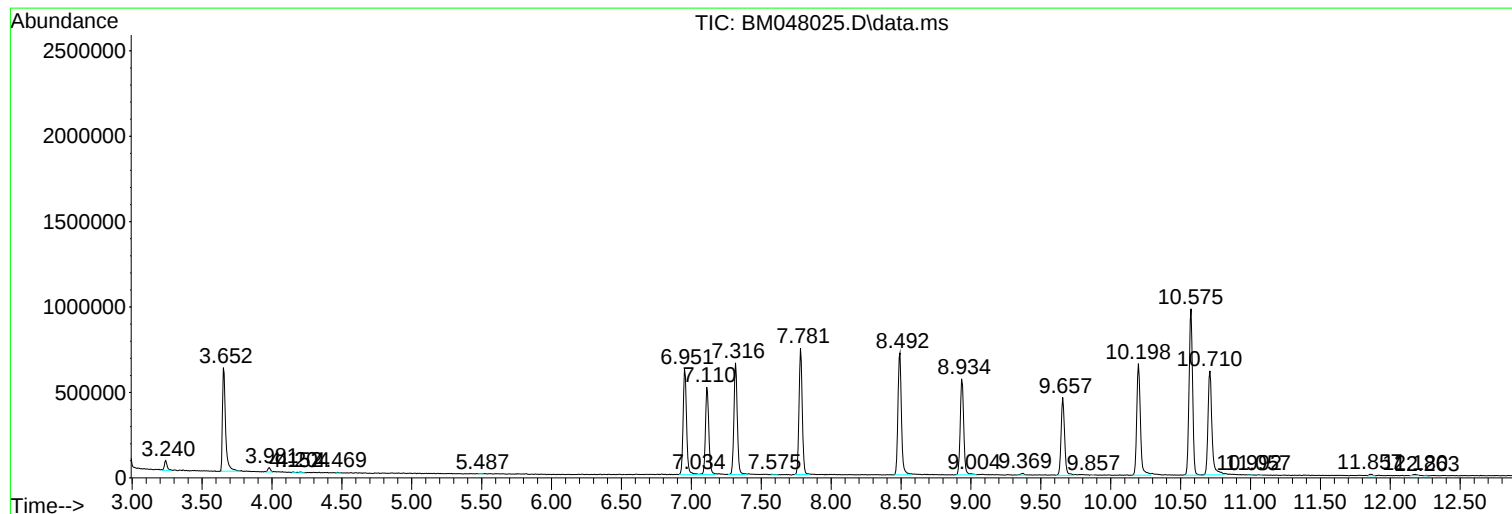

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101424\
Data File : BM048025.D
Acq On : 14 Oct 2024 12:55
Operator : RC/JU
Sample : PB163884BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK884

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101424\
Data File : BM048025.D
Acq On : 14 Oct 2024 12:55
Operator : RC/JU
Sample : PB163884BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK884

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc