

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101424\
 Data File : BM048048.D
 Acq On : 15 Oct 2024 04:46
 Operator : RC/JU
 Sample : PB163836BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK836

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048048.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	39	42	50	rVB	66885	88857	1.81%	0.169%
2	3.652	109	113	135	rBV	849418	1244530	25.36%	2.368%
3	3.981	165	169	174	rVB	25318	36560	0.75%	0.070%
4	6.957	667	675	690	rBV	845129	1421324	28.97%	2.705%
5	7.110	695	701	716	rVB	699241	1143805	23.31%	2.176%
6	7.316	728	736	747	rBV	934959	1511490	30.80%	2.876%
7	7.781	808	815	830	rBV	891971	1471367	29.99%	2.800%
8	8.240	888	893	898	rBV9	3594	6455	0.13%	0.012%
9	8.493	929	936	953	rBV	1000815	1723465	35.12%	3.279%
10	8.934	1004	1011	1025	rBV	767492	1333826	27.18%	2.538%
11	9.369	1082	1085	1088	rVB4	4197	5571	0.11%	0.011%
12	9.657	1126	1134	1144	rBV	641168	1093665	22.29%	2.081%
13	10.198	1219	1226	1238	rBV	947181	1685749	34.36%	3.208%
14	10.575	1282	1290	1301	rBV	1164246	1981126	40.37%	3.770%
15	10.710	1305	1313	1335	rBV	915282	1718730	35.03%	3.270%
16	11.863	1506	1509	1514	rVB6	4081	6714	0.14%	0.013%
17	12.175	1557	1562	1567	rBV5	14162	31667	0.65%	0.060%
18	13.827	1835	1843	1857	rBV	1537982	2244477	45.74%	4.271%
19	14.110	1880	1891	1904	rBV	1924612	2919299	59.49%	5.555%
20	14.422	1937	1944	1957	rBV	1597094	2479218	50.53%	4.718%
21	14.627	1972	1979	1998	rBV	455460	1011619	20.62%	1.925%
22	14.839	2012	2015	2020	rVB6	5304	6832	0.14%	0.013%
23	15.410	2106	2112	2127	rBV	2329247	3453049	70.37%	6.571%
24	15.533	2127	2133	2144	rVV	559483	815236	16.61%	1.551%
25	15.651	2150	2153	2161	rVB6	12638	20786	0.42%	0.040%
26	16.645	2320	2322	2328	rVB7	3847	5837	0.12%	0.011%
27	16.839	2352	2355	2358	rBV5	4620	5930	0.12%	0.011%
28	16.951	2372	2374	2377	rVB4	4696	5390	0.11%	0.010%
29	17.157	2403	2409	2420	rVV	1826841	2773349	56.52%	5.277%
30	17.257	2420	2426	2440	rVV	2636140	3727513	75.97%	7.093%
31	17.439	2452	2457	2459	rBV6	6279	11289	0.23%	0.021%
32	19.115	2738	2742	2746	rBV3	38707	52781	1.08%	0.100%
33	19.186	2750	2754	2759	rVV2	30794	46250	0.94%	0.088%
34	19.545	2809	2815	2827	rBV	3046756	4530739	92.34%	8.621%
35	21.386	3122	3128	3138	rBV2	2103632	3323800	67.74%	6.325%
36	24.180	3594	3603	3618	rVB	1937020	4906841	100.00%	9.337%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101424\
Data File : BM048048.D
Acq On : 15 Oct 2024 04:46
Operator : RC/JU
Sample : PB163836BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK836

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Title : SVOA CALIBRATION

37 24.380 3629 3637 3649 rVB 1448217 3707763 75.56% 7.055%




Sum of corrected areas: 52552899

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101424\
Data File : BM048048.D
Acq On : 15 Oct 2024 04:46
Operator : RC/JU
Sample : PB163836BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK836

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

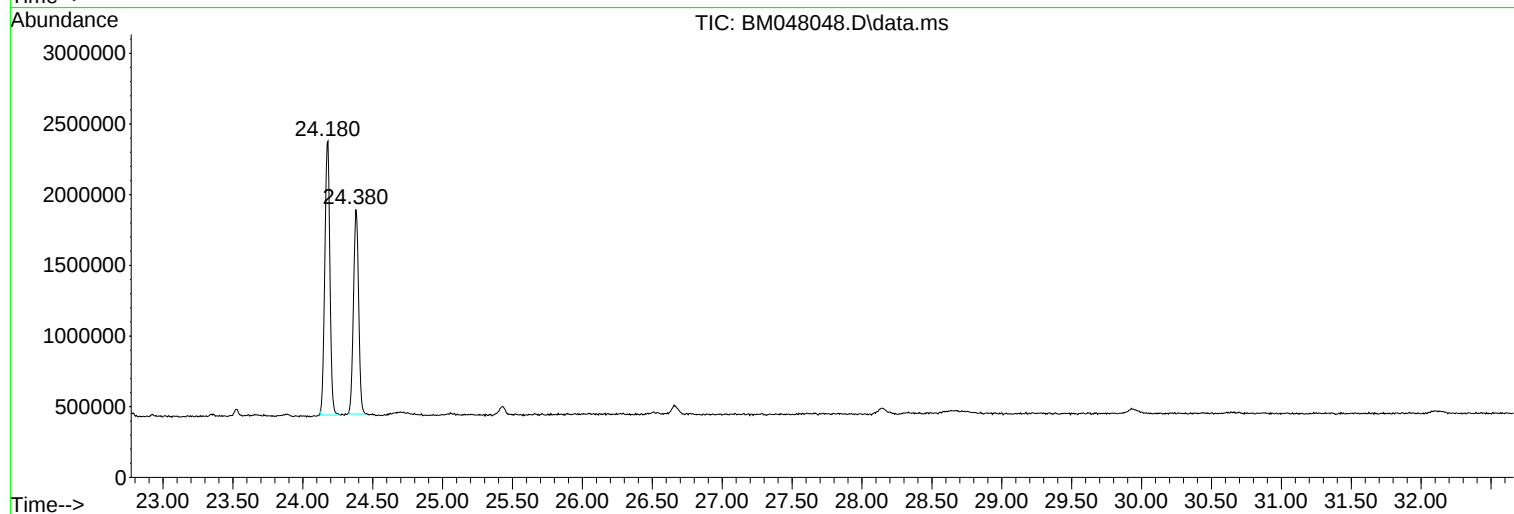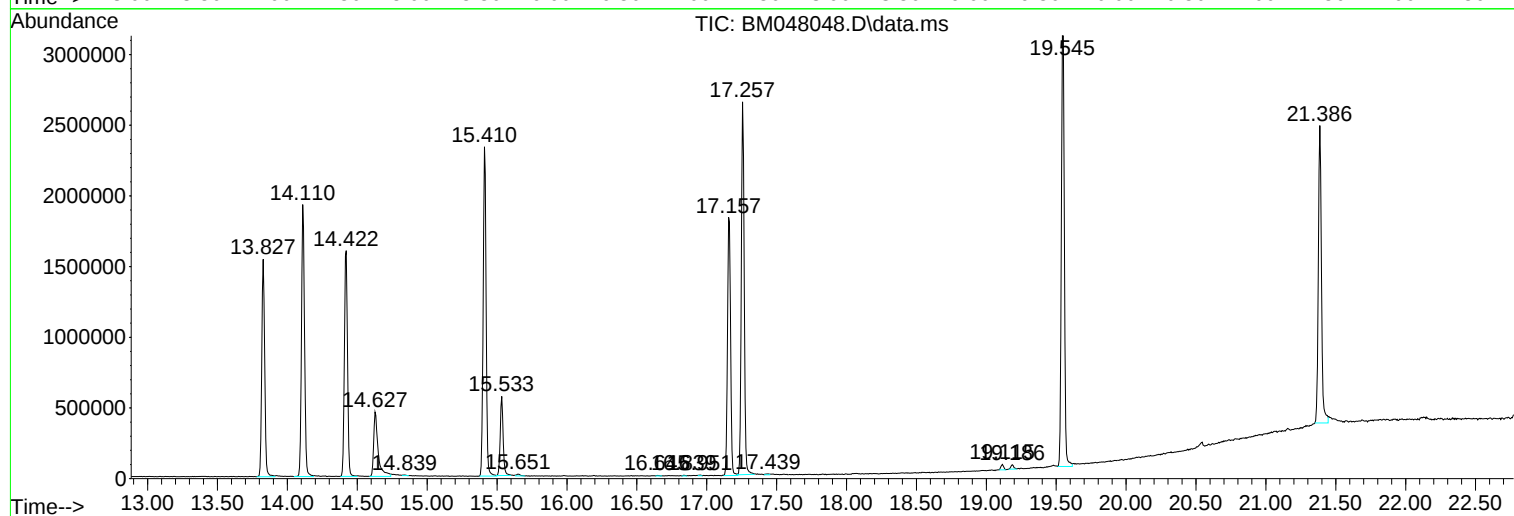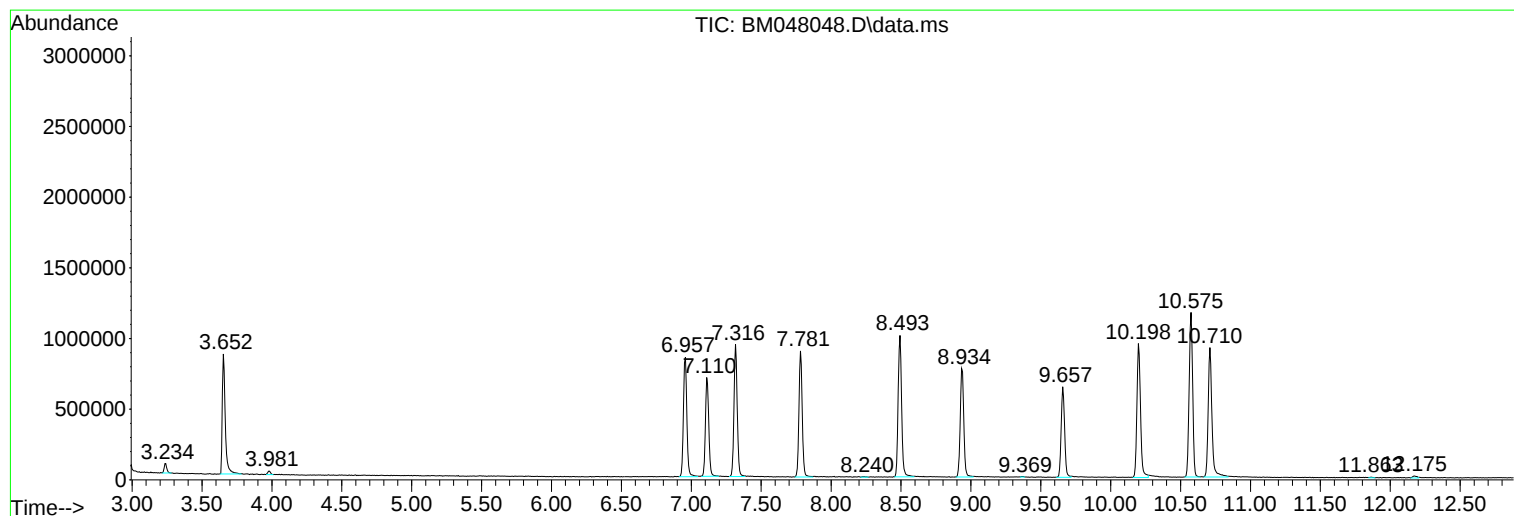

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101424\
Data File : BM048048.D
Acq On : 15 Oct 2024 04:46
Operator : RC/JU
Sample : PB163836BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK836

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101424\
Data File : BM048048.D
Acq On : 15 Oct 2024 04:46
Operator : RC/JU
Sample : PB163836BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK836

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM092724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------