
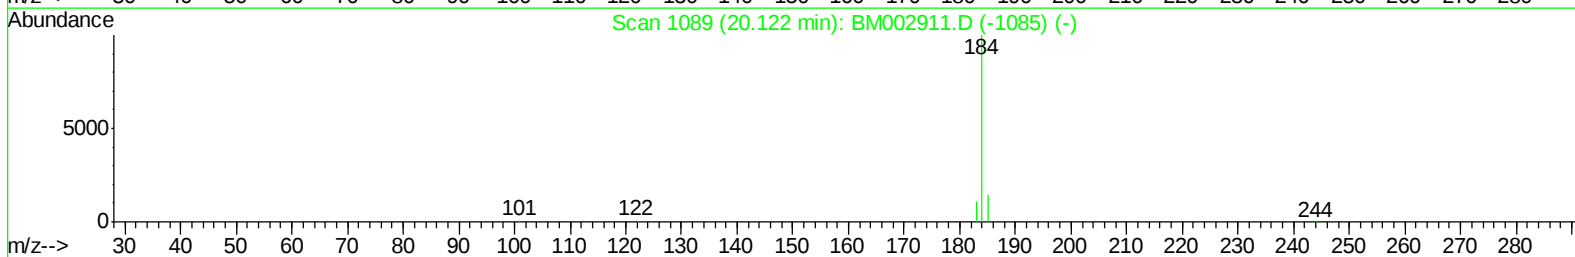
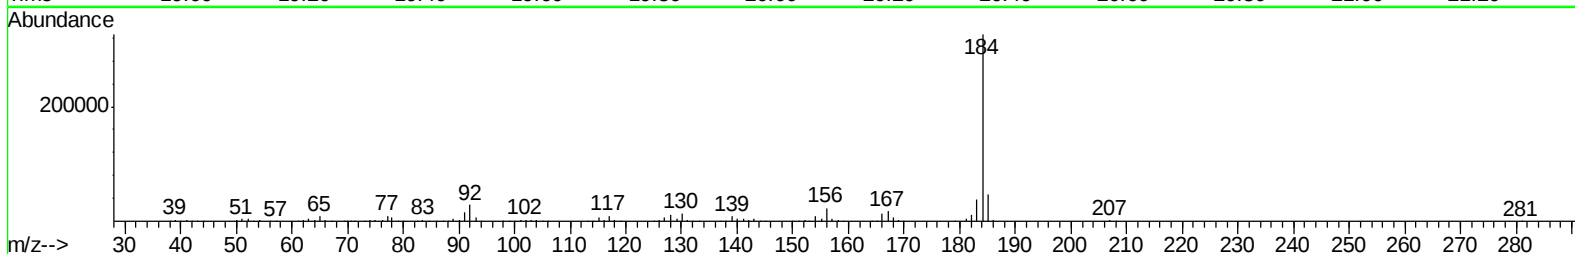


Data Path : Z:\HPCHEM1\BNA M\DATA\BM101515\  
Data File : BM002918.D  
Acq On : 15 Oct 2015 17:32  
Operator : UM/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 16 07:33:27 2015  
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-SIM-BM101515.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Oct 16 06:59:27 2015  
Response via : Initial Calibration

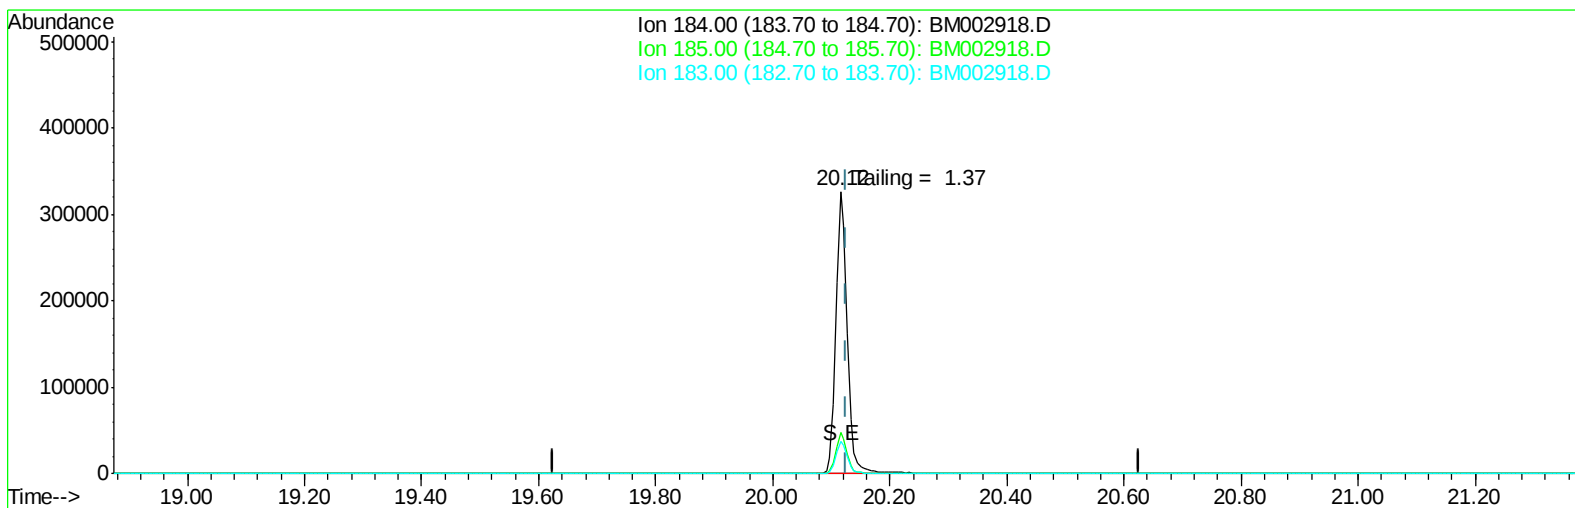

TIC: BM002918.D

(27) Benzidine




20.115min (-0.011) 0.00ng

response 436804

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.00 | 14.49 |
| 183.00 | 11.10 | 11.57 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA M\DATA\BM101515\  
Data File : BM002918.D  
Acq On : 15 Oct 2015 17:32  
Operator : UM/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 16 07:33:27 2015  
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-SIM-BM101515.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Oct 16 06:59:27 2015  
Response via : Initial Calibration

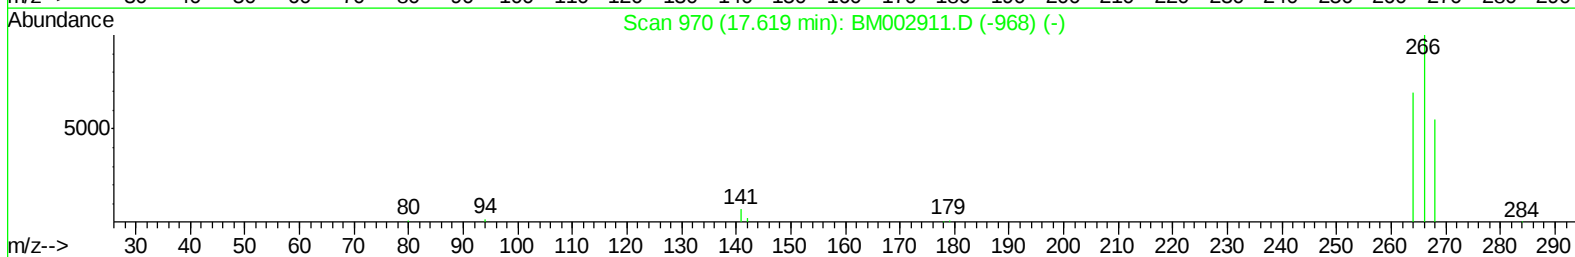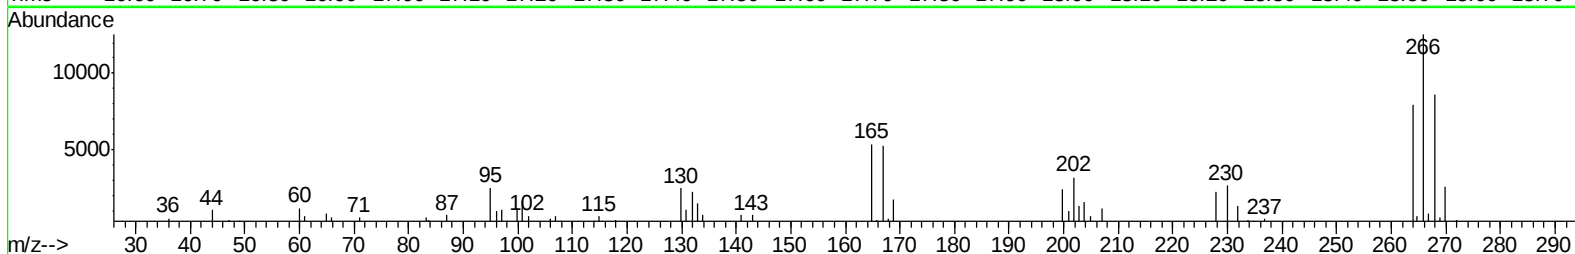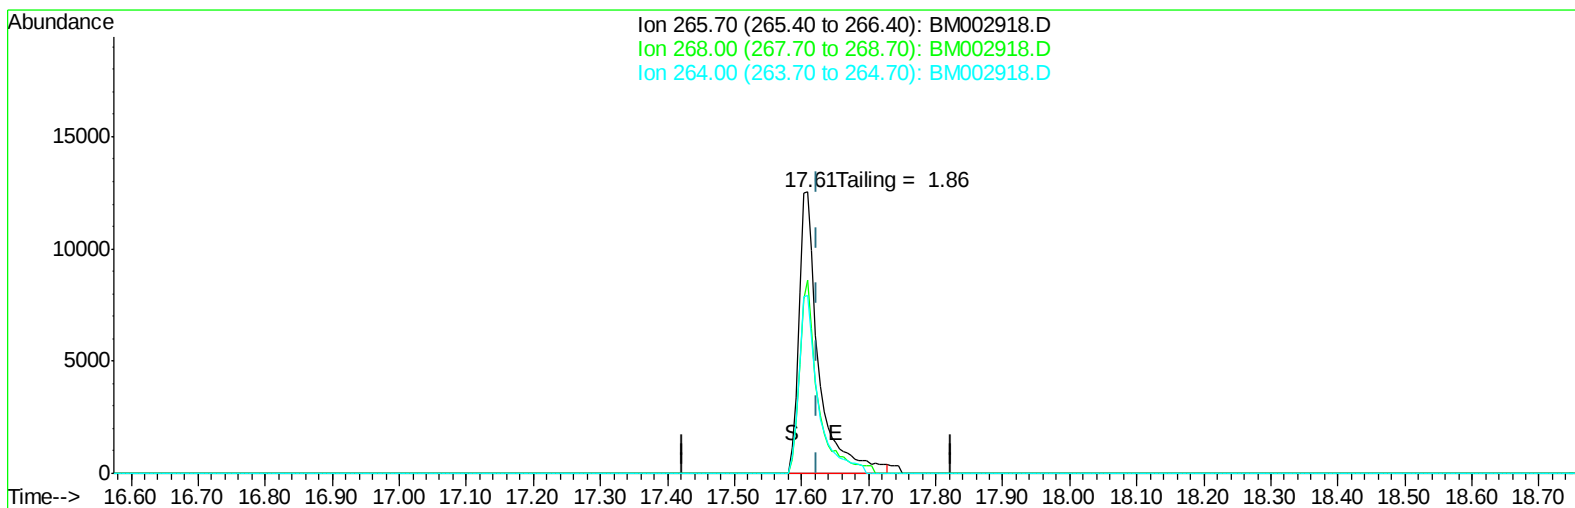

TIC: BM002918.D

(22) Pentachlorophenol

17.609min (-0.014) 0.00ng

response 26348

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 72.90 | 68.71 |
| 264.00 | 67.70 | 63.37 |
| 0.00   | 0.00  | 0.00  |