


Data Path : Z:\HPCHEM1\BNA M\DATA\BM101515\
 Data File : BM002905.D
 Acq On : 15 Oct 2015 09:01
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM101515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 15 16:21:18 2015

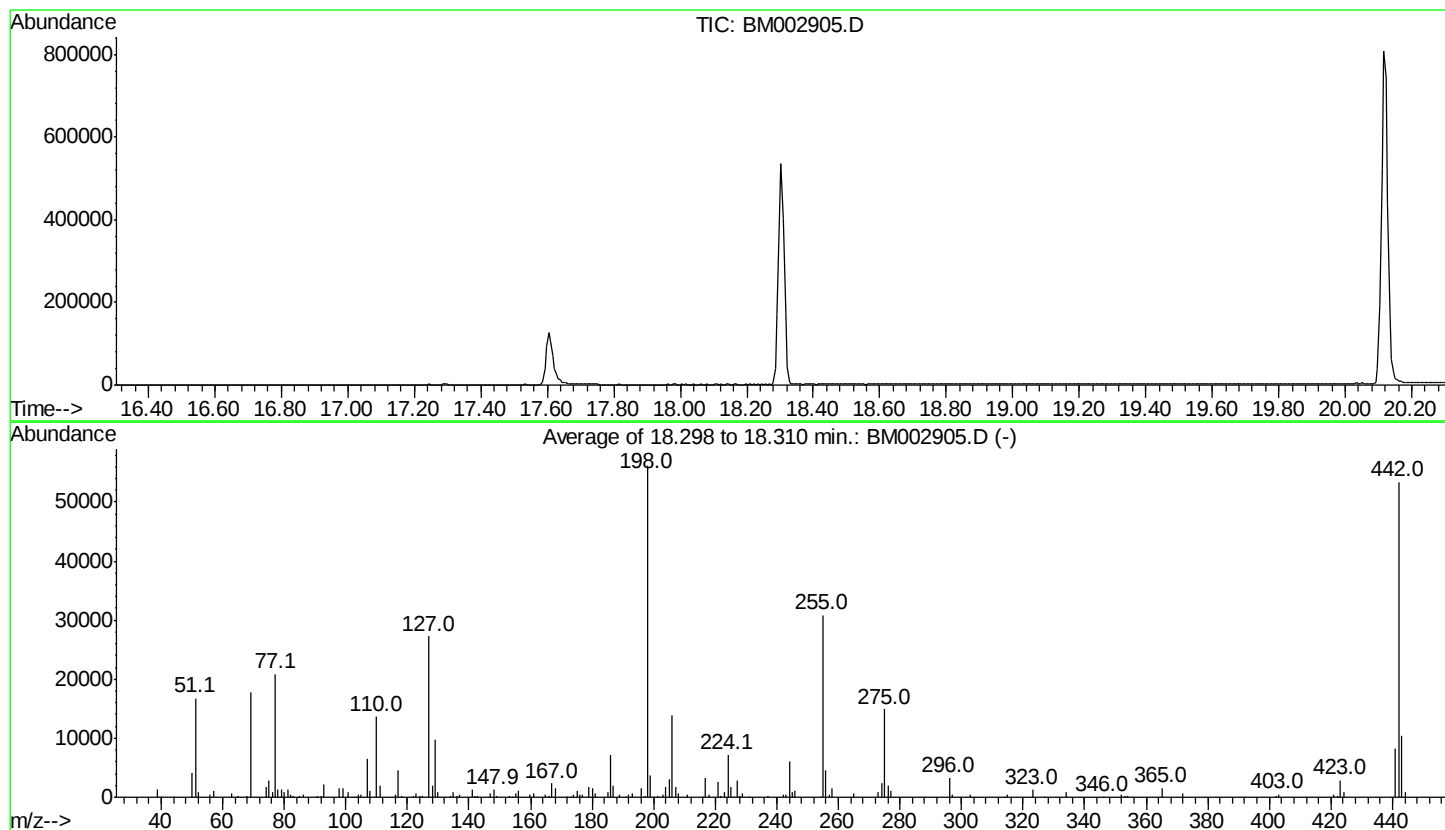

AutoFind: Scans 2586, 2587, 2588; Background Corrected with Scan 2580

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.8	16738	PASS
68	69	0.00	2	1.3	239	PASS
69	198	0.00	100	31.8	17843	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.5	27261	PASS
197	198	0.00	2	0.4	241	PASS
198	198	100	100	100.0	56173	PASS
199	198	5	9	6.7	3789	PASS
275	198	10	60	26.5	14873	PASS
365	198	1	100	2.8	1594	PASS
441	442	0.01	24	15.3	8182	PASS
442	198	50	100	95.2	53456	PASS
443	442	15	24	19.4	10386	PASS