

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101521\
 Data File : BM032543.D
 Acq On : 16 Oct 2021 01:43
 Operator : CG/JU
 Sample : M4029-20
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00T1

Quant Time: Oct 18 04:10:35 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 15 12:37:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.553	152	6661	0.40	ng/ul	0.00
4) Naphthalene-d8	10.339	136	19850	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.209	164	9296	0.40	ng/ul	0.00
13) Phenanthrene-d10	16.946	188	16609	0.40	ng/ul	0.00
17) Chrysene-d12	21.123	240	11883	0.40	ng/ul	-0.01
23) Perylene-d12	23.256	264	12795	0.40	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.923	96	11813	1.58	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.936	152	2409	0.09	ng/ul	0.00
18) Fluoranthene-d10	18.973	212	3935	0.11	ng/ul	0.00
Target Compounds						
						Qvalue
19) Fluoranthene	19.004	202	1400	0.02	ng/ul#	81
20) Pyrene	19.366	202	1349	0.02	ng/ul#	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101521\
Data File : BM032543.D
Acq On : 16 Oct 2021 01:43
Operator : CG/JU
Sample : M4029-20
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00T1

Quant Time: Oct 18 04:10:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 15 12:37:00 2021
Response via : Initial Calibration




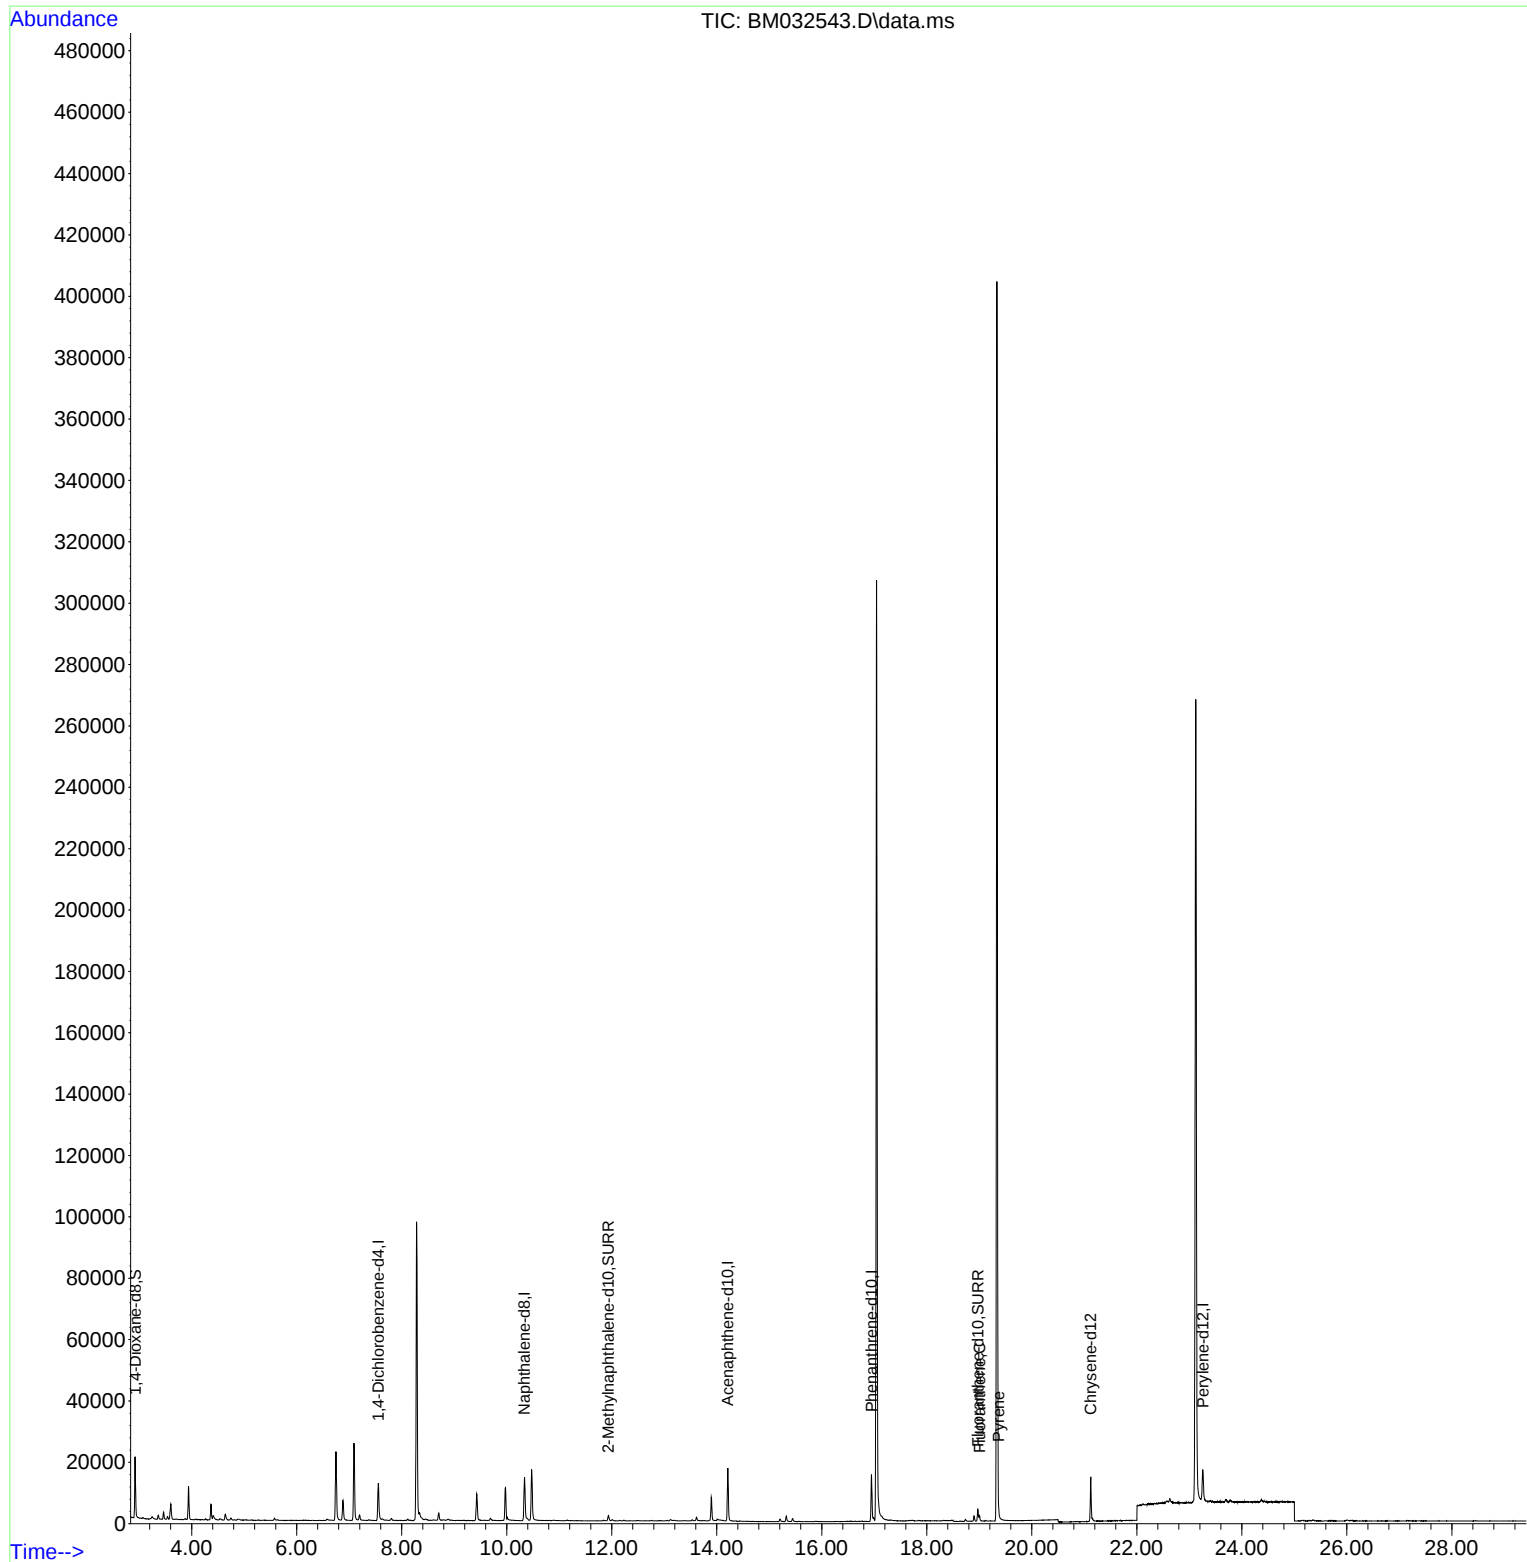


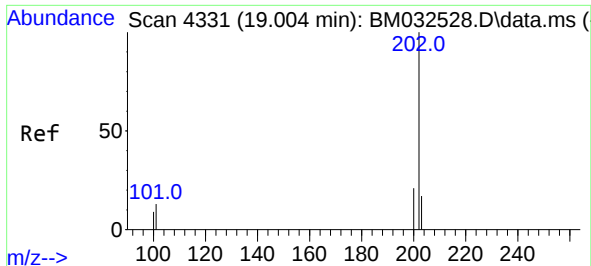

#19
Fluoranthene
Concen: 0.02 ng/ul
RT: 19.004 min Scan# 4331
Delta R.T. -0.008 min
Lab File: BM032543.D
Acq: 16 Oct 2021 01:43

Instrument :
BNA_M
ClientSampleId :
C00T1

Tgt Ion:	202	Resp:	1400
Ion	Ratio	Lower	Upper
202	100		
101	21.8	10.6	16.0#
100	16.0	7.8	11.8#

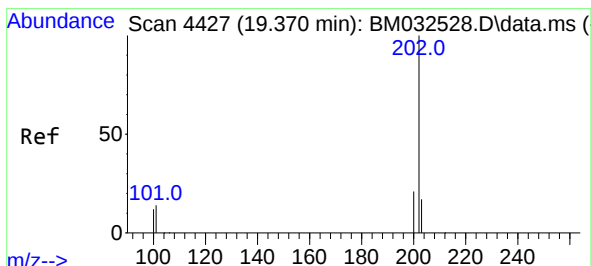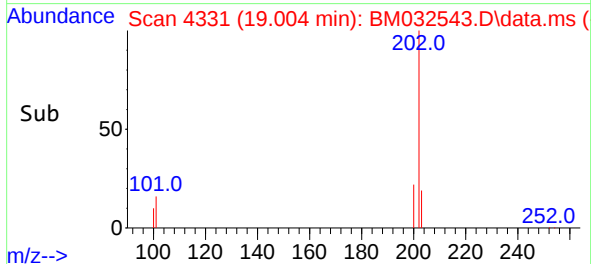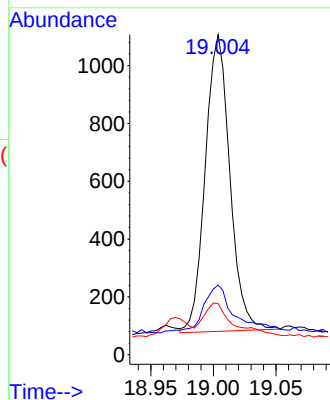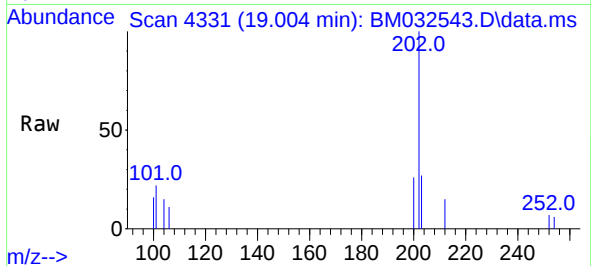

#20
Pyrene
Concen: 0.02 ng/ul
RT: 19.366 min Scan# 4426
Delta R.T. -0.008 min
Lab File: BM032543.D
Acq: 16 Oct 2021 01:43

Tgt Ion:	202	Resp:	1349
Ion	Ratio	Lower	Upper
202	100		
101	21.4	12.3	18.5#
100	20.9	10.1	15.1#

