

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101521\
 Data File : BM032549.D
 Acq On : 16 Oct 2021 05:58
 Operator : CG/JU
 Sample : M4110-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00T3

Quant Time: Oct 18 05:27:40 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 15 12:37:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.553	152	4431	0.40	ng/ul	0.00
4) Naphthalene-d8	10.339	136	13247	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.209	164	6632	0.40	ng/ul	0.00
13) Phenanthrene-d10	16.946	188	12330	0.40	ng/ul	0.00
17) Chrysene-d12	21.123	240	9503	0.40	ng/ul	-0.01
23) Perylene-d12	23.254	264	10785	0.40	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.920	96	11756	2.37	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.936	152	5561	0.31	ng/ul	0.00
18) Fluoranthene-d10	18.970	212	11902	0.40	ng/ul	-0.01
Target Compounds						
15) Phenanthrene	16.984	178	1278	0.03	ng/ul#	Qvalue 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101521\
Data File : BM032549.D
Acq On : 16 Oct 2021 05:58
Operator : CG/JU
Sample : M4110-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00T3


Quant Time: Oct 18 05:27:40 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 15 12:37:00 2021
Response via : Initial Calibration

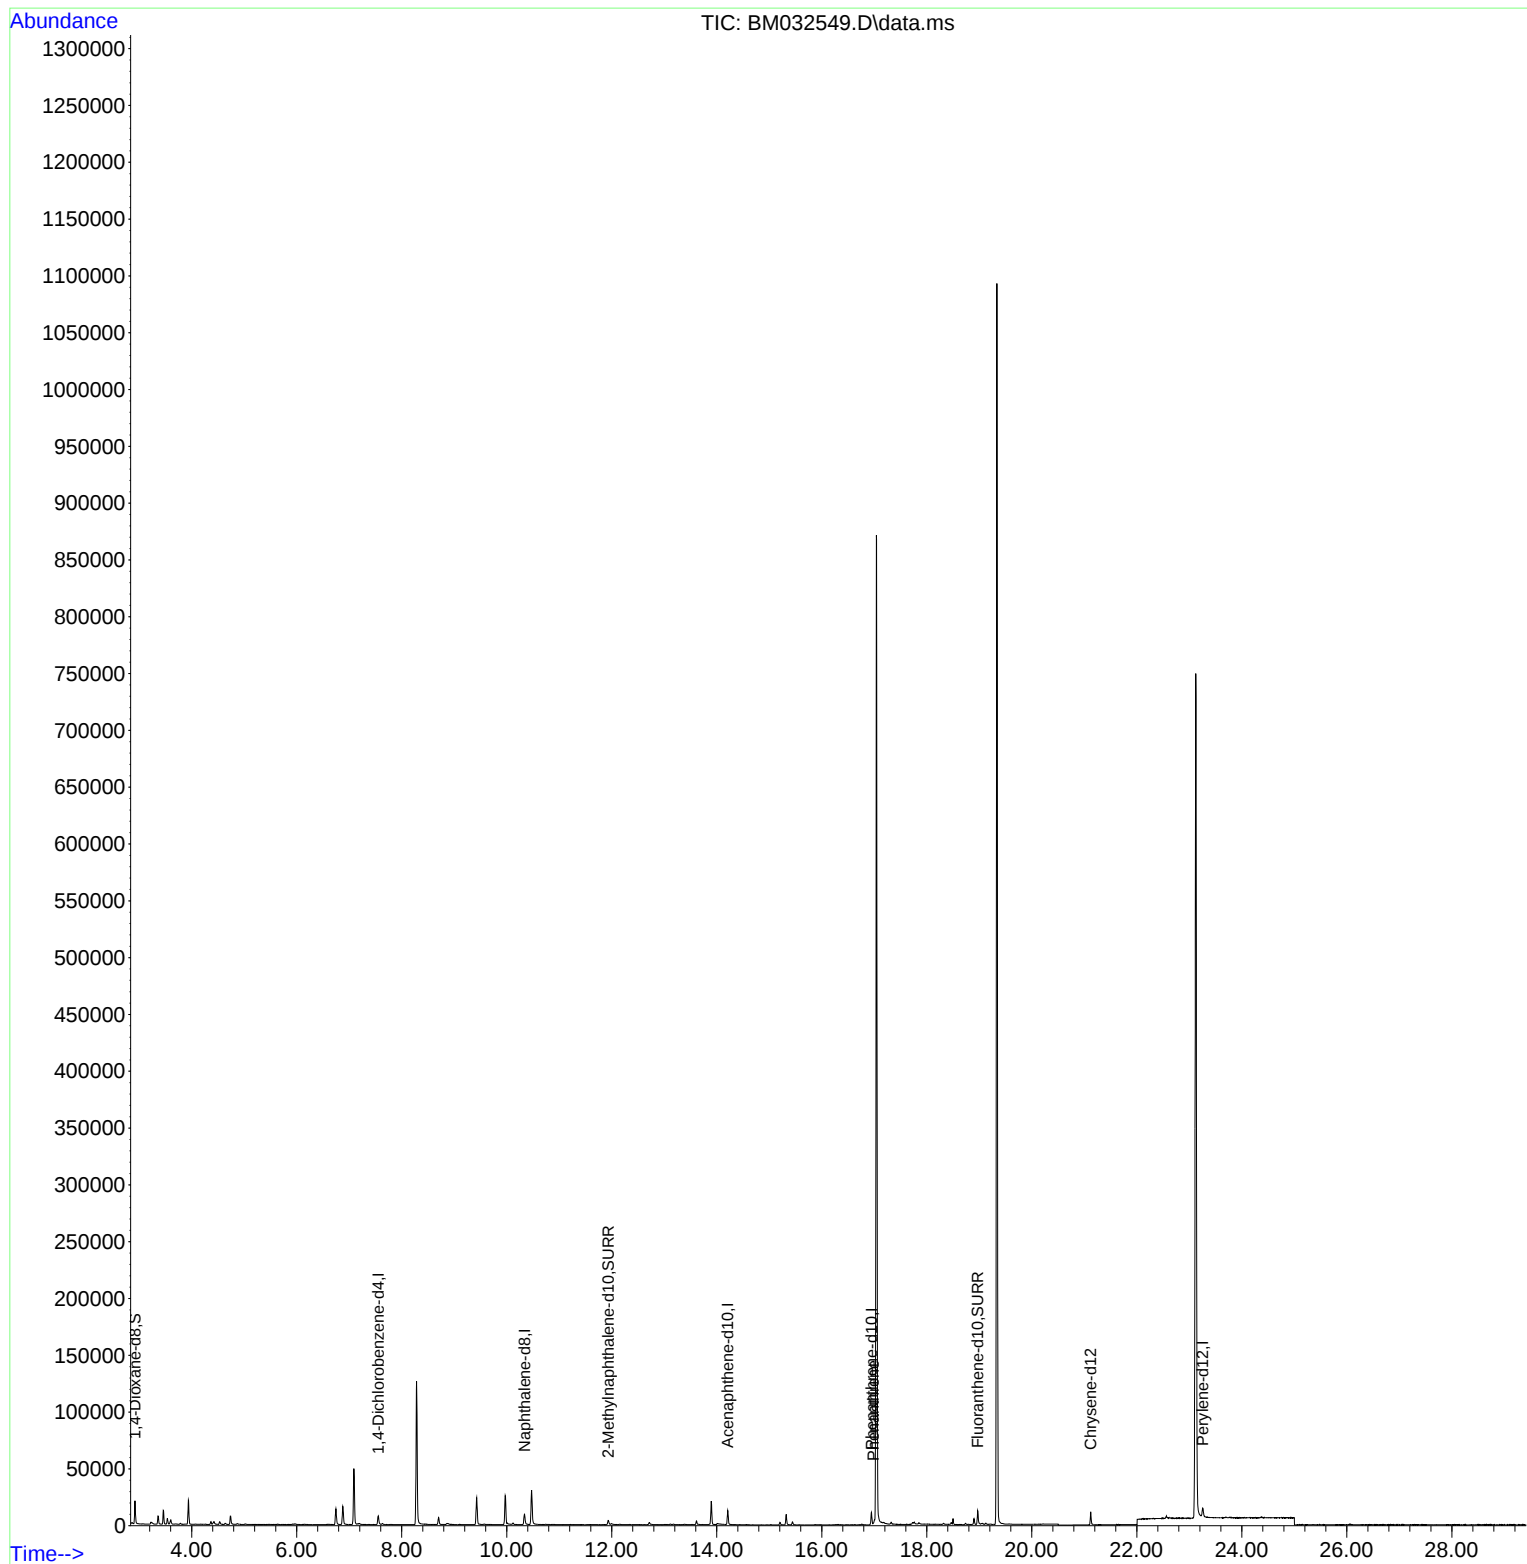

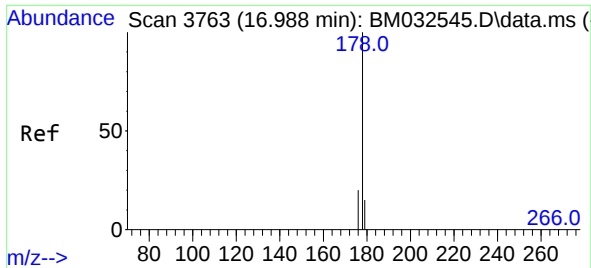

#15
 Phenanthrene
 Concen: 0.03 ng/ul
 RT: 16.984 min Scan# 3762
 Delta R.T. -0.010 min
 Lab File: BM032549.D
 Acq: 16 Oct 2021 05:58

Instrument :
 BNA_M
 ClientSampleId :
 C00T3

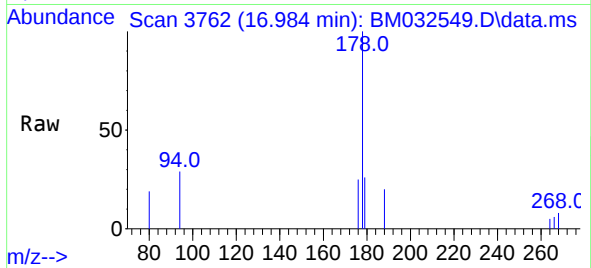

Tgt Ion:	178	Resp:	1278
Ion	Ratio	Lower	Upper
178	100		
179	26.1	12.9	19.3#
176	25.5	16.1	24.1#

