

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101521\
 Data File : BM032559.D
 Acq On : 16 Oct 2021 11:59
 Operator : CG/JU
 Sample : M4110-04
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00U1

Quant Time: Oct 18 05:29:05 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 15 12:37:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.553	152	6270	0.40	ng/ul	0.00
4) Naphthalene-d8	10.339	136	19250	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.209	164	9662	0.40	ng/ul	0.00
13) Phenanthrene-d10	16.946	188	16887	0.40	ng/ul	0.00
17) Chrysene-d12	21.123	240	9882	0.40	ng/ul	-0.01
23) Perylene-d12	23.259	264	11156	0.40	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.924	96	14571	2.07	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.931	152	8362	0.33	ng/ul	0.00
18) Fluoranthene-d10	18.973	212	15782	0.51	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	2.962	88	790	0.10	ng/ul#	81

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101521\
Data File : BM032559.D
Acq On : 16 Oct 2021 11:59
Operator : CG/JU
Sample : M4110-04
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00U1


Quant Time: Oct 18 05:29:05 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 15 12:37:00 2021
Response via : Initial Calibration

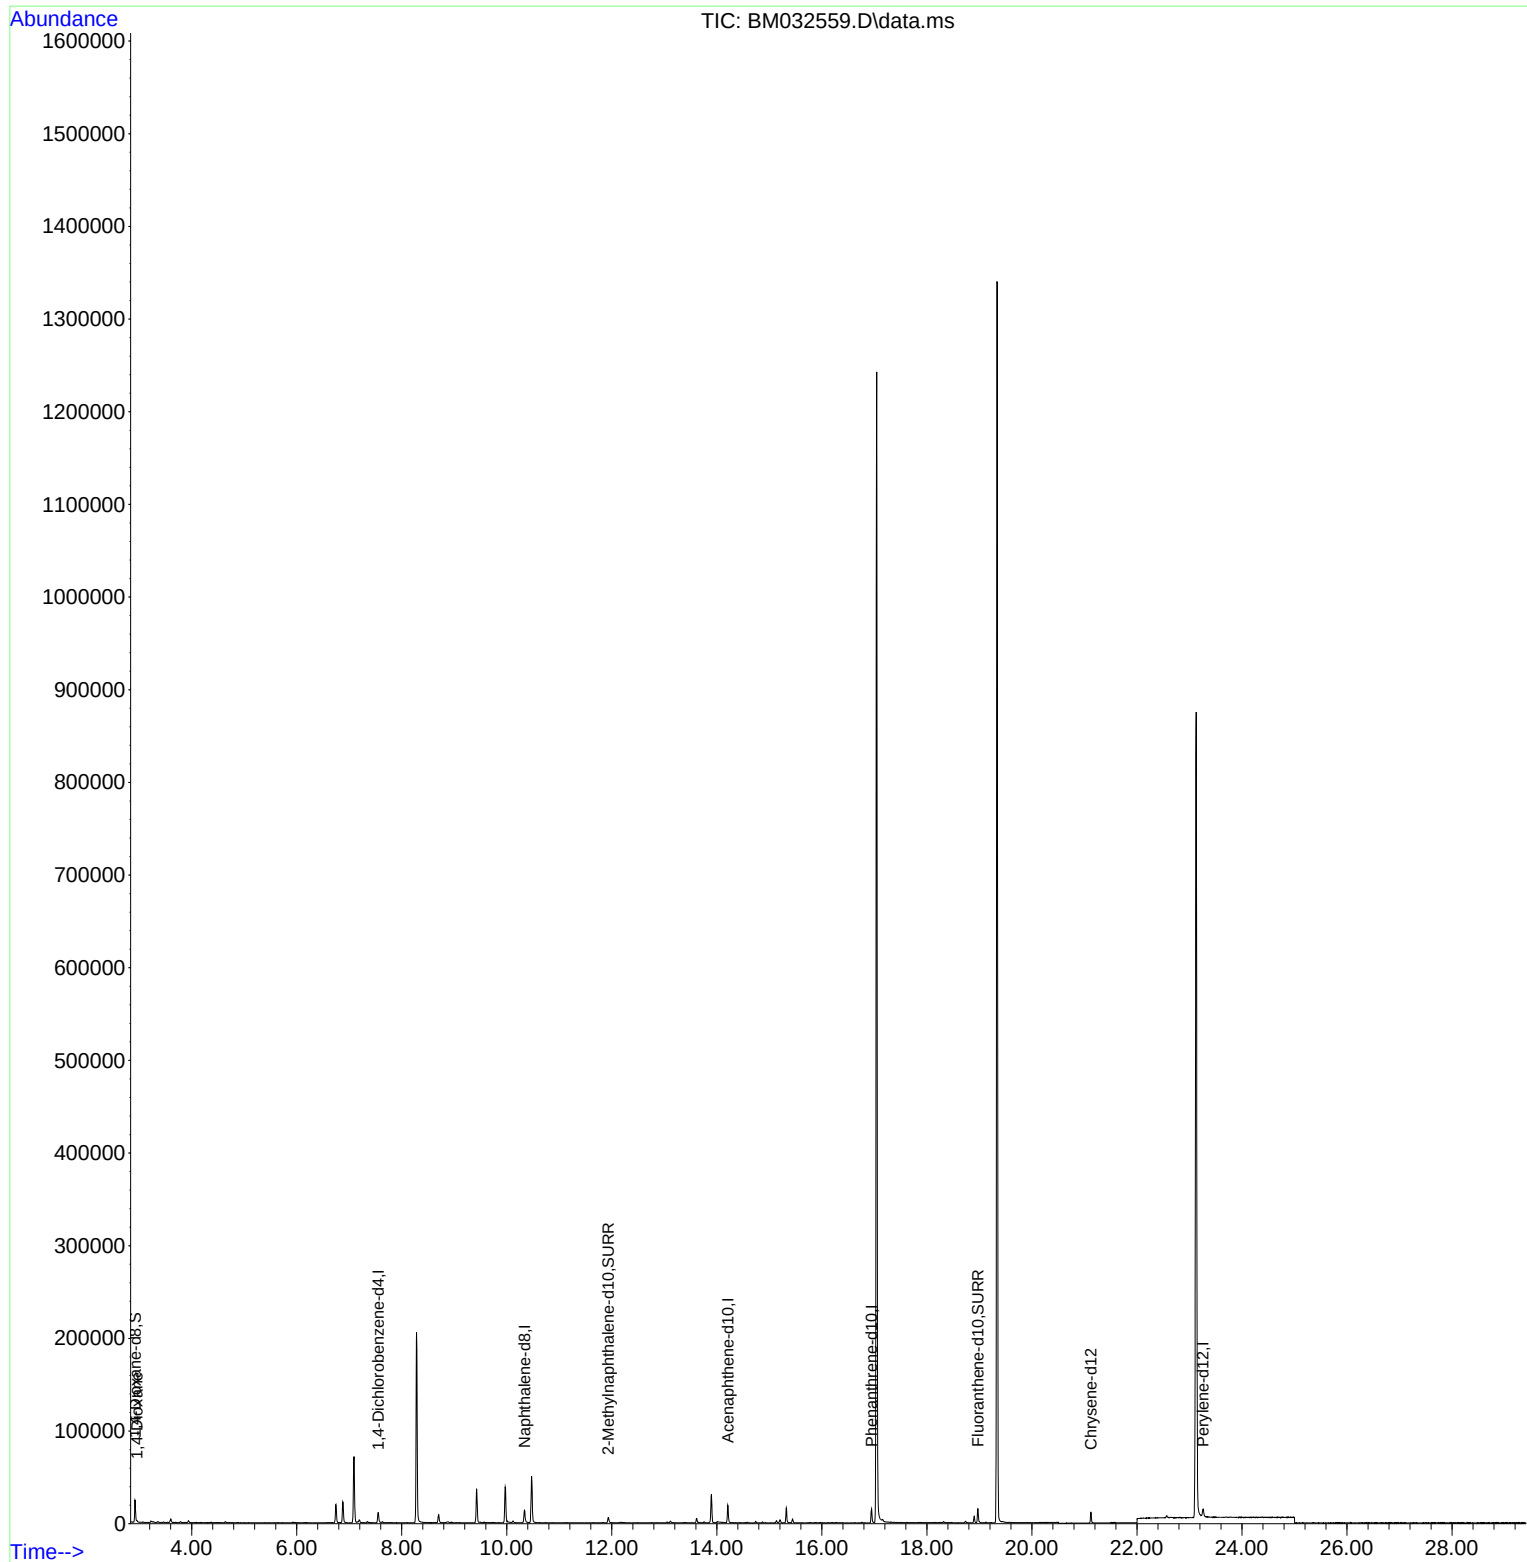


Abundance Scan 37 (2.961 min): BM032545.D\data.ms (-27)

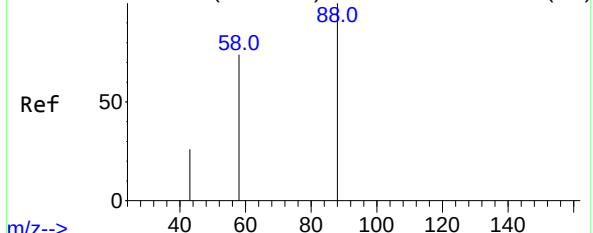

m/z-->

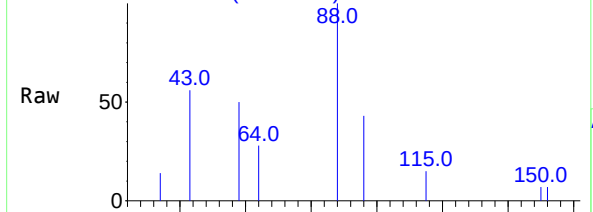


m/z-->

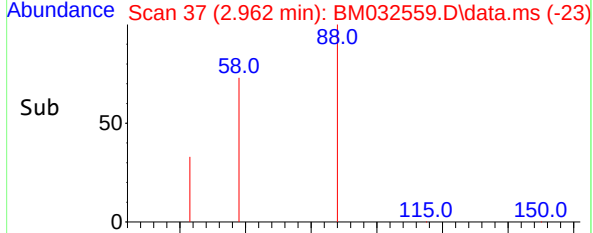

m/z-->

#2
1,4-Dioxane
Concen: 0.10 ng/ul
RT: 2.962 min Scan# 37
Delta R.T. 0.000 min
Lab File: BM032559.D
Acq: 16 Oct 2021 11:59

Tgt Ion:	88	Resp:	790
Ion	Ratio	Lower	Upper
88	100		
43	56.1	46.6	69.8
58	49.6	60.7	91.1#

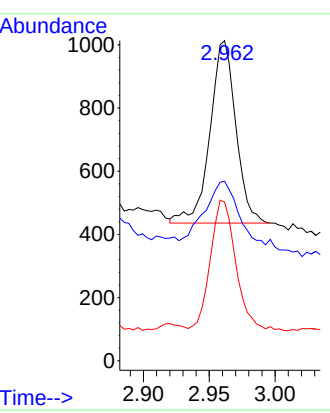

Instrument :
BNA_M
ClientSampleId :
C00U1