
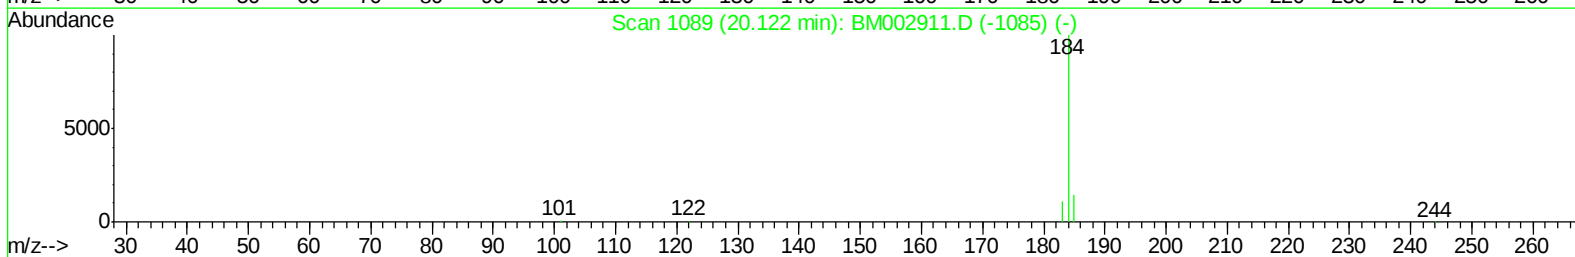
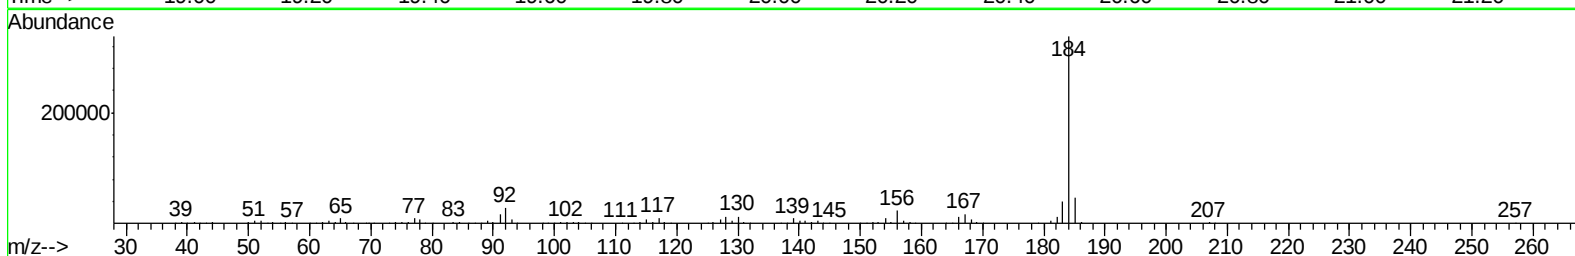


Data Path : Z:\HPCHEM1\BNA M\DATA\BM101615\
Data File : BM002929.D
Acq On : 16 Oct 2015 11:09
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 16 23:26:24 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-SIM-BM101515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 16 22:59:32 2015
Response via : Initial Calibration

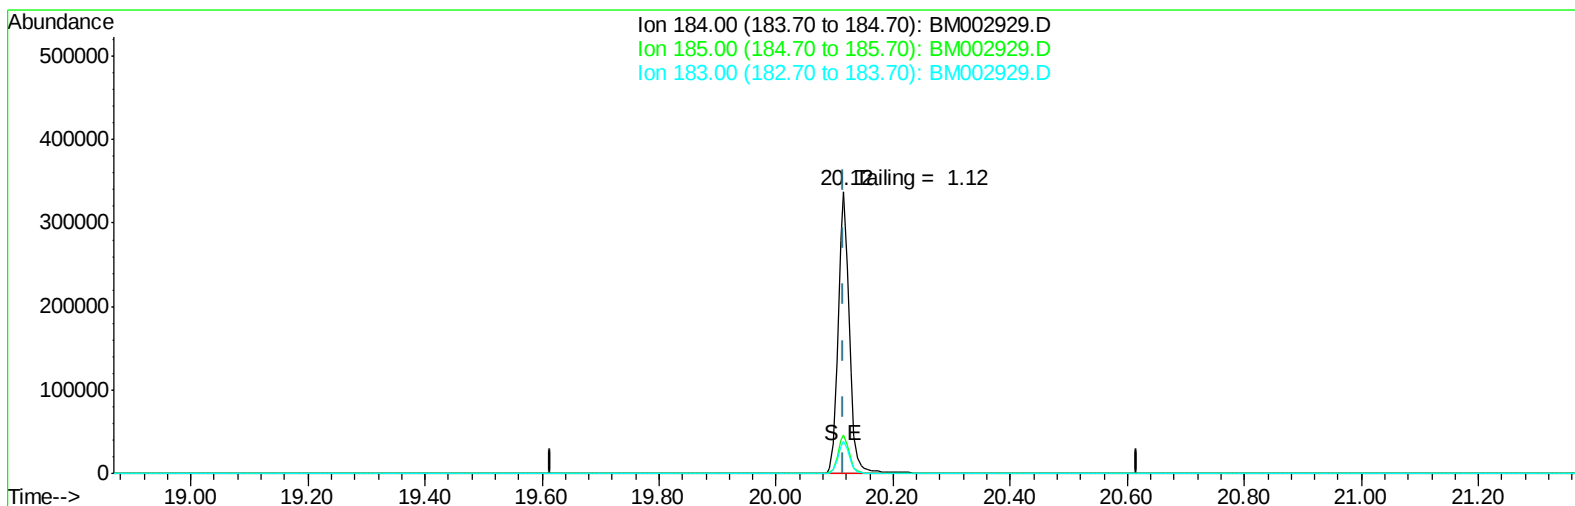

TIC: BM002929.D

(27) Benzidine




20.115min (-0.001) 0.00ng

response 448173

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	13.68
183.00	11.10	11.53
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM101615\
Data File : BM002929.D
Acq On : 16 Oct 2015 11:09
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 16 23:26:24 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-SIM-BM101515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 16 22:59:32 2015
Response via : Initial Calibration

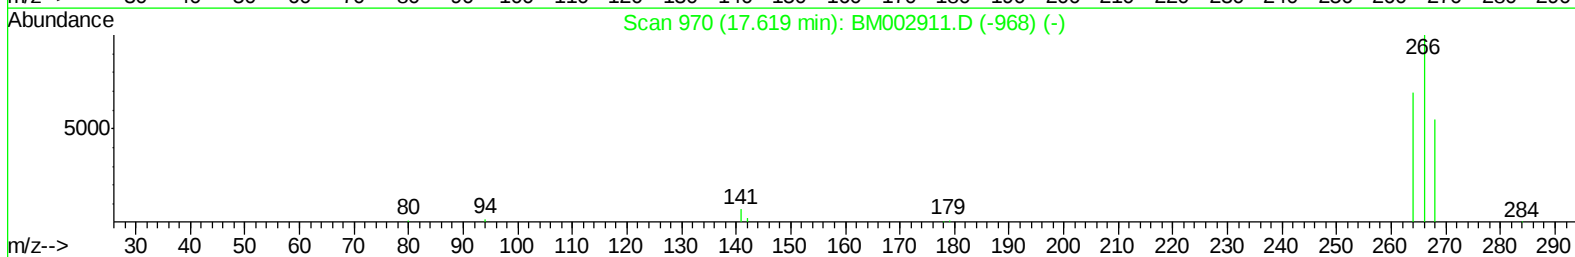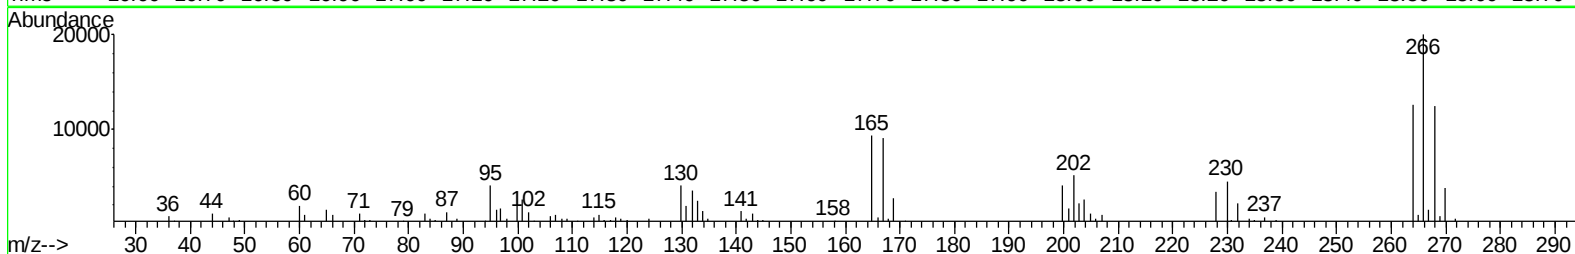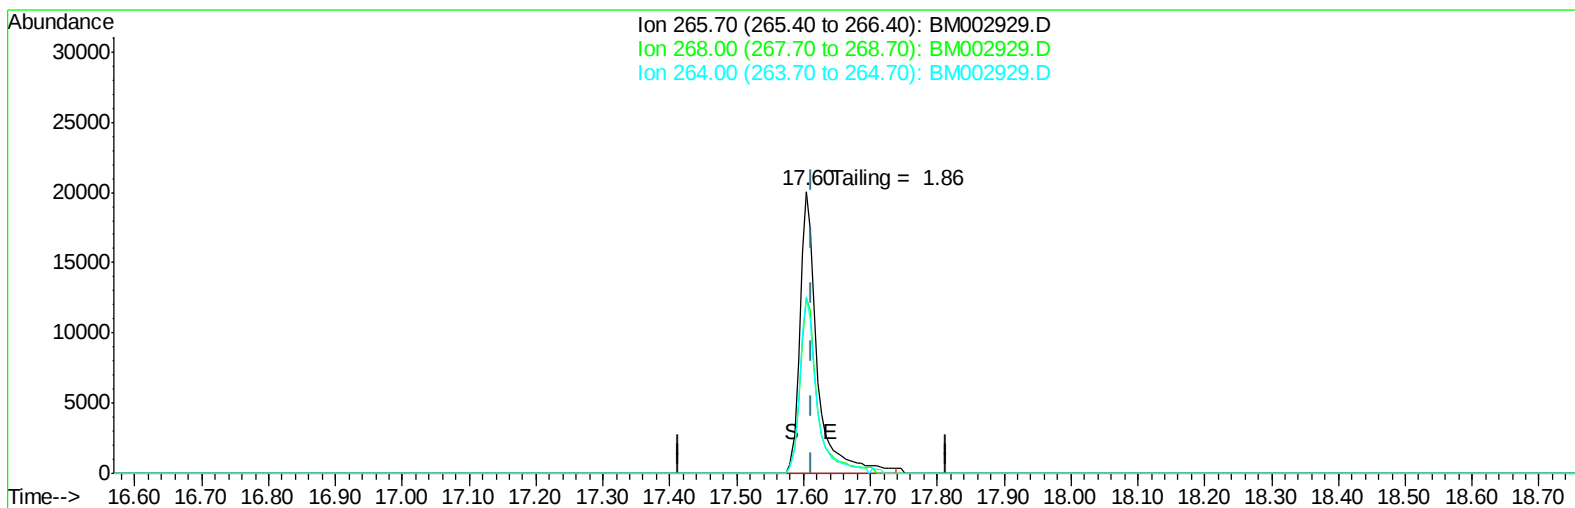

TIC: BM002929.D

(22) Pentachlorophenol

17.604min (-0.009) 0.00ng

response 37052

Ion	Exp%	Act%
265.70	100	100
268.00	72.90	62.40
264.00	67.70	62.78
0.00	0.00	0.00