

Data Path : Z:\HPCHEM1\BNA M\DATA\BM101615\  
 Data File : BM002935.D  
 Acq On : 16 Oct 2015 15:29  
 Operator : UM/IZ  
 Sample : G4037-05  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 RAV-GT-113

Quant Time: Oct 19 17:49:38 2015  
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-SIM-BM101515.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Oct 16 22:59:32 2015  
 Response via : Initial Calibration


| Internal Standards             | R.T.  | QIon | Response | Conc | Units | Dev(Min) |
|--------------------------------|-------|------|----------|------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4      | 8.66  | 152  | 99316    | 5.00 | ng    | 0.00     |
| 7) Naphthalene-d8              | 11.49 | 136  | 432584   | 5.00 | ng    | 0.00     |
| 13) Acenaphthene-d10           | 15.23 | 164  | 239449   | 5.00 | ng    | 0.00     |
| 19) Phenanthrene-d10           | 17.95 | 188  | 555549   | 5.00 | ng    | 0.00     |
| 26) Chrysene-d12               | 22.03 | 240  | 401516   | 5.00 | ng    | 0.00     |
| 35) Perylene-d12               | 24.61 | 264  | 357369   | 5.00 | ng    | 0.01     |
| System Monitoring Compounds    |       |      |          |      |       |          |
| 4) 2-Fluorophenol              | 6.12  | 112  | 51353    | 2.76 | ng    | -0.03    |
| 5) Phenol-d6                   | 7.79  | 99   | 46244    | 1.95 | ng    | 0.00     |
| 8) Nitrobenzene-d5             | 9.86  | 82   | 75112    | 3.62 | ng    | 0.00     |
| 14) 2,4,6-Tribromophenol       | 16.71 | 330  | 70478    | 7.53 | ng    | 0.00     |
| 15) 2-Fluorobiphenyl           | 13.87 | 172  | 245761   | 3.21 | ng    | 0.00     |
| 29) Terphenyl-d14              | 20.48 | 244  | 238363   | 3.97 | ng    | 0.00     |
| Target Compounds               |       |      |          |      |       | Qvalue   |
| 10) Naphthalene                | 11.54 | 128  | 180328   | 1.88 | ng    | 94       |
| 17) Acenaphthene               | 15.29 | 154  | 20909    | 0.29 | ng    | # 100    |
| 18) Fluorene                   | 16.27 | 166  | 27248    | 0.32 | ng    | # 95     |
| 25) Fluoranthene               | 19.96 | 202  | 6236     | 0.04 | ng    | # 91     |
| 28) Pyrene                     | 20.32 | 202  | 6225     | 0.05 | ng    | # 94     |
| 30) Benzo(a)anthracene         | 22.03 | 228  | 4681     | 0.04 | ng    | # 47     |
| 32) Chrysene                   | 22.07 | 228  | 4123m    | 0.04 | ng    |          |
| 33) Bis(2-ethylhexyl)phthalate | 21.85 | 149  | 7842     | 0.38 | ng    | # 83     |
| 34) Indeno(1,2,3-cd)pyrene     | 27.32 | 276  | 2320     | 0.02 | ng    | # 90     |
| 39) Dibenzo(a,h)anthracene     | 27.31 | 278  | 2648     | 0.03 | ng    | # 32     |
| 40) Benzo(g,h,i)perylene       | 28.16 | 276  | 1960     | 0.02 | ng    | # 35     |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM101615\  
Data File : BM002935.D  
Acq On : 16 Oct 2015 15:29  
Operator : UM/IZ  
Sample : G4037-05  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
RAV-GT-113

Quant Time: Oct 19 17:49:38 2015  
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-SIM-BM101515.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Oct 16 22:59:32 2015  
Response via : Initial Calibration

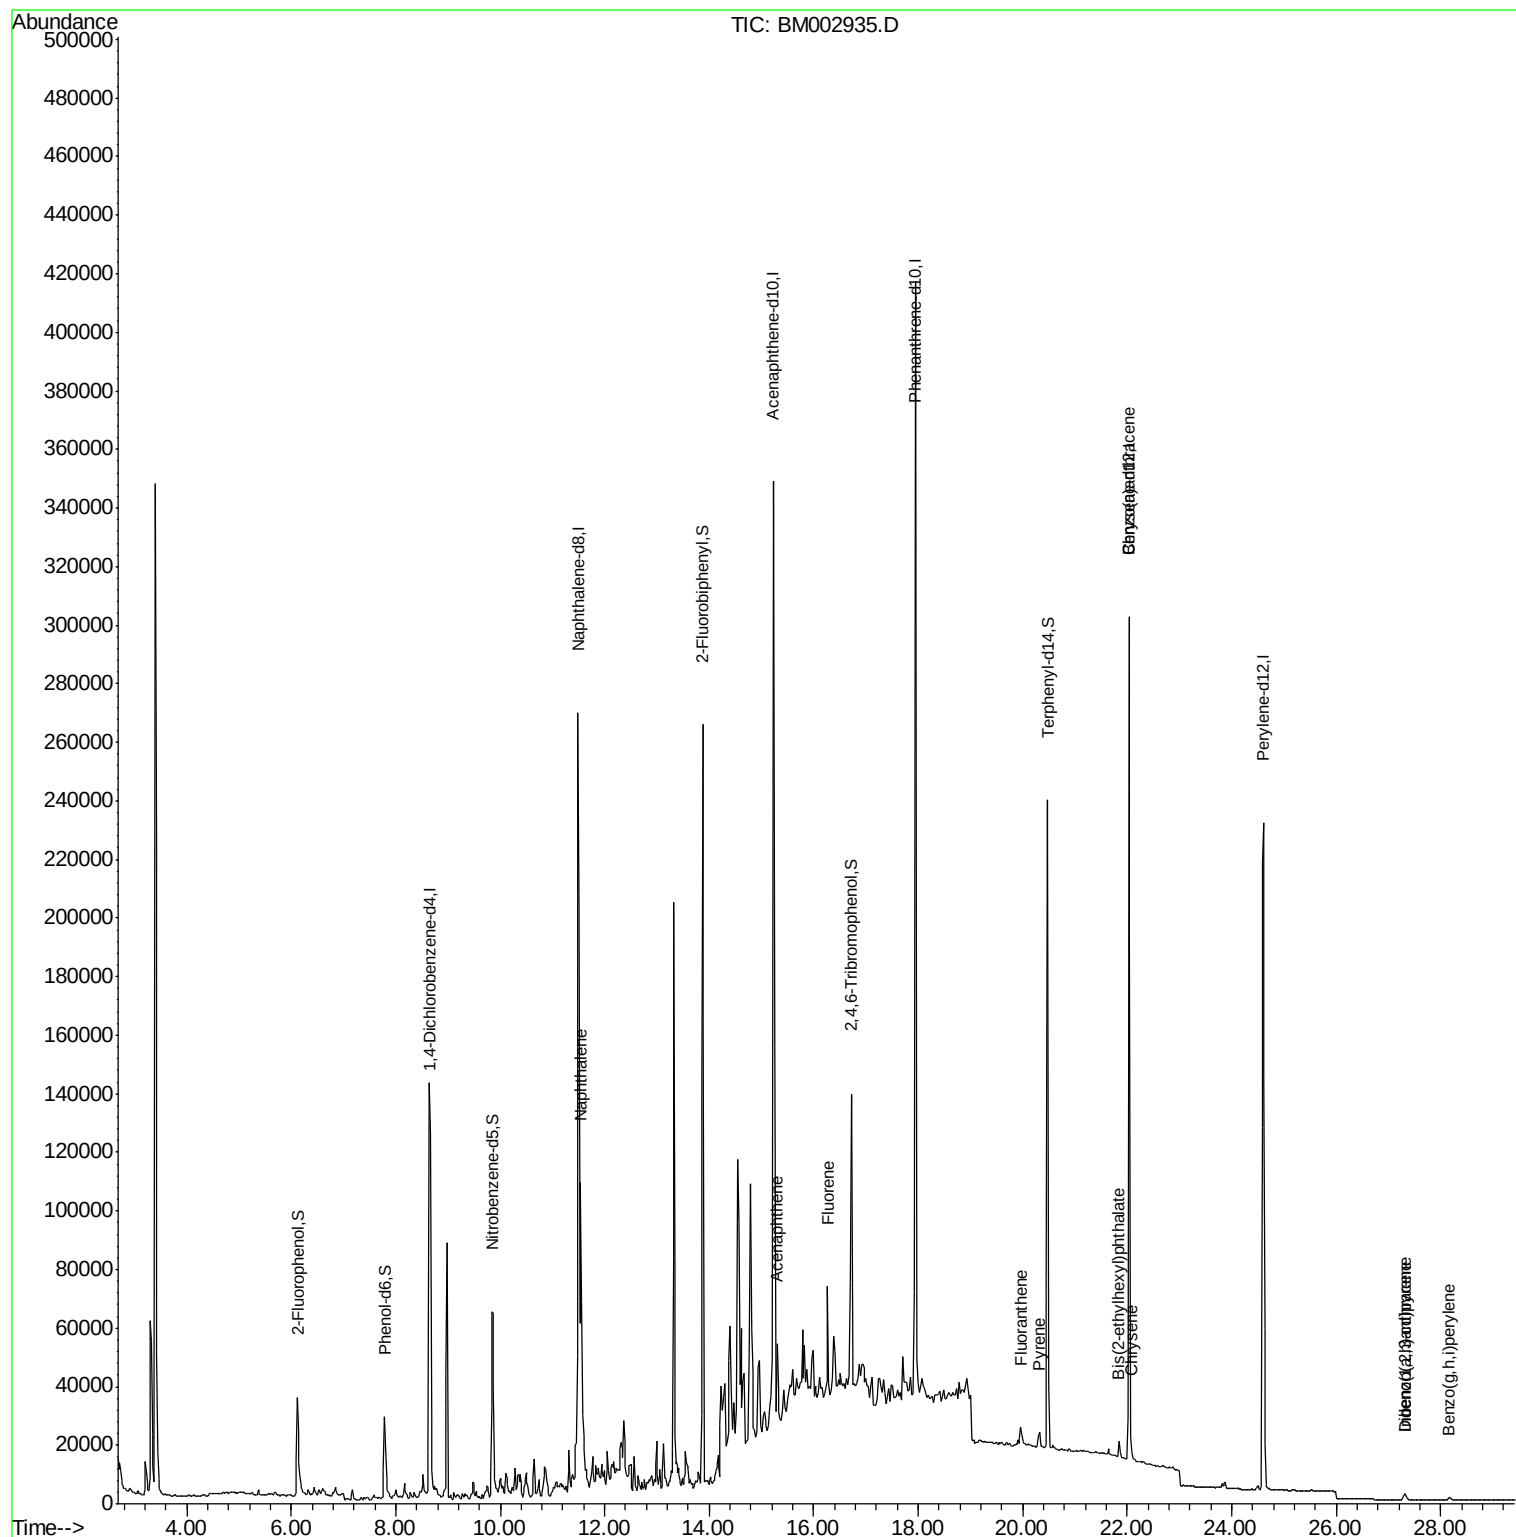



#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 8.66 min Scan# 377

Delta R.T. -0.00 min

Lab File: BM002935.D

Acq: 16 Oct 2015 15:29

Instrument :

BNA\_M

ClientSampleId :

RAV-GT-113


Tot Ion:152 Resp: 99316

Ion Ratio Lower Upper

152 100

150 139.2 113.0 169.6




115 47.9 37.9 56.9

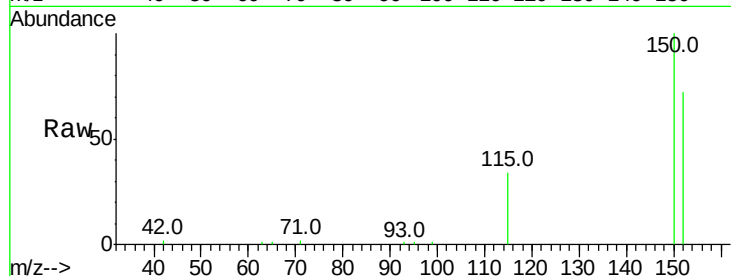

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

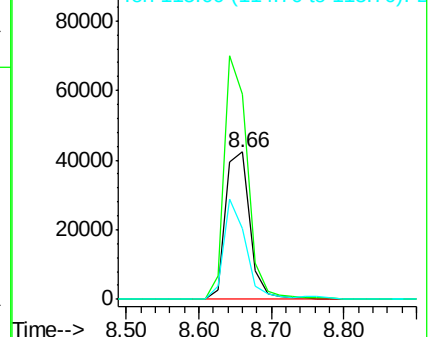

#4

2-Fluorophenol

Concen: 2.76 ng

RT: 6.12 min Scan# 223

Delta R.T. -0.03 min

Lab File: BM002935.D

Acq: 16 Oct 2015 15:29


Tgt Ion:112 Resp: 51353

Ion Ratio Lower Upper

112 100

64 51.1 42.0 63.0



63 24.3 20.0 30.0




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

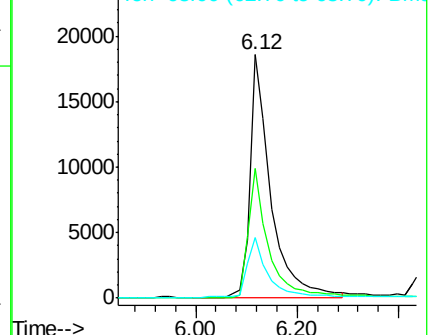



#5

Phenol-d6

Concen: 1.95 ng

RT: 7.79 min Scan# 326

Delta R.T. -0.00 min

Lab File: BM002935.D

Acq: 16 Oct 2015 15:29

Instrument :

BNA\_M

ClientSampleId :

RAV-GT-113


Tot Ion: 99 Resp: 46244

Ion Ratio Lower Upper

99 100

42 15.5 12.4 18.6

71 37.2 21.4 32.0#



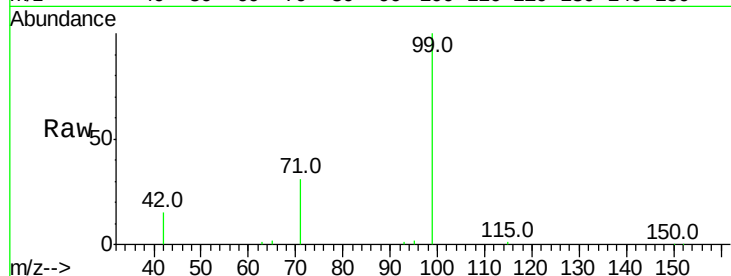


Abundance Ion 99.00 (98.70 to 99.70): BM002911.D (-320) (-)

Ion 42.00 (41.70 to 42.70): BM002911.D (-320) (-)

Ion 71.00 (70.70 to 71.70): BM002911.D (-320) (-)

Time-->

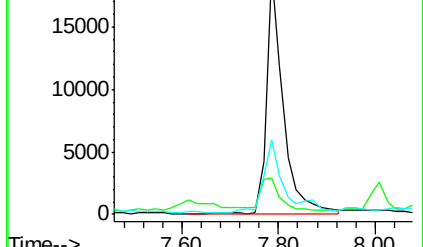

#7

Naphthalene-d8

Concen: 5.00 ng

RT: 11.49 min Scan# 599

Delta R.T. -0.00 min

Lab File: BM002935.D

Acq: 16 Oct 2015 15:29

Tgt Ion: 136 Resp: 432584


Ion Ratio Lower Upper

136 100

137 10.4 9.1 13.7

54 10.0 3.5 5.3#

68 8.7 3.3 4.9#





Abundance Ion 136.00 (135.70 to 136.70): BM002911.D (-593) (-)


Ion 137.00 (136.70 to 137.70): BM002911.D (-593) (-)

Ion 54.00 (53.70 to 54.70): BM002911.D (-593) (-)

Ion 68.00 (67.70 to 68.70): BM002911.D (-593) (-)

Time-->




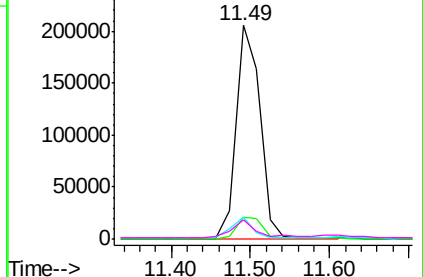


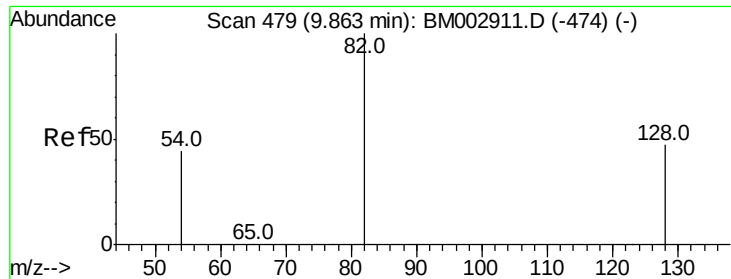

#8  
 Nitrobenzene-d5  
 Concen: 3.62 ng  
 RT: 9.86 min Scan# 479  
 Delta R.T. -0.00 min  
 Lab File: BM002935.D  
 Acq: 16 Oct 2015 15:29




Instrument :  
 BNA\_M  
 ClientSampleId :  
 RAV-GT-113


Tot Ion: 82 Resp: 75112  
 Ion Ratio Lower Upper  
 82 100  
 128 55.2 34.1 51.1#  
 54 39.7 42.6 63.8#

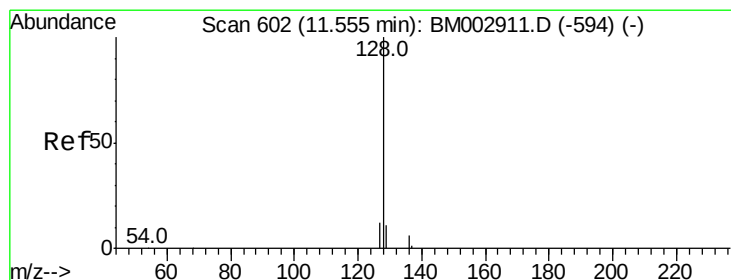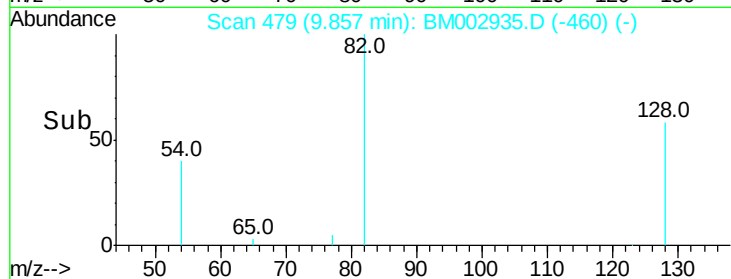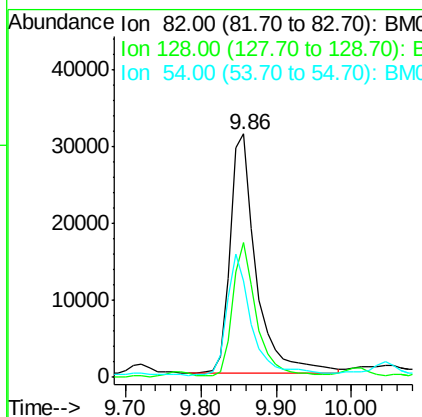

#10  
 Naphthalene  
 Concen: 1.88 ng  
 RT: 11.54 min Scan# 602  
 Delta R.T. -0.00 min  
 Lab File: BM002935.D  
 Acq: 16 Oct 2015 15:29

Tgt Ion: 128 Resp: 180328  
 Ion Ratio Lower Upper  
 128 100  
 129 13.9 9.4 14.2  
 127 14.3 9.6 14.4

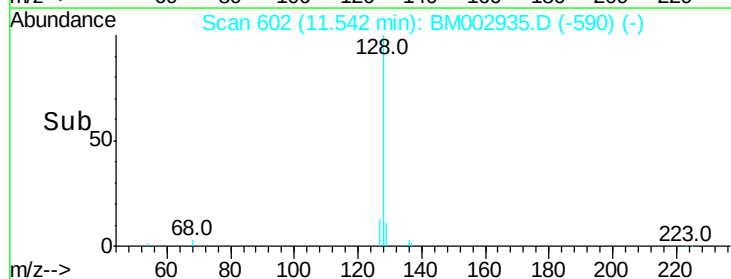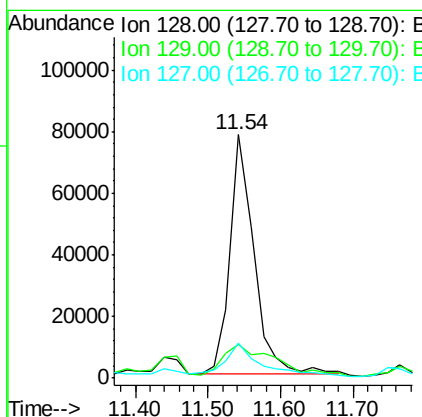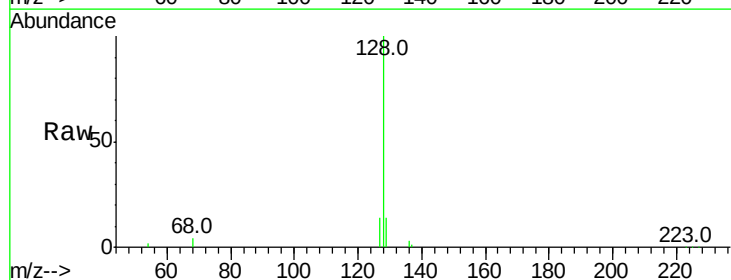

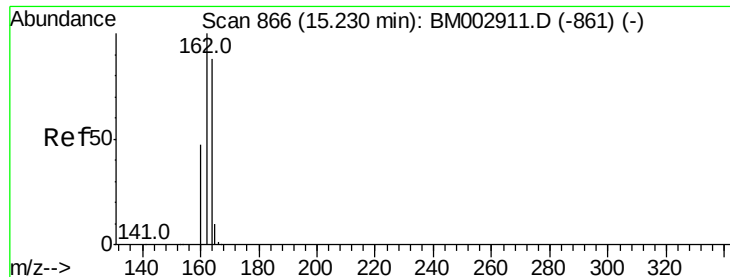

#13

Acenaphthene-d10

Concen: 5.00 ng

RT: 15.23 min Scan# 867

Delta R.T. -0.00 min

Lab File: BM002935.D

Acq: 16 Oct 2015 15:29

Instrument :

BNA\_M

ClientSampleId :

RAV-GT-113


Tot Ion:164 Resp: 239449

Ion Ratio Lower Upper

164 100

162 112.5 79.6 119.4




160 57.6 33.1 49.7#

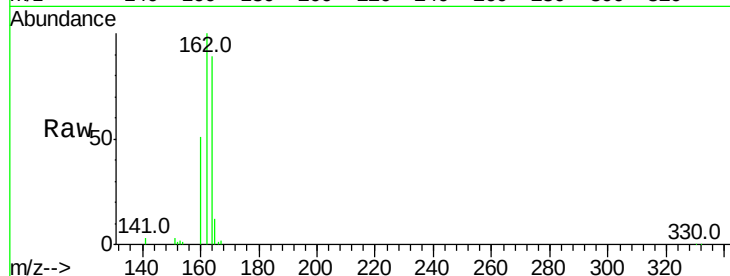

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

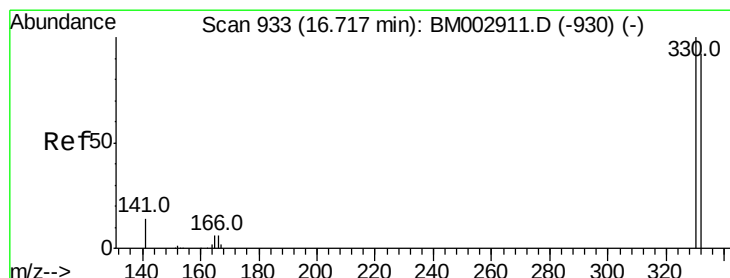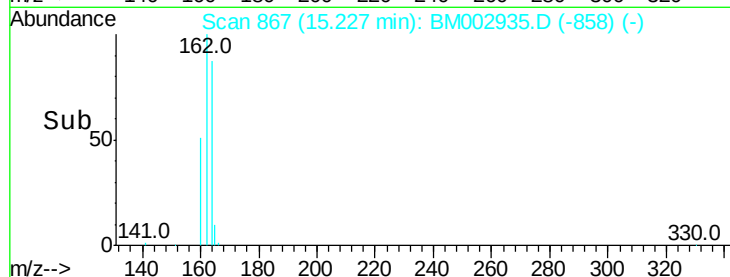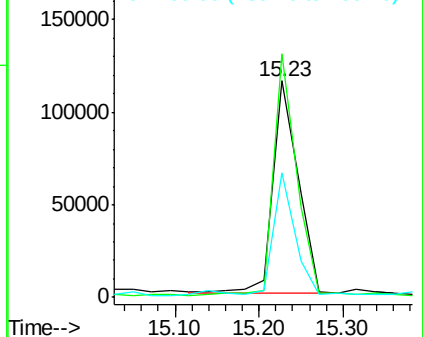

#14

2,4,6-Tribromophenol

Concen: 7.53 ng

RT: 16.71 min Scan# 934

Delta R.T. -0.00 min

Lab File: BM002935.D

Acq: 16 Oct 2015 15:29


Tgt Ion:330 Resp: 70478

Ion Ratio Lower Upper

330 100

332 97.4 76.6 115.0



141 0.0 0.0 0.0

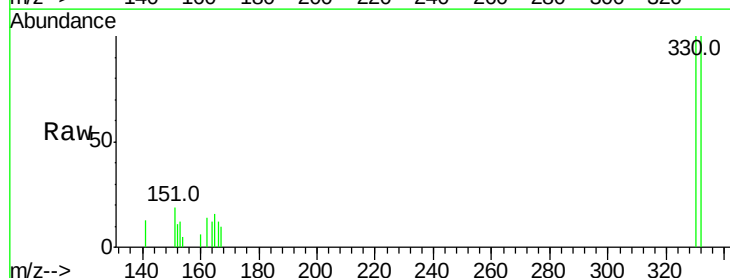


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



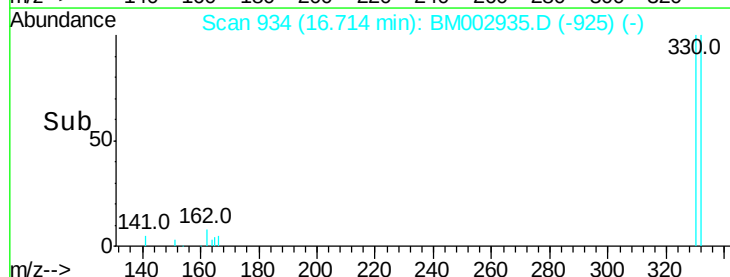
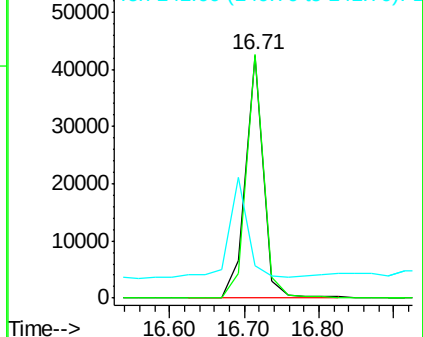


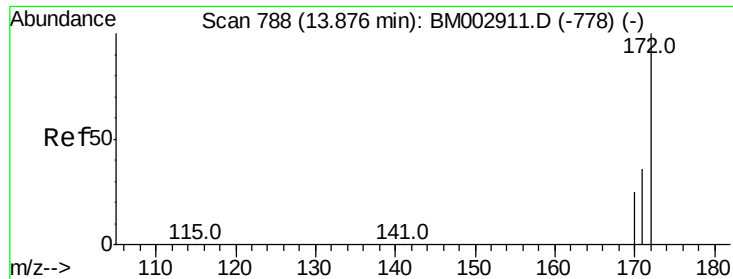

#15  
2-Fluorobiphenyl  
Concen: 3.21 ng  
RT: 13.87 min Scan# 789  
Delta R.T. -0.00 min  
Lab File: BM002935.D  
Acq: 16 Oct 2015 15:29




Instrument :  
BNA\_M  
ClientSampleId :  
RAV-GT-113


Tot Ion:172 Resp: 245761  
Ion Ratio Lower Upper  
172 100  
171 34.8 26.1 39.1  
170 22.6 15.7 23.5

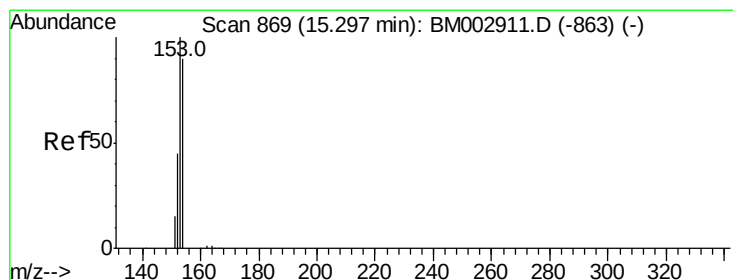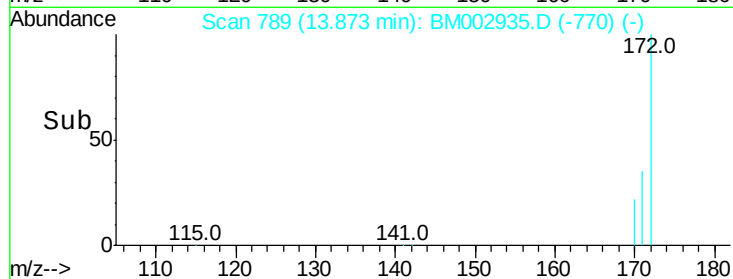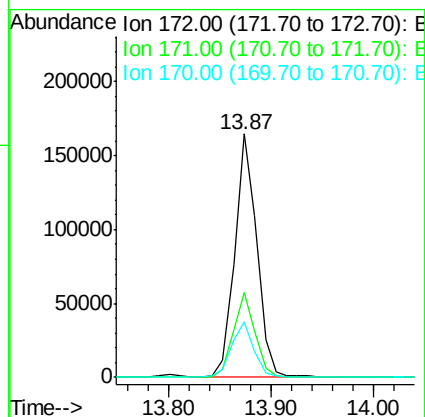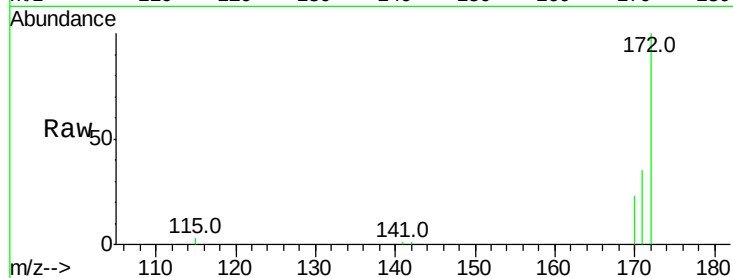

#17  
Acenaphthene  
Concen: 0.29 ng  
RT: 15.29 min Scan# 870  
Delta R.T. -0.00 min  
Lab File: BM002935.D  
Acq: 16 Oct 2015 15:29

Tgt Ion:154 Resp: 20909  
Ion Ratio Lower Upper  
154 100  
153 91.6 0.0 0.0#  
152 59.6 0.0 0.0#

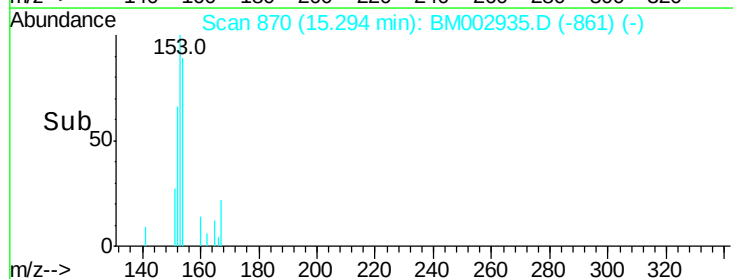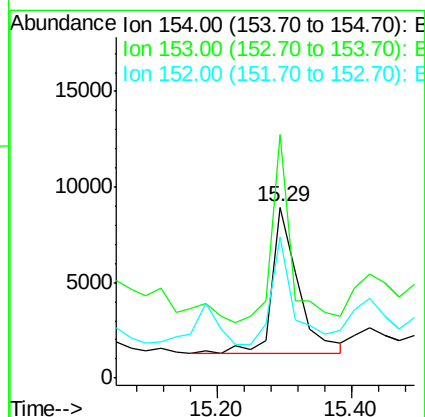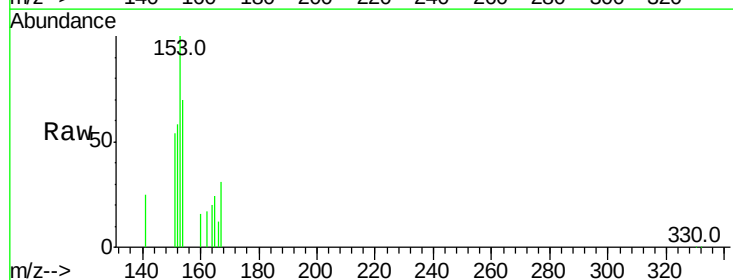

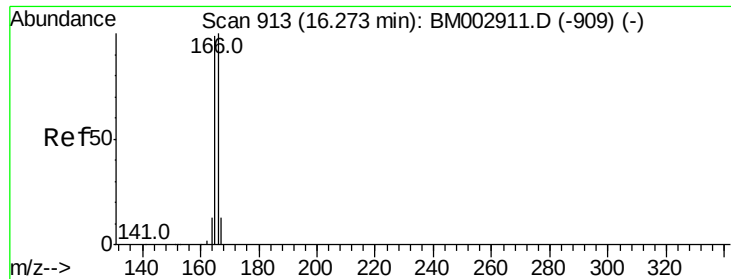

#18

Fluorene

Concen: 0.32 ng

RT: 16.27 min Scan# 914

Delta R.T. -0.00 min

Lab File: BM002935.D

Acq: 16 Oct 2015 15:29

Instrument :

BNA\_M

ClientSampleId :

RAV-GT-113





Tot Ion:166 Resp: 27248

Ion Ratio Lower Upper

166 100

165 97.4 77.3 115.9

167 28.1 10.9 16.3#

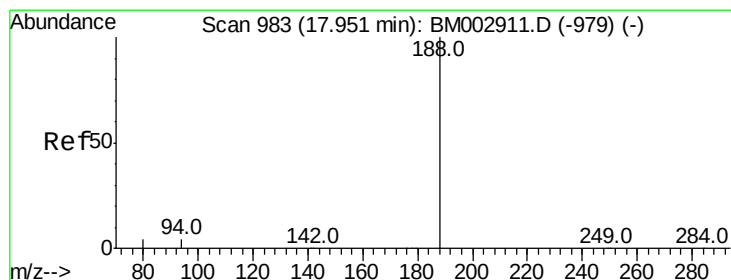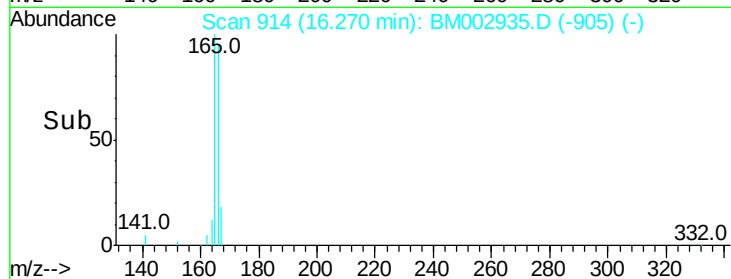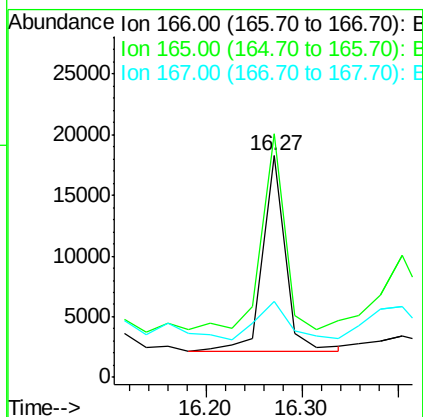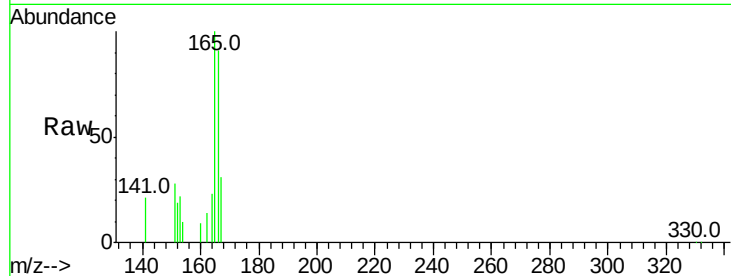

#19

Phenanthrene-d10

Concen: 5.00 ng

RT: 17.95 min Scan# 984

Delta R.T. -0.00 min

Lab File: BM002935.D

Acq: 16 Oct 2015 15:29




Tgt Ion:188 Resp: 555549

Ion Ratio Lower Upper


188 100

94 8.7 15.2 22.8#

80 7.2 15.9 23.9#

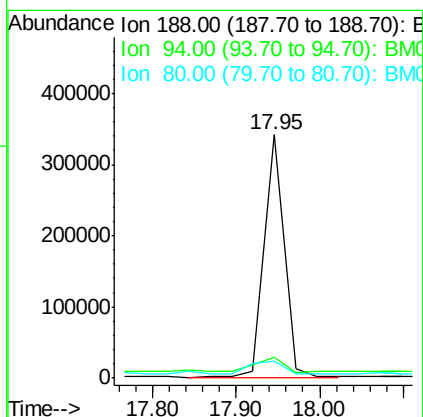



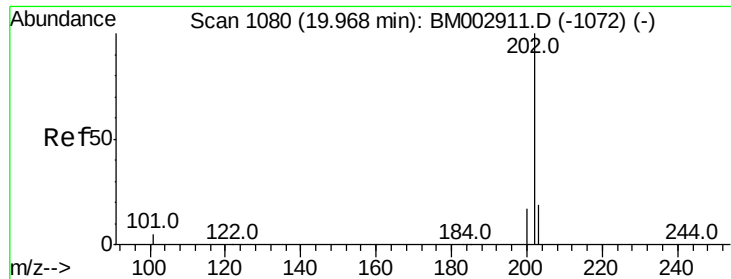

#25

Fluoranthene

Concen: 0.04 ng

RT: 19.96 min Scan# 1081

Delta R.T. -0.00 min

Lab File: BM002935.D

Acq: 16 Oct 2015 15:29

Instrument :

BNA\_M

ClientSampleId :

RAV-GT-113


Tot Ion:202 Resp: 6236

Ion Ratio Lower Upper

202 100

101 15.5 11.0 16.6




203 23.1 13.8 20.6#

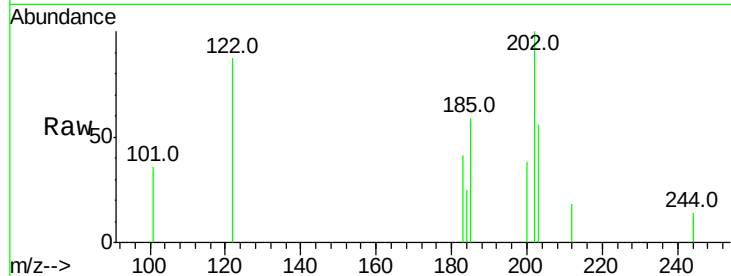

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

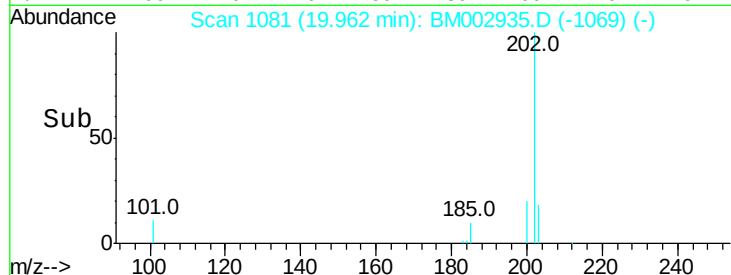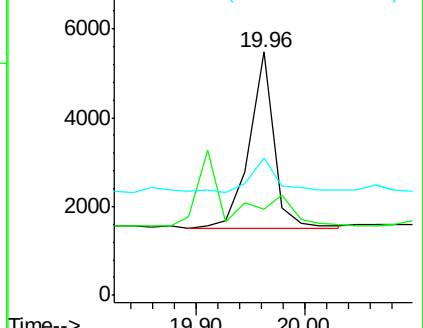

#26

Chrysene-d12

Concen: 5.00 ng

RT: 22.03 min Scan# 1192

Delta R.T. -0.00 min

Lab File: BM002935.D

Acq: 16 Oct 2015 15:29


Tgt Ion:240 Resp: 401516

Ion Ratio Lower Upper

240 100

120 29.9 3.3 4.9#



236 32.4 19.5 29.3#




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



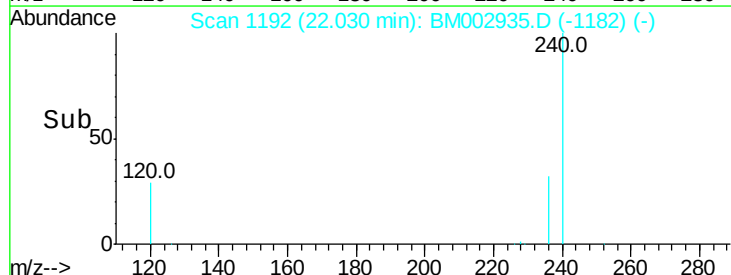
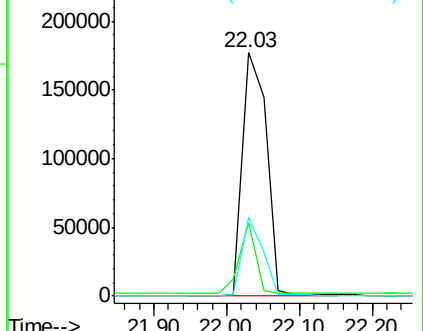




#28  
Pvrene  
Concen: 0.05 ng  
RT: 20.32 min Scan# 1102  
Delta R.T. -0.00 min  
Lab File: BM002935.D  
Acq: 16 Oct 2015 15:29




Instrument :  
BNA\_M  
ClientSampleId :  
RAV-GT-113


Tot Ion:202 Resp: 6225  
Ion Ratio Lower Upper  
202 100  
200 21.7 16.2 24.4  
203 21.1 13.8 20.8#

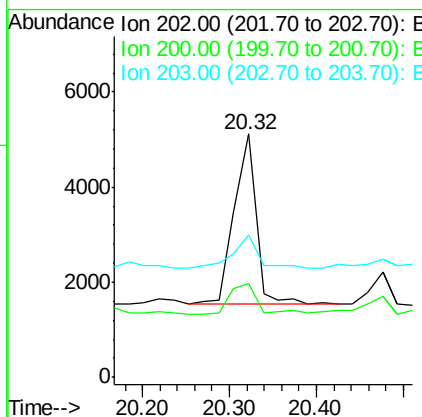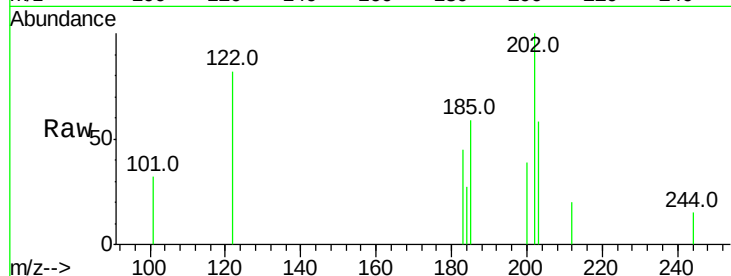

#29  
Terphenyl-d14  
Concen: 3.97 ng  
RT: 20.48 min Scan# 1111  
Delta R.T. -0.00 min  
Lab File: BM002935.D  
Acq: 16 Oct 2015 15:29

Tgt Ion:244 Resp: 238363  
Ion Ratio Lower Upper  
244 100  
212 8.7 5.6 8.4#  
122 7.0 2.2 3.2#

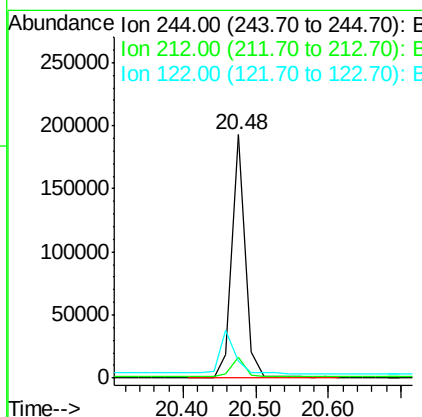

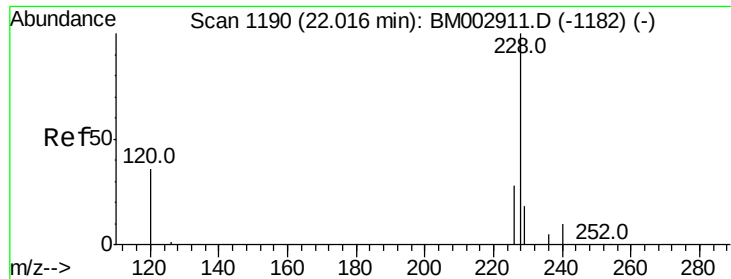

#30

Benzo(a)anthracene

Concen: 0.04 ng

RT: 22.03 min Scan# 1192

Delta R.T. 0.02 min

Lab File: BM002935.D

Acq: 16 Oct 2015 15:29

Instrument :

BNA\_M

ClientSampleId :

RAV-GT-113





Tot Ion:228 Resp: 4681

Ion Ratio Lower Upper

228 100

226 41.3 19.0 28.6#

229 55.0 16.8 25.2#

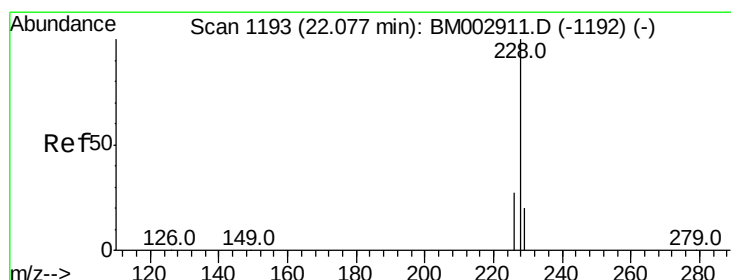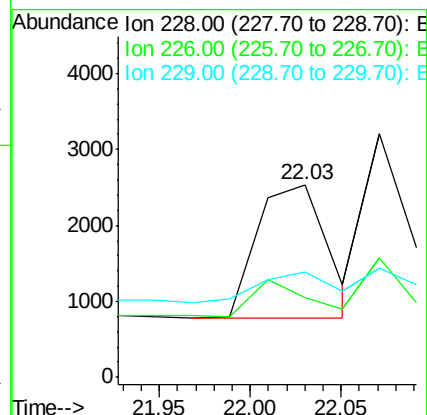

#32

Chrysene

Concen: 0.04 ng m

RT: 22.07 min Scan# 1194

Delta R.T. -0.00 min

Lab File: BM002935.D

Acq: 16 Oct 2015 15:29




Tgt Ion:228 Resp: 4123


Ion Ratio Lower Upper

228 100

226 48.9 20.6 30.8#

229 44.6 17.4 26.2#

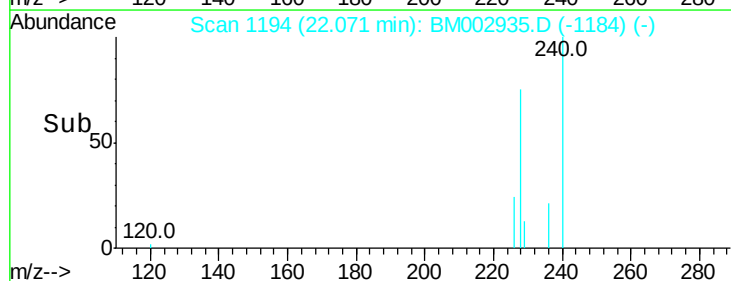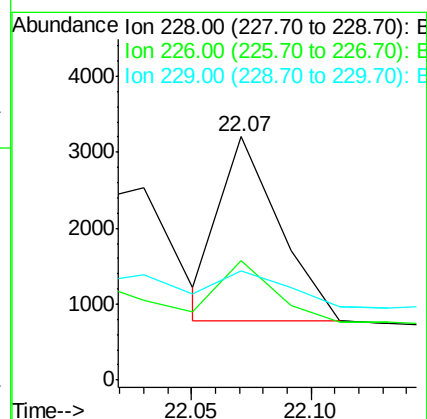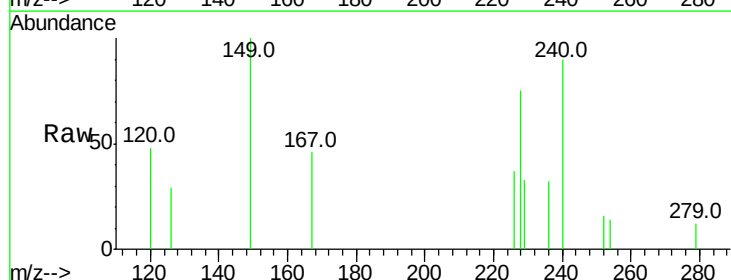



#33

Bis(2-ethylhexyl)phthalate

Concen: 0.38 ng

RT: 21.85 min Scan# 1183

Delta R.T. -0.00 min

Lab File: BM002935.D

Acq: 16 Oct 2015 15:29

Instrument :

BNA\_M

ClientSampleId :

RAV-GT-113


Tot Ion:149 Resp: 7842

Ion Ratio Lower Upper

149 100

167 30.1 17.2 25.8#




279 0.0 2.2 3.4#

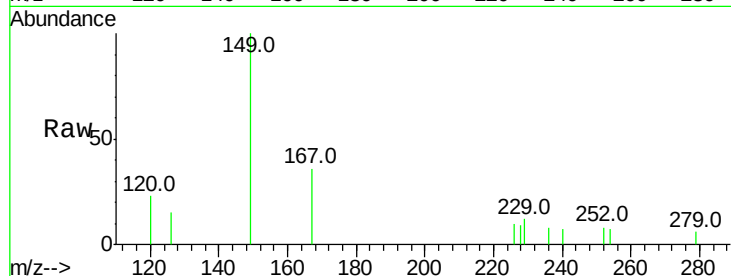

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

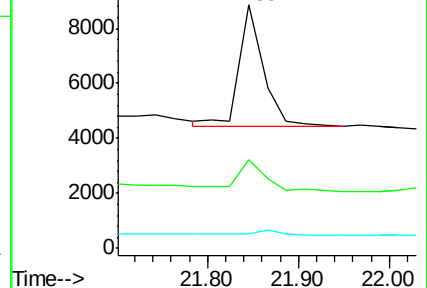

#34

Indeno(1,2,3-cd)pyrene

Concen: 0.02 ng

RT: 27.32 min Scan# 1653

Delta R.T. 0.01 min

Lab File: BM002935.D

Acq: 16 Oct 2015 15:29


Tgt Ion:276 Resp: 2320

Ion Ratio Lower Upper

276 100

138 44.6 29.0 43.6#



277 26.9 19.8 29.8






Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E




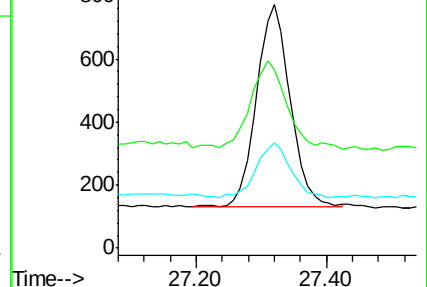


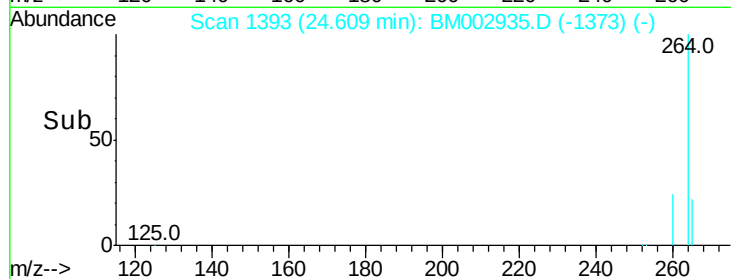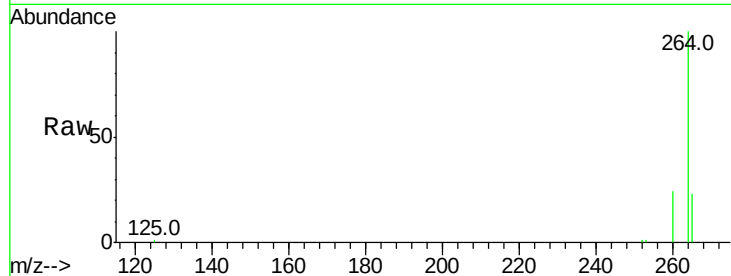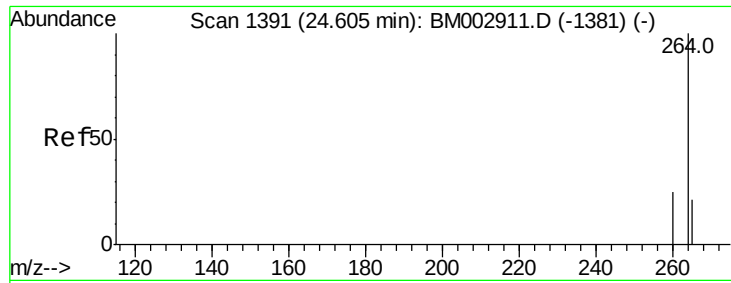

#35  
 Pervlene-d12  
 Concen: 5.00 ng  
 RT: 24.61 min Scan# 1393  
 Delta R.T. 0.01 min  
 Lab File: BM002935.D  
 Acq: 16 Oct 2015 15:29


Instrument :  
 BNA\_M  
 ClientSampleId :  
 RAV-GT-113


Tot Ion:264 Resp: 357369  
 Ion Ratio Lower Upper  
 264 100  
 260 24.2 20.1 30.1  
 265 22.7 17.6 26.4

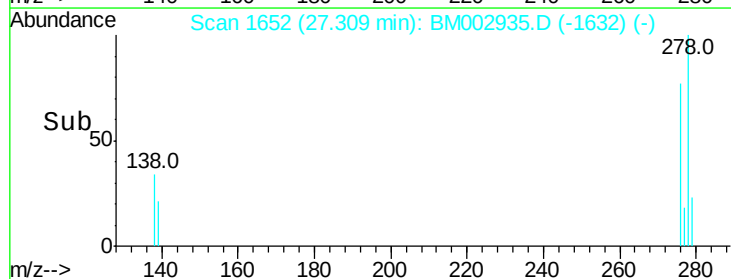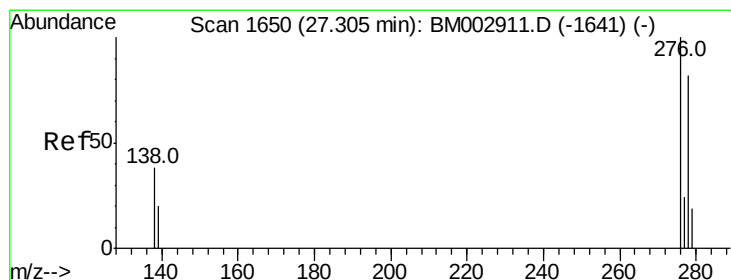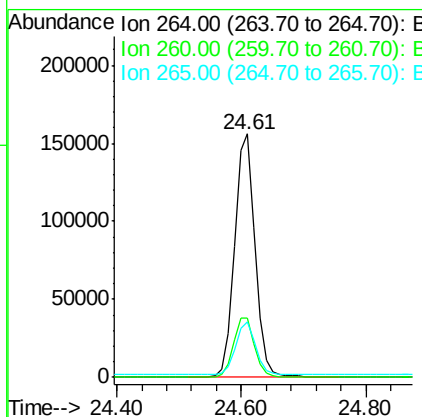

#39  
 Dibenzo(a,h)anthracene  
 Concen: 0.03 ng  
 RT: 27.31 min Scan# 1652  
 Delta R.T. 0.01 min  
 Lab File: BM002935.D  
 Acq: 16 Oct 2015 15:29

Tgt Ion:278 Resp: 2648  
 Ion Ratio Lower Upper  
 278 100  
 139 68.8 19.8 29.6#  
 279 47.2 19.1 28.7#

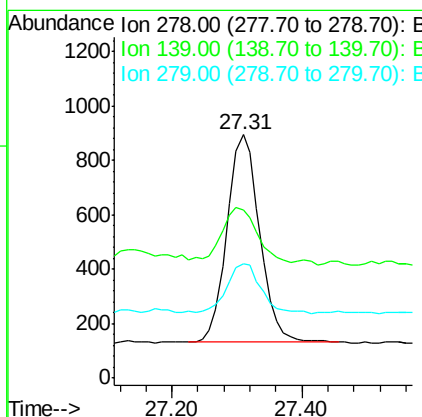

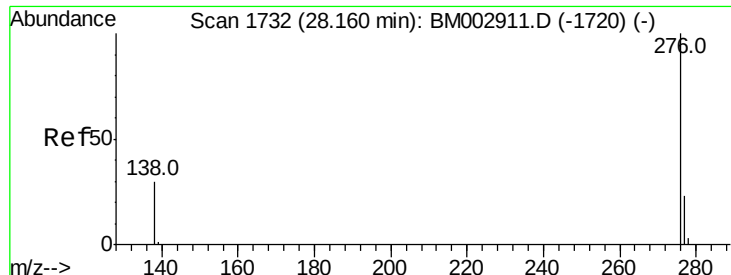

#40

Benzo(a,h,i)perylene

Concen: 0.02 ng

RT: 28.16 min Scan# 1734

Delta R.T. 0.01 min

Lab File: BM002935.D


Acq: 16 Oct 2015 15:29

Instrument :

BNA\_M

ClientSampleId :

RAV-GT-113

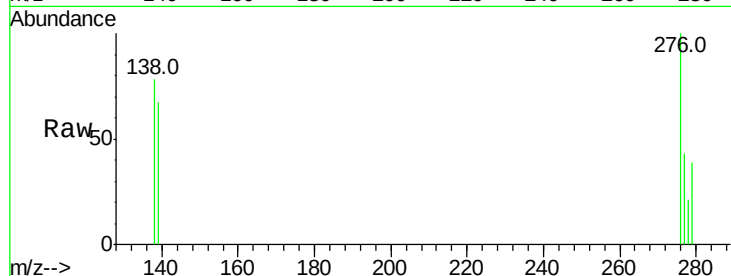


Tot Ion: 276 Resp: 1960

Ion Ratio Lower Upper

276 100

277 43.2 19.4 29.0#

138 77.7 24.4 36.6#



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

