


Data Path : Z:\HPCHEM1\BNA_M\Data\BM101717\
Data File : BM012277.D
Acq On : 18 Oct 2017 08:20
Operator : SJ/JU
Sample : I5747-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Oct 18 12:26:43 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 18 08:12:28 2017
Response via : Initial Calibration

Instrument :
BNA_M
Client Sampled :
B-23(1-3)-100517

Manual Integrations
APPROVED

Sohil
10/18/2017 7:33:53 PM

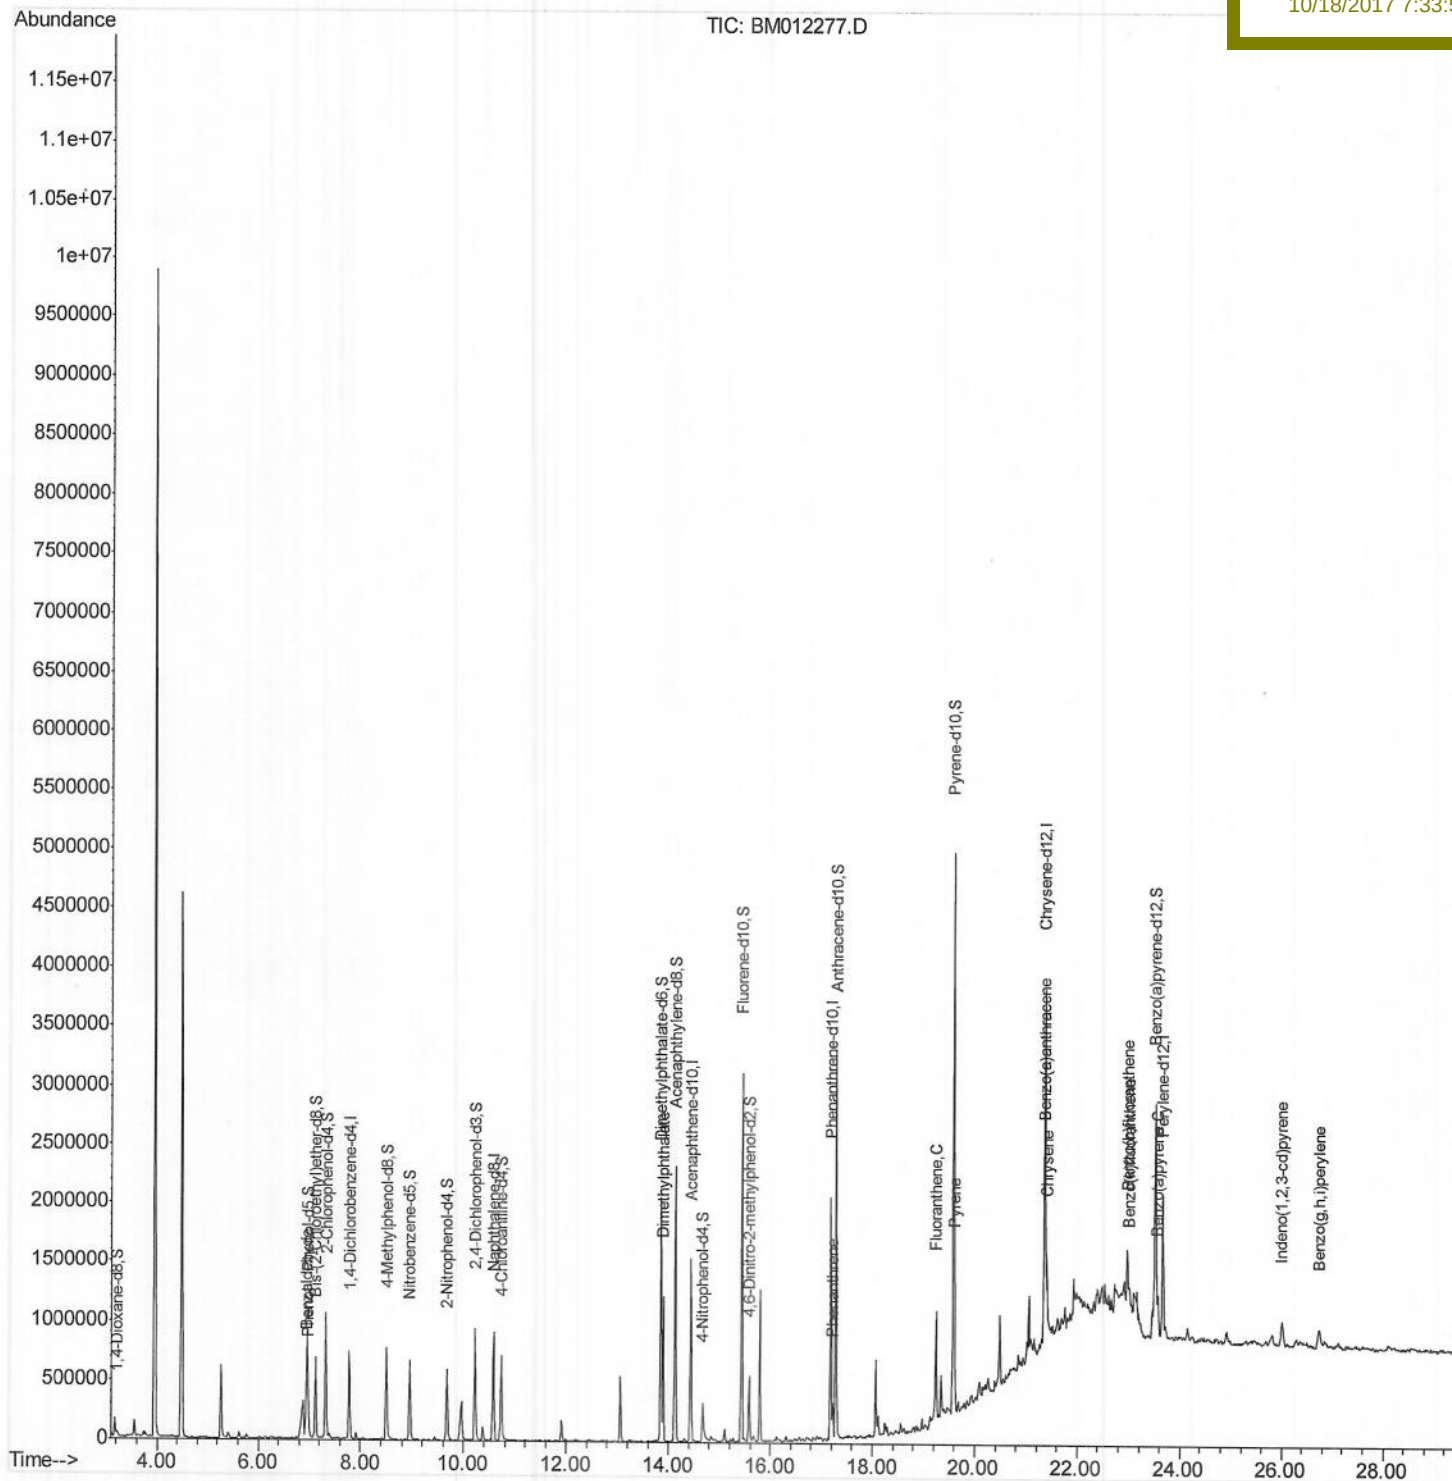

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM101717\
Data File : BM012277.D
Acq On : 18 Oct 2017 08:20
Operator : SJ/JU
Sample : I5747-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Oct 18 12:21:56 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 18 08:12:28 2017
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
B-23(1-3)-100517

Manual Integrations
APPROVED

Sohil
10/18/2017 7:33:53 PM

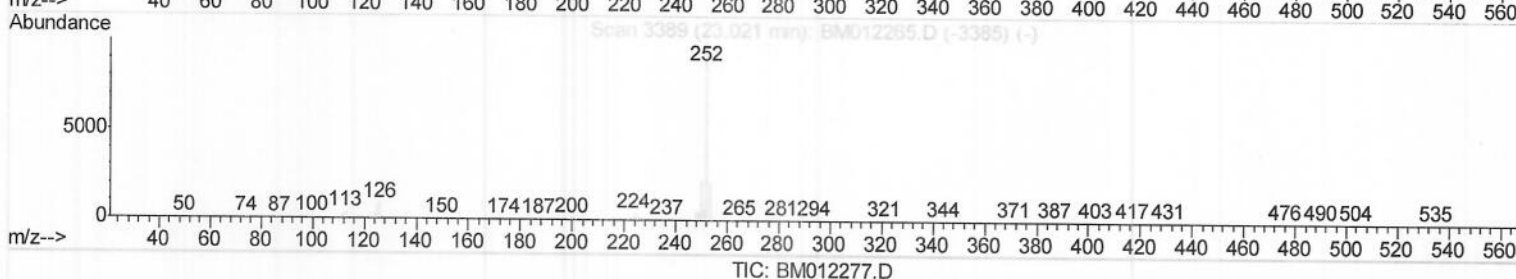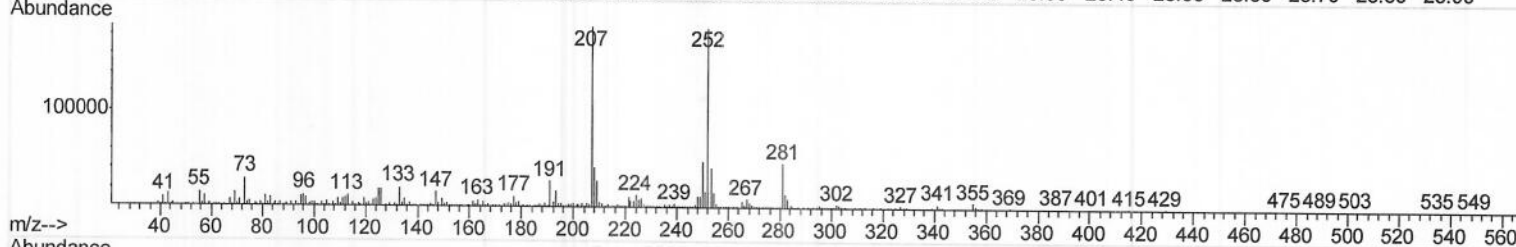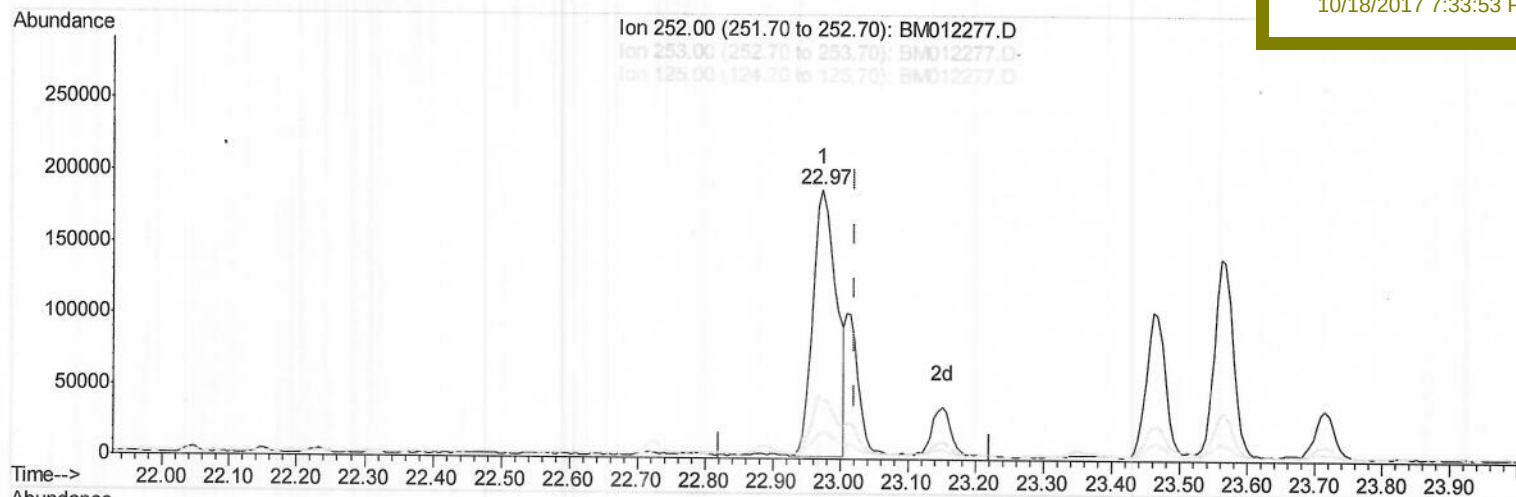

(86) Benzo(k)fluoranthene

22.974min (-0.047) 7.57ng/ui

response 446582

Ion	Exp%	Act%
252.00	100	100
253.00	22.20	22.32
125.00	6.10	9.61#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM101717\
Data File : BM012277.D
Acq On : 18 Oct 2017 08:20
Operator : SJ/JU
Sample : I5747-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Oct 18 12:21:56 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 18 08:12:28 2017
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
B-23(1-3)-100517

Manual Integrations
APPROVED

Sohil
10/18/2017 7:33:53 PM

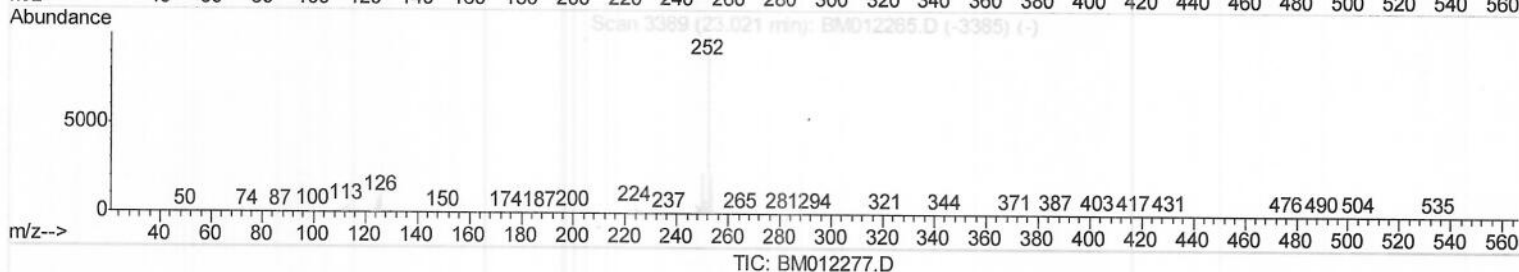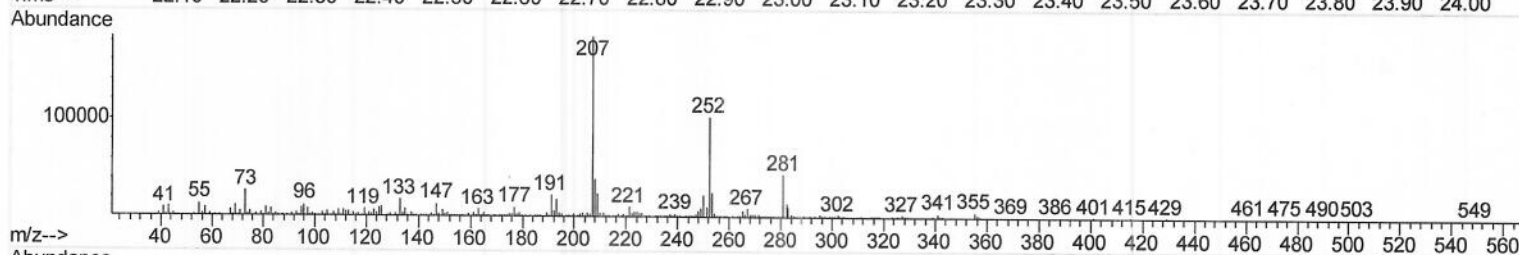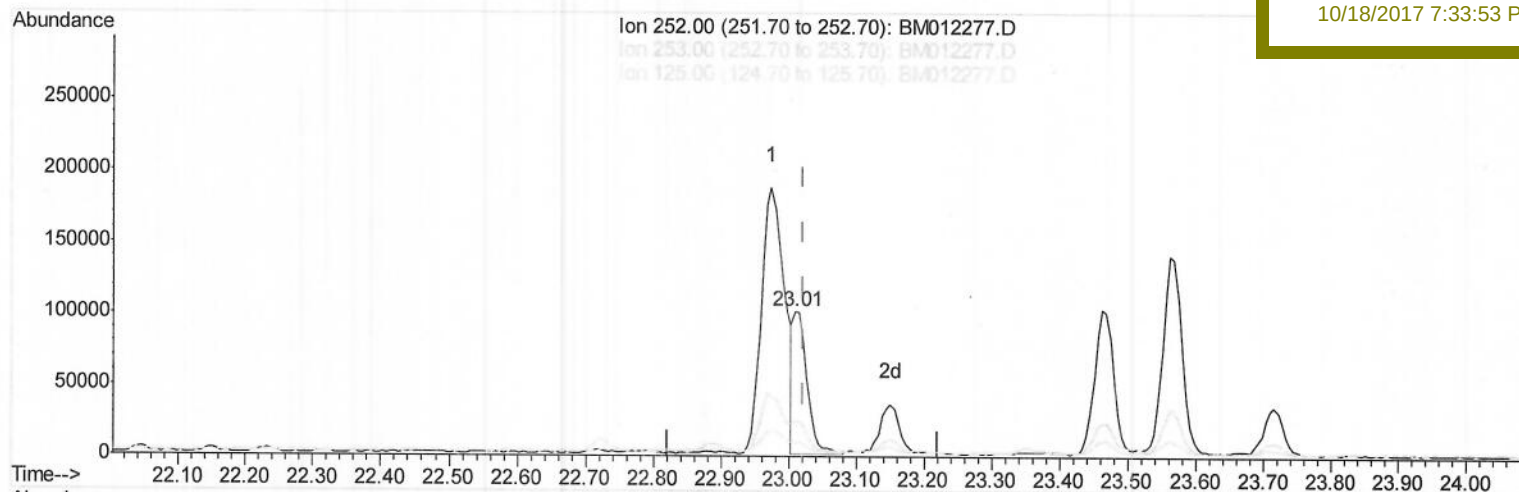

(86) Benzo(k)fluoranthene

23.009min (-0.012) 2.37ng/ul m) SJ 06/27/18

response 140024

Ion	Exp%	Act%
252.00	100	100
253.00	22.20	24.46
125.00	6.10	9.54#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\Data\BM101717\
 Data File : BM012277.D
 Acq On : 18 Oct 2017 08:20
 Operator : SJ/JU
 Sample : I5747-02
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 B-23(1-3)-100517

Quant Time: Oct 18 12:26:43 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101217.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 18 08:12:28 2017
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 10/18/2017 7:33:53 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.78	152	211813	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	778803	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.44	164	511141	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	1202718	20.00	ng/ul	0.00
75) Chrysene-d12	21.37	240	1232564	20.00	ng/ul	0.00
83) Perylene-d12	23.66	264	937661	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	17945	4.03	ng/uL	0.00
5) Phenol-d5	6.96	99	486732	28.32	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	296845	28.80	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	461793	31.68	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	304788	20.60	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	175538	29.54	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	213724	30.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	406887	30.69	ng/ul	0.00
29) 4-Chloroaniline-d4	10.73	131	424151	34.18	ng/ul	0.00
43) Dimethylphthalate-d6	13.84	166	1413148	31.28	ng/ul	0.00
46) Acenaphthylene-d8	14.13	160	1693544	30.97	ng/ul	0.00
51) 4-Nitrophenol-d4	14.67	143	131537	19.37	ng/ul	0.00
57) Fluorene-d10	15.43	176	1192824	32.17	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.58	200	158140	19.16	ng/ul	0.00
70) Anthracene-d10	17.29	188	1836111	30.87	ng/ul	0.00
76) Pyrene-d10	19.58	212	2404402	38.43	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.52	264	1426056	31.55	ng/ul	0.00

Target Compounds

					Qvalue	
4) Benzaldehyde	6.93	77	62438	5.437	ng/ul	96
6) Phenol	6.98	94	113833	6.407	ng/ul	97
44) Dimethylphthalate	13.89	163	802824	17.738	ng/ul	99
69) Phenanthrene	17.23	178	208432	3.046	ng/ul	98
74) Fluoranthene	19.24	202	523948	6.346	ng/ul#	96
77) Pyrene	19.61	202	592706	7.281	ng/ul#	95
80) Benzo(a)anthracene	21.35	228	299598	3.736	ng/ul	97
82) Chrysene	21.40	228	330067	4.383	ng/ul	96
85) Benzo(b)fluoranthene	22.97	252	446582	7.298	ng/ul#	97
86) Benzo(k)fluoranthene	23.01	252	140024m	2.375	ng/ul	95
88) Benzo(a)pyrene	23.56	252	267604	4.640	ng/ul#	95
89) Indeno(1,2,3-cd)pyrene	26.00	276	210948	3.444	ng/ul	97
91) Benzo(g,h,i)perylene	26.73	276	189464	3.777	ng/ul	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

) SJ 06/27/18