

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101722\
 Data File : BM037109.D
 Acq On : 17 Oct 2022 12:51
 Operator : CG/JU
 Sample : N4980-11DL 20X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8Z1DL

Quant Time: Oct 17 23:54:14 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 17 02:26:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.930	152	5077	0.400	ng/ul	0.00
4) Naphthalene-d8	10.732	136	18169	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.557	164	9417	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.296	188	15730	0.400	ng/ul	0.00
17) Chrysene-d12	21.468	240	9040	0.400	ng/ul	0.00
23) Perylene-d12	23.853	264	7040	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	819	0.114	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.316	152	279	0.010	ng/ul	0.00
18) Fluoranthene-d10	19.317	212	431	0.016	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.373	88	13480	1.926	ng/ul#	77
11) Acenaphthene	14.617	153	739	0.022	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101722\
Data File : BM037109.D
Acq On : 17 Oct 2022 12:51
Operator : CG/JU
Sample : N4980-11DL 20X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8Z1DL

Quant Time: Oct 17 23:54:14 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 17 02:26:13 2022
Response via : Initial Calibration




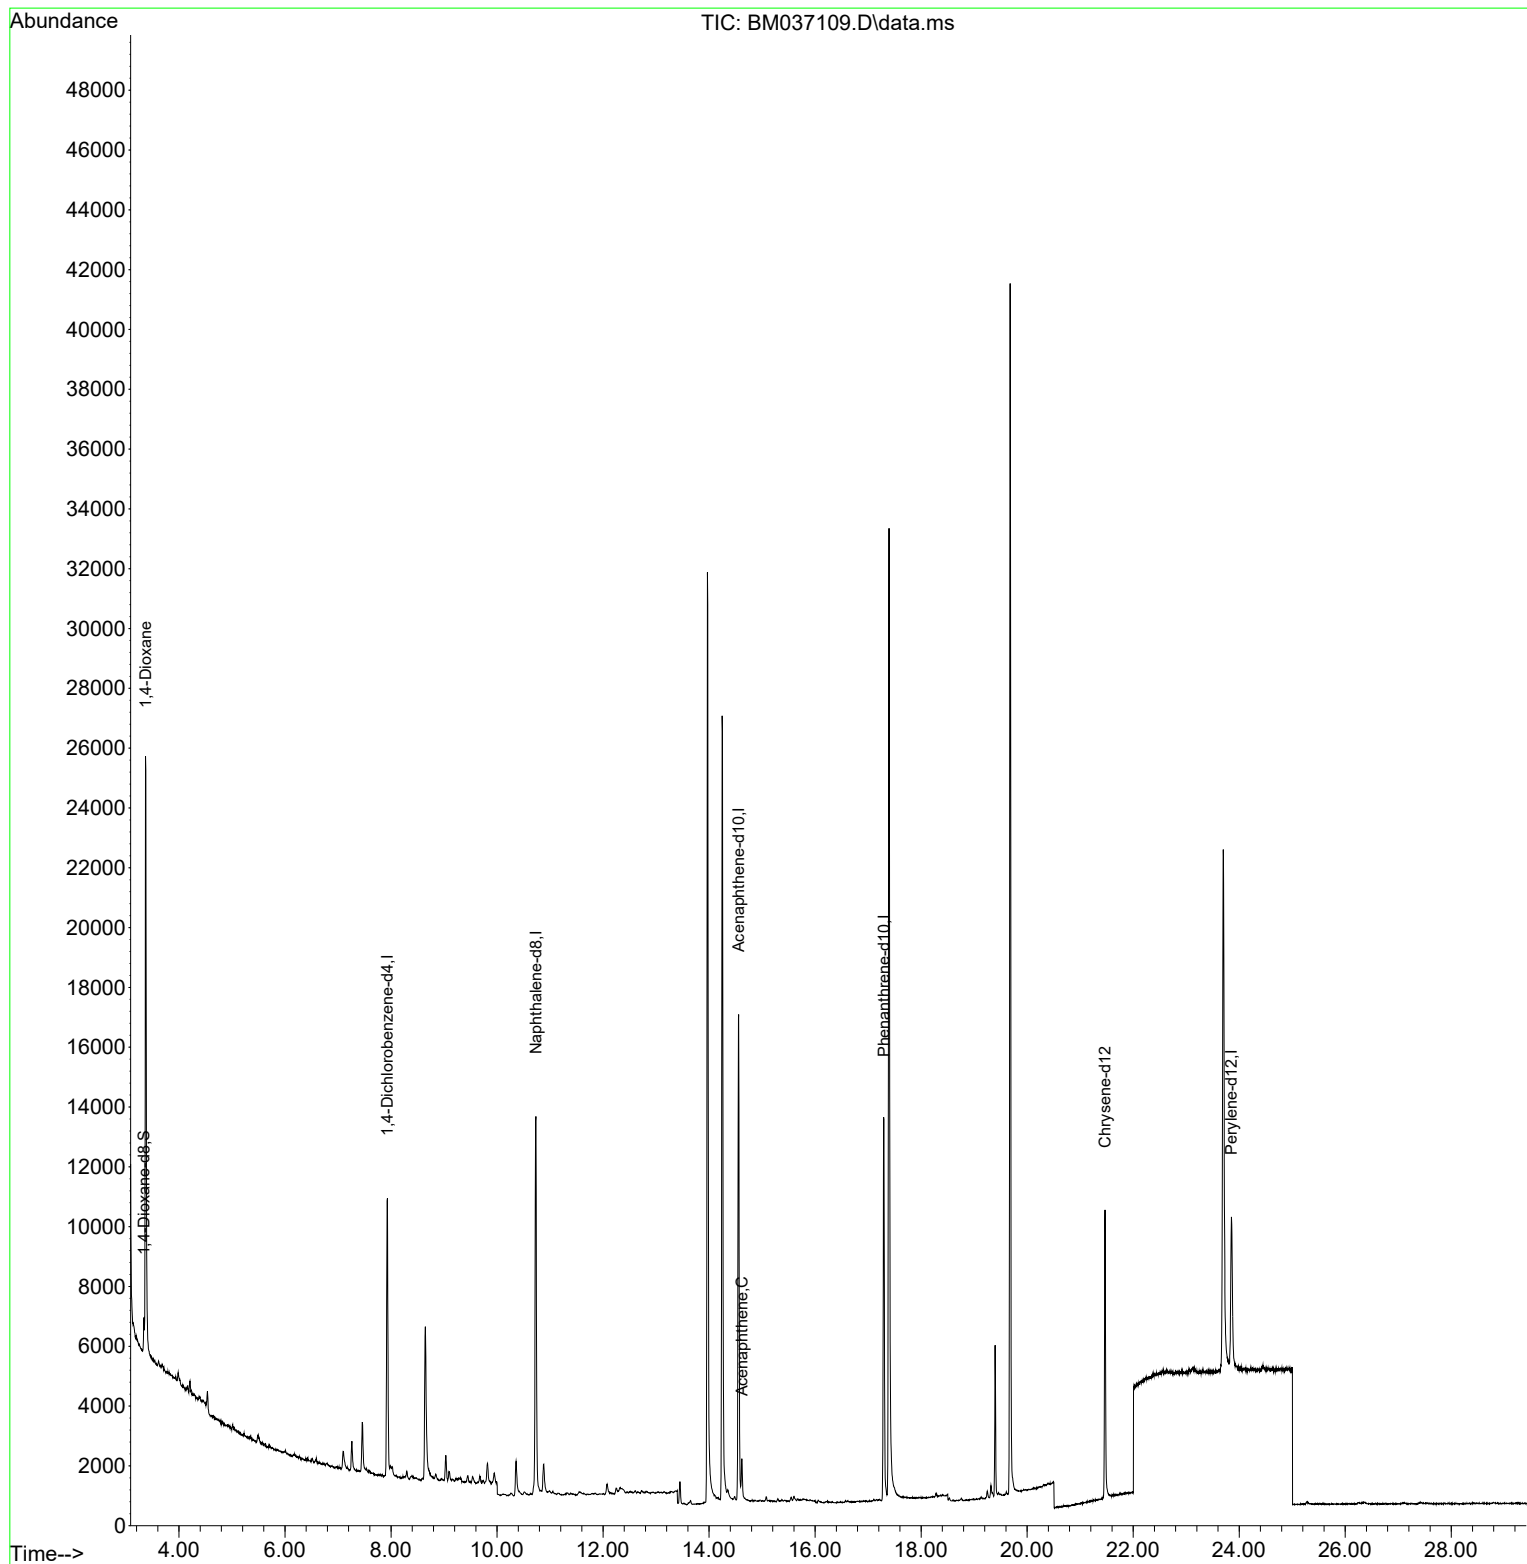


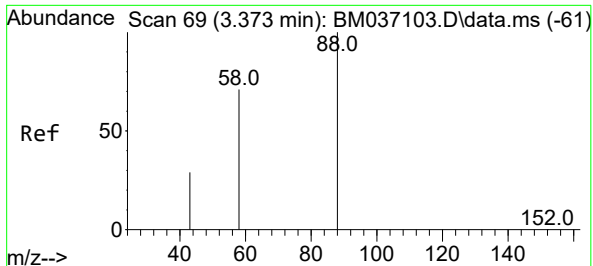

#2
1,4-Dioxane
Concen: 1.926 ng/ul
RT: 3.373 min Scan# 69
Delta R.T. 0.000 min
Lab File: BM037109.D
Acq: 17 Oct 2022 12:51

Instrument :
BNA_M
ClientSampleId :
CB8Z1DL

Tgt Ion: 88 Resp: 13480
Ion Ratio Lower Upper
88 100
43 31.7 37.8 56.6#
58 69.3 42.6 63.8#

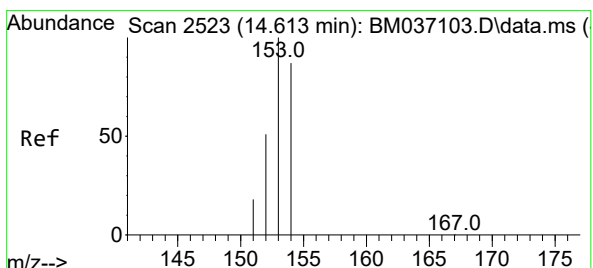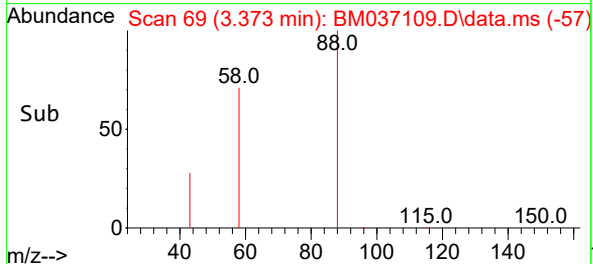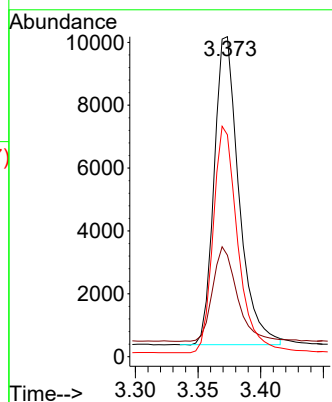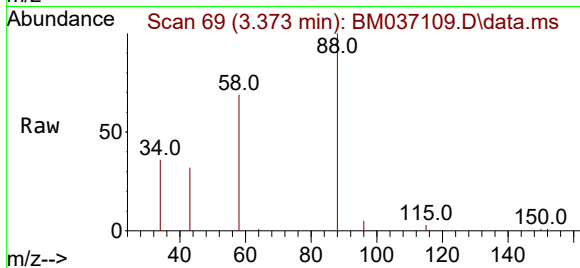

#11
Acenaphthene
Concen: 0.022 ng/ul
RT: 14.617 min Scan# 2524
Delta R.T. 0.000 min
Lab File: BM037109.D
Acq: 17 Oct 2022 12:51

Tgt Ion: 153 Resp: 739
Ion Ratio Lower Upper
153 100
152 56.2 40.2 60.4
154 86.2 69.7 104.5

