

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101722\
 Data File : BM037110.D
 Acq On : 17 Oct 2022 13:27
 Operator : CG/JU
 Sample : N4980-12DL 20X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8Z2DL

Quant Time: Oct 17 23:54:20 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 17 02:26:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.930	152	5647	0.400	ng/ul	0.00
4) Naphthalene-d8	10.732	136	18815	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.556	164	8794	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.296	188	14455	0.400	ng/ul	0.00
17) Chrysene-d12	21.468	240	10487	0.400	ng/ul	0.00
23) Perylene-d12	23.856	264	8492	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	1186	0.149	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.316	152	435	0.015	ng/ul	0.00
18) Fluoranthene-d10	19.317	212	571	0.018	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.373	88	17485	2.246	ng/ul#	77
11) Acenaphthene	14.617	153	2160	0.068	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101722\
Data File : BM037110.D
Acq On : 17 Oct 2022 13:27
Operator : CG/JU
Sample : N4980-12DL 20X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8Z2DL

Quant Time: Oct 17 23:54:20 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 17 02:26:13 2022
Response via : Initial Calibration




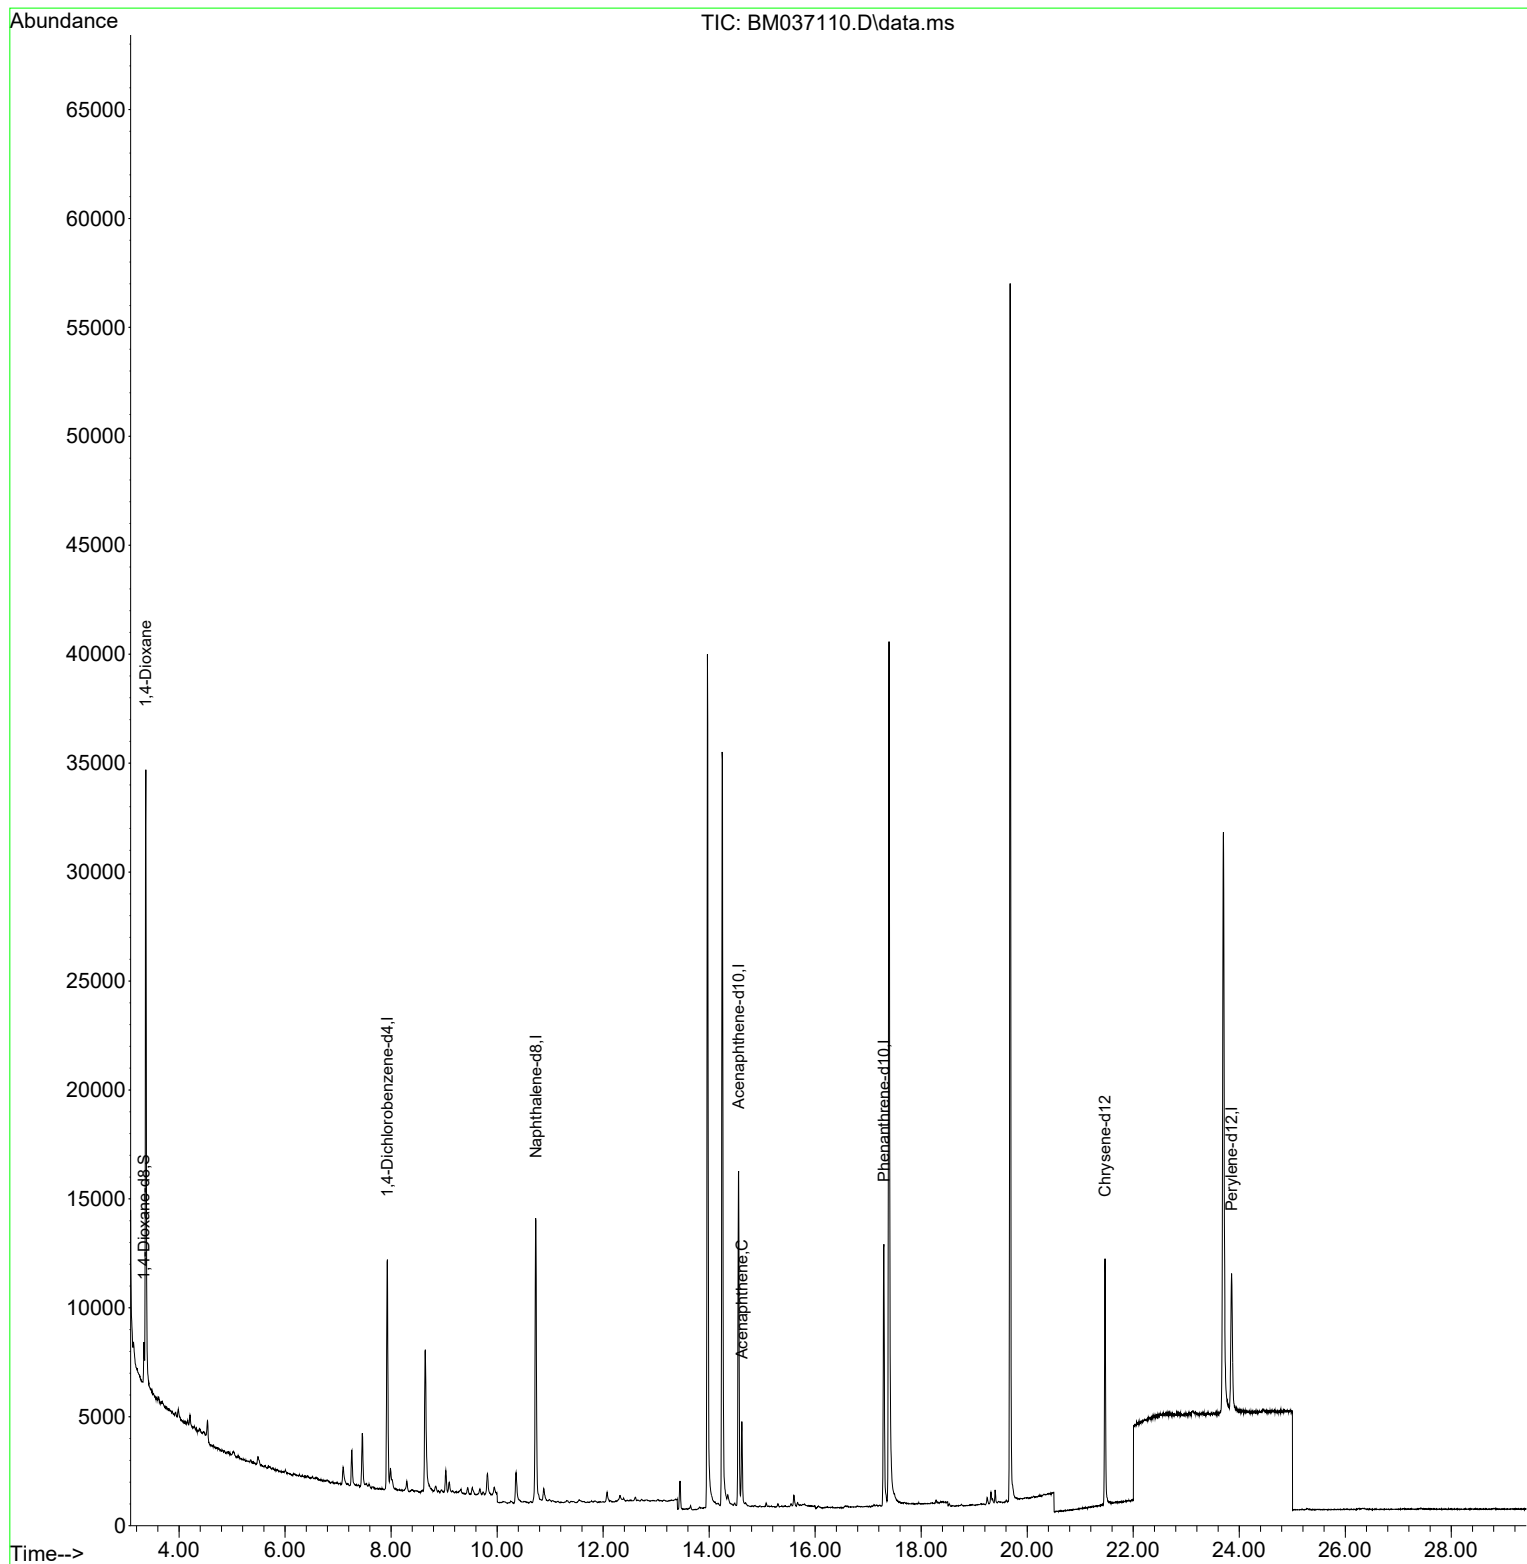


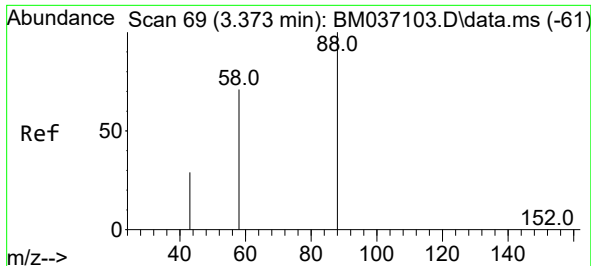

#2
1,4-Dioxane
Concen: 2.246 ng/ul
RT: 3.373 min Scan# 61
Delta R.T. -0.000 min
Lab File: BM037110.D
Acq: 17 Oct 2022 13:27

Instrument :
BNA_M
ClientSampleId :
CB8Z2DL

Tgt Ion: 88 Resp: 17485
Ion Ratio Lower Upper
88 100
43 31.1 37.8 56.6#
58 68.4 42.6 63.8#

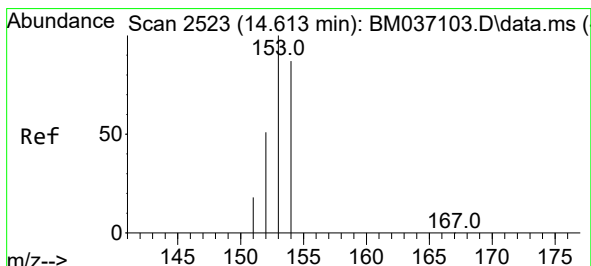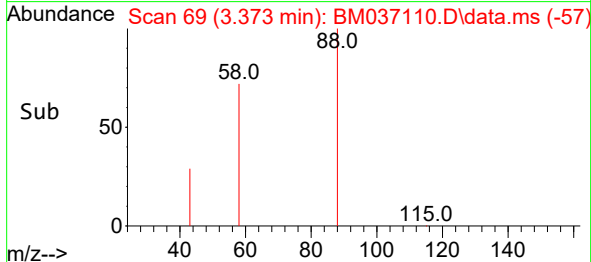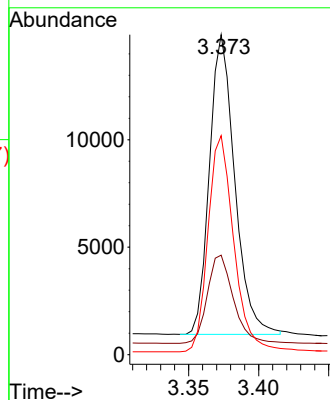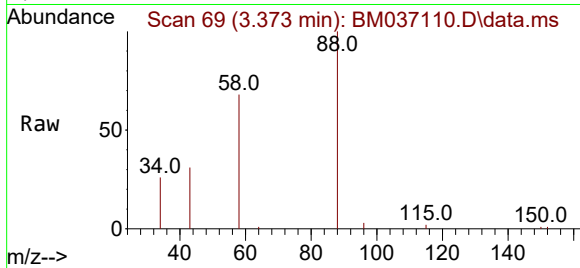

#11
Acenaphthene
Concen: 0.068 ng/ul
RT: 14.617 min Scan# 2524
Delta R.T. -0.000 min
Lab File: BM037110.D
Acq: 17 Oct 2022 13:27

Tgt Ion: 153 Resp: 2160
Ion Ratio Lower Upper
153 100
152 54.3 40.2 60.4
154 86.1 69.7 104.5

