

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101722\
 Data File : BM037121.D
 Acq On : 17 Oct 2022 20:37
 Operator : CG/JU
 Sample : PB148300BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK300

Quant Time: Oct 17 23:56:05 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 17 02:26:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.926	152	4487	0.400	ng/ul	0.00
4) Naphthalene-d8	10.726	136	16472	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.552	164	8691	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.292	188	16588	0.400	ng/ul	0.00
17) Chrysene-d12	21.468	240	9750	0.400	ng/ul	0.00
23) Perylene-d12	23.853	264	9402	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.335	96	34395	5.436	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.316	152	6914	0.278	ng/ul	0.00
18) Fluoranthene-d10	19.317	212	11169	0.383	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.547	166	2262	0.064	ng/ul#	14
20) Pyrene	19.680	202	1984	0.049	ng/ul#	1
26) Benzo(a)pyrene	23.701	252	2936	0.086	ng/ul#	56


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101722\
Data File : BM037121.D
Acq On : 17 Oct 2022 20:37
Operator : CG/JU
Sample : PB148300BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK300

Quant Time: Oct 17 23:56:05 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 17 02:26:13 2022
Response via : Initial Calibration




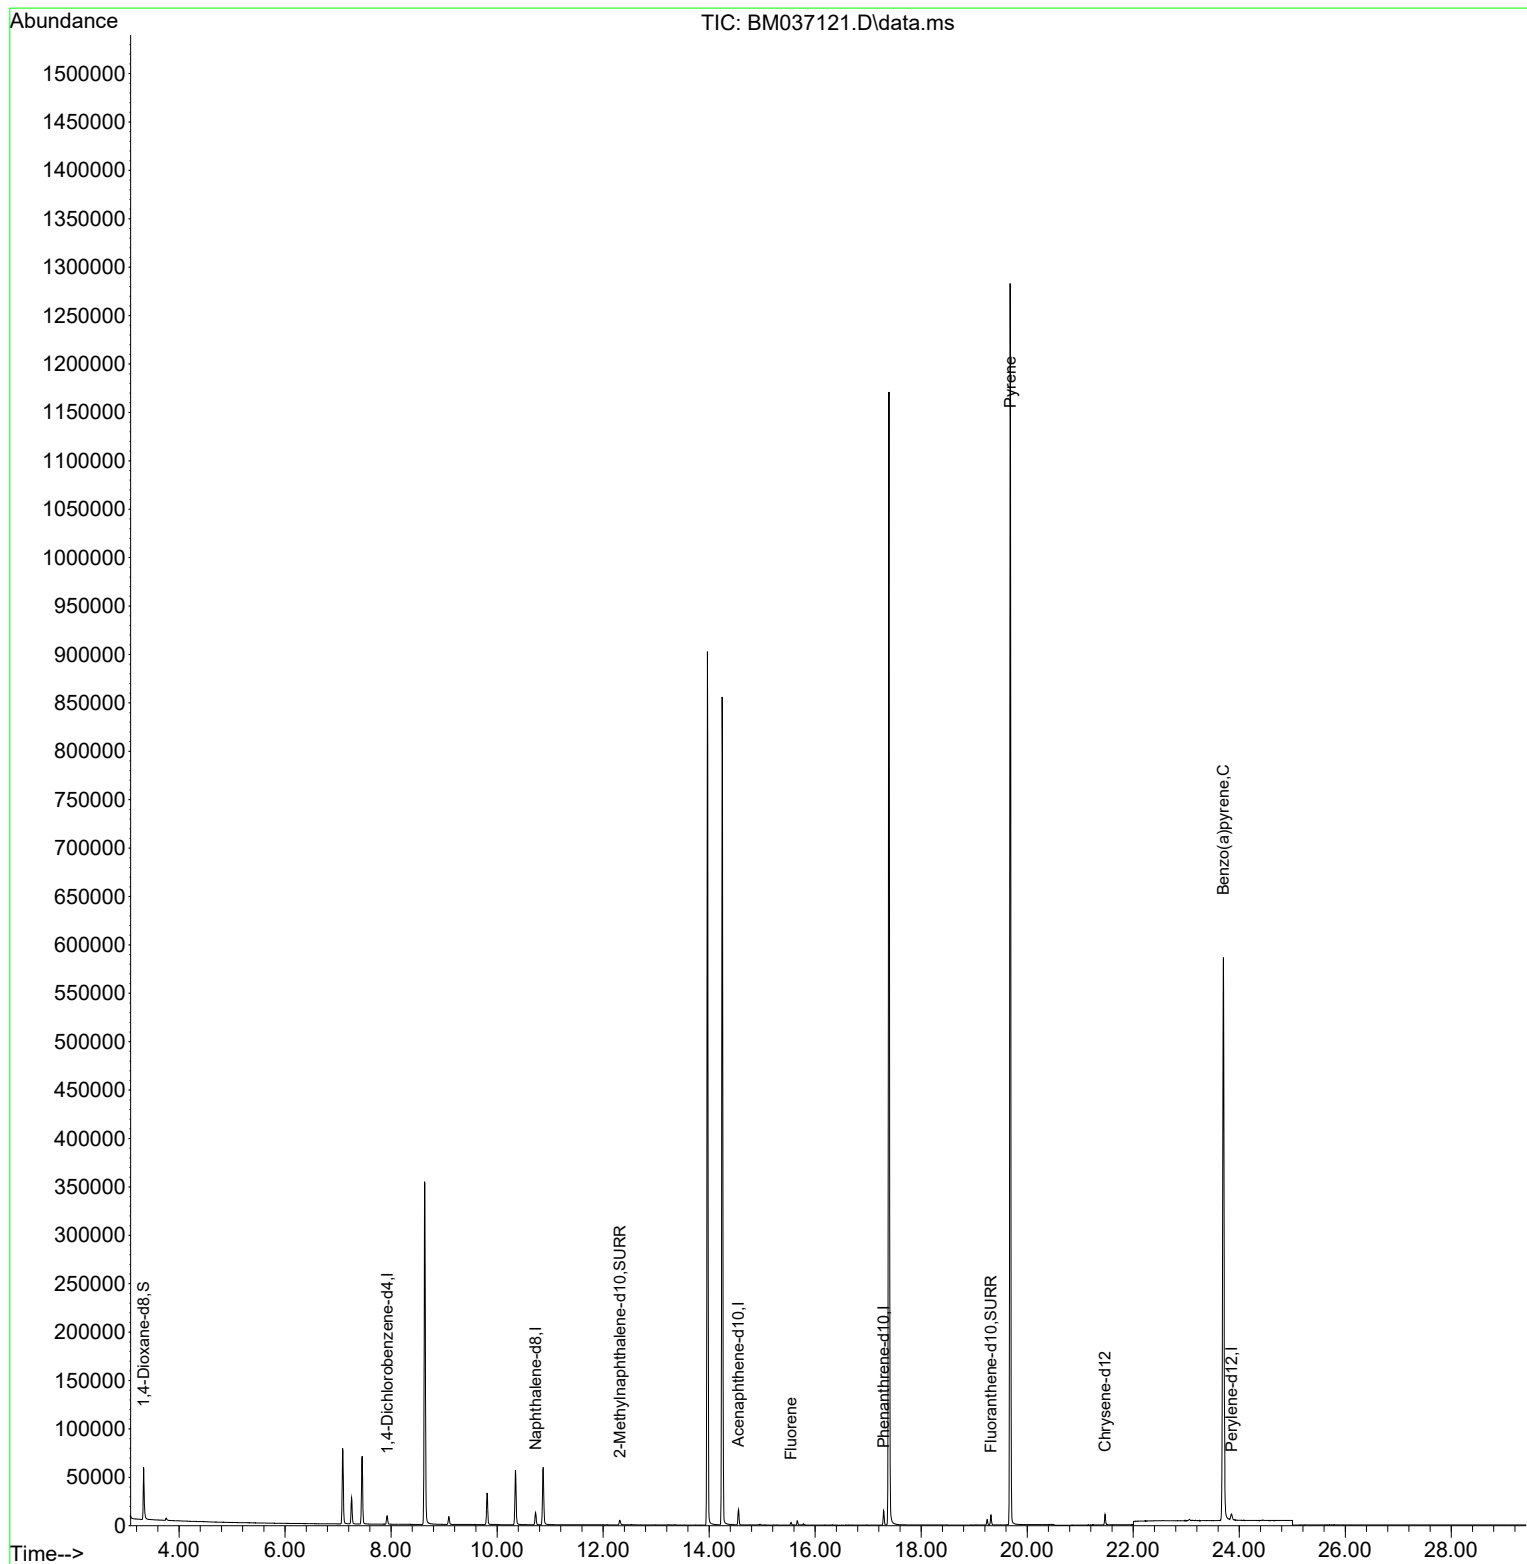


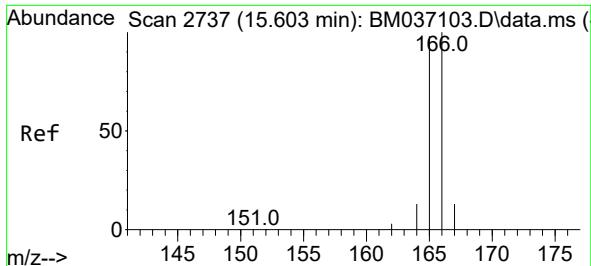

#12
Fluorene
Concen: 0.064 ng/ul
RT: 15.547 min Scan# 21
Delta R.T. -0.056 min
Lab File: BM037121.D
Acq: 17 Oct 2022 20:37




Instrument :
BNA_M
ClientSampleId :
SBLK300


Tgt Ion:166 Resp: 2262
Ion Ratio Lower Upper
166 100
165 9.3 78.9 118.3#
167 36.9 11.3 16.9#

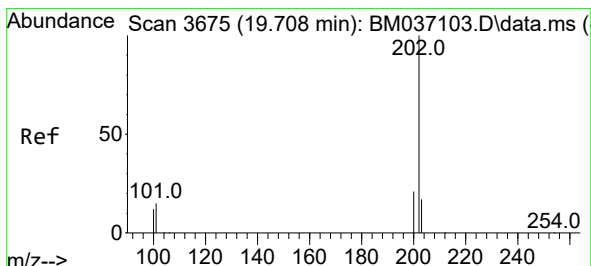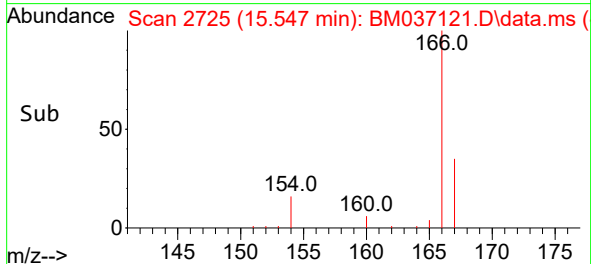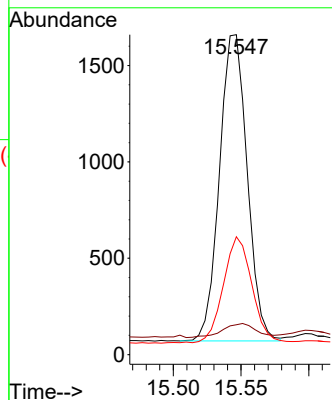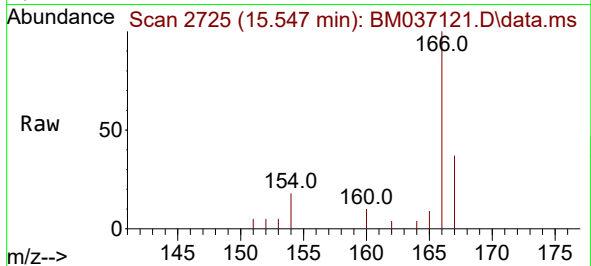

#20
Pyrene
Concen: 0.049 ng/ul
RT: 19.680 min Scan# 3669
Delta R.T. -0.028 min
Lab File: BM037121.D
Acq: 17 Oct 2022 20:37


Tgt Ion:202 Resp: 1984
Ion Ratio Lower Upper
202 100
101 177.9 12.0 18.0#
100 1333.5 9.8 14.6#

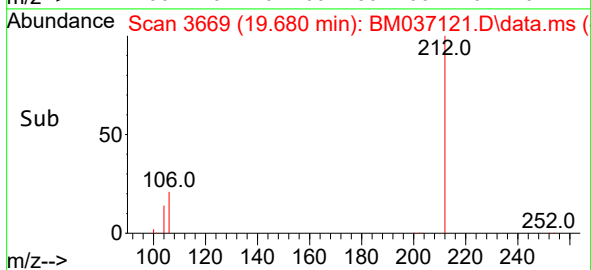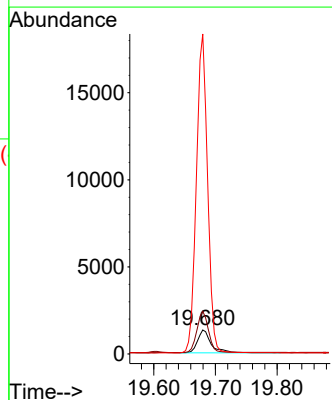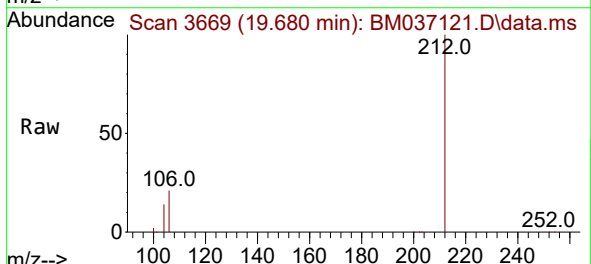

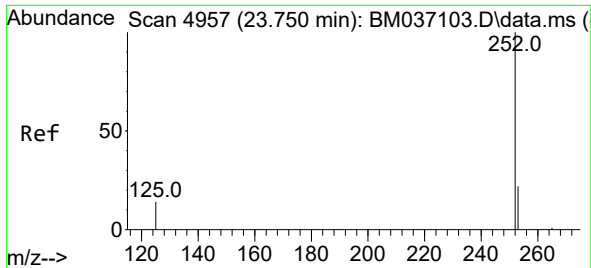

#26
Benzo(a)pyrene
Concen: 0.086 ng/ul
RT: 23.701 min Scan# 4957
Delta R.T. -0.044 min
Lab File: BM037121.D
Acq: 17 Oct 2022 20:37

Instrument :
BNA_M
ClientSampleId :
SBLK300

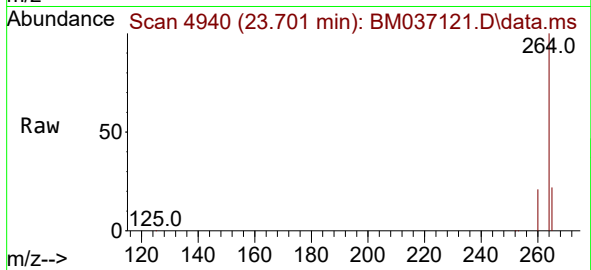

Tgt Ion:252 Resp: 2936
Ion Ratio Lower Upper
252 100
253 52.8 29.7 44.5#
125 65.4 23.6 35.4#

