

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101722\
 Data File : BM037124.D
 Acq On : 17 Oct 2022 22:23
 Operator : CG/JU
 Sample : N5071-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0BS7

Quant Time: Oct 17 23:56:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 17 02:26:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.926	152	4637	0.400	ng/ul	0.00
4) Naphthalene-d8	10.726	136	16847	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.552	164	8837	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.292	188	17732	0.400	ng/ul	0.00
17) Chrysene-d12	21.465	240	9800	0.400	ng/ul	0.00
23) Perylene-d12	23.850	264	9233	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.335	96	25599	3.915	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.316	152	7062	0.278	ng/ul	0.00
18) Fluoranthene-d10	19.312	212	14011	0.478	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.373	88	705	0.110	ng/ul#	74
20) Pyrene	19.680	202	2266	0.056	ng/ul#	1
26) Benzo(a)pyrene	23.695	252	3381	0.101	ng/ul#	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101722\
Data File : BM037124.D
Acq On : 17 Oct 2022 22:23
Operator : CG/JU
Sample : N5071-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0BS7

Quant Time: Oct 17 23:56:28 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 17 02:26:13 2022
Response via : Initial Calibration




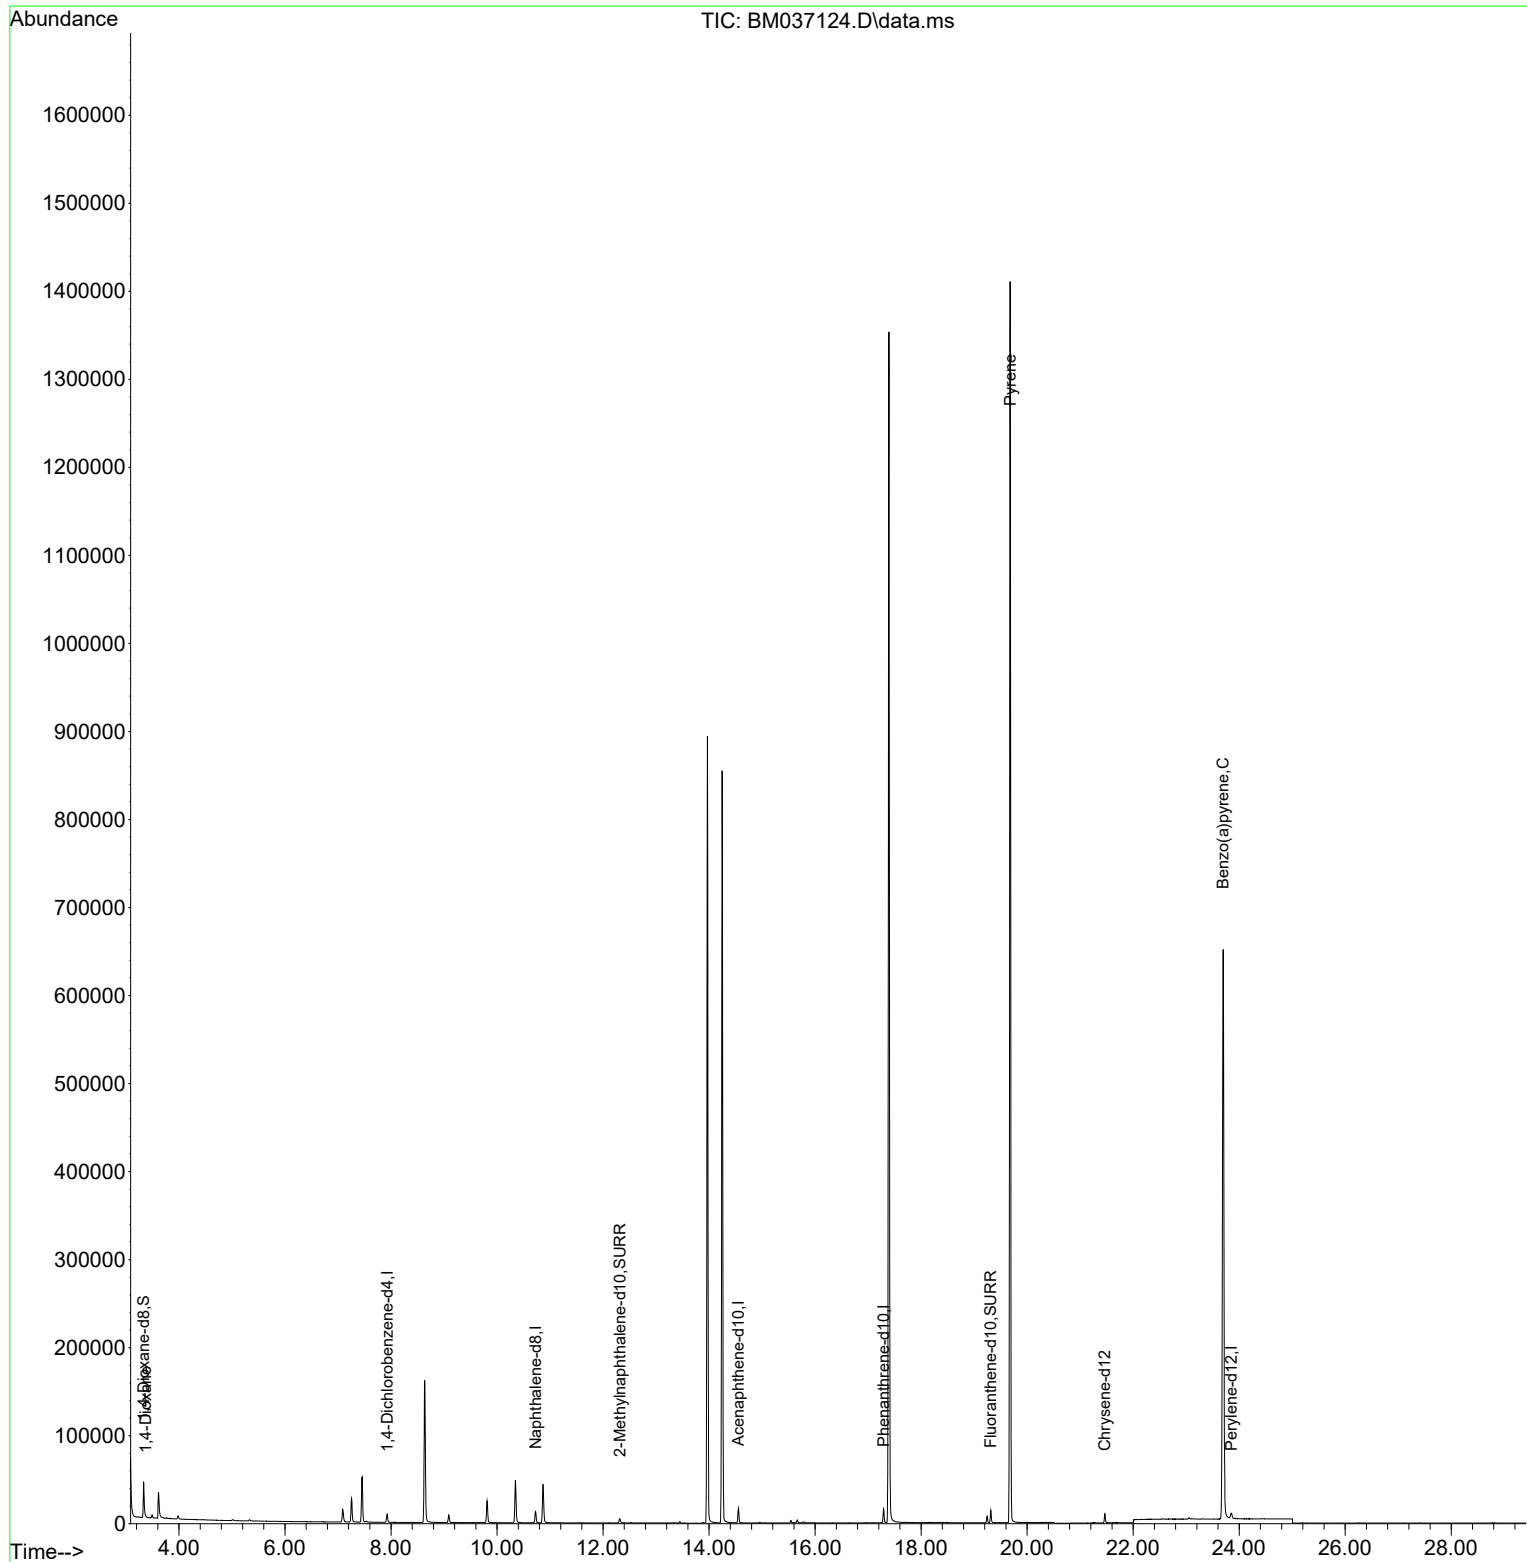


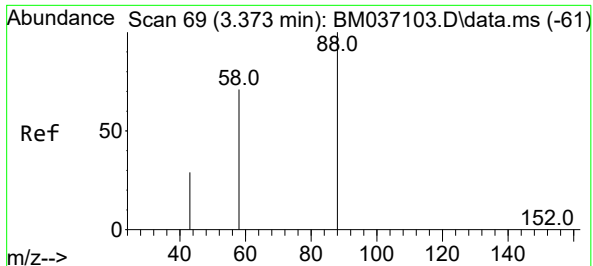

#2
1,4-Dioxane
Concen: 0.110 ng/ul
RT: 3.373 min Scan# 61
Delta R.T. 0.000 min
Lab File: BM037124.D
Acq: 17 Oct 2022 22:23




Instrument :
BNA_M
ClientSampleId :
C0BS7


Tgt Ion: 88 Resp: 705
Ion Ratio Lower Upper
88 100
43 82.4 37.8 56.6#
58 51.5 42.6 63.8

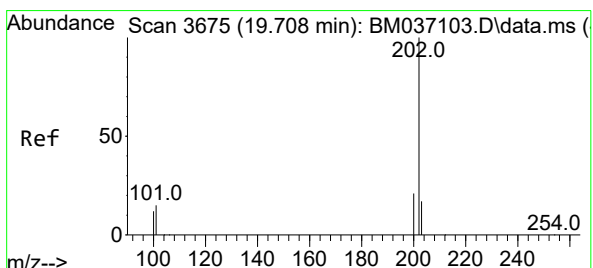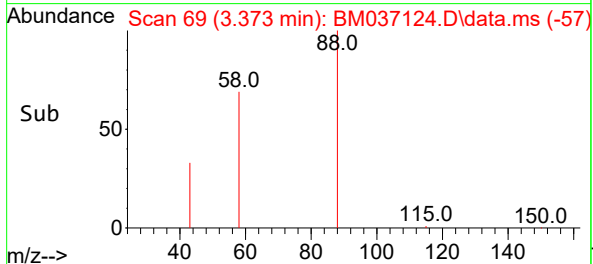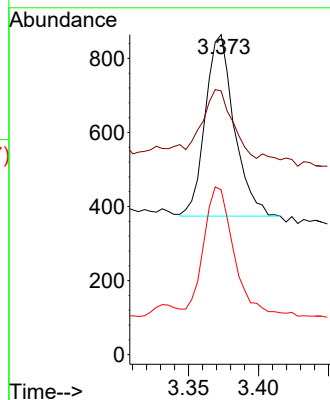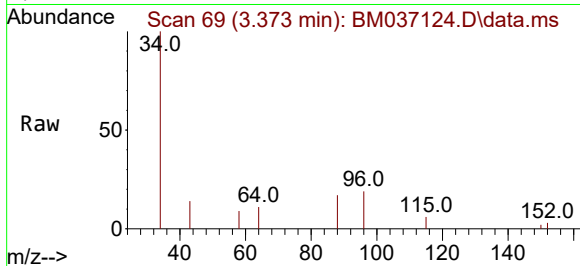

#20
Pyrene
Concen: 0.056 ng/ul
RT: 19.680 min Scan# 3669
Delta R.T. -0.028 min
Lab File: BM037124.D
Acq: 17 Oct 2022 22:23


Tgt Ion: 202 Resp: 2266
Ion Ratio Lower Upper
202 100
101 167.3 12.0 18.0#
100 1200.0 9.8 14.6#

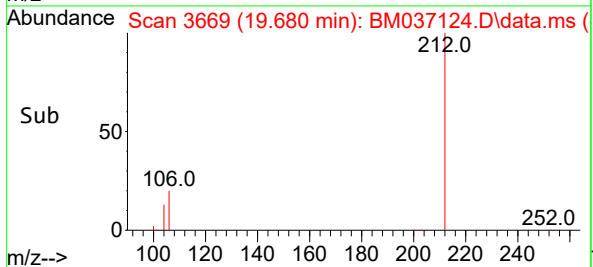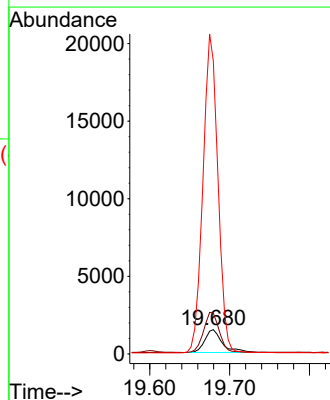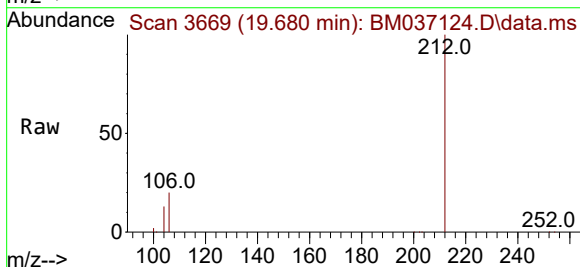

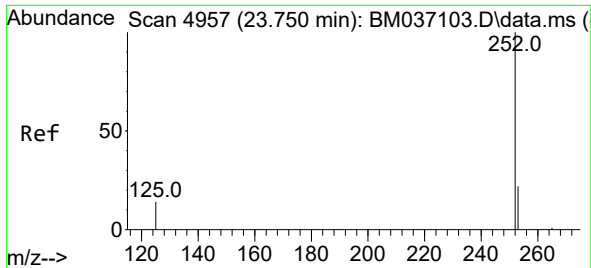

#26
Benzo(a)pyrene
Concen: 0.101 ng/ul
RT: 23.695 min Scan# 4957
Delta R.T. -0.050 min
Lab File: BM037124.D
Acq: 17 Oct 2022 22:23

Instrument :
BNA_M
ClientSampleId :
C0BS7

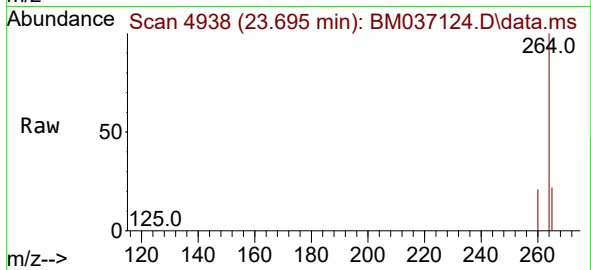

Tgt Ion:252 Resp: 3381
Ion Ratio Lower Upper
252 100
253 51.5 29.7 44.5#
125 62.9 23.6 35.4#

