

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101722\
 Data File : BM037106.D
 Acq On : 17 Oct 2022 11:04
 Operator : CG/JU
 Sample : N4984-06
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGNJ1

Quant Time: Oct 17 23:53:54 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 17 02:26:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.926	152	5542	0.400	ng/ul	0.00
4) Naphthalene-d8	10.727	136	18634	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.552	164	9153	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.292	188	14678	0.400	ng/ul	0.00
17) Chrysene-d12	21.471	240	10325	0.400	ng/ul	0.00
23) Perylene-d12	23.859	264	10753	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.336	96	35477	4.539	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.316	152	9234	0.328	ng/ul	0.00
18) Fluoranthene-d10	19.317	212	12835	0.416	ng/ul	0.00
Target Compounds						
5) Naphthalene	10.776	128	1185	0.022	ng/ul#	Qvalue 81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101722\
Data File : BM037106.D
Acq On : 17 Oct 2022 11:04
Operator : CG/JU
Sample : N4984-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGNJ1


Quant Time: Oct 17 23:53:54 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 17 02:26:13 2022
Response via : Initial Calibration

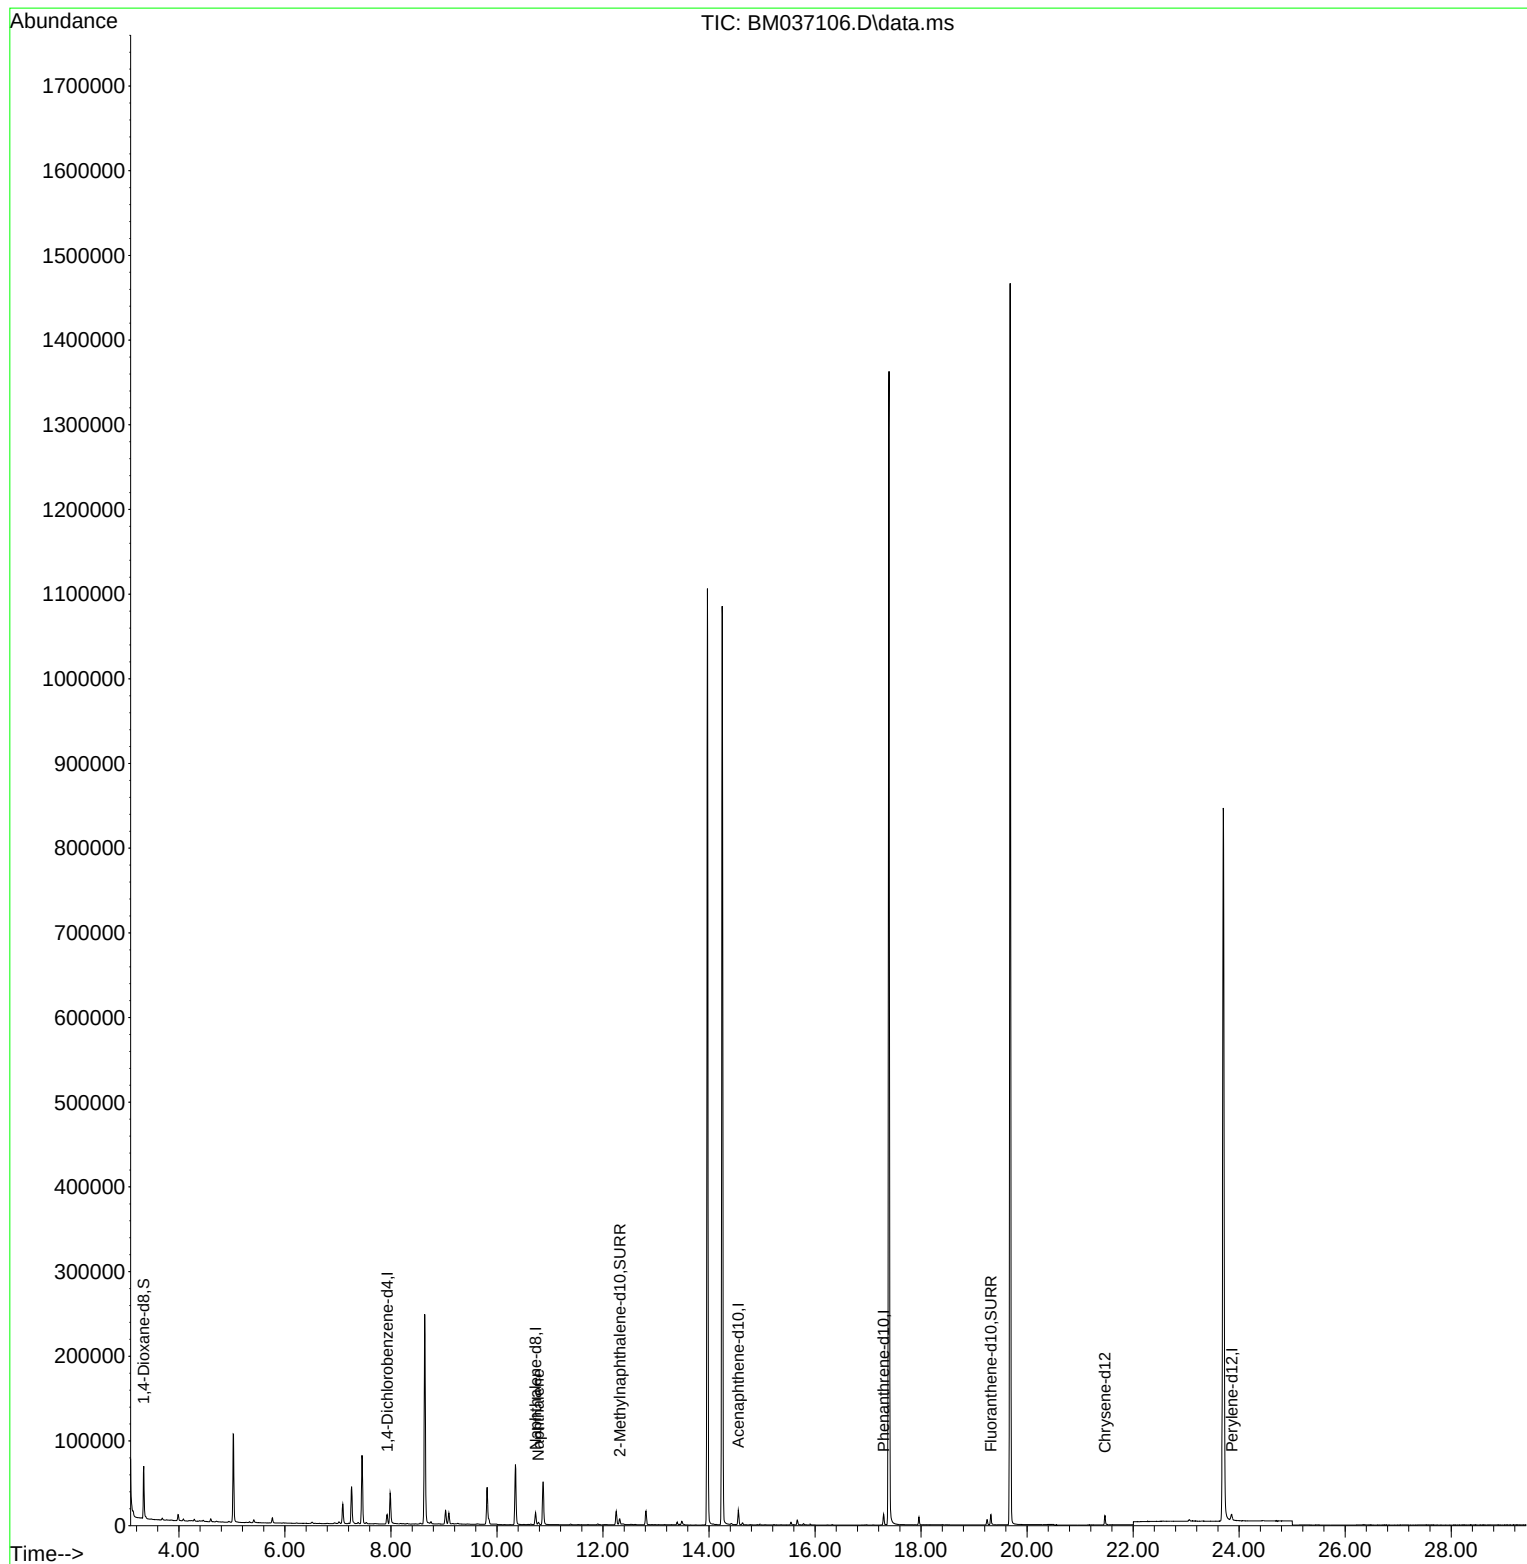

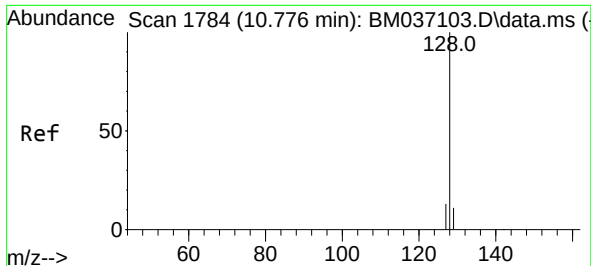

#5
Naphthalene
Concen: 0.022 ng/ul
RT: 10.776 min Scan# 11
Delta R.T. -0.005 min
Lab File: BM037106.D
Acq: 17 Oct 2022 11:04

Instrument :
BNA_M
ClientSampleId :
BGNJ1

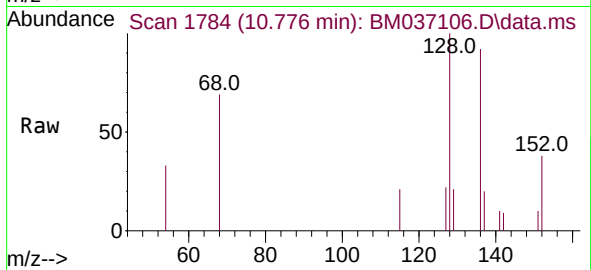

Tgt Ion:128 Resp: 1185
Ion Ratio Lower Upper
128 100
129 20.6 10.2 15.2#
127 22.3 11.7 17.5#

