

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101722\
 Data File : BM037107.D
 Acq On : 17 Oct 2022 11:40
 Operator : CG/JU
 Sample : N4984-12
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGNM1

Quant Time: Oct 17 23:54:01 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 17 02:26:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.926	152	4958	0.400	ng/ul	0.00
4) Naphthalene-d8	10.727	136	17673	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.557	164	9312	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.292	188	14900	0.400	ng/ul	0.00
17) Chrysene-d12	21.471	240	8305	0.400	ng/ul	0.00
23) Perylene-d12	23.853	264	8748	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.336	96	33782	4.831	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.316	152	9844	0.369	ng/ul	0.00
18) Fluoranthene-d10	19.317	212	12773	0.514	ng/ul	0.00
Target Compounds						
5) Naphthalene	10.776	128	1155	0.023	ng/ul#	Qvalue 77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101722\
Data File : BM037107.D
Acq On : 17 Oct 2022 11:40
Operator : CG/JU
Sample : N4984-12
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGNM1


Quant Time: Oct 17 23:54:01 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM100622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 17 02:26:13 2022
Response via : Initial Calibration

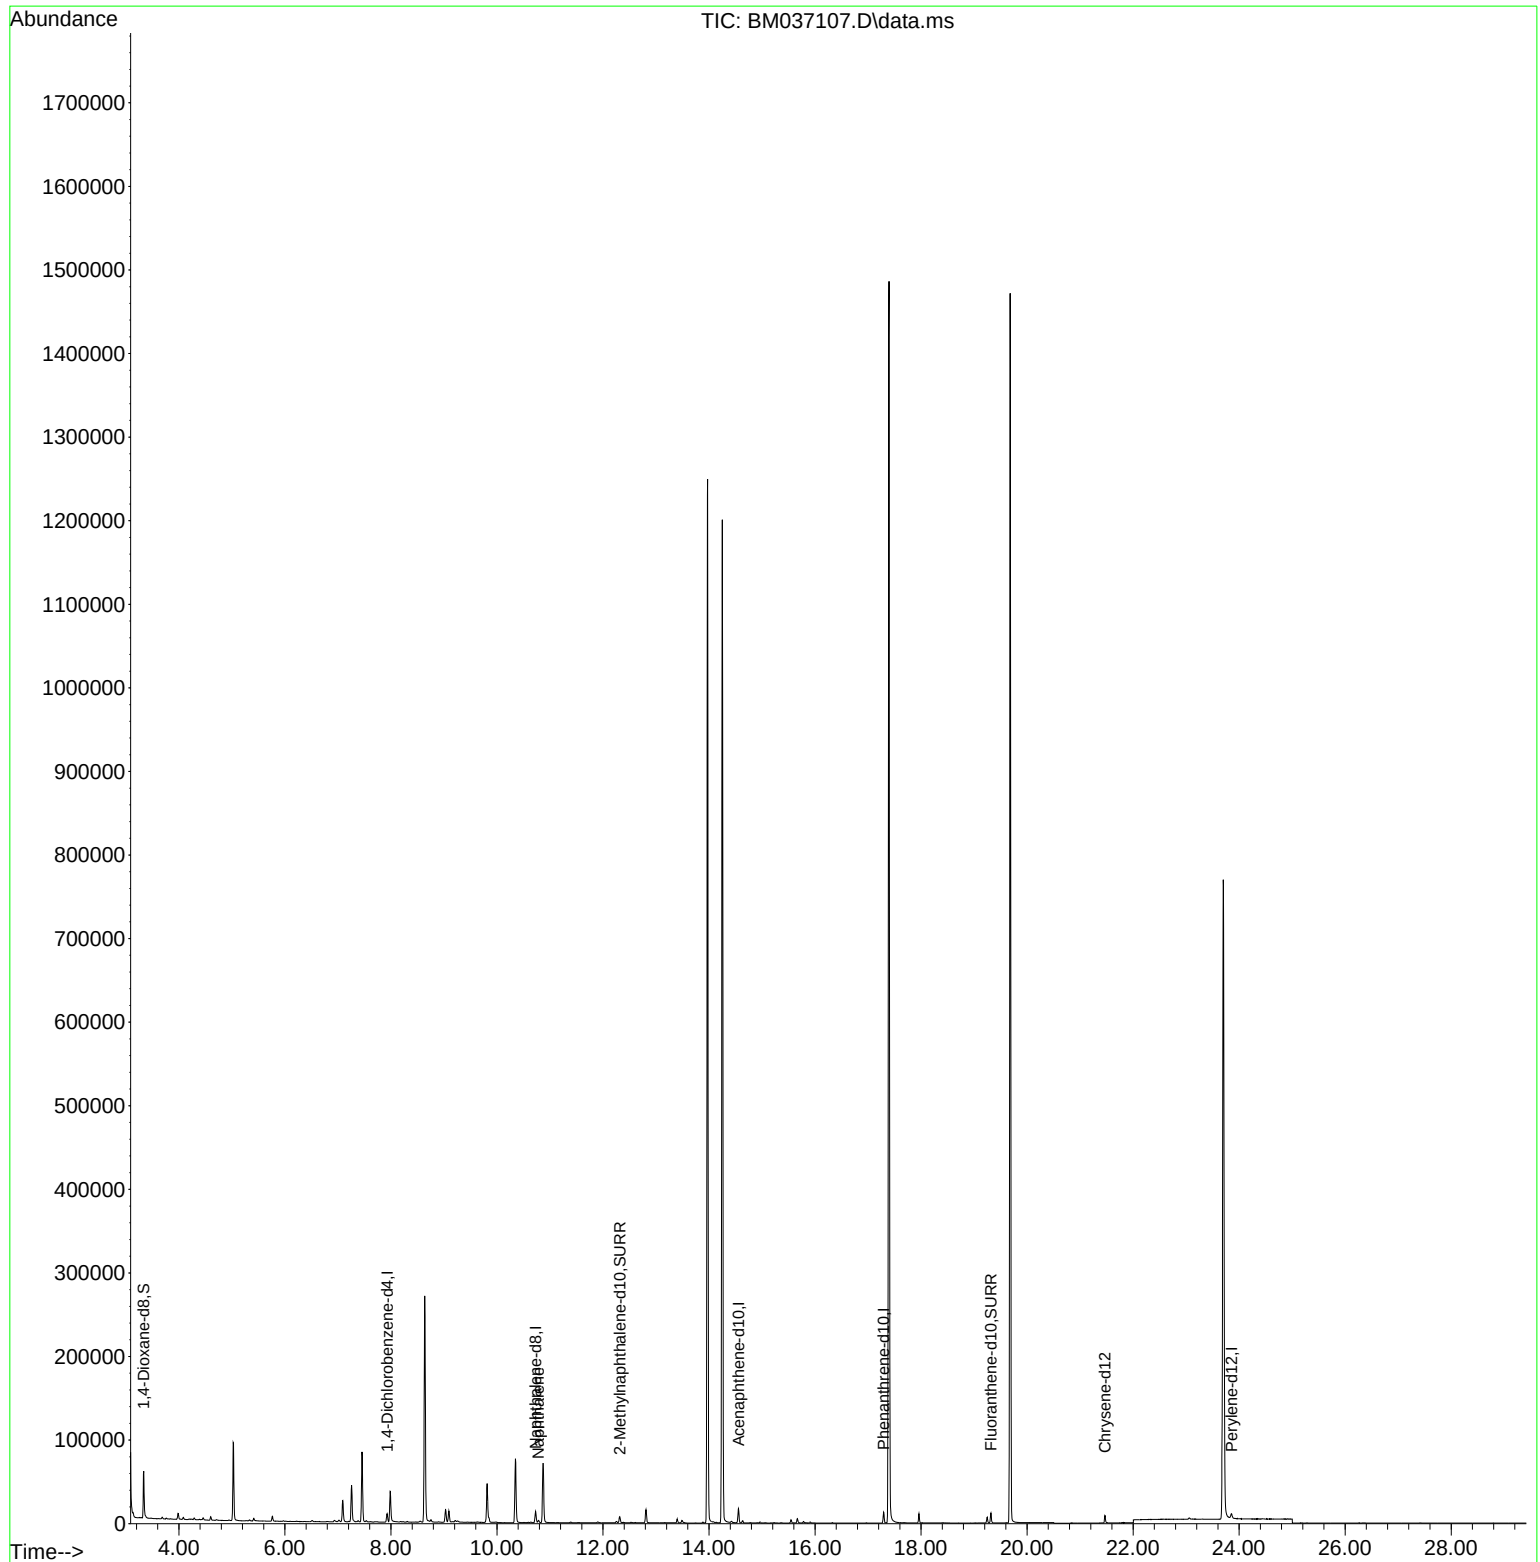

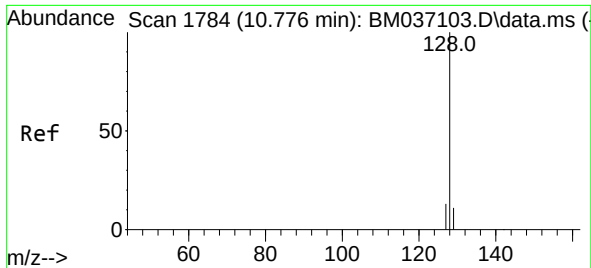

#5
Naphthalene
Concen: 0.023 ng/ul
RT: 10.776 min Scan# 11
Delta R.T. -0.005 min
Lab File: BM037107.D
Acq: 17 Oct 2022 11:40

Instrument :
BNA_M
ClientSampleId :
BGNM1

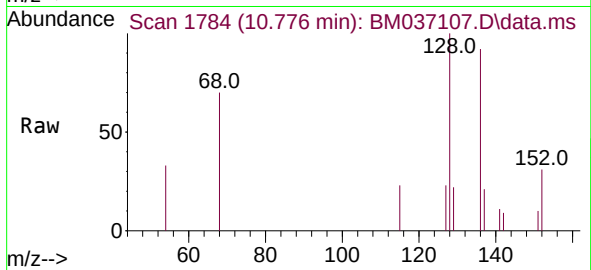

Tgt Ion:128 Resp: 1155
Ion Ratio Lower Upper
128 100
129 22.3 10.2 15.2#
127 23.3 11.7 17.5#

