

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
 Data File : BM048131.D
 Acq On : 18 Oct 2024 12:04
 Operator : RC/JU
 Sample : P4380-10
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E27J6

Quant Time: Oct 18 12:49:43 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 17 15:44:59 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	273150	20.000	ng/ul	0.00
20) Naphthalene-d8	10.557	136	1082905	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.404	164	660372	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.145	188	1270240	20.000	ng/ul	0.00
79) Chrysene-d12	21.368	240	1160055	20.000	ng/ul	0.00
88) Perylene-d12	24.350	264	1312531	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	33048	4.594	ng/uL	0.00
4) Pyridine-d5	3.657	84	72670	3.755	ng/ul	0.00
7) Phenol-d5	6.945	99	209963	9.489	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.098	67	455894	34.688	ng/ul	0.00
11) 2-Chlorophenol-d4	7.304	132	584919	30.564	ng/ul	0.00
15) 4-Methylphenol-d8	8.481	113	372348	21.622	ng/ul	0.00
21) Nitrobenzene-d5	8.928	128	302281	33.078	ng/ul	0.00
24) 2-Nitrophenol-d4	9.645	143	339951	33.618	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.186	165	550119	30.889	ng/ul	0.00
31) 4-Chloroaniline-d4	10.698	131	354804	15.221	ng/ul	0.00
46) Dimethylphthalate-d6	13.816	166	1646387	34.326	ng/ul	0.00
49) Acenaphthylene-d8	14.098	160	1867397	32.745	ng/ul	0.00
54) 4-Nitrophenol-d4	14.627	143	55006	6.205	ng/ul	0.00
60) Fluorene-d10	15.398	176	1421466	34.714	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.521	200	249197	30.331	ng/ul	0.00
73) Anthracene-d10	17.245	188	2180185	36.190	ng/ul	0.00
81) Pyrene-d10	19.533	212	2464216	34.763	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.150	264	2543928	36.288	ng/ul	0.00
Target Compounds						
16) Acetophenone	8.592	105	43878	1.662	ng/ul#	94
59) Diethylphthalate	15.221	149	103646	2.167	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
Data File : BM048131.D
Acq On : 18 Oct 2024 12:04
Operator : RC/JU
Sample : P4380-10
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J6

Quant Time: Oct 18 12:49:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 17 15:44:59 2024
Response via : Initial Calibration




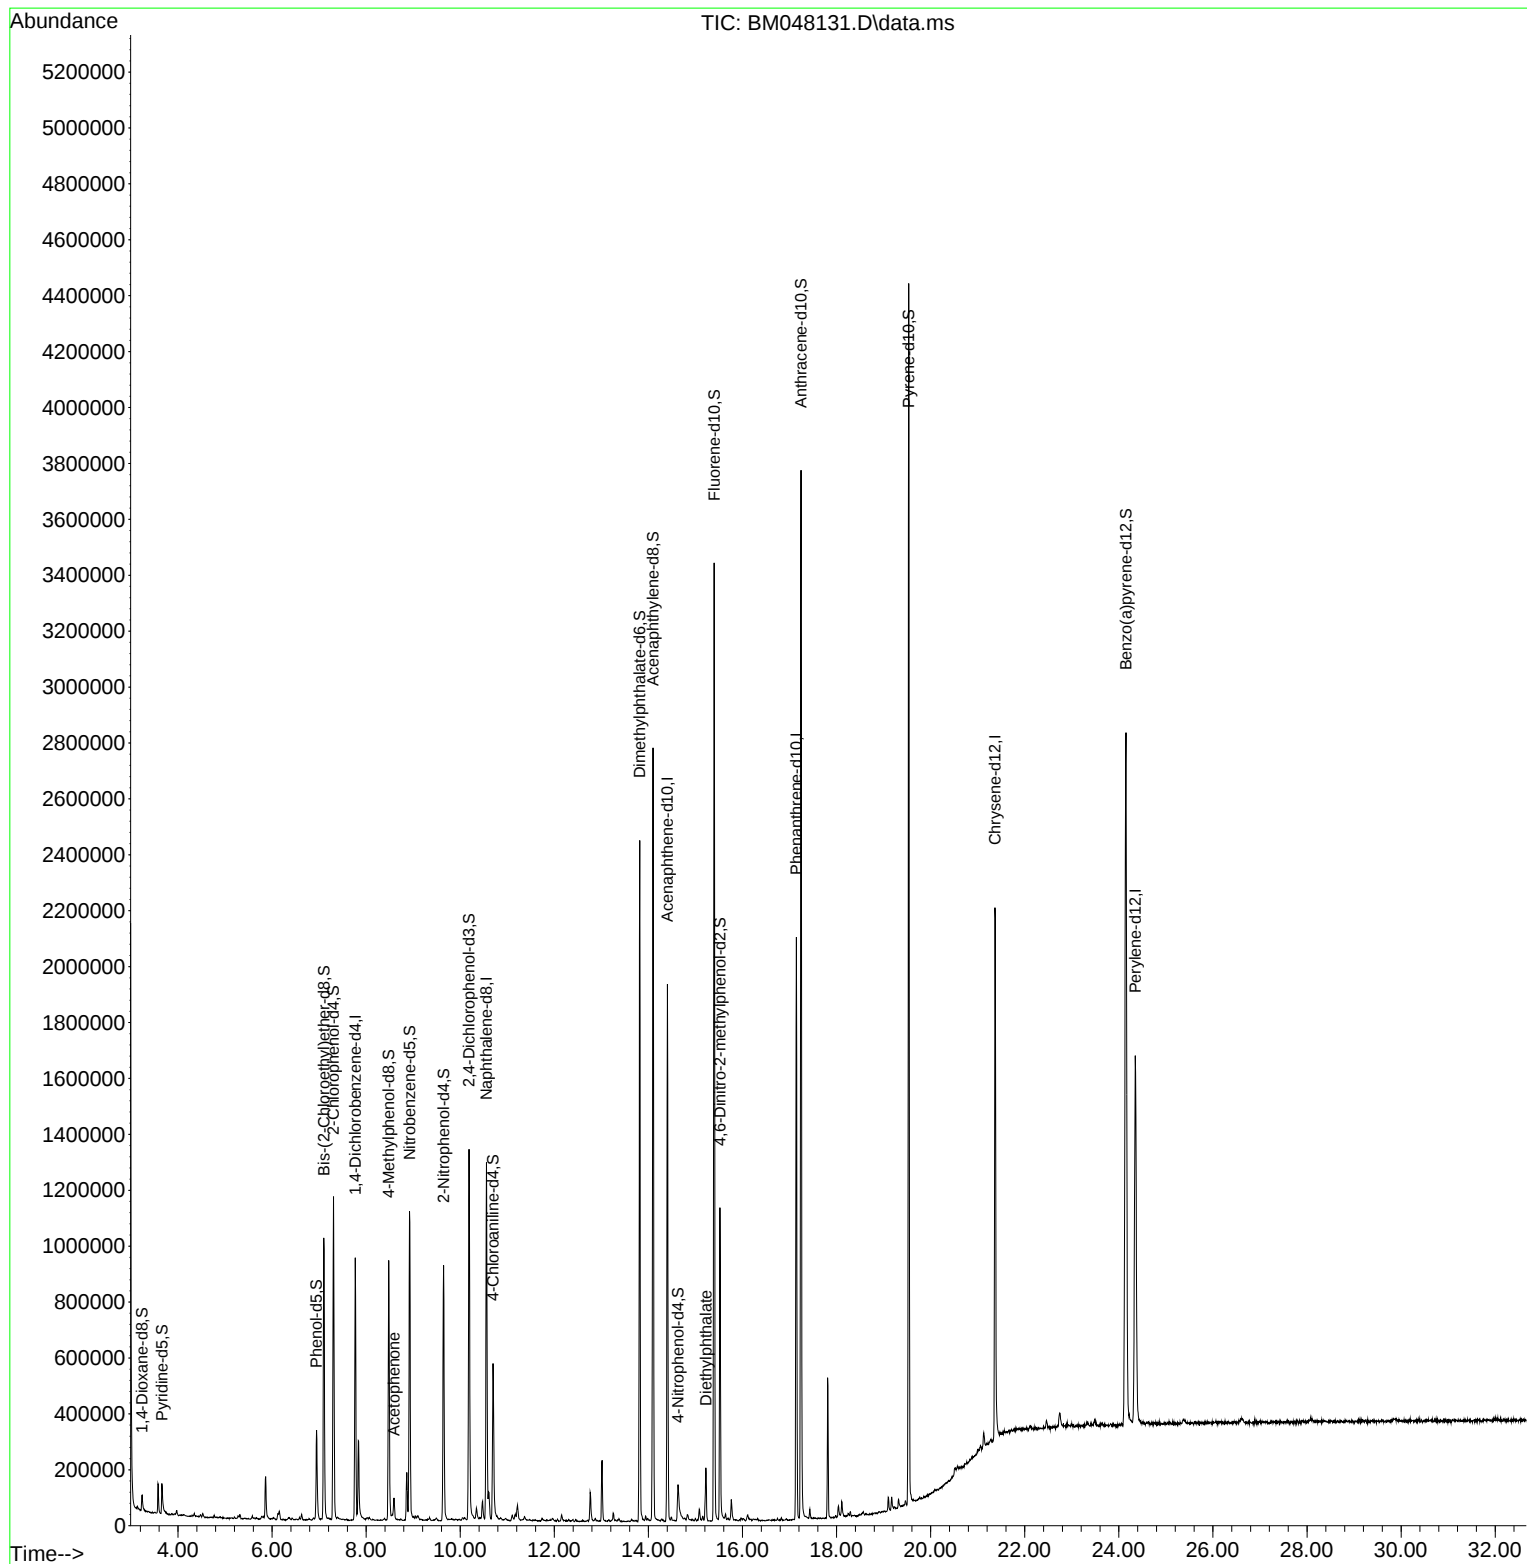


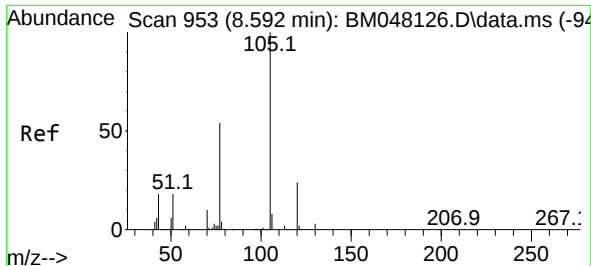

#16
Acetophenone
Concen: 1.662 ng/ul
RT: 8.592 min Scan# 91
Delta R.T. -0.000 min
Lab File: BM048131.D
Acq: 18 Oct 2024 12:04

Instrument :
BNA_M
ClientSampleId :
E27J6

Tgt Ion:105 Resp: 43878
Ion Ratio Lower Upper
105 100
77 77.3 59.3 88.9
51 30.6 19.9 29.9#

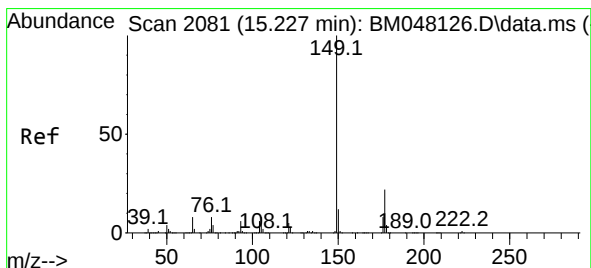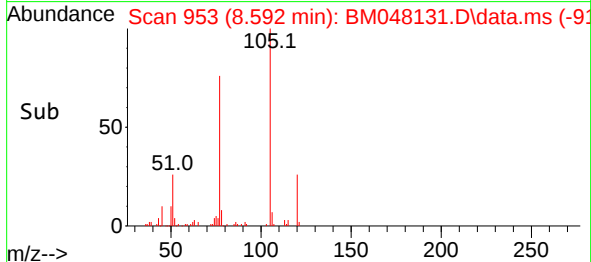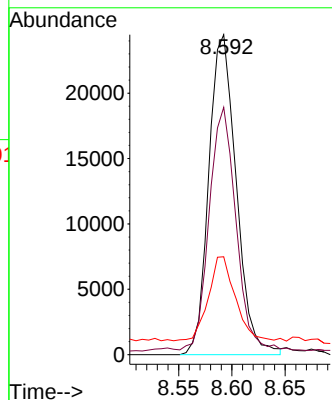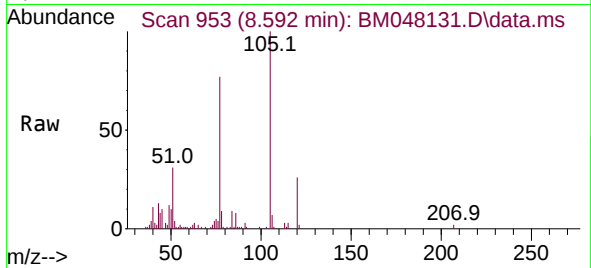

#59
Diethylphthalate
Concen: 2.167 ng/ul
RT: 15.221 min Scan# 2080
Delta R.T. -0.006 min
Lab File: BM048131.D
Acq: 18 Oct 2024 12:04

Tgt Ion:149 Resp: 103646
Ion Ratio Lower Upper
149 100
177 22.0 17.5 26.3
150 12.3 9.8 14.8

