

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
 Data File : BM048136.D
 Acq On : 18 Oct 2024 15:22
 Operator : RC/JU
 Sample : PB164048BS
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLCS048

Quant Time: Oct 18 15:56:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 17 15:44:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	260717	20.000	ng/u1	0.00
20) Naphthalene-d8	10.557	136	1024420	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.404	164	605356	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.145	188	1163886	20.000	ng/u1	0.00
79) Chrysene-d12	21.368	240	1028539	20.000	ng/u1	0.00
88) Perylene-d12	24.350	264	1157344	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	37194	5.417	ng/uL	0.00
4) Pyridine-d5	3.646	84	526086	28.477	ng/u1	0.00
7) Phenol-d5	6.945	99	619680	29.343	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.098	67	373868	29.803	ng/u1	0.00
11) 2-Chlorophenol-d4	7.304	132	538309	29.470	ng/u1	0.00
15) 4-Methylphenol-d8	8.481	113	484169	29.456	ng/u1	0.00
21) Nitrobenzene-d5	8.922	128	251529	29.096	ng/u1	0.00
24) 2-Nitrophenol-d4	9.645	143	279046	29.170	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.186	165	494915	29.376	ng/u1	0.00
31) 4-Chloroaniline-d4	10.698	131	613453	27.819	ng/u1	0.00
46) Dimethylphthalate-d6	13.816	166	1316556	29.944	ng/u1	0.00
49) Acenaphthylene-d8	14.098	160	1545310	29.560	ng/u1	0.00
54) 4-Nitrophenol-d4	14.621	143	240461	29.589	ng/u1	0.00
60) Fluorene-d10	15.398	176	1118246	29.791	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.521	200	225509	29.956	ng/u1	0.00
73) Anthracene-d10	17.245	188	1658349	30.043	ng/u1	0.00
81) Pyrene-d10	19.533	212	1873916	29.816	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.150	264	1909005	30.882	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.269	88	76698	10.667	ng/uL	94
5) Pyridine	3.669	79	518734	27.480	ng/u1	96
6) Benzaldehyde	6.910	77	287863	29.455	ng/u1	99
8) Phenol	6.975	94	632818	29.131	ng/u1	98
10) Bis(2-Chloroethyl)ether	7.192	93	506751	29.066	ng/u1	99
12) 2-Chlorophenol	7.340	128	540560	29.370	ng/u1	98
13) 2-Methylphenol	8.216	108	477488	29.058	ng/u1	100
14) 2,2'-oxybis(1-Chloropr...	8.287	45	738025	29.987	ng/u1	98
16) Acetophenone	8.592	105	762572	30.253	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.575	70	355303	29.771	ng/u1	98
18) 4-Methylphenol	8.545	108	518282	29.315	ng/u1	99
19) Hexachloroethane	8.845	117	226834	28.992	ng/u1	99
22) Nitrobenzene	8.969	77	542226	28.987	ng/u1	99
23) Isophorone	9.492	82	1036887	28.985	ng/u1	98
25) 2-Nitrophenol	9.675	139	293891	28.810	ng/u1	99
26) 2,4-Dimethylphenol	9.739	107	464266	26.126	ng/u1	98
27) Bis(2-Chloroethoxy)met...	9.969	93	644881	28.773	ng/u1	100
29) 2,4-Dichlorophenol	10.216	162	486075	28.802	ng/u1	99
30) Naphthalene	10.610	128	1622581	28.653	ng/u1	100
32) 4-Chloroaniline	10.722	127	471006	22.150	ng/u1	99
33) Hexachlorobutadiene	10.892	225	316204	28.346	ng/u1	99
34) Caprolactam	11.504	113	147795	28.313	ng/u1	96
35) 4-Chloro-3-methylphenol	11.857	107	476659	29.381	ng/u1	99
36) 2-Methylnaphthalene	12.222	142	1060780	28.782	ng/u1	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
 Data File : BM048136.D
 Acq On : 18 Oct 2024 15:22
 Operator : RC/JU
 Sample : PB164048BS
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLCS048

Quant Time: Oct 18 15:56:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 17 15:44:59 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.439	142	1054963	28.422	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.592	216	565903	28.692	ng/ul	99
40) Hexachlorocyclopentadiene	12.574	237	309024	27.999	ng/ul	99
41) 2,4,6-Trichlorophenol	12.839	196	360825	27.818	ng/ul	98
42) 2,4,5-Trichlorophenol	12.916	196	389506	28.516	ng/ul	97
43) 1,1'-Biphenyl	13.239	154	1367498	29.250	ng/ul	99
44) 2-Chloronaphthalene	13.280	162	1070936	28.888	ng/ul	99
45) 2-Nitroaniline	13.486	65	290613	30.161	ng/ul	98
47) Dimethylphthalate	13.863	163	1301565	29.439	ng/ul	99
48) 2,6-Dinitrotoluene	13.980	165	265885	30.281	ng/ul	99
50) Acenaphthylene	14.127	152	1676861	29.651	ng/ul	99
51) 3-Nitroaniline	14.316	138	265625	29.002	ng/ul	95
52) Acenaphthene	14.468	153	1121297	28.657	ng/ul	99
53) 2,4-Dinitrophenol	14.527	184	161654	27.903	ng/ul	97
55) 4-Nitrophenol	14.633	109	164610	29.114	ng/ul	97
56) Dibenzofuran	14.804	168	1571321	29.352	ng/ul	100
57) 2,4-Dinitrotoluene	14.774	165	386263	30.967	ng/ul	98
58) 2,3,4,6-Tetrachlorophenol	15.033	232	310264	28.158	ng/ul#	98
59) Diethylphthalate	15.227	149	1294770	29.530	ng/ul	99
61) Fluorene	15.451	166	1237618	29.580	ng/ul	98
62) 4-Chlorophenyl-phenyle...	15.445	204	617284	29.665	ng/ul	99
63) 4-Nitroaniline	15.474	138	280712	35.389	ng/ul	95
66) 4,6-Dinitro-2-methylph...	15.539	198	243846	30.112	ng/ul	97
67) N-Nitrosodiphenylamine	15.663	169	1053760	30.106	ng/ul	99
68) 4-Bromophenyl-phenylether	16.339	248	375747	29.757	ng/ul	97
69) Hexachlorobenzene	16.457	284	443157	29.695	ng/ul	100
70) Atrazine	16.610	200	239031	20.349	ng/ul	97
71) Pentachlorophenol	16.804	266	259555	26.976	ng/ul	98
72) Phenanthrene	17.186	178	1907583	29.962	ng/ul	99
74) Anthracene	17.280	178	1918652	30.031	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.204	216	546058	27.909	ng/ul	98
76) Pentachlorobenzene	14.727	250	524668	27.539	ng/ul	97
77) Carbazole	17.551	167	1752142	30.961	ng/ul	100
78) Di-n-butylphthalate	18.109	149	2234114	29.973	ng/ul	99
80) Fluoranthene	19.198	202	2161407	29.557	ng/ul	99
82) Pyrene	19.562	202	2295657	29.470	ng/ul	99
83) Butylbenzylphthalate	20.456	149	1003617	29.657	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.274	252	699904	30.511	ng/ul	100
85) Benzo(a)anthracene	21.350	228	2209493	29.544	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.268	149	1442483	29.487	ng/ul	100
87) Chrysene	21.415	228	2066921	29.328	ng/ul	99
89) Di-n-octyl phthalate	22.391	149	2537902	30.391	ng/ul	100
90) Benzo(b)fluoranthene	23.409	252	2200619	30.187	ng/ul	99
91) Benzo(k)fluoranthene	23.468	252	2239738	30.849	ng/ul	99
93) Benzo(a)pyrene	24.215	252	2012842	29.661	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	27.721	276	2639334	30.000	ng/ul	100
95) Dibenzo(a,h)anthracene	27.768	278	2167814	30.498	ng/ul	99
96) Benzo(g,h,i)perylene	28.762	276	2068082	30.205	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
Data File : BM048136.D
Acq On : 18 Oct 2024 15:22
Operator : RC/JU
Sample : PB164048BS
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SLCS048

Quant Time: Oct 18 15:56:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 17 15:44:59 2024
Response via : Initial Calibration




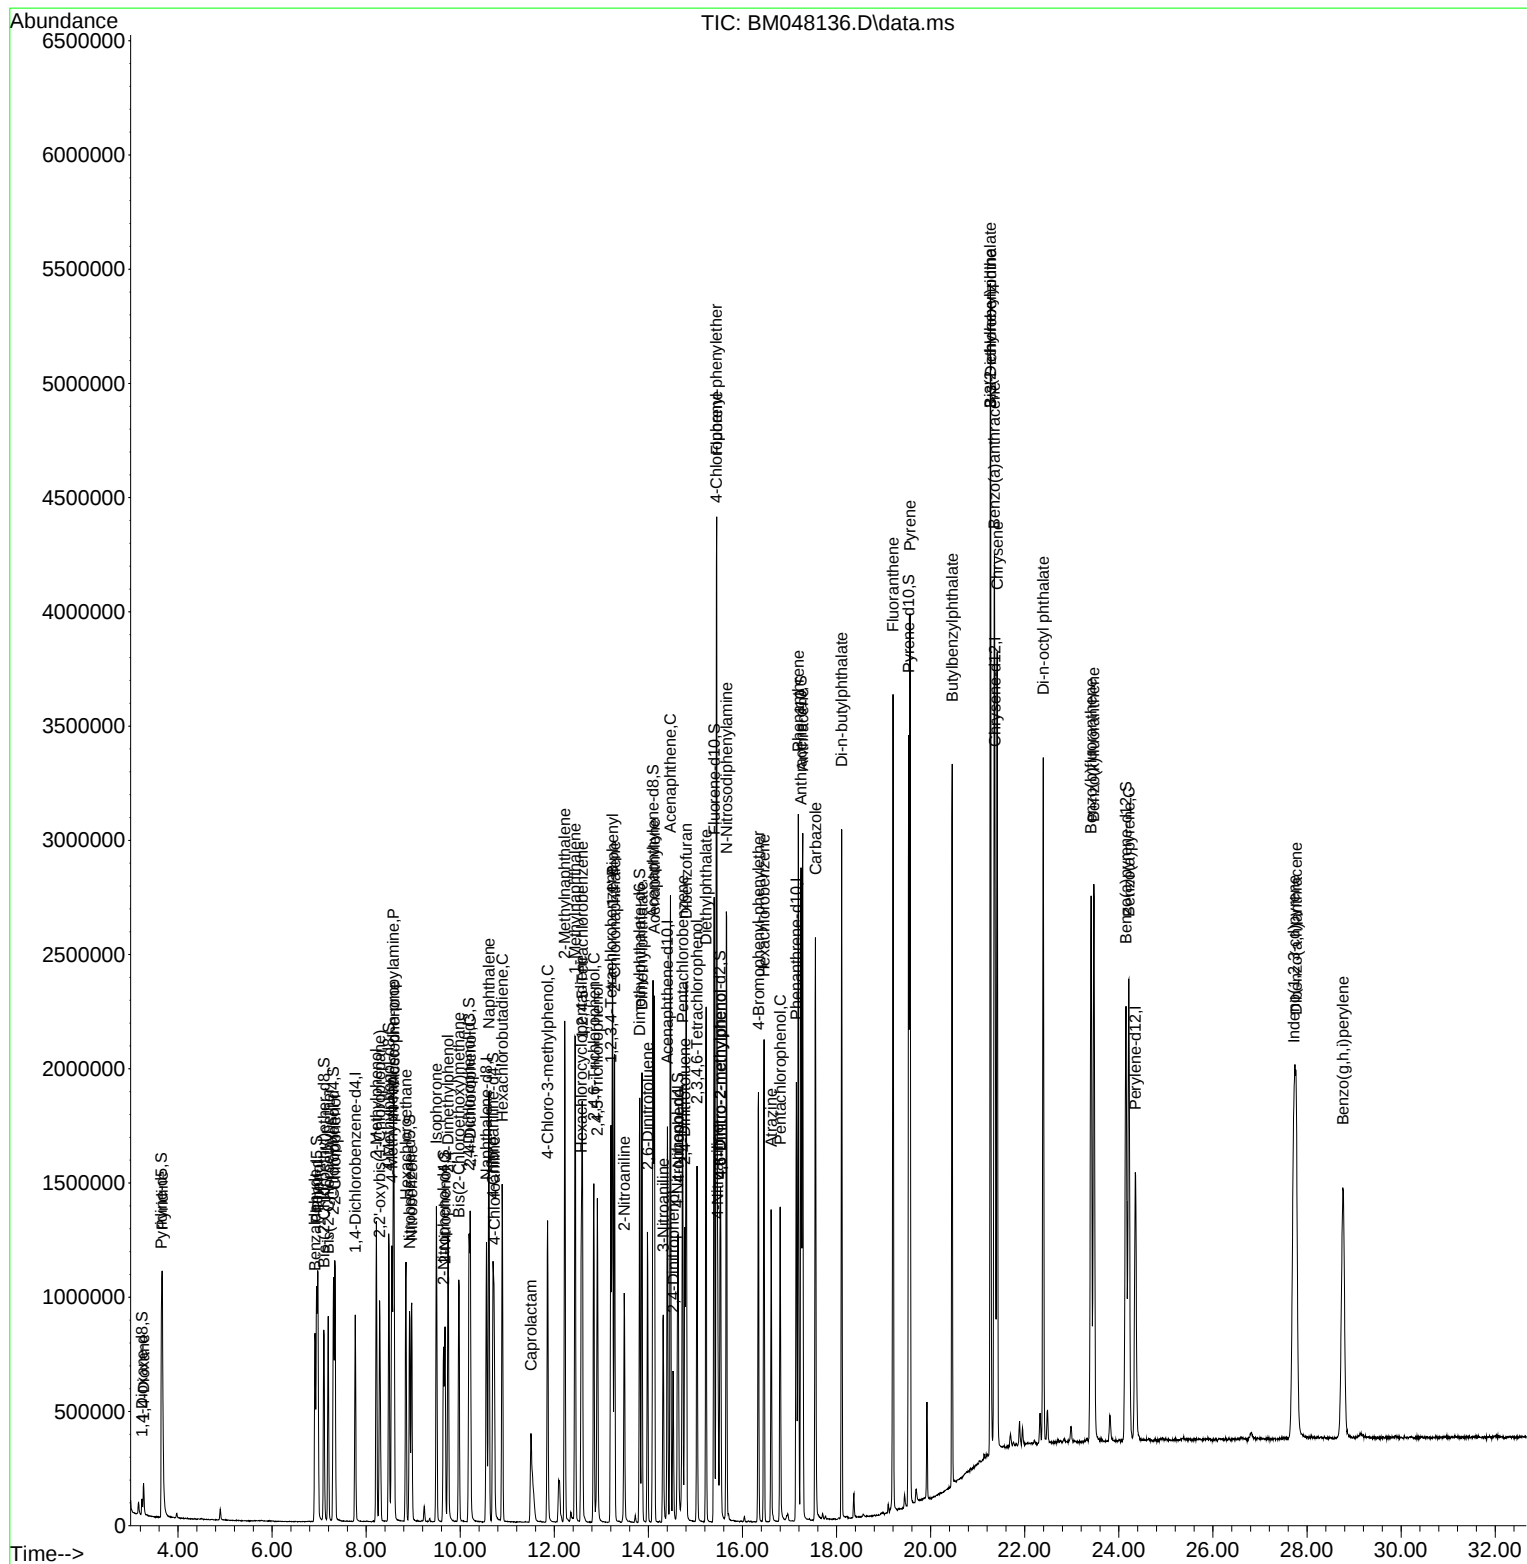




#2
1,4-Dioxane
Concen: 10.667 ng/uL
RT: 3.269 min Scan# 48
Delta R.T. -0.000 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22




Instrument :
BNA_M
ClientSampleId :
SLCS048


Tgt Ion: 88 Resp: 76698
Ion Ratio Lower Upper
88 100
43 27.9 22.5 33.7
58 78.3 57.2 85.8



#5
Pyridine
Concen: 27.480 ng/uL
RT: 3.669 min Scan# 116
Delta R.T. -0.000 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22

Tgt Ion: 79 Resp: 518734
Ion Ratio Lower Upper
79 100
52 73.5 62.6 93.8
51 33.8 27.4 41.0





#6

Benzaldehyde

Concen: 29.455 ng/ul

RT: 6.910 min Scan# 668

Delta R.T. -0.006 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22

Instrument :

BNA_M

ClientSampleId :

SLCS048





Tgt Ion: 77 Resp: 287863

Ion Ratio Lower Upper

77 100

105 101.9 83.0 124.4

106 100.0 79.3 118.9

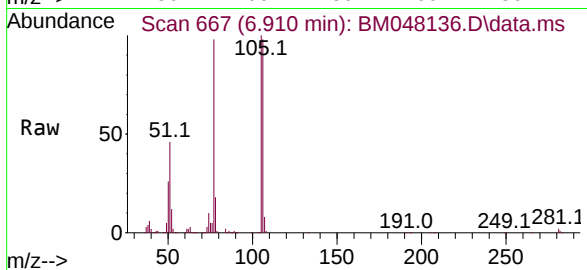

#8

Phenol

Concen: 29.131 ng/ul

RT: 6.975 min Scan# 678

Delta R.T. -0.000 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22




Tgt Ion: 94 Resp: 632818


Ion Ratio Lower Upper

94 100

65 25.4 21.0 31.4

66 32.7 25.0 37.6

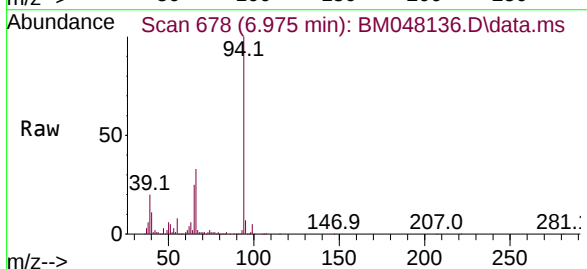



#10

Bis(2-Chloroethyl)ether

Concen: 29.066 ng/ul

RT: 7.192 min Scan# 715

Delta R.T. -0.006 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22

Instrument :

BNA_M

ClientSampleId :

SLCS048





Tgt Ion: 93 Resp: 506751

Ion Ratio Lower Upper

93 100

63 72.0 58.7 88.1

95 31.7 25.4 38.2



#12

2-Chlorophenol

Concen: 29.370 ng/ul

RT: 7.340 min Scan# 740

Delta R.T. -0.000 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22




Tgt Ion: 128 Resp: 540560


Ion Ratio Lower Upper

128 100

64 41.9 34.8 52.2

130 32.6 26.2 39.4









#13
2-Methylphenol
Concen: 29.058 ng/ul
RT: 8.216 min Scan# 889
Delta R.T. -0.006 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22




Instrument :
BNA_M
ClientSampleId :
SLCS048


Tgt Ion:108 Resp: 477488
Ion Ratio Lower Upper
108 100
107 87.5 70.2 105.2

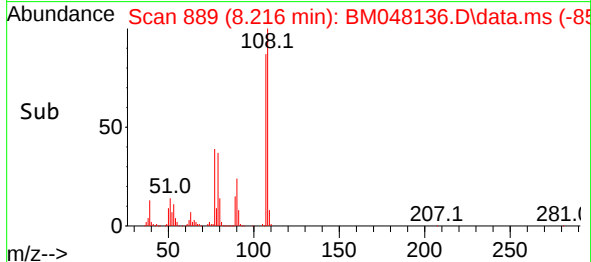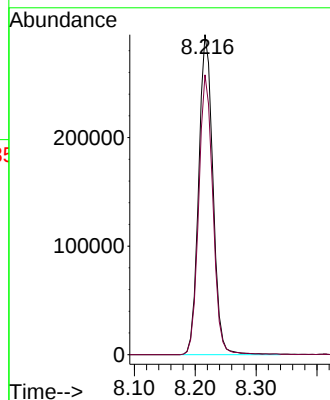

#14
2,2'-oxybis(1-Chloropropane)
Concen: 29.987 ng/ul
RT: 8.287 min Scan# 901
Delta R.T. -0.006 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22

Tgt Ion: 45 Resp: 738025
Ion Ratio Lower Upper
45 100
77 13.2 11.4 17.0
79 10.1 8.3 12.5



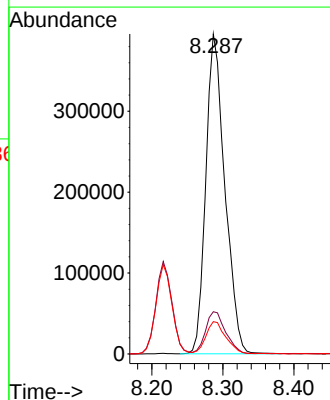





#16
Acetophenone
Concen: 30.253 ng/ul
RT: 8.592 min Scan# 91
Delta R.T. -0.000 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22




Instrument :
BNA_M
ClientSampleId :
SLCS048


Tgt Ion:105 Resp: 762572
Ion Ratio Lower Upper
105 100
77 72.8 59.3 88.9
51 24.1 19.9 29.9

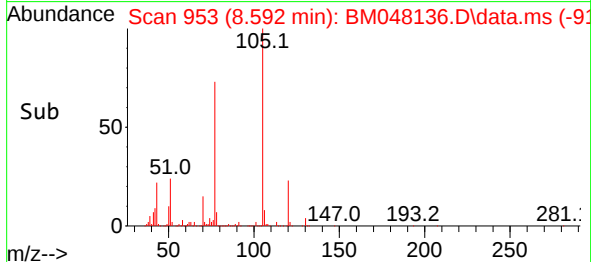

#17
N-Nitroso-di-n-propylamine
Concen: 29.771 ng/ul
RT: 8.575 min Scan# 950
Delta R.T. -0.000 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22

Tgt Ion: 70 Resp: 355303
Ion Ratio Lower Upper
70 100
42 56.6 43.6 65.4
101 10.3 7.9 11.9
130 22.6 17.8 26.8







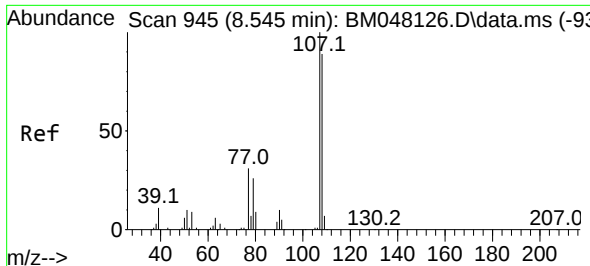

#18
4-Methylphenol
Concen: 29.315 ng/ul
RT: 8.545 min Scan# 945
Delta R.T. -0.000 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22




Instrument :
BNA_M
ClientSampleId :
SLCS048


Tgt Ion:108 Resp: 518282
Ion Ratio Lower Upper
108 100
107 111.7 90.2 135.4

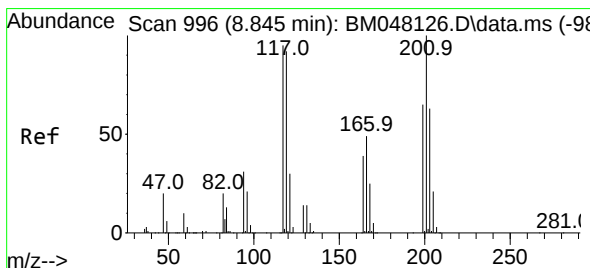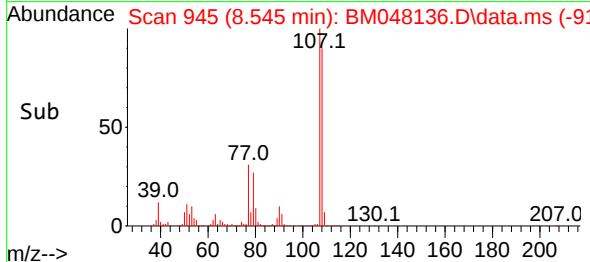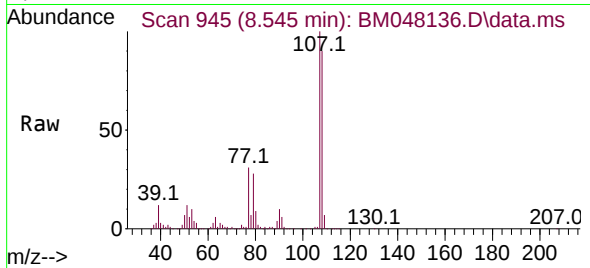

#19
Hexachloroethane
Concen: 28.992 ng/ul
RT: 8.845 min Scan# 996
Delta R.T. -0.000 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22

Tgt Ion:117 Resp: 226834
Ion Ratio Lower Upper
117 100
201 101.7 81.5 122.3
199 64.4 49.4 74.0


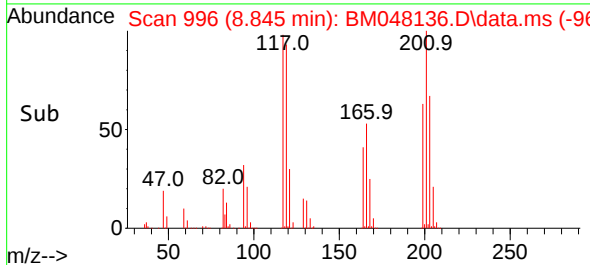

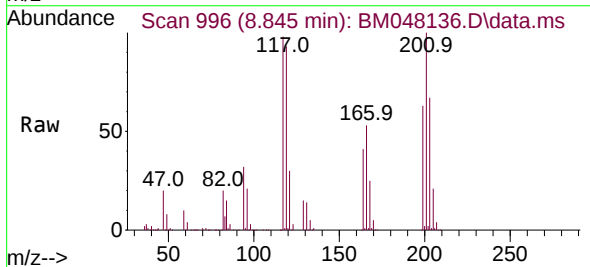




#22
Nitrobenzene
Concen: 28.987 ng/ul
RT: 8.969 min Scan# 1017
Delta R.T. -0.000 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22




Instrument :
BNA_M
ClientSampleId :
SLCS048


Tgt Ion: 77 Resp: 542226
Ion Ratio Lower Upper
77 100
123 49.6 39.6 59.4
65 12.6 11.0 16.4

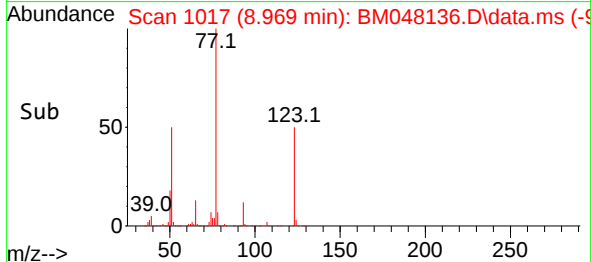

#23
Isophorone
Concen: 28.985 ng/ul
RT: 9.492 min Scan# 1106
Delta R.T. -0.006 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22

Tgt Ion: 82 Resp: 1036887
Ion Ratio Lower Upper
82 100
95 6.4 5.2 7.8
138 17.6 15.2 22.8





#25

2-Nitrophenol

Concen: 28.810 ng/ul

RT: 9.675 min Scan# 1137

Delta R.T. -0.006 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22

Instrument :

BNA_M

ClientSampleId :

SLCS048





Tgt Ion:139 Resp: 293891

Ion Ratio Lower Upper

139 100

65 45.1 36.4 54.6

109 26.4 20.9 31.3



#26

2,4-Dimethylphenol

Concen: 26.126 ng/ul

RT: 9.739 min Scan# 1148

Delta R.T. -0.006 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22




Tgt Ion:107 Resp: 464266


Ion Ratio Lower Upper

107 100

121 52.0 40.4 60.6

122 89.9 70.6 106.0




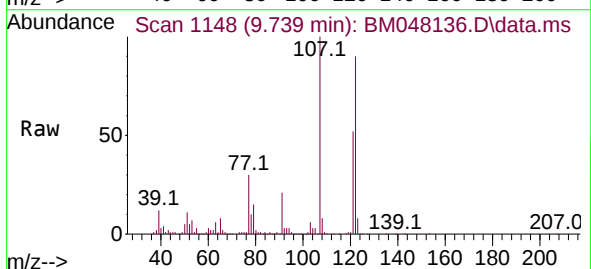




#27
 Bis(2-Chloroethoxy)methane
 Concen: 28.773 ng/ul
 RT: 9.969 min Scan# 1187
 Delta R.T. -0.006 min
 Lab File: BM048136.D
 Acq: 18 Oct 2024 15:22




Instrument :
 BNA_M
 ClientSampleId :
 SLCS048


Tgt Ion: 93 Resp: 644881
 Ion Ratio Lower Upper
 93 100
 95 32.7 26.3 39.5
 123 11.9 9.6 14.4

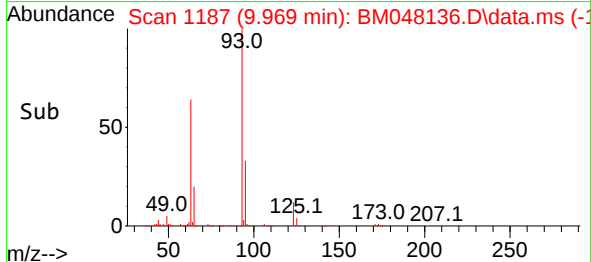

#29
 2,4-Dichlorophenol
 Concen: 28.802 ng/ul
 RT: 10.216 min Scan# 1229
 Delta R.T. -0.000 min
 Lab File: BM048136.D
 Acq: 18 Oct 2024 15:22

Tgt Ion:162 Resp: 486075
 Ion Ratio Lower Upper
 162 100
 164 64.7 52.0 78.0
 98 34.8 27.4 41.0









#30
Naphthalene
Concen: 28.653 ng/ul
RT: 10.610 min Scan# 1296
Delta R.T. -0.000 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22




Instrument :
BNA_M
ClientSampleId :
SLCS048


Tgt Ion:128 Resp: 1622581
Ion Ratio Lower Upper
128 100
129 11.2 8.7 13.1
127 12.9 10.3 15.5



#32
4-Chloroaniline
Concen: 22.150 ng/ul
RT: 10.722 min Scan# 1315
Delta R.T. -0.000 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22

Tgt Ion:127 Resp: 471006
Ion Ratio Lower Upper
127 100
129 32.4 26.4 39.6









#33
Hexachlorobutadiene
Concen: 28.346 ng/ul
RT: 10.892 min Scan# 11
Delta R.T. -0.006 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22




Instrument :
BNA_M
ClientSampleId :
SLCS048


Tgt Ion:225 Resp: 316204
Ion Ratio Lower Upper
225 100
223 64.5 50.6 76.0
227 65.1 51.3 76.9



#34
Caprolactam
Concen: 28.313 ng/ul
RT: 11.504 min Scan# 1448
Delta R.T. -0.000 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22

Tgt Ion:113 Resp: 147795
Ion Ratio Lower Upper
113 100
55 161.2 123.8 185.8
56 119.4 92.9 139.3









#35
4-Chloro-3-methylphenol
Concen: 29.381 ng/ul
RT: 11.857 min Scan# 11
Delta R.T. -0.000 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22




Instrument :
BNA_M
ClientSampleId :
SLCS048


Tgt Ion:107 Resp: 476659
Ion Ratio Lower Upper
107 100
144 26.6 22.2 33.2
142 81.9 65.7 98.5

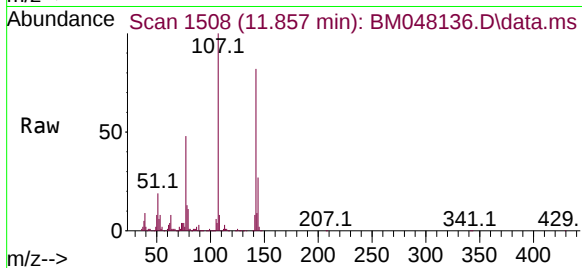

#36
2-Methylnaphthalene
Concen: 28.782 ng/ul
RT: 12.222 min Scan# 1570
Delta R.T. -0.006 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22

Tgt Ion:142 Resp: 1060780
Ion Ratio Lower Upper
142 100
141 88.1 71.1 106.7

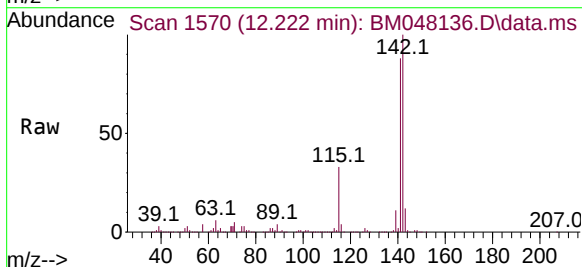

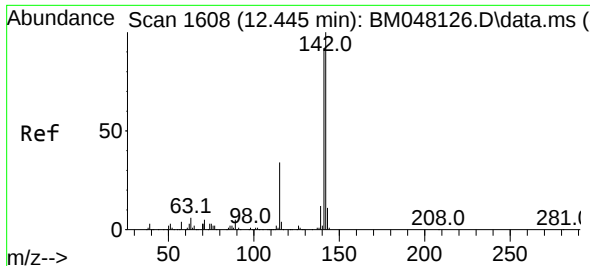

#37

1-Methylnaphthalene

Concen: 28.422 ng/ul

RT: 12.439 min Scan# 1

Delta R.T. -0.006 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22

Instrument :

BNA_M

ClientSampleId :

SLCS048





Tgt Ion:142 Resp: 1054963

Ion Ratio Lower Upper

142 100

141 91.8 72.8 109.2

116 3.6 2.7 4.1

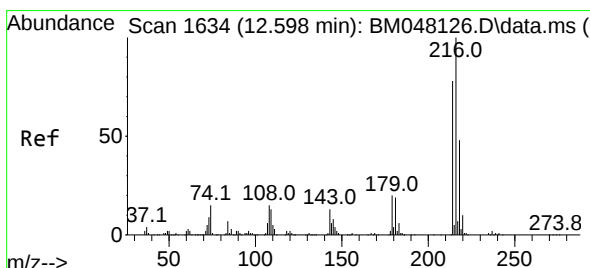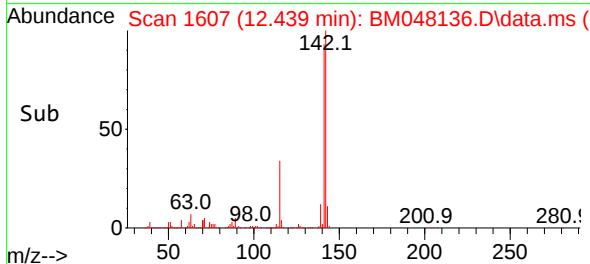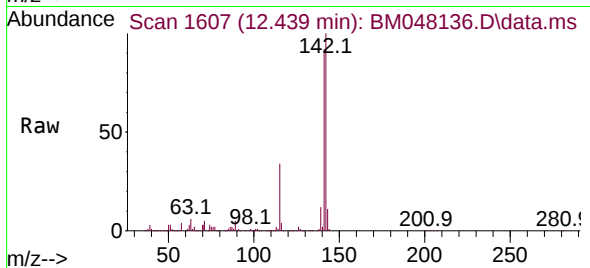

#39

1,2,4,5-Tetrachlorobenzene

Concen: 28.692 ng/ul

RT: 12.592 min Scan# 1633

Delta R.T. -0.006 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22

Tgt Ion:216 Resp: 565903




Ion Ratio Lower Upper


216 100

214 78.1 62.6 94.0

179 20.6 16.2 24.2

108 17.2 13.0 19.4


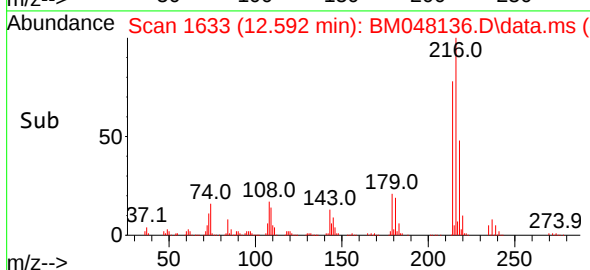
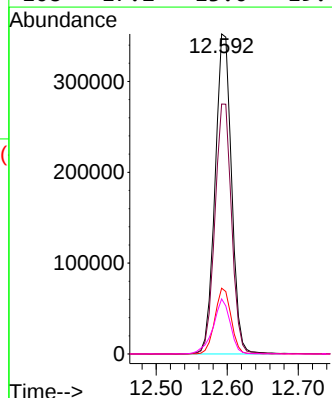
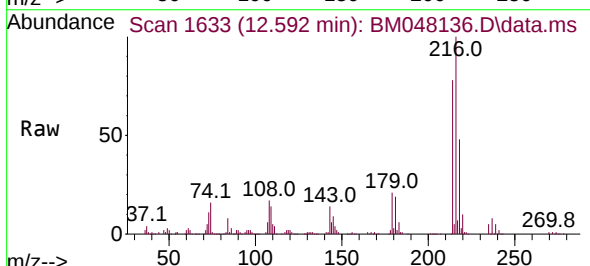




#40
Hexachlorocyclopentadiene
Concen: 27.999 ng/ul
RT: 12.574 min Scan# 1630
Delta R.T. -0.000 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22




Instrument :
BNA_M
ClientSampleId :
SLCS048


Tgt Ion:237 Resp: 309024
Ion Ratio Lower Upper
237 100
235 62.4 50.1 75.1
272 13.1 10.0 15.0

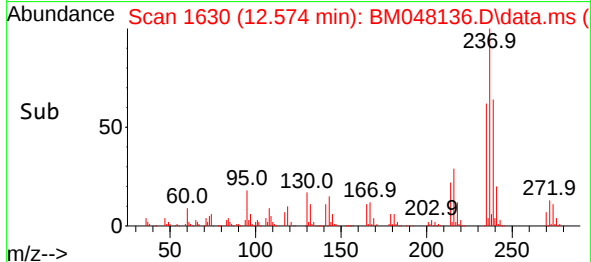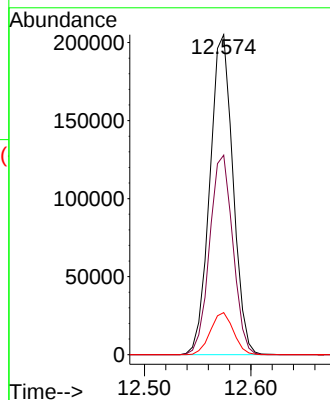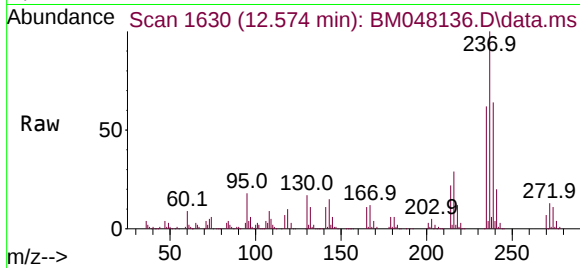

#41
2,4,6-Trichlorophenol
Concen: 27.818 ng/ul
RT: 12.839 min Scan# 1675
Delta R.T. -0.006 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22

Tgt Ion:196 Resp: 360825
Ion Ratio Lower Upper
196 100
198 98.3 77.0 115.4
200 31.2 24.9 37.3



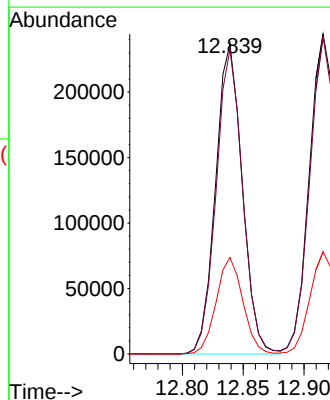
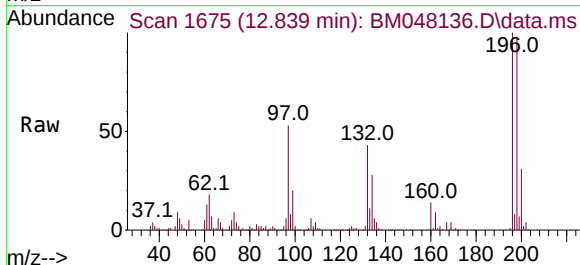




#42
2,4,5-Trichlorophenol
Concen: 28.516 ng/ul
RT: 12.916 min Scan# 1
Delta R.T. -0.000 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22




Instrument :
BNA_M
ClientSampleId :
SLCS048


Tgt Ion:196 Resp: 389506
Ion Ratio Lower Upper
196 100
198 99.1 76.1 114.1
200 32.0 25.3 37.9

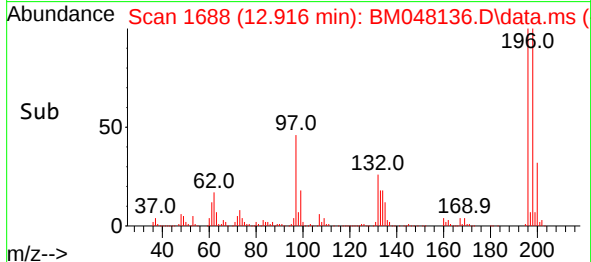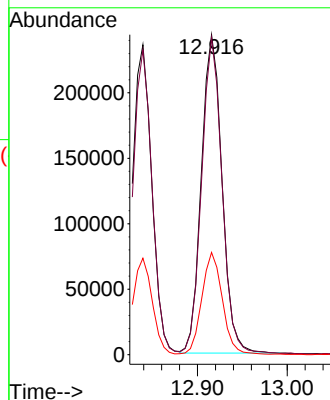

#43
1,1'-Biphenyl
Concen: 29.250 ng/ul
RT: 13.239 min Scan# 1743
Delta R.T. -0.000 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22

Tgt Ion:154 Resp: 1367498
Ion Ratio Lower Upper
154 100
153 39.2 31.5 47.3
76 11.6 9.6 14.4

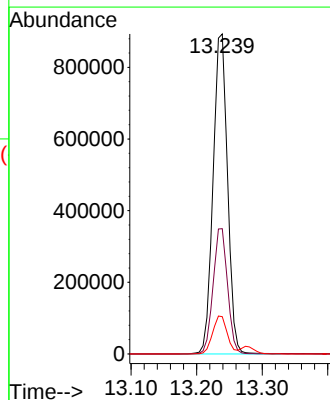



#44

2-Chloronaphthalene

Concen: 28.888 ng/ul

RT: 13.280 min Scan# 1

Delta R.T. -0.000 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22

Instrument :

BNA_M

ClientSampleId :

SLCS048





Tgt Ion:162 Resp: 1070936

Ion Ratio Lower Upper

162 100

164 33.2 26.2 39.2

127 37.2 30.6 46.0

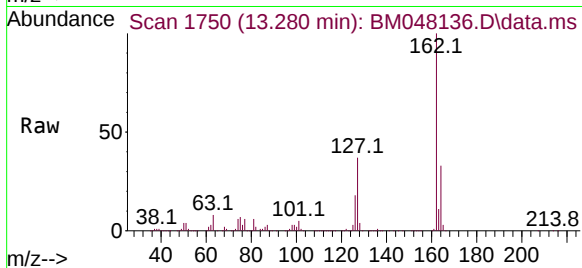

#45

2-Nitroaniline

Concen: 30.161 ng/ul

RT: 13.486 min Scan# 1785

Delta R.T. -0.000 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22




Tgt Ion: 65 Resp: 290613


Ion Ratio Lower Upper

65 100

92 70.8 59.2 88.8

138 118.0 95.2 142.8

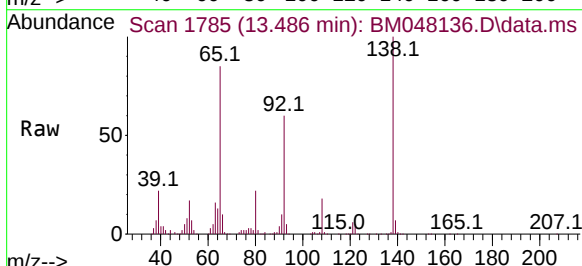



#47

Dimethylphthalate

Concen: 29.439 ng/ul

RT: 13.863 min Scan# 1

Delta R.T. -0.000 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22

Instrument :

BNA_M

ClientSampleId :

SLCS048





Tgt Ion:163 Resp: 1301565

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.0

164 10.1 8.2 12.4



#48

2,6-Dinitrotoluene

Concen: 30.281 ng/ul

RT: 13.980 min Scan# 1869

Delta R.T. -0.006 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22




Tgt Ion:165 Resp: 265885


Ion Ratio Lower Upper

165 100

89 53.6 42.1 63.1

121 21.3 17.1 25.7



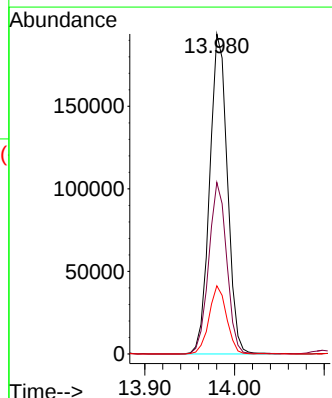





#50
Acenaphthylene
Concen: 29.651 ng/ul
RT: 14.127 min Scan# 1894
Delta R.T. -0.000 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22




Instrument :
BNA_M
ClientSampleId :
SLCS048


Tgt Ion:152 Resp: 1676861
Ion Ratio Lower Upper
152 100
151 19.8 15.4 23.0
153 13.1 10.6 15.8

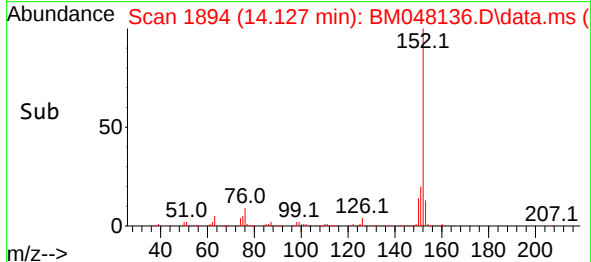

#51
3-Nitroaniline
Concen: 29.002 ng/ul
RT: 14.316 min Scan# 1926
Delta R.T. -0.000 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22

Tgt Ion:138 Resp: 265625
Ion Ratio Lower Upper
138 100
108 10.1 8.7 13.1
92 107.5 90.2 135.2









#52
Acenaphthene
Concen: 28.657 ng/ul
RT: 14.468 min Scan# 1952
Delta R.T. -0.006 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22




Instrument :
BNA_M
ClientSampleId :
SLCS048


Tgt Ion:153 Resp: 1121297
Ion Ratio Lower Upper
153 100
152 47.6 37.0 55.4
154 88.4 71.4 107.2



#53
2,4-Dinitrophenol
Concen: 27.903 ng/ul
RT: 14.527 min Scan# 1962
Delta R.T. -0.000 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22

Tgt Ion:184 Resp: 161654
Ion Ratio Lower Upper
184 100
63 56.5 47.9 71.9
154 59.5 46.4 69.6









#55
4-Nitrophenol
Concen: 29.114 ng/ul
RT: 14.633 min Scan# 1980
Delta R.T. -0.000 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22




Instrument :
BNA_M
ClientSampleId :
SLCS048


Tgt Ion:109 Resp: 164610
Ion Ratio Lower Upper
109 100
139 153.9 120.9 181.3
65 133.5 110.9 166.3



#56
Dibenzofuran
Concen: 29.352 ng/ul
RT: 14.804 min Scan# 2009
Delta R.T. -0.006 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22

Tgt Ion:168 Resp: 1571321
Ion Ratio Lower Upper
168 100
139 35.8 28.4 42.6


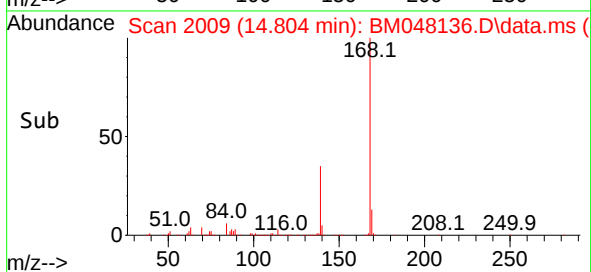

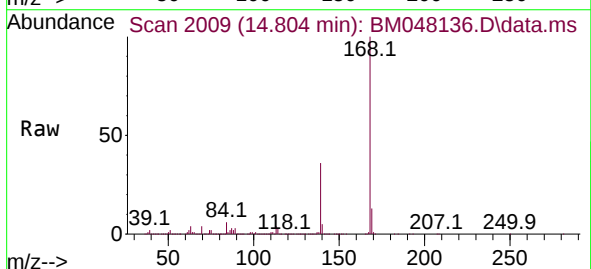




#57
2,4-Dinitrotoluene
Concen: 30.967 ng/ul
RT: 14.774 min Scan# 2004
Delta R.T. -0.000 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22




Instrument :
BNA_M
ClientSampleId :
SLCS048


Tgt Ion:165 Resp: 386263
Ion Ratio Lower Upper
165 100
63 38.2 31.4 47.0
182 2.7 2.0 3.0



#58
2,3,4,6-Tetrachlorophenol
Concen: 28.158 ng/ul
RT: 15.033 min Scan# 2048
Delta R.T. -0.006 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22

Tgt Ion:232 Resp: 310264
Ion Ratio Lower Upper
232 100
131 44.6 34.7 52.1
130 2.6 1.7 2.5#
166 30.2 25.2 37.8

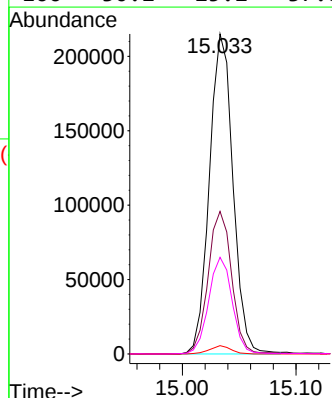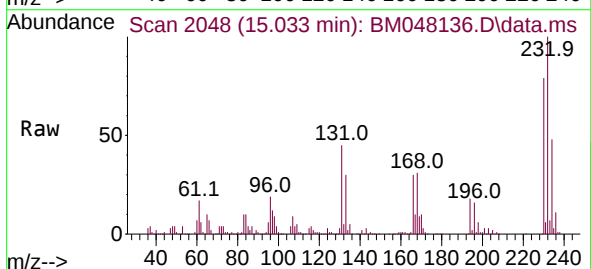



#59

Diethylphthalate

Concen: 29.530 ng/ul

RT: 15.227 min Scan# 2081

Delta R.T. -0.000 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22

Instrument :

BNA_M

ClientSampleId :

SLCS048





Tgt Ion:149 Resp: 1294770

Ion Ratio Lower Upper

149 100

177 22.4 17.5 26.3

150 12.3 9.8 14.8



#61

Fluorene

Concen: 29.580 ng/ul

RT: 15.451 min Scan# 2119

Delta R.T. -0.006 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22




Tgt Ion:166 Resp: 1237618


Ion Ratio Lower Upper

166 100

165 95.9 78.2 117.2

167 13.5 10.8 16.2









#62
4-Chlorophenyl-phenylether
Concen: 29.665 ng/ul
RT: 15.445 min Scan# 2118
Delta R.T. -0.006 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22




Instrument :
BNA_M
ClientSampleId :
SLCS048


Tgt Ion:204 Resp: 617284
Ion Ratio Lower Upper
204 100
206 32.6 26.6 39.8
141 56.7 44.6 66.8

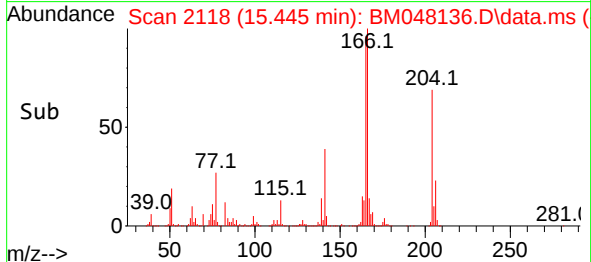

#63
4-Nitroaniline
Concen: 35.389 ng/ul
RT: 15.474 min Scan# 2123
Delta R.T. -0.000 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22

Tgt Ion:138 Resp: 280712
Ion Ratio Lower Upper
138 100
92 49.3 36.6 55.0
108 70.8 53.8 80.6







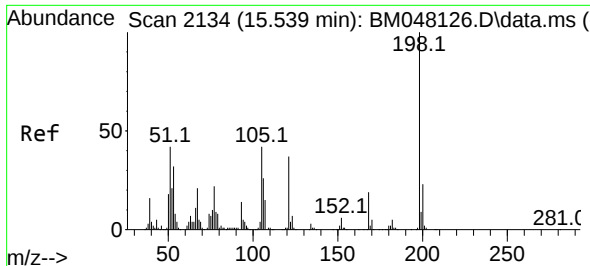

#66
4,6-Dinitro-2-methylphenol
Concen: 30.112 ng/ul
RT: 15.539 min Scan# 2134
Delta R.T. -0.000 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22




Instrument :
BNA_M
ClientSampleId :
SLCS048


Tgt Ion:198 Resp: 243846
Ion Ratio Lower Upper
198 100
182 4.2 3.9 5.9
77 22.2 19.3 28.9

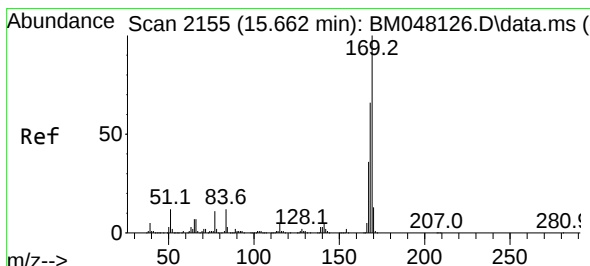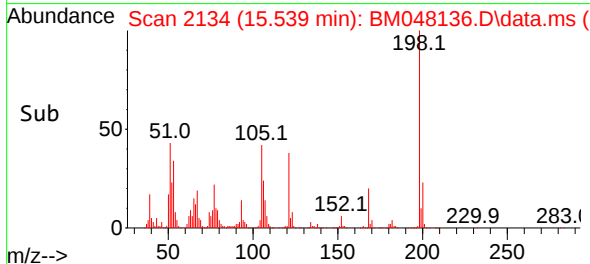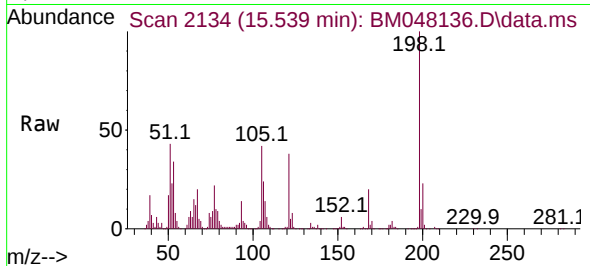

#67
N-Nitrosodiphenylamine
Concen: 30.106 ng/ul
RT: 15.663 min Scan# 2155
Delta R.T. -0.000 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22

Tgt Ion:169 Resp: 1053760
Ion Ratio Lower Upper
169 100
168 67.3 53.5 80.3
167 36.3 30.1 45.1


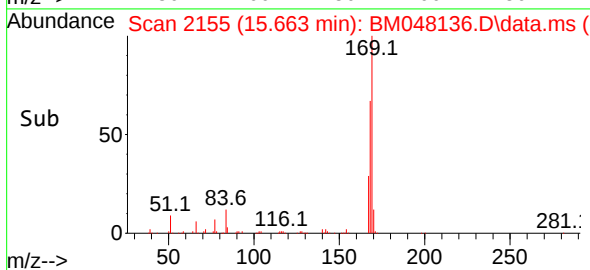

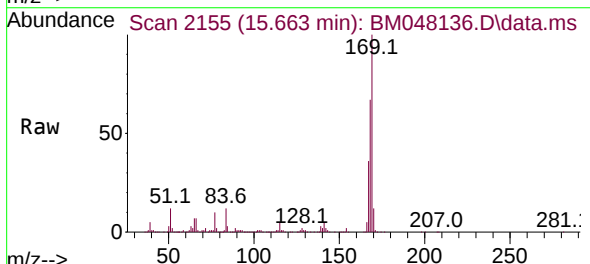




#68
4-Bromophenyl-phenylether
Concen: 29.757 ng/ul
RT: 16.339 min Scan# 21
Delta R.T. -0.000 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22




Instrument :
BNA_M
ClientSampleId :
SLCS048


Tgt Ion:248 Resp: 375747
Ion Ratio Lower Upper
248 100
250 99.0 78.2 117.4
141 69.0 58.2 87.2

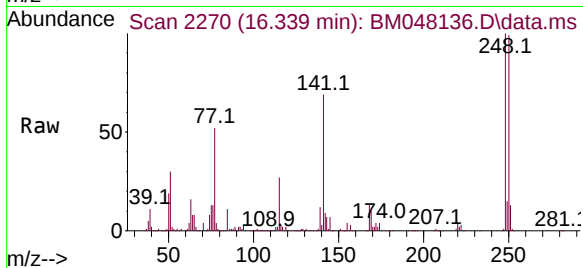

#69
Hexachlorobenzene
Concen: 29.695 ng/ul
RT: 16.457 min Scan# 2290
Delta R.T. -0.006 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22

Tgt Ion:284 Resp: 443157
Ion Ratio Lower Upper
284 100
142 33.4 26.8 40.2
249 30.5 24.6 36.8

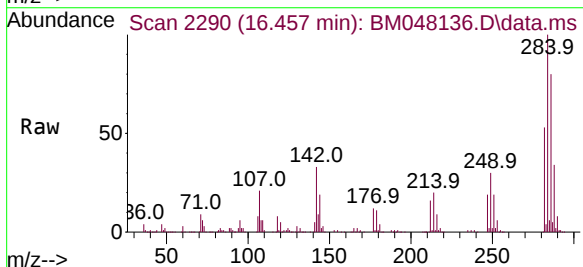



#70

Atrazine

Concen: 20.349 ng/ul

RT: 16.610 min Scan# 21

Delta R.T. -0.006 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22

Instrument :

BNA_M

ClientSampleId :

SLCS048





Tgt Ion:200 Resp: 239031

Ion Ratio Lower Upper

200 100

173 26.8 21.0 31.6

215 47.9 40.5 60.7



#71

Pentachlorophenol

Concen: 26.976 ng/ul

RT: 16.804 min Scan# 2349

Delta R.T. -0.000 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22




Tgt Ion:266 Resp: 259555


Ion Ratio Lower Upper

266 100

264 61.8 48.8 73.2

268 64.5 50.3 75.5

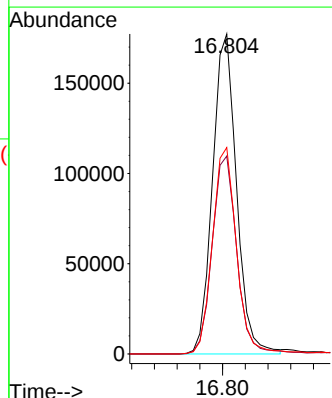



#72

Phenanthrene

Concen: 29.962 ng/u1

RT: 17.186 min Scan# 2414

Delta R.T. -0.006 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22

Instrument :

BNA_M

ClientSampleId :

SLCS048





Tgt Ion:178 Resp: 1907583

Ion Ratio Lower Upper

178 100

179 15.2 12.4 18.6

176 19.1 15.6 23.4



#74

Anthracene

Concen: 30.031 ng/u1

RT: 17.280 min Scan# 2430

Delta R.T. -0.000 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22




Tgt Ion:178 Resp: 1918652


Ion Ratio Lower Upper

178 100

179 15.2 12.6 19.0

176 18.2 14.8 22.2





#75

1,2,3,4-Tetrachlorobenzene

Concen: 27.909 ng/uL

RT: 13.204 min Scan# 1

Delta R.T. -0.006 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22

Instrument :

BNA_M

ClientSampleId :

SLCS048





Tgt Ion:216 Resp: 546058

Ion Ratio Lower Upper

216 100

214 78.5 61.0 91.6

218 48.7 38.6 58.0



#76

Pentachlorobenzene

Concen: 27.539 ng/uL

RT: 14.727 min Scan# 1996

Delta R.T. -0.000 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22




Tgt Ion:250 Resp: 524668


Ion Ratio Lower Upper

250 100

248 63.1 49.0 73.4

252 64.4 49.7 74.5





#77

Carbazole

Concen: 30.961 ng/ul

RT: 17.551 min Scan# 2476

Delta R.T. -0.000 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22

Instrument :





BNA_M

ClientSampleId :

SLCS048

Tgt Ion:167 Resp: 1752142

Ion	Ratio	Lower	Upper
167	100		
166	21.2	16.9	25.3
139	12.4	9.9	14.9

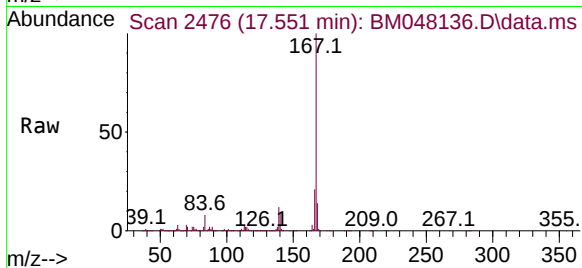

#78

Di-n-butylphthalate

Concen: 29.973 ng/ul

RT: 18.109 min Scan# 2571




Delta R.T. -0.000 min


Lab File: BM048136.D

Acq: 18 Oct 2024 15:22

Tgt Ion:149 Resp: 2234114

Ion	Ratio	Lower	Upper
149	100		
150	8.9	7.4	11.2
104	4.6	3.7	5.5

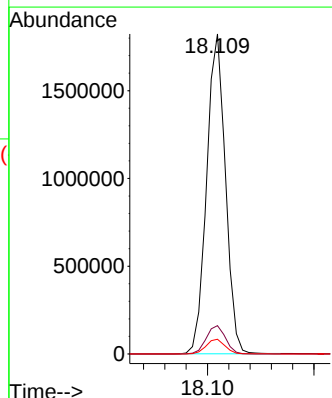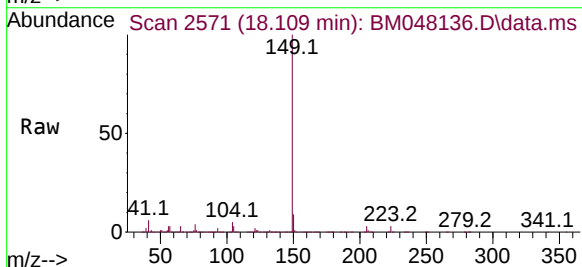



#80

Fluoranthene

Concen: 29.557 ng/ul

RT: 19.198 min Scan# 21

Delta R.T. -0.006 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22

Instrument :

BNA_M

ClientSampleId :

SLCS048





Tgt Ion:202 Resp: 2161407

Ion Ratio Lower Upper

202 100

101 11.4 8.6 12.8

100 8.7 6.6 10.0

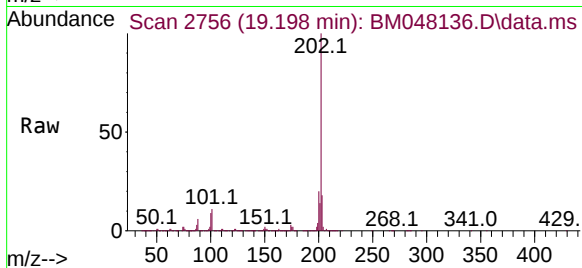

#82

Pyrene

Concen: 29.470 ng/ul

RT: 19.562 min Scan# 2818

Delta R.T. -0.000 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22




Tgt Ion:202 Resp: 2295657


Ion Ratio Lower Upper

202 100

101 12.7 10.4 15.6

100 10.4 8.5 12.7




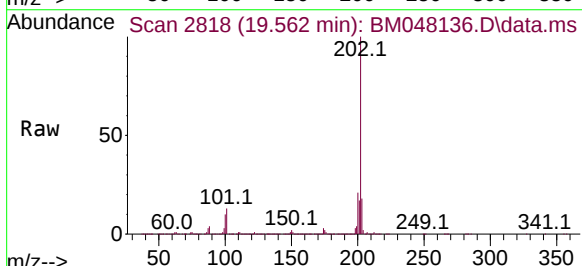




#83
Butylbenzylphthalate
Concen: 29.657 ng/ul
RT: 20.456 min Scan# 2970
Delta R.T. -0.000 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22




Instrument :
BNA_M
ClientSampleId :
SLCS048


Tgt Ion:149 Resp: 1003617
Ion Ratio Lower Upper
149 100
91 65.3 53.2 79.8
206 20.8 16.6 24.8

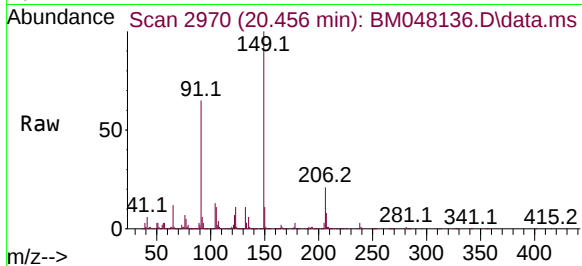

#84
3,3'-Dichlorobenzidine
Concen: 30.511 ng/ul
RT: 21.274 min Scan# 3109
Delta R.T. -0.006 min
Lab File: BM048136.D
Acq: 18 Oct 2024 15:22

Tgt Ion:252 Resp: 699904
Ion Ratio Lower Upper
252 100
254 63.8 51.0 76.6
126 11.0 8.5 12.7

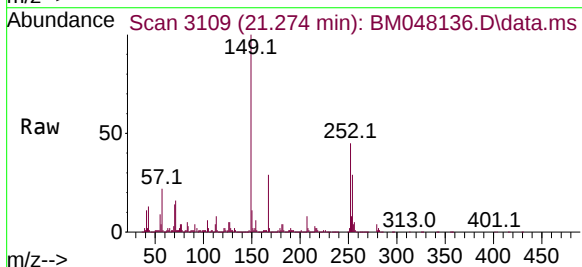



#85

Benzo(a)anthracene

Concen: 29.544 ng/ul

RT: 21.350 min Scan# 3122

Delta R.T. -0.006 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22

Instrument :

BNA_M

ClientSampleId :

SLCS048





Tgt Ion:228 Resp: 2209493

Ion Ratio Lower Upper

228 100

229 19.8 15.4 23.2

226 26.6 21.3 31.9



#86

Bis(2-ethylhexyl)phthalate

Concen: 29.487 ng/ul

RT: 21.268 min Scan# 3108

Delta R.T. -0.006 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22




Tgt Ion:149 Resp: 1442483


Ion Ratio Lower Upper

149 100

167 28.0 22.5 33.7

279 3.8 3.4 5.0





#87

Chrysene

Concen: 29.328 ng/ul

RT: 21.415 min Scan# 3133

Delta R.T. -0.000 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22

Instrument :

BNA_M

ClientSampleId :

SLCS048





Tgt Ion:228 Resp: 2066921

Ion Ratio Lower Upper

228 100

226 30.2 23.6 35.4

229 19.7 15.9 23.9



#89

Di-n-octyl phthalate

Concen: 30.391 ng/ul




RT: 22.391 min Scan# 3299


Delta R.T. -0.006 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22

Tgt Ion:149 Resp: 2537902





#90

Benzo(b)fluoranthene

Concen: 30.187 ng/ul

RT: 23.409 min Scan# 3472

Delta R.T. -0.006 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22

Instrument :

BNA_M

ClientSampleId :

SLCS048





Tgt Ion:252 Resp: 2200619

Ion Ratio Lower Upper

252 100

253 22.0 17.6 26.4

125 10.6 7.8 11.6

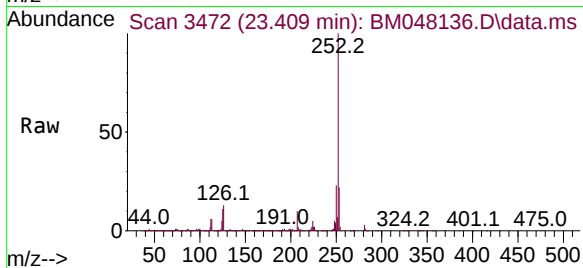

#91

Benzo(k)fluoranthene

Concen: 30.849 ng/ul

RT: 23.468 min Scan# 3482

Delta R.T. -0.012 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22




Tgt Ion:252 Resp: 2239738


Ion Ratio Lower Upper

252 100

253 22.3 17.3 25.9

125 10.2 7.8 11.6

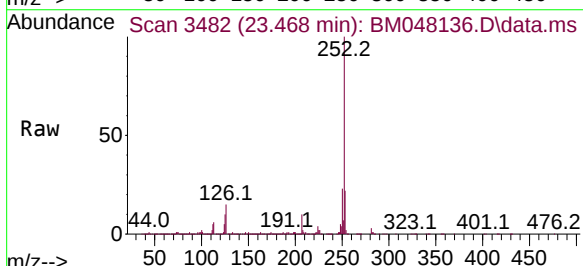



#93

Benzo(a)pyrene

Concen: 29.661 ng/ul

RT: 24.215 min Scan# 3

Delta R.T. -0.006 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22

Instrument :

BNA_M

ClientSampleId :

SLCS048





Tgt Ion:252 Resp: 2012842

Ion Ratio Lower Upper

252 100

253 21.8 17.3 25.9

125 10.6 8.7 13.1



#94

Indeno(1,2,3-cd)pyrene

Concen: 30.000 ng/ul

RT: 27.721 min Scan# 4205

Delta R.T. -0.012 min

Lab File: BM048136.D

Acq: 18 Oct 2024 15:22




Tgt Ion:276 Resp: 2639334


Ion Ratio Lower Upper

276 100

138 20.7 16.7 25.1

277 24.1 19.1 28.7









#95
 Dibenzo(a,h)anthracene
 Concen: 30.498 ng/ul
 RT: 27.768 min Scan# 41
 Delta R.T. -0.012 min
 Lab File: BM048136.D
 Acq: 18 Oct 2024 15:22

Instrument :
 BNA_M
 ClientSampleId :
 SLCS048

Tgt Ion:278 Resp: 2167814

Ion	Ratio	Lower	Upper
278	100		
139	15.8	12.3	18.5
279	24.3	19.3	28.9

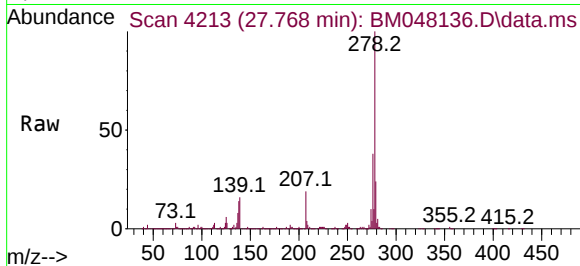

#96
 Benzo(g,h,i)perylene
 Concen: 30.205 ng/ul
 RT: 28.762 min Scan# 4382
 Delta R.T. -0.018 min
 Lab File: BM048136.D
 Acq: 18 Oct 2024 15:22

Tgt Ion:276 Resp: 2068082

Ion	Ratio	Lower	Upper
276	100		
138	20.9	17.8	26.6
277	23.2	19.0	28.6

