

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
 Data File : BM048113.D
 Acq On : 17 Oct 2024 19:44
 Operator : RC/JU
 Sample : PB164043BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK043

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048113.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	38	42	50	rVB	70503	103924	2.26%	0.199%
2	3.651	108	113	132	rBV	808939	1404990	30.51%	2.685%
3	3.975	164	168	174	rVB3	13611	24743	0.54%	0.047%
4	6.945	664	673	685	rBV	922888	1557511	33.82%	2.976%
5	7.104	693	700	715	rVB	778703	1285968	27.92%	2.457%
6	7.304	727	734	750	rBV	1000506	1660195	36.05%	3.172%
7	7.769	806	813	821	rBV	753269	1273634	27.66%	2.434%
8	8.481	926	934	953	rBV	1143914	1930814	41.93%	3.689%
9	8.928	1002	1010	1027	rBV	860653	1494971	32.46%	2.857%
10	9.351	1077	1082	1086	rBV4	11666	15798	0.34%	0.030%
11	9.645	1125	1132	1141	rBV	711374	1225142	26.60%	2.341%
12	10.186	1217	1224	1250	rBV	991483	1874544	40.70%	3.582%
13	10.563	1280	1288	1298	rBV	1010065	1735224	37.68%	3.316%
14	10.698	1303	1311	1334	rBV	946228	1876364	40.74%	3.585%
15	11.845	1502	1506	1510	rVB3	9036	12326	0.27%	0.024%
16	12.180	1555	1563	1571	rBV3	13972	32812	0.71%	0.063%
17	13.816	1834	1841	1852	rBV	1720170	2516112	54.63%	4.808%
18	14.098	1882	1889	1899	rBV	2099505	3197075	69.42%	6.109%
19	14.404	1935	1941	1953	rBV	1410139	2156818	46.83%	4.121%
20	14.621	1971	1978	2001	rBV	486424	1070549	23.25%	2.046%
21	14.780	2003	2005	2009	rVV5	7799	12313	0.27%	0.024%
22	14.815	2009	2011	2016	rVB6	5463	9800	0.21%	0.019%
23	15.398	2104	2110	2126	rBV	2625340	3804636	82.61%	7.270%
24	15.527	2126	2132	2147	rVV	710350	1134074	24.63%	2.167%
25	15.639	2148	2151	2158	rVV4	16557	33427	0.73%	0.064%
26	15.968	2204	2207	2213	rVB6	3118	4614	0.10%	0.009%
27	16.639	2318	2321	2325	rVB5	4010	4789	0.10%	0.009%
28	16.939	2370	2372	2378	rVB7	4527	6191	0.13%	0.012%
29	17.145	2401	2407	2418	rBV	1632982	2411221	52.36%	4.607%
30	17.245	2418	2424	2437	rVV	2620123	3967791	86.16%	7.582%
31	18.056	2557	2562	2566	rBV7	8656	17210	0.37%	0.033%
32	19.103	2736	2740	2746	rBV3	34738	53958	1.17%	0.103%
33	19.174	2748	2752	2756	rBV	29381	41183	0.89%	0.079%
34	19.533	2807	2813	2831	rBV	3254218	4605322	100.00%	8.800%
35	21.374	3121	3126	3139	rBV2	1534494	2517416	54.66%	4.810%
36	24.156	3590	3599	3613	rBV	1766895	4546310	98.72%	8.687%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
Data File : BM048113.D
Acq On : 17 Oct 2024 19:44
Operator : RC/JU
Sample : PB164043BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK043

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
Title : SVOA CALIBRATION

37	24.356	3626	3633	3645	rVB	1044894	2714368	58.94%	5.187%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 52334137

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
Data File : BM048113.D
Acq On : 17 Oct 2024 19:44
Operator : RC/JU
Sample : PB164043BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK043

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

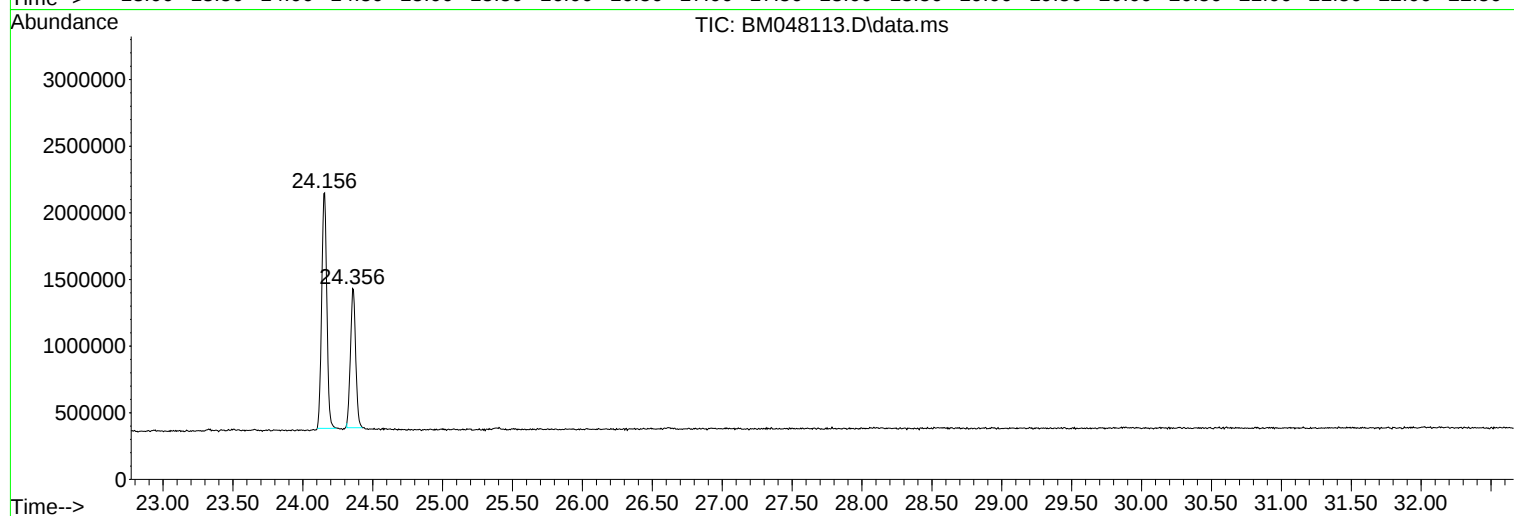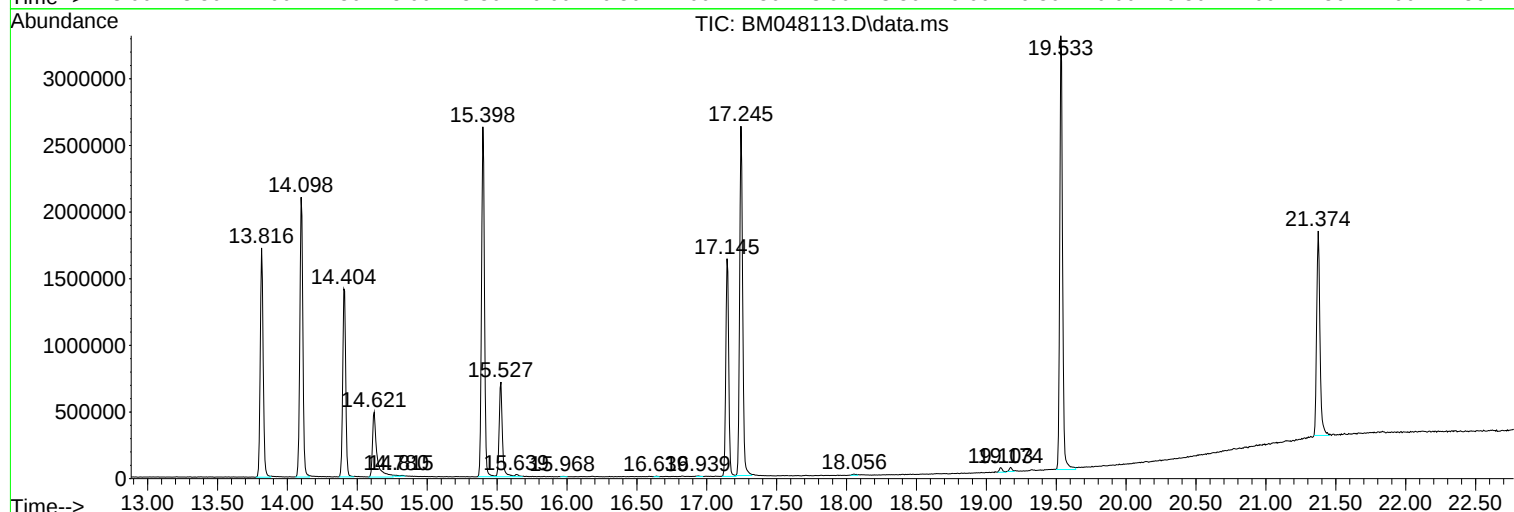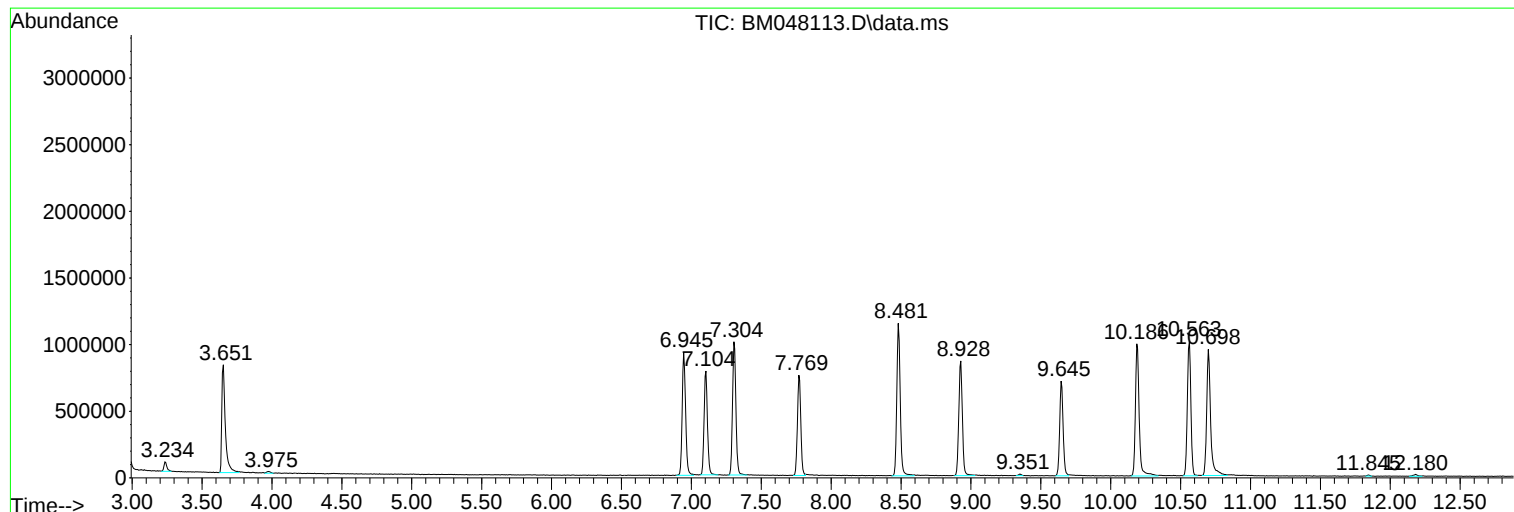

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
Data File : BM048113.D
Acq On : 17 Oct 2024 19:44
Operator : RC/JU
Sample : PB164043BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK043

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
Data File : BM048113.D
Acq On : 17 Oct 2024 19:44
Operator : RC/JU
Sample : PB164043BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK043

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc