

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
 Data File : BM048114.D
 Acq On : 17 Oct 2024 20:23
 Operator : RC/JU
 Sample : PB164163BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK163

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048114.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	38	42	55	rVB	73462	125992	2.73%	0.240%
2	3.651	109	113	131	rBV	801003	1410000	30.59%	2.681%
3	3.975	164	168	172	rBV2	11605	17090	0.37%	0.032%
4	6.945	663	673	684	rBV	909602	1559833	33.84%	2.966%
5	7.104	692	700	710	rBV	790068	1290098	27.99%	2.453%
6	7.304	726	734	748	rBV	982869	1668686	36.20%	3.173%
7	7.769	806	813	823	rBV	762641	1278919	27.75%	2.432%
8	8.481	927	934	949	rBV	1117016	1910482	41.45%	3.633%
9	8.928	1002	1010	1024	rBV	852491	1484961	32.22%	2.824%
10	9.345	1078	1081	1087	rVB4	8298	11879	0.26%	0.023%
11	9.645	1123	1132	1145	rBV	702383	1231766	26.72%	2.342%
12	10.186	1217	1224	1252	rBV	986681	1875980	40.70%	3.567%
13	10.563	1280	1288	1296	rBV	995590	1733001	37.60%	3.295%
14	10.698	1303	1311	1334	rBV	934665	1878303	40.75%	3.572%
15	11.845	1501	1506	1509	rBV4	9858	11367	0.25%	0.022%
16	12.186	1557	1564	1567	rBV2	12279	26470	0.57%	0.050%
17	13.816	1835	1841	1852	rBV	1734481	2513973	54.54%	4.780%
18	13.916	1856	1858	1863	rVB6	3328	5319	0.12%	0.010%
19	14.098	1880	1889	1904	rBV	2093706	3221393	69.89%	6.126%
20	14.404	1934	1941	1953	rBV	1430412	2187175	47.45%	4.159%
21	14.621	1971	1978	2001	rBV	487798	1056385	22.92%	2.009%
22	15.398	2103	2110	2121	rBV	2476011	3798996	82.42%	7.224%
23	15.527	2125	2132	2148	rVV	704590	1134437	24.61%	2.157%
24	15.639	2148	2151	2158	rVB4	16346	27584	0.60%	0.052%
25	16.186	2240	2244	2248	rBV7	3400	4611	0.10%	0.009%
26	16.645	2318	2322	2326	rVB4	4349	5301	0.12%	0.010%
27	16.827	2348	2353	2357	rBV5	5342	10939	0.24%	0.021%
28	16.939	2368	2372	2376	rVB5	3144	5081	0.11%	0.010%
29	17.145	2401	2407	2418	rBV	1667207	2418932	52.48%	4.600%
30	17.245	2418	2424	2439	rVV2	2613871	3985065	86.46%	7.578%
31	17.704	2499	2502	2506	rVB6	3589	4675	0.10%	0.009%
32	18.056	2557	2562	2566	rBV7	8332	18196	0.39%	0.035%
33	19.103	2736	2740	2745	rBV	34213	49606	1.08%	0.094%
34	19.174	2748	2752	2757	rBV	30399	50872	1.10%	0.097%
35	19.539	2808	2814	2826	rBV	3147565	4528080	98.24%	8.610%
36	21.374	3120	3126	3141	rBV	1495822	2635510	57.18%	5.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
Data File : BM048114.D
Acq On : 17 Oct 2024 20:23
Operator : RC/JU
Sample : PB164163BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK163

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
Title : SVOA CALIBRATION

37	24.156	3590	3599	3615	rVB	1811065	4609242	100.00%	8.765%
38	24.356	3626	3633	3651	rVB	1022748	2802182	60.79%	5.329%




Sum of corrected areas: 52588381

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
Data File : BM048114.D
Acq On : 17 Oct 2024 20:23
Operator : RC/JU
Sample : PB164163BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK163

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

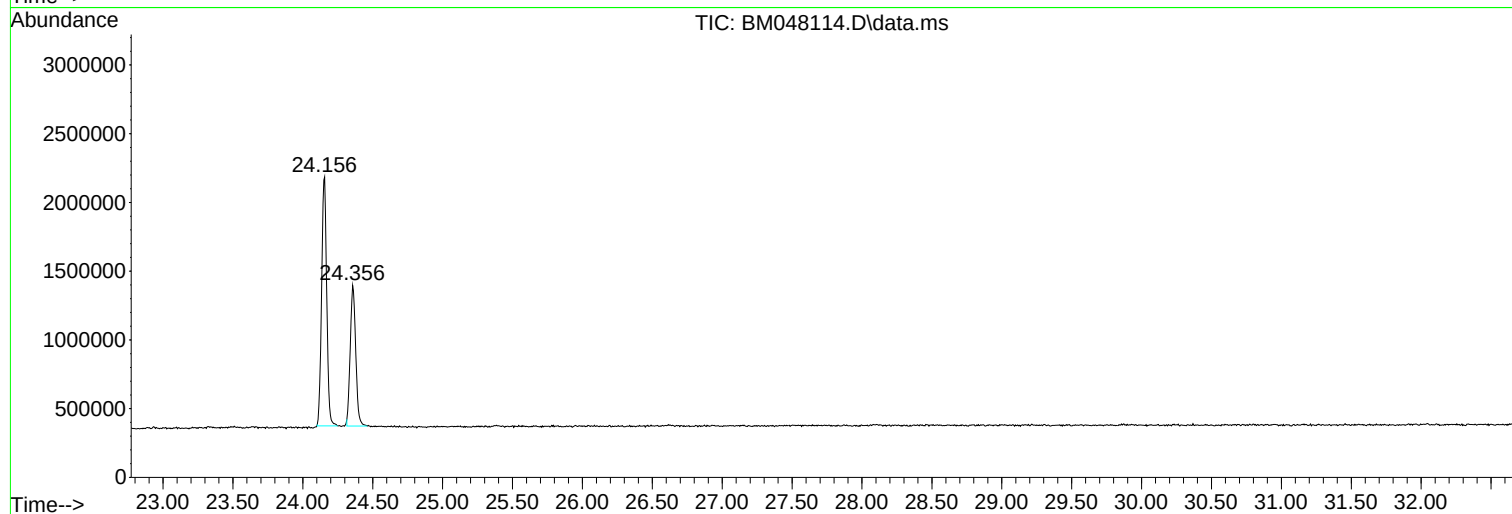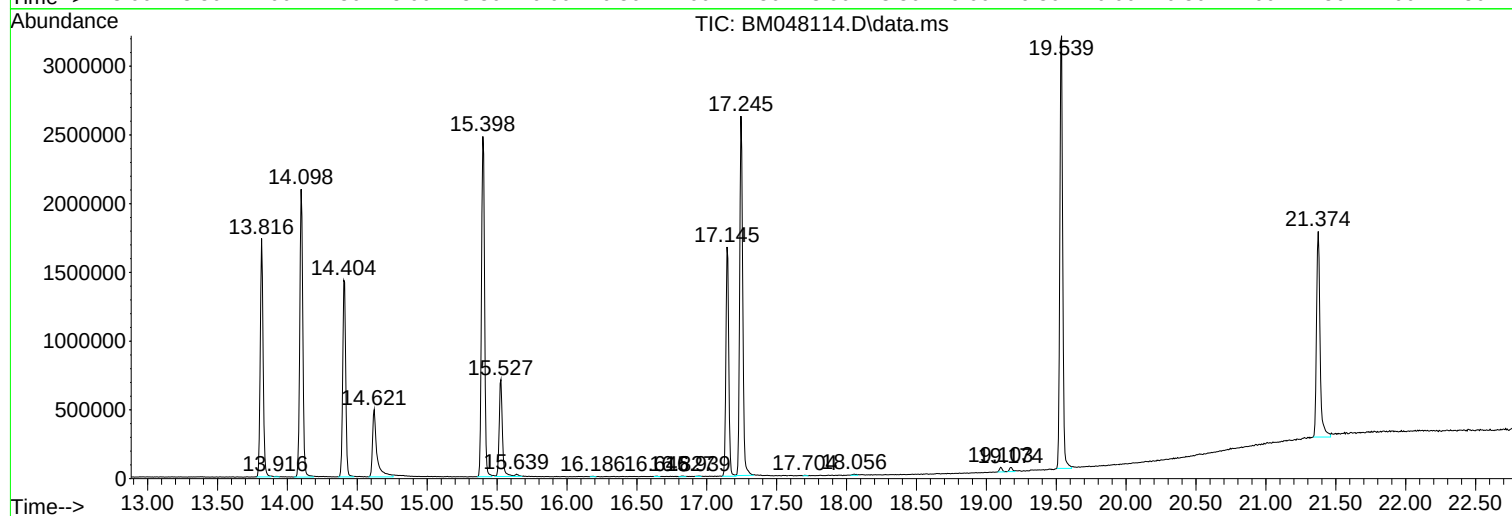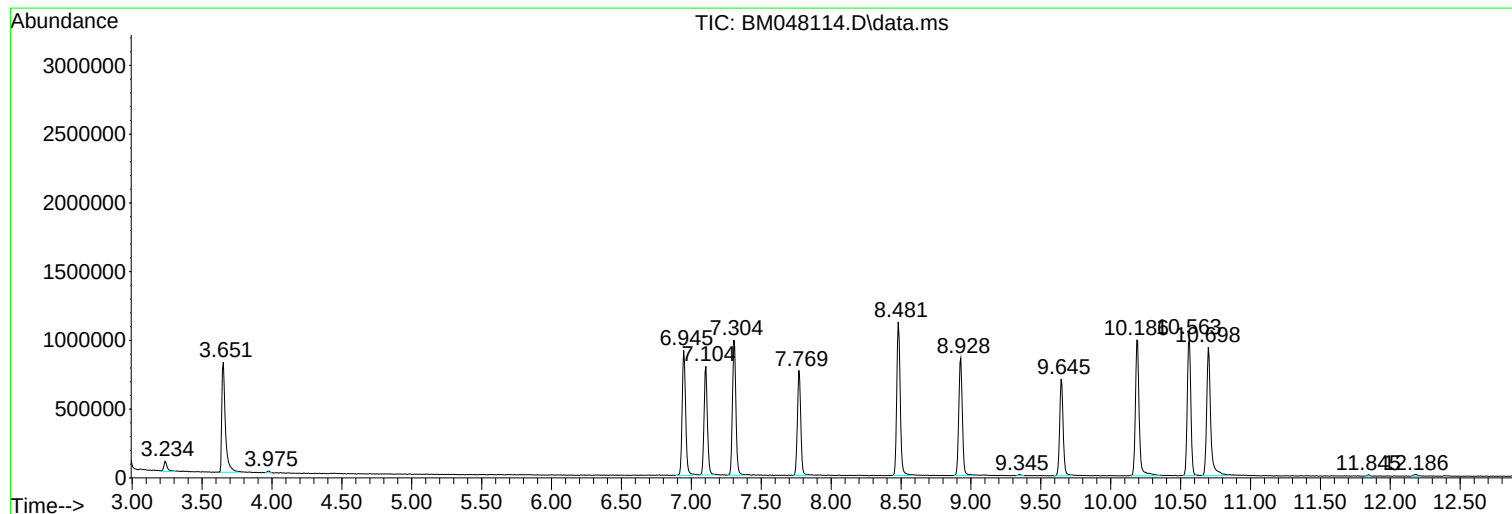

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
Data File : BM048114.D
Acq On : 17 Oct 2024 20:23
Operator : RC/JU
Sample : PB164163BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK163

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
Data File : BM048114.D
Acq On : 17 Oct 2024 20:23
Operator : RC/JU
Sample : PB164163BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK163

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------