

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
 Data File : BM048122.D
 Acq On : 18 Oct 2024 01:39
 Operator : RC/JU
 Sample : P4389-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E27J8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048122.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	39	43	52	rVB	57505	94611	1.53%	0.149%
2	3.657	110	114	130	rBV	233580	441773	7.15%	0.695%
3	3.934	159	161	164	rBV3	6356	6826	0.11%	0.011%
4	3.975	164	168	175	rVB	23561	41674	0.67%	0.066%
5	5.822	479	482	490	rVB8	6586	10311	0.17%	0.016%
6	6.951	664	674	684	rBV	266635	484317	7.84%	0.762%
7	7.104	693	700	712	rBV	1000667	1648893	26.70%	2.595%
8	7.228	717	721	725	rBV7	4934	7553	0.12%	0.012%
9	7.304	728	734	746	rBV	1066969	1844989	29.87%	2.904%
10	7.769	804	813	821	rBV	873433	1439123	23.30%	2.265%
11	7.839	821	825	831	rVB2	19707	36880	0.60%	0.058%
12	8.481	926	934	946	rBV	797076	1429658	23.15%	2.250%
13	8.592	951	953	957	rVB4	8646	12460	0.20%	0.020%
14	8.863	995	999	1003	rBV5	9682	16123	0.26%	0.025%
15	8.928	1003	1010	1022	rVV	1124844	1901197	30.78%	2.992%
16	9.092	1034	1038	1044	rVB8	7387	13842	0.22%	0.022%
17	9.351	1078	1082	1086	rVB3	13080	21080	0.34%	0.033%
18	9.645	1125	1132	1145	rBV	942069	1619542	26.22%	2.549%
19	10.192	1217	1225	1239	rBV	1282282	2371375	38.40%	3.732%
20	10.563	1280	1288	1295	rBV	1152546	1993048	32.27%	3.137%
21	10.698	1304	1311	1333	rBV	1098838	2121957	34.36%	3.340%
22	11.216	1396	1399	1406	rBV4	7014	14048	0.23%	0.022%
23	11.745	1488	1489	1499	rVB8	3418	6703	0.11%	0.011%
24	11.845	1499	1506	1512	rVB6	11192	18499	0.30%	0.029%
25	12.163	1553	1560	1570	rBV	18373	44803	0.73%	0.071%
26	12.769	1660	1663	1669	rVB6	5377	10753	0.17%	0.017%
27	13.016	1699	1705	1712	rBV9	6571	11518	0.19%	0.018%
28	13.386	1764	1768	1774	rVB5	5086	8710	0.14%	0.014%
29	13.816	1835	1841	1853	rBV	2317687	3327309	53.87%	5.237%
30	14.098	1879	1889	1900	rBV	2838177	4263445	69.03%	6.710%
31	14.404	1932	1941	1951	rBV	1649888	2479638	40.15%	3.903%
32	14.527	1958	1962	1966	rVB6	5231	8688	0.14%	0.014%
33	14.633	1974	1980	2001	rBV2	104915	312823	5.07%	0.492%
34	14.833	2010	2014	2022	rVB5	25292	49105	0.80%	0.077%
35	15.398	2103	2110	2125	rBV	3462305	5040926	81.62%	7.934%
36	15.521	2125	2131	2144	rVV	1062323	1635682	26.48%	2.574%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
 Data File : BM048122.D
 Acq On : 18 Oct 2024 01:39
 Operator : RC/JU
 Sample : P4389-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E27J8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
 Title : SVOA CALIBRATION

37	15.639	2148	2151	2156	rVB2	18099	28980	0.47%	0.046%
38	15.763	2165	2172	2185	rBV	1255146	1771061	28.68%	2.788%
39	15.962	2202	2206	2211	rBV8	4791	9136	0.15%	0.014%
40	16.104	2223	2230	2238	rBV	50655	106661	1.73%	0.168%
41	16.180	2241	2243	2247	rVB5	7248	8335	0.13%	0.013%
42	16.821	2347	2352	2357	rBV9	5686	11001	0.18%	0.017%
43	16.933	2367	2371	2374	rBV4	5184	7838	0.13%	0.012%
44	17.145	2400	2407	2418	rBV	1879296	2735105	44.29%	4.305%
45	17.245	2418	2424	2438	rVV2	3613138	5292442	85.69%	8.330%
46	17.439	2454	2457	2460	rVB4	8378	8506	0.14%	0.013%
47	17.809	2517	2520	2525	rBV7	6448	10732	0.17%	0.017%
48	18.039	2555	2559	2565	rBV4	34426	61322	0.99%	0.097%
49	19.103	2734	2740	2744	rBV3	50414	81506	1.32%	0.128%
50	19.174	2748	2752	2757	rBV	49420	74020	1.20%	0.117%
51	19.321	2774	2777	2784	rBV6	23367	35124	0.57%	0.055%
52	19.462	2799	2801	2806	rVB5	19724	23102	0.37%	0.036%
53	19.539	2807	2814	2827	rBV	4205282	6133390	99.31%	9.654%
54	21.374	3120	3126	3136	rBV	1781195	2920240	47.28%	4.596%
55	24.150	3589	3598	3614	rVB	2409944	6176000	100.00%	9.721%
56	24.356	3625	3633	3649	rVB	1221886	3250830	52.64%	5.117%




Sum of corrected areas: 63535213

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
Data File : BM048122.D
Acq On : 18 Oct 2024 01:39
Operator : RC/JU
Sample : P4389-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

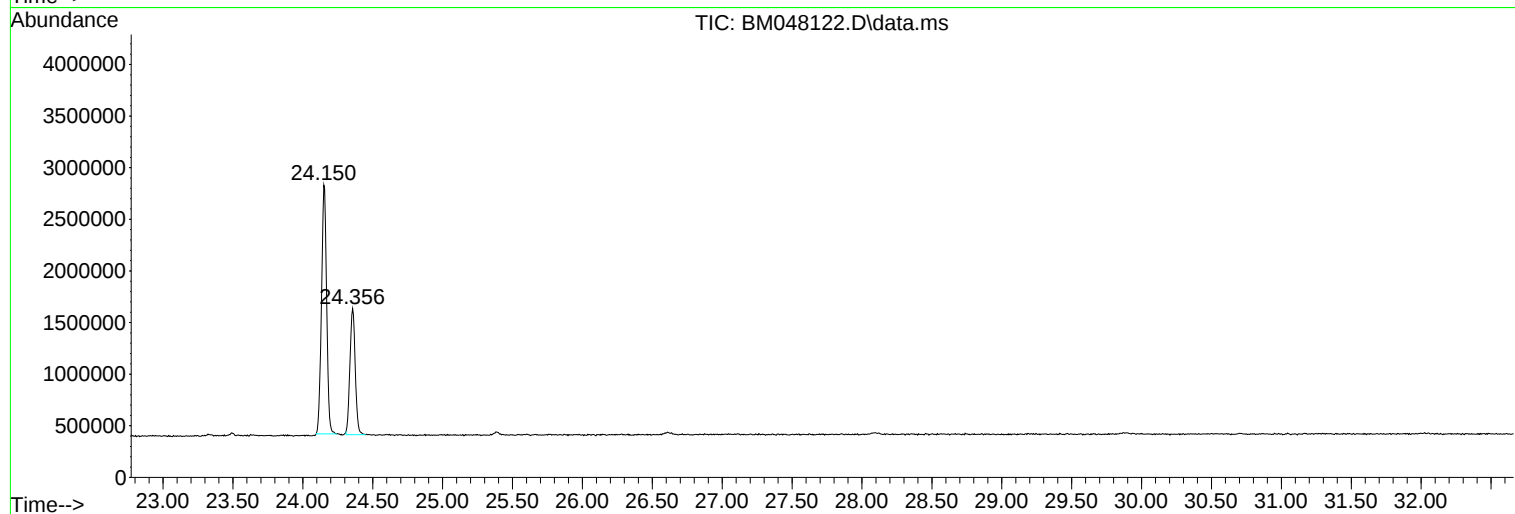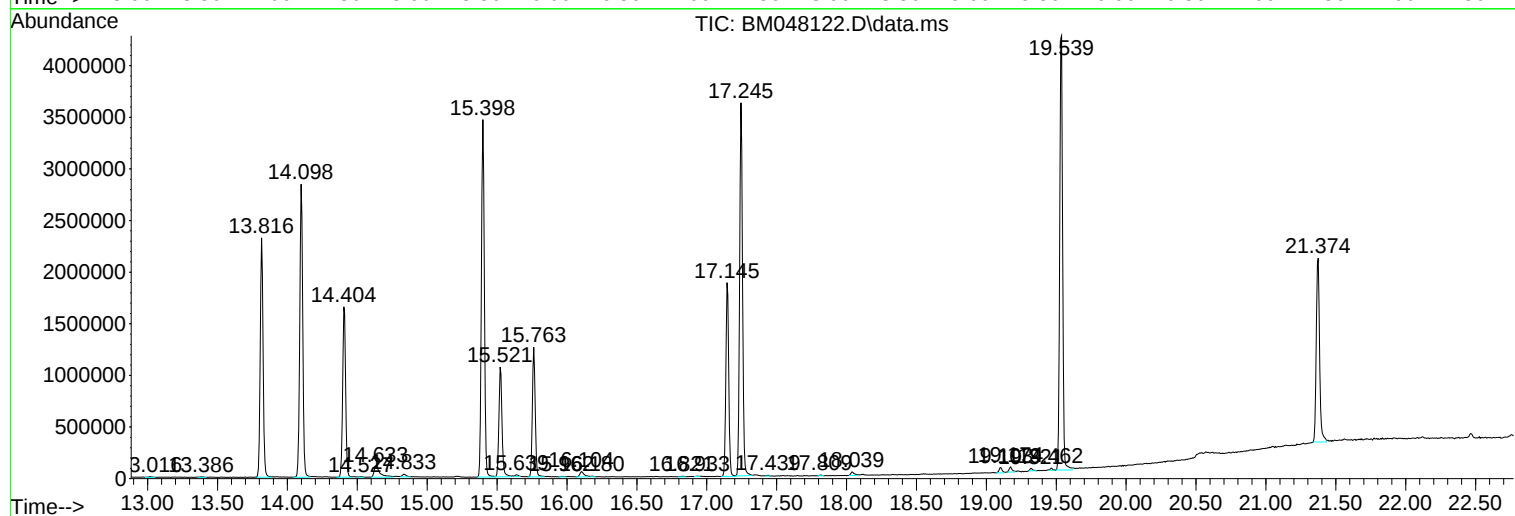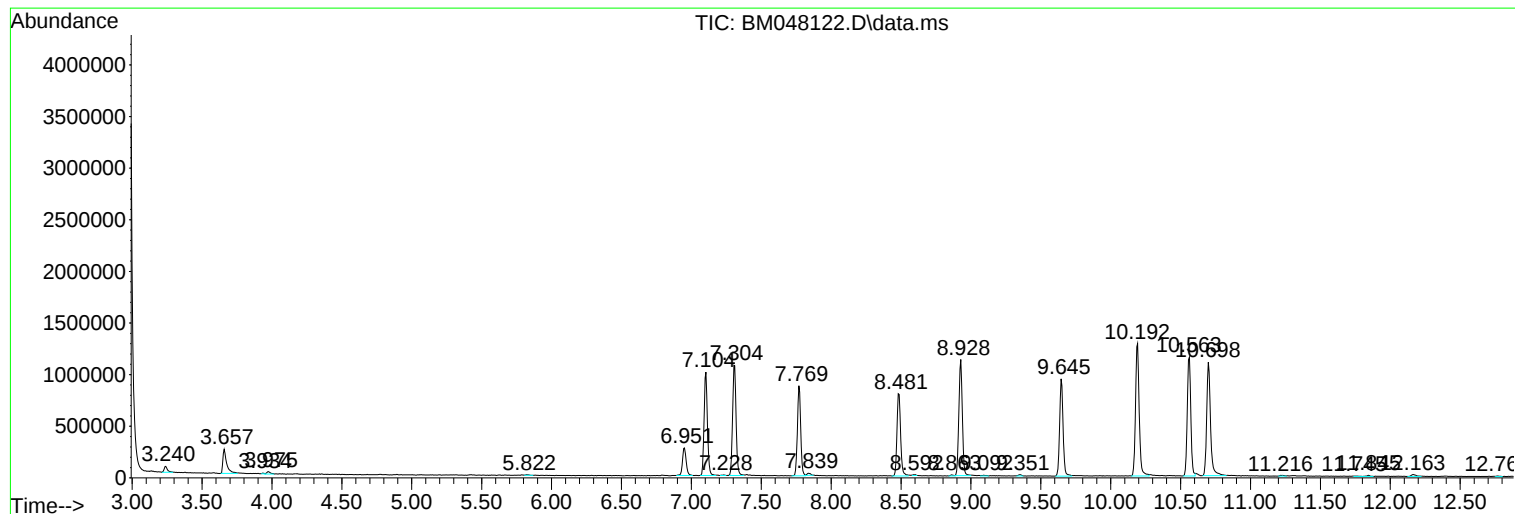

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
Data File : BM048122.D
Acq On : 18 Oct 2024 01:39
Operator : RC/JU
Sample : P4389-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J8










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.762	14.28 ng/ul	1771060	Acenaphthene-d10	14.404

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	97
2			Benzophenone	182	C13H10O	000119-61-9	96
3			Benzophenone	182	C13H10O	000119-61-9	95
4			Benzophenone	182	C13H10O	000119-61-9	93
5			Acetophenone, 2-chloro-	154	C8H7ClO	000532-27-4	49

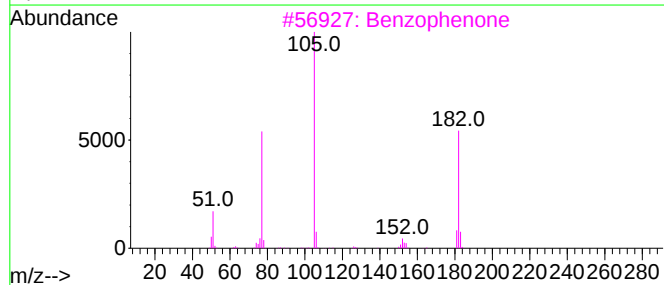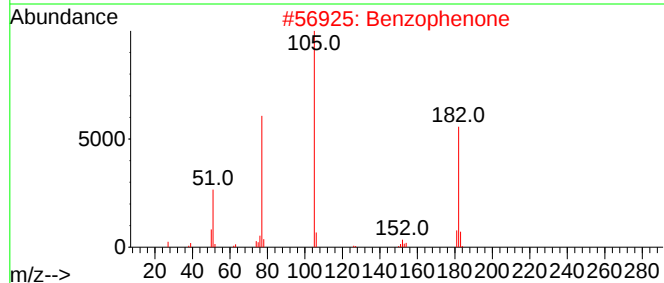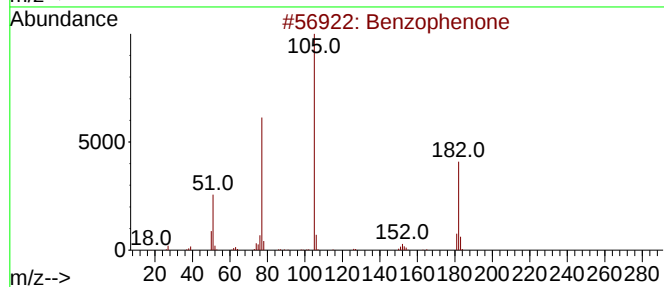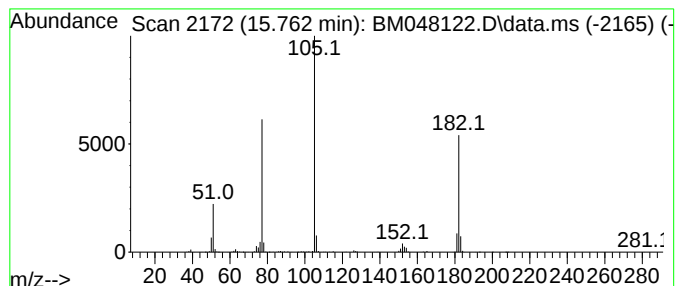

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
Data File : BM048122.D
Acq On : 18 Oct 2024 01:39
Operator : RC/JU
Sample : P4389-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	15.762	14.3	ng/ul	1771060	3	14.404	2479640	20.0