

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
 Data File : BM048128.D
 Acq On : 18 Oct 2024 10:06
 Operator : RC/JU
 Sample : P4380-07DL 10X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E27H9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048128.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.675	114	117	120	rBV2	9840	14393	0.50%	0.071%
2	3.969	165	167	172	rVB2	10891	11995	0.42%	0.059%
3	4.898	321	325	329	rBV5	5297	8946	0.31%	0.044%
4	6.351	569	572	573	rBV2	3379	3600	0.13%	0.018%
5	6.910	663	667	671	rBV	34496	50300	1.75%	0.247%
6	6.951	671	674	687	rVB4	16731	43982	1.53%	0.216%
7	7.104	694	700	710	rBV	54496	110599	3.85%	0.542%
8	7.310	729	735	745	rVV	71411	137035	4.77%	0.672%
9	7.445	757	758	761	rVB3	3169	3024	0.11%	0.015%
10	7.769	806	813	827	rBV	743943	1339867	46.60%	6.572%
11	8.145	875	877	881	rVB4	5527	6230	0.22%	0.031%
12	8.222	888	890	893	rVB3	2485	3094	0.11%	0.015%
13	8.304	898	904	910	rVV9	5813	12135	0.42%	0.060%
14	8.492	931	936	952	rVB	49868	115226	4.01%	0.565%
15	8.857	994	998	1004	rVB5	2365	3969	0.14%	0.019%
16	8.933	1004	1011	1021	rBV3	54946	123014	4.28%	0.603%
17	9.351	1076	1082	1090	rVB	41228	59815	2.08%	0.293%
18	9.539	1112	1114	1123	rVB6	1699	3797	0.13%	0.019%
19	9.651	1128	1133	1142	rBV2	43958	93323	3.25%	0.458%
20	10.210	1221	1228	1237	rBV	47091	133784	4.65%	0.656%
21	10.557	1280	1287	1291	rBV	1026663	1789334	62.23%	8.776%
22	10.610	1291	1296	1307	rVV	1542551	2694953	93.72%	13.218%
23	10.727	1309	1316	1328	rVB3	53201	142333	4.95%	0.698%
24	11.504	1446	1448	1452	rVB5	2002	2899	0.10%	0.014%
25	11.663	1473	1475	1479	rVV4	3252	4004	0.14%	0.020%
26	11.845	1499	1506	1513	rBV2	14999	25339	0.88%	0.124%
27	12.245	1565	1574	1586	rVB3	31529	96275	3.35%	0.472%
28	12.457	1604	1610	1620	rVV2	24540	57970	2.02%	0.284%
29	12.598	1631	1634	1639	rVB6	2805	3292	0.11%	0.016%
30	12.763	1659	1662	1666	rBV4	2233	3474	0.12%	0.017%
31	13.251	1739	1745	1753	rBV4	11715	27713	0.96%	0.136%
32	13.386	1763	1768	1769	rBV4	2276	3169	0.11%	0.016%
33	13.410	1769	1772	1774	rVB3	2809	3260	0.11%	0.016%
34	13.727	1822	1826	1831	rBV6	5024	8405	0.29%	0.041%
35	13.816	1831	1841	1851	rBV	161158	282703	9.83%	1.387%
36	14.098	1884	1889	1903	rBV2	202033	342908	11.93%	1.682%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
 Data File : BM048128.D
 Acq On : 18 Oct 2024 10:06
 Operator : RC/JU
 Sample : P4380-07DL 10X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E27H9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
 Title : SVOA CALIBRATION

37	14.404	1934	1941	1947	rVV	1508127	2241605	77.96%	10.995%
38	14.468	1947	1952	1962	rVB	206939	327588	11.39%	1.607%
39	14.621	1974	1978	1983	rVB7	2938	4683	0.16%	0.023%
40	14.680	1983	1988	1990	rBV5	4126	6786	0.24%	0.033%
41	14.810	2005	2010	2022	rBV	39642	77062	2.68%	0.378%
42	14.898	2022	2025	2028	rVV5	2807	4191	0.15%	0.021%
43	14.957	2032	2035	2039	rVB6	2762	4245	0.15%	0.021%
44	15.162	2066	2070	2073	rBV6	2744	4296	0.15%	0.021%
45	15.398	2104	2110	2116	rBV	245456	408929	14.22%	2.006%
46	15.457	2116	2120	2128	rVB	59502	105204	3.66%	0.516%
47	15.539	2128	2134	2139	rBV2	38056	73885	2.57%	0.362%
48	15.768	2167	2173	2181	rBV	52498	90396	3.14%	0.443%
49	15.904	2194	2196	2200	rVB5	2687	3576	0.12%	0.018%
50	16.133	2230	2235	2239	rBV6	10836	19524	0.68%	0.096%
51	16.292	2260	2262	2265	rBV4	2877	3364	0.12%	0.016%
52	16.333	2267	2269	2274	rVB6	3481	4686	0.16%	0.023%
53	16.457	2287	2290	2292	rBV4	2839	3214	0.11%	0.016%
54	16.645	2318	2322	2326	rBV5	11372	18124	0.63%	0.089%
55	16.786	2343	2346	2347	rBV3	2506	3181	0.11%	0.016%
56	17.092	2394	2398	2401	rBV2	12638	18559	0.65%	0.091%
57	17.145	2401	2407	2413	rBV	1702778	2470750	85.93%	12.119%
58	17.245	2419	2424	2438	rVB	247340	443879	15.44%	2.177%
59	17.562	2473	2478	2487	rBV	17699	40146	1.40%	0.197%
60	17.756	2508	2511	2513	rBV3	4516	4910	0.17%	0.024%
61	17.774	2513	2514	2517	rVB3	4042	2942	0.10%	0.014%
62	18.039	2554	2559	2564	rBV8	23160	46055	1.60%	0.226%
63	18.151	2576	2578	2583	rVB6	4833	5622	0.20%	0.028%
64	18.221	2587	2590	2594	rVB3	9236	15196	0.53%	0.075%
65	19.203	2753	2757	2764	rVB	34582	51652	1.80%	0.253%
66	19.533	2808	2813	2824	rBV	369229	598147	20.80%	2.934%
67	21.368	3120	3125	3139	rBV	1626523	2643932	91.95%	12.968%
68	24.350	3624	3632	3645	rVB	1085876	2875425	100.00%	14.104%




Sum of corrected areas: 20387913

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
Data File : BM048128.D
Acq On : 18 Oct 2024 10:06
Operator : RC/JU
Sample : P4380-07DL 10X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27H9DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

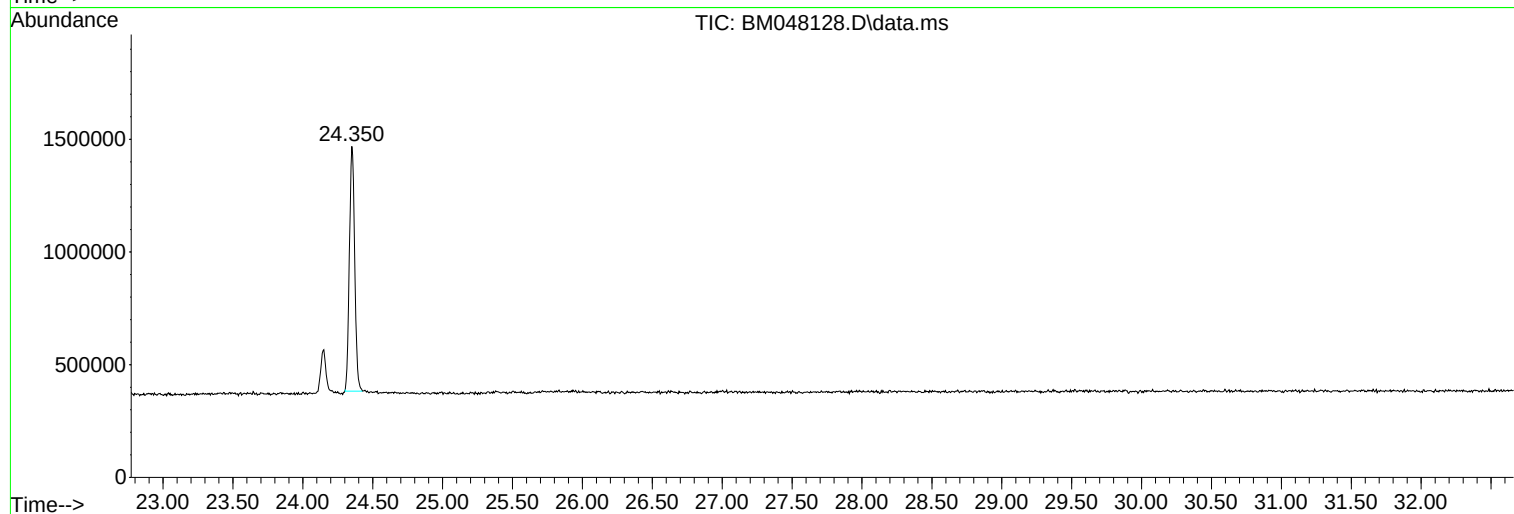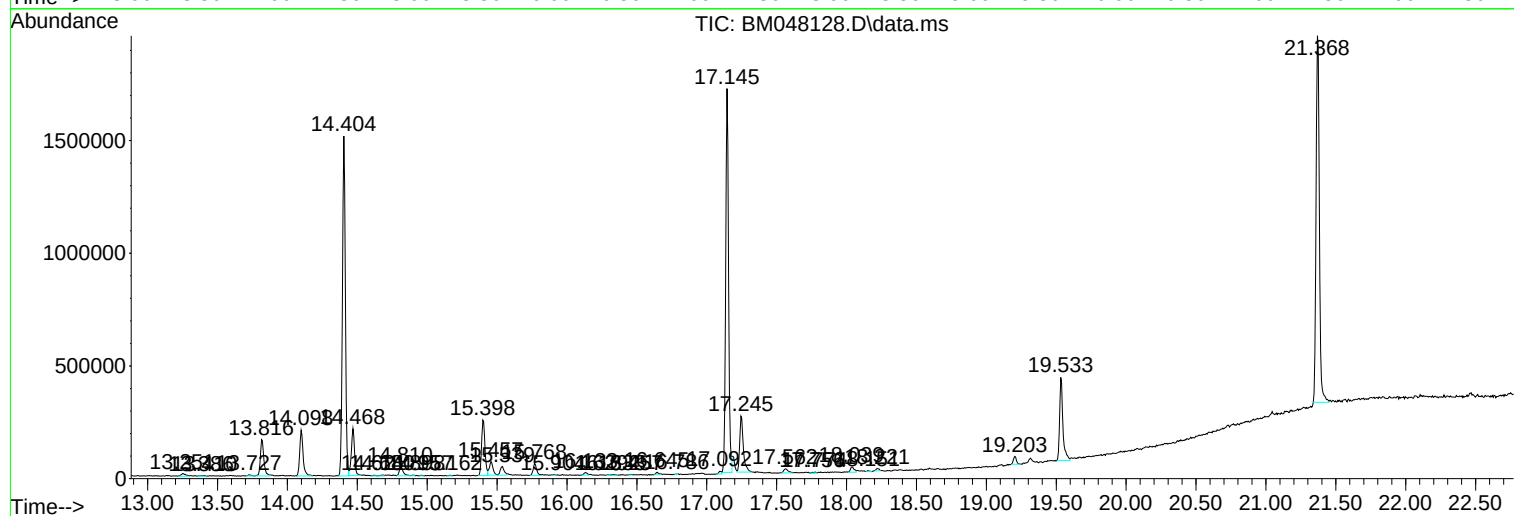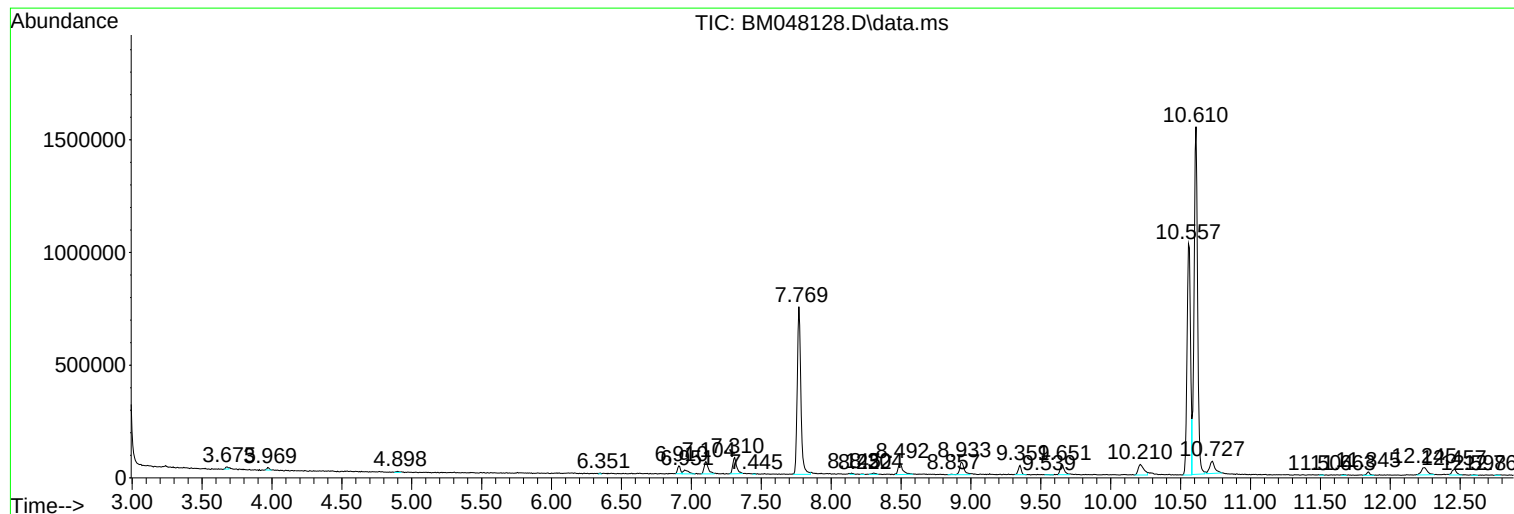

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
Data File : BM048128.D
Acq On : 18 Oct 2024 10:06
Operator : RC/JU
Sample : P4380-07DL 10X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27H9DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
Data File : BM048128.D
Acq On : 18 Oct 2024 10:06
Operator : RC/JU
Sample : P4380-07DL 10X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27H9DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc