

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
 Data File : BM048133.D
 Acq On : 18 Oct 2024 13:23
 Operator : RC/JU
 Sample : P4380-13
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E27H2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048133.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	39	42	47	rBV	49399	67062	1.25%	0.142%
2	3.651	109	113	135	rVB	553101	973176	18.12%	2.065%
3	3.969	164	167	180	rVB	25579	47016	0.88%	0.100%
4	4.346	227	231	236	rVB8	5562	9017	0.17%	0.019%
5	4.769	299	303	307	rVB4	8303	9924	0.18%	0.021%
6	5.140	364	366	373	rVB8	3850	6515	0.12%	0.014%
7	5.422	410	414	421	rVB5	7438	18588	0.35%	0.039%
8	5.657	450	454	461	rVB8	3453	6837	0.13%	0.015%
9	5.787	472	476	480	rVB4	12450	17813	0.33%	0.038%
10	6.263	554	557	561	rVB3	8308	9704	0.18%	0.021%
11	6.451	586	589	595	rVB7	11809	21107	0.39%	0.045%
12	6.916	663	668	670	rBV6	7601	12067	0.22%	0.026%
13	6.951	671	674	678	rVV3	12910	23192	0.43%	0.049%
14	6.992	678	681	689	rVB2	23500	38376	0.71%	0.081%
15	7.098	693	699	715	rBV	766995	1326552	24.70%	2.814%
16	7.292	728	732	733	rBV3	8207	9408	0.18%	0.020%
17	7.387	742	748	750	rBV7	4299	6308	0.12%	0.013%
18	7.422	750	754	757	rVB6	6409	10403	0.19%	0.022%
19	7.769	805	813	823	rBV	800732	1359762	25.32%	2.885%
20	7.839	823	825	828	rVV3	18275	23518	0.44%	0.050%
21	7.886	828	833	840	rVV2	17885	40673	0.76%	0.086%
22	8.081	860	866	871	rBV	18030	32287	0.60%	0.068%
23	8.139	871	876	880	rVB6	6813	10429	0.19%	0.022%
24	8.410	919	922	925	rVB4	5163	7120	0.13%	0.015%
25	8.486	929	935	946	rBV	96478	215958	4.02%	0.458%
26	8.586	949	952	960	rVV8	7867	21087	0.39%	0.045%
27	8.663	960	965	970	rVB3	7875	12967	0.24%	0.028%
28	8.869	993	1000	1002	rBV5	8698	13928	0.26%	0.030%
29	8.928	1002	1010	1018	rBV	795809	1460106	27.19%	3.097%
30	9.192	1053	1055	1060	rVB6	4602	6425	0.12%	0.014%
31	9.328	1071	1078	1079	rBV4	17977	27249	0.51%	0.058%
32	9.457	1095	1100	1102	rBV4	11612	18204	0.34%	0.039%
33	9.651	1126	1133	1134	rBV6	6366	11143	0.21%	0.024%
34	9.969	1181	1187	1194	rBV5	30294	57719	1.07%	0.122%
35	10.122	1208	1213	1220	rBV5	13218	26842	0.50%	0.057%
36	10.204	1220	1227	1231	rVB9	6180	13898	0.26%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
 Data File : BM048133.D
 Acq On : 18 Oct 2024 13:23
 Operator : RC/JU
 Sample : P4380-13
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E27H2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
 Title : SVOA CALIBRATION

37	10.369	1246	1255	1268	rBV6	16579	70334	1.31%	0.149%
38	10.557	1280	1287	1294	rBV	1063944	1847722	34.41%	3.920%
39	10.610	1294	1296	1303	rVB3	40978	60992	1.14%	0.129%
40	10.698	1303	1311	1333	rBV	981887	1941242	36.15%	4.118%
41	11.186	1387	1394	1396	rBV8	4928	10645	0.20%	0.023%
42	11.422	1430	1434	1435	rBV4	4788	5756	0.11%	0.012%
43	11.651	1469	1473	1475	rBV4	3555	5575	0.10%	0.012%
44	11.774	1488	1494	1498	rBV7	4801	9822	0.18%	0.021%
45	11.839	1503	1505	1510	rVB5	6711	8159	0.15%	0.017%
46	12.074	1540	1545	1549	rBV2	16199	32108	0.60%	0.068%
47	12.163	1555	1560	1566	rBV2	14248	25141	0.47%	0.053%
48	12.369	1589	1595	1597	rBV5	7167	10701	0.20%	0.023%
49	12.445	1605	1608	1618	rVB3	15468	30550	0.57%	0.065%
50	12.951	1689	1694	1701	rBV5	16605	33379	0.62%	0.071%
51	13.010	1701	1704	1710	rVB8	5040	9203	0.17%	0.020%
52	13.251	1739	1745	1750	rBV8	11405	23977	0.45%	0.051%
53	13.380	1758	1767	1772	rVB9	7423	17160	0.32%	0.036%
54	13.521	1788	1791	1795	rVB3	4173	5482	0.10%	0.012%
55	13.574	1795	1800	1801	rBV4	10319	14401	0.27%	0.031%
56	13.727	1818	1826	1831	rBV	34397	65830	1.23%	0.140%
57	13.816	1831	1841	1851	rVV	1616434	2408165	44.84%	5.109%
58	13.898	1852	1855	1857	rVV4	7137	8794	0.16%	0.019%
59	13.939	1857	1862	1869	rVB4	30645	63731	1.19%	0.135%
60	14.051	1876	1881	1882	rBV5	5474	6547	0.12%	0.014%
61	14.098	1882	1889	1904	rVV	2258521	3512910	65.41%	7.452%
62	14.404	1929	1941	1948	rBV	1605170	2372597	44.18%	5.033%
63	14.468	1948	1952	1959	rVV	40544	73366	1.37%	0.156%
64	14.545	1960	1965	1970	rVB8	11294	20097	0.37%	0.043%
65	14.686	1982	1989	1997	rVB10	10145	26533	0.49%	0.056%
66	14.810	2006	2010	2014	rVB5	11677	17548	0.33%	0.037%
67	14.886	2017	2023	2028	rBV2	37905	61353	1.14%	0.130%
68	15.021	2041	2046	2052	rBV8	12057	28948	0.54%	0.061%
69	15.074	2053	2055	2064	rVB9	5053	9093	0.17%	0.019%
70	15.151	2064	2068	2071	rBV4	10225	11862	0.22%	0.025%
71	15.198	2073	2076	2079	rBV5	8038	11834	0.22%	0.025%
72	15.286	2087	2091	2095	rVB7	4737	8637	0.16%	0.018%
73	15.333	2095	2099	2100	rVB3	5271	7438	0.14%	0.016%
74	15.398	2103	2110	2117	rBV	2782466	4240157	78.96%	8.995%
75	15.568	2138	2139	2146	rBV7	5445	9690	0.18%	0.021%
76	15.639	2146	2151	2155	rBV4	22473	35370	0.66%	0.075%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
 Data File : BM048133.D
 Acq On : 18 Oct 2024 13:23
 Operator : RC/JU
 Sample : P4380-13
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E27H2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
 Title : SVOA CALIBRATION

77	15.751	2166	2170	2171	rBV4	8342	8565	0.16%	0.018%
78	15.857	2184	2188	2192	rVB3	17010	23504	0.44%	0.050%
79	15.974	2203	2208	2212	rBV7	9484	16132	0.30%	0.034%
80	16.104	2222	2230	2241	rBV7	29213	84556	1.57%	0.179%
81	16.215	2247	2249	2254	rVB6	5433	6014	0.11%	0.013%
82	16.357	2269	2273	2276	rBV6	7883	13310	0.25%	0.028%
83	16.427	2280	2285	2290	rBV	30777	55947	1.04%	0.119%
84	16.674	2323	2327	2332	rBV5	34826	55767	1.04%	0.118%
85	16.804	2345	2349	2351	rBV2	12971	18430	0.34%	0.039%
86	16.915	2364	2368	2373	rVV7	14289	26665	0.50%	0.057%
87	17.145	2401	2407	2412	rBV	1777568	2589846	48.23%	5.494%
88	17.186	2412	2414	2417	rVV	58264	66456	1.24%	0.141%
89	17.245	2417	2424	2434	rVV	3058650	4527295	84.30%	9.604%
90	19.098	2736	2739	2745	rVB4	42919	58168	1.08%	0.123%
91	19.168	2748	2751	2754	rBV2	38931	54468	1.01%	0.116%
92	19.533	2807	2813	2825	rBV	4018940	5370256	100.00%	11.392%
93	21.368	3120	3125	3139	rVB2	1719858	2714462	50.55%	5.758%
94	24.150	3589	3598	3610	rVB	2164473	5303083	98.75%	11.250%
95	24.350	3624	3632	3644	rVB	1154274	3010427	56.06%	6.386%




Sum of corrected areas: 47138580

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
Data File : BM048133.D
Acq On : 18 Oct 2024 13:23
Operator : RC/JU
Sample : P4380-13
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27H2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

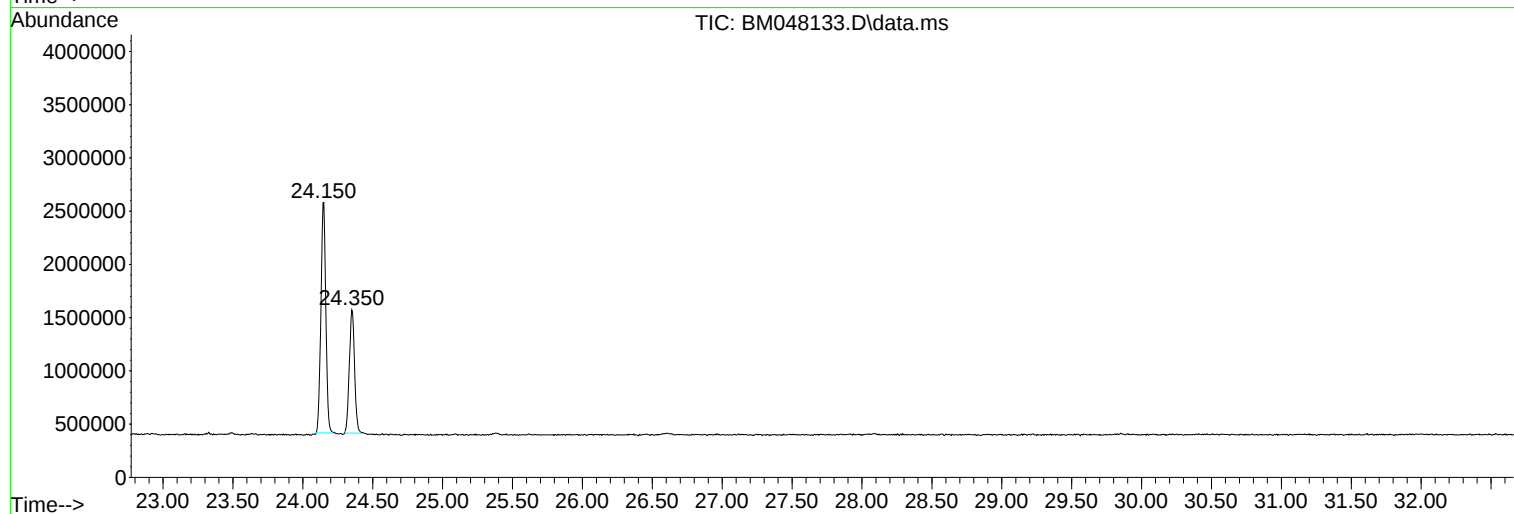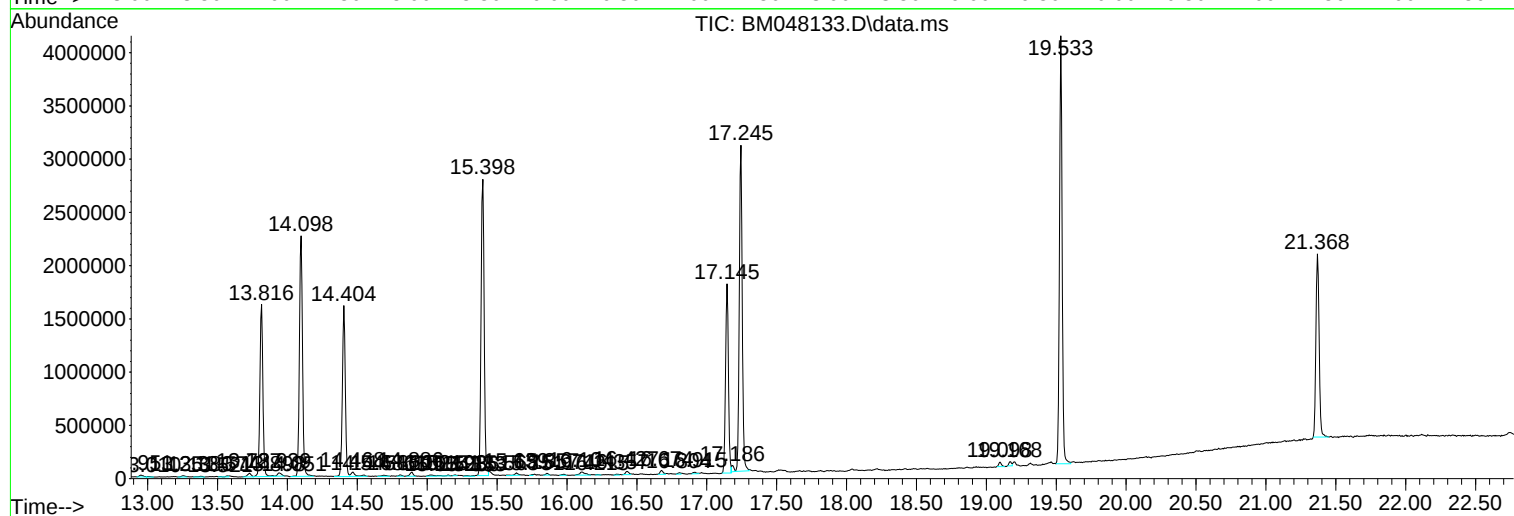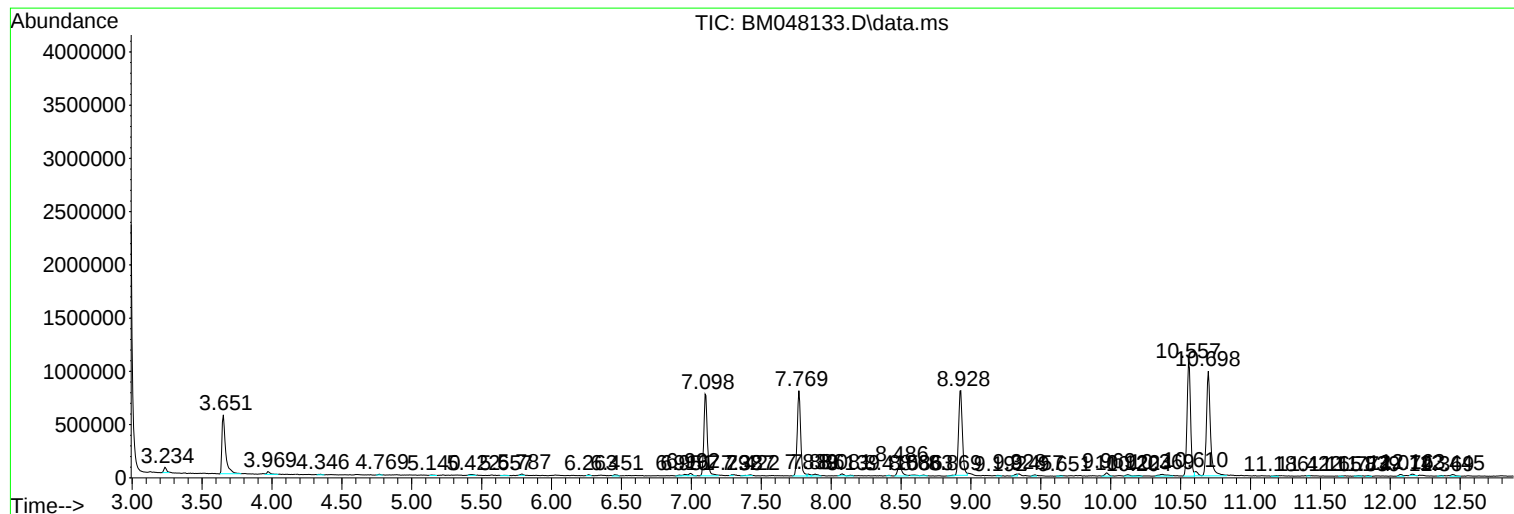

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
Data File : BM048133.D
Acq On : 18 Oct 2024 13:23
Operator : RC/JU
Sample : P4380-13
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27H2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101724\
Data File : BM048133.D
Acq On : 18 Oct 2024 13:23
Operator : RC/JU
Sample : P4380-13
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27H2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM101724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------