

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM101818\
 Data File : BM017214.D
 Acq On : 19 Oct 2018 03:58
 Operator : MJ/SJ
 Sample : PB113953BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB113953BL

Quant Time: Oct 19 13:56:11 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 17 14:23:17 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	323811	20.00	ng	0.00
21) Naphthalene-d8	10.45	136	1285636	20.00	ng	0.00
39) Acenaphthene-d10	14.31	164	755060	20.00	ng	0.00
64) Phenanthrene-d10	17.06	188	1695105	20.00	ng	-0.01
76) Chrysene-d12	21.25	240	1525539	20.00	ng	-0.01
87) Perylene-d12	23.46	264	1264046	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.29	112	2380273	124.33	ng	0.00
7) Phenol-d6	6.85	99	3135080	120.23	ng	0.00
23) Nitrobenzene-d5	8.82	82	1885690	85.78	ng	-0.01
42) 2,4,6-Tribromophenol	15.81	330	1267397	124.12	ng	0.00
45) 2-Fluorobiphenyl	12.93	172	4551298	80.20	ng	0.00
79) Terphenyl-d14	19.70	244	6240229	92.20	ng	0.00
Target Compounds						
80) Butylbenzylphthalate	20.40	149	956	7.201	ng	# 27
84) Bis(2-ethylhexyl)phthalate	21.17	149	563	5.318	ng	# 52
85) Di-n-octyl phthalate	22.07	149	1978	5.592	ng	# 77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM101818\
Data File : BM017214.D
Acq On : 19 Oct 2018 03:58
Operator : MJ/SJ
Sample : PB113953BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB113953BL

Quant Time: Oct 19 13:56:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 17 14:23:17 2018
Response via : Initial Calibration

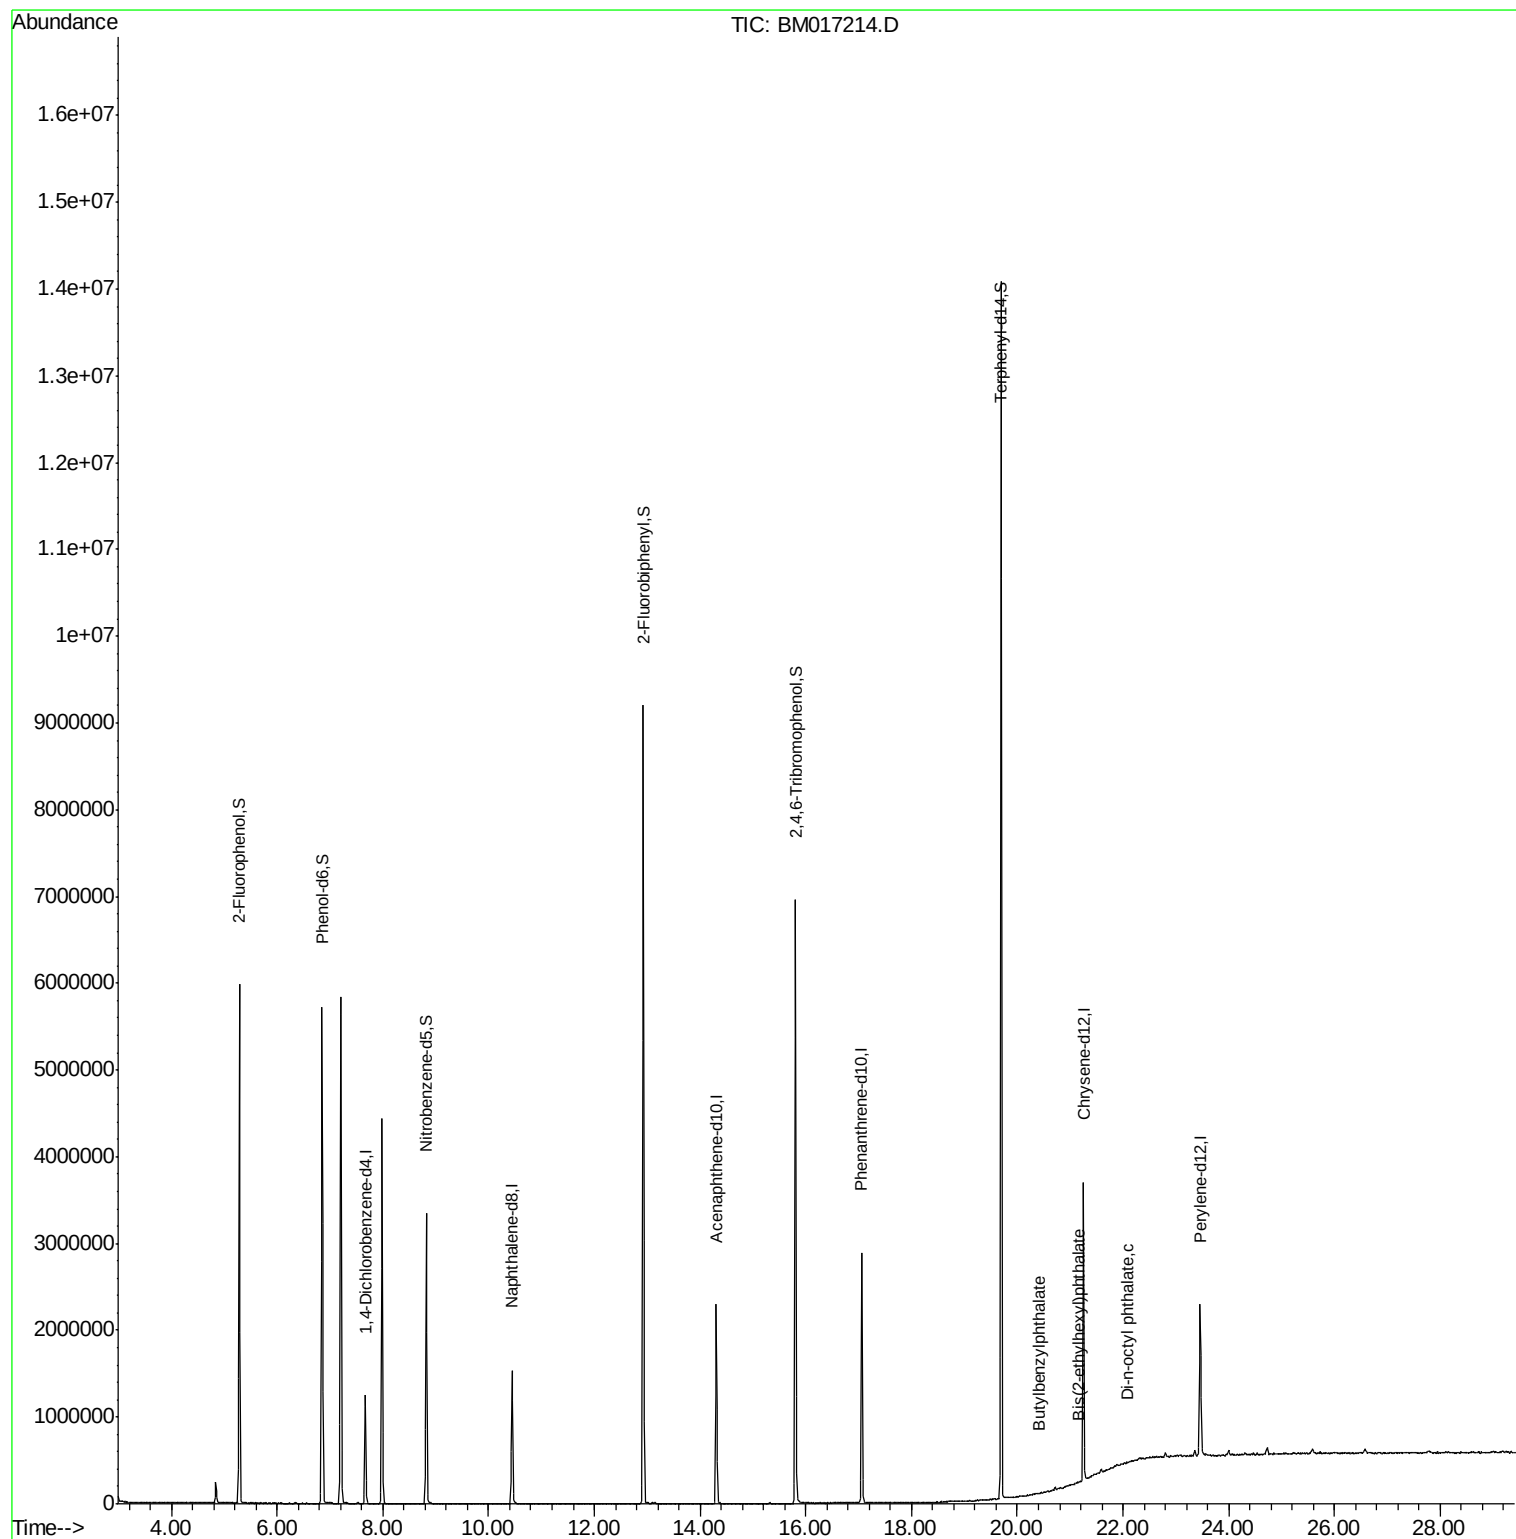

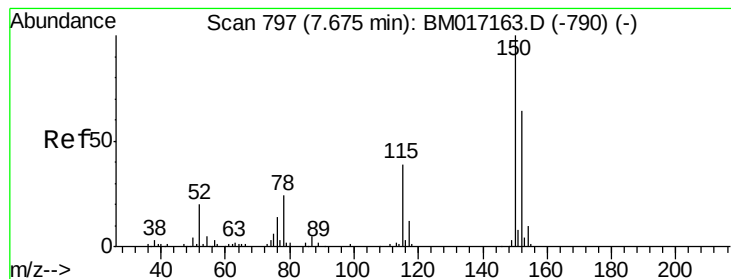


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.67 min Scan# 796
Delta R.T. -0.01 min
Lab File: BM017214.D
Acq: 19 Oct 2018 03:58

Instrument :
BNA_M
ClientSampleId :
PB113953BL

Tgt Ion:152 Resp: 323811
Ion Ratio Lower Upper
152 100
150 152.7 124.3 186.5
115 60.7 48.1 72.1

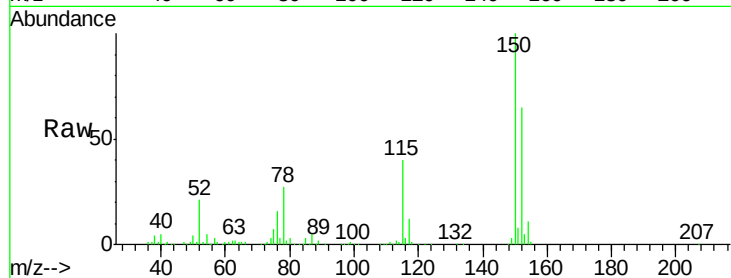


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

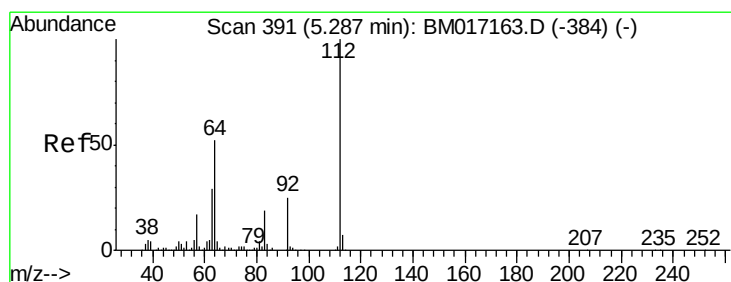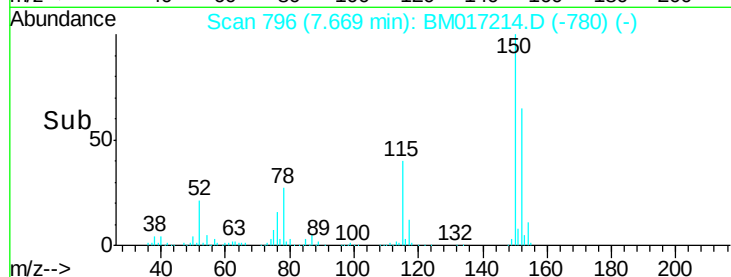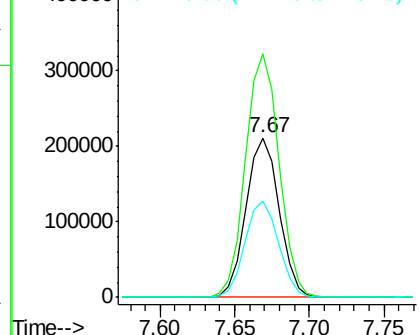



#5


2-Fluorophenol
Concen: 124.327 ng
RT: 5.29 min Scan# 391
Delta R.T. 0.00 min
Lab File: BM017214.D
Acq: 19 Oct 2018 03:58

Tgt Ion:112 Resp: 2380273
Ion Ratio Lower Upper
112 100
64 58.2 41.7 62.5
63 31.2 23.0 34.4

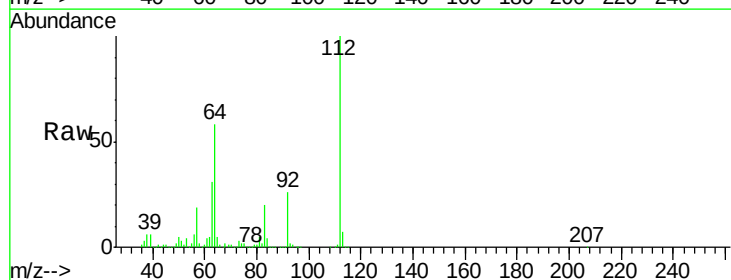

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

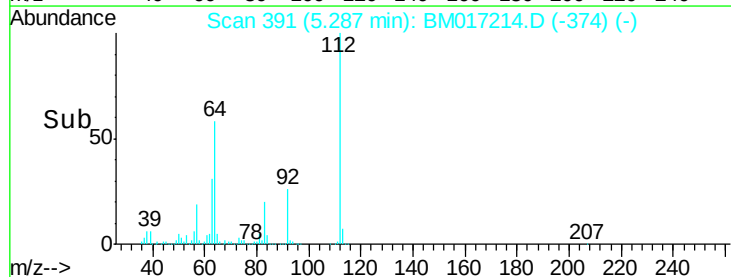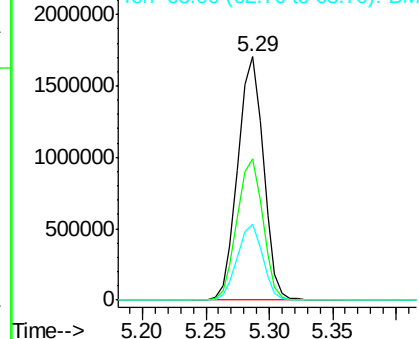

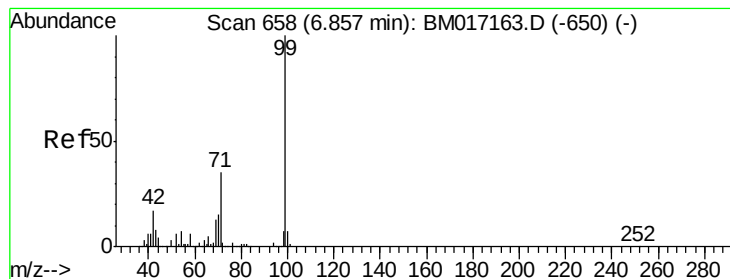

#7

Phenol-d6

Concen: 120.234 ng

RT: 6.85 min Scan# 657

Delta R.T. -0.01 min

Lab File: BM017214.D

Acq: 19 Oct 2018 03:58

Instrument :

BNA_M

ClientSampleId :

PB113953BL


Tgt Ion: 99 Resp: 3135080

Ion Ratio Lower Upper

99 100

42 18.4 13.3 19.9




71 36.8 28.0 42.0

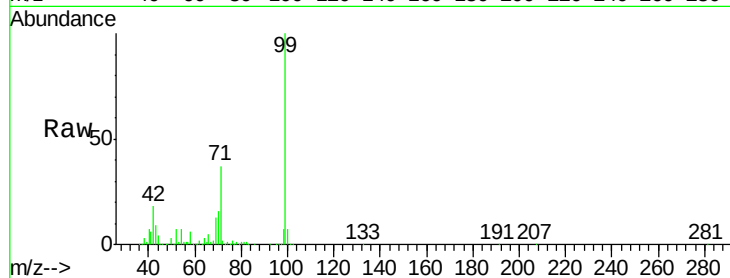

Abundance Ion 99.00 (98.70 to 99.70): BM017214.D (-641) (-)

Ion 42.00 (41.70 to 42.70): BM017214.D (-641) (-)

Ion 71.00 (70.70 to 71.70): BM017214.D (-641) (-)

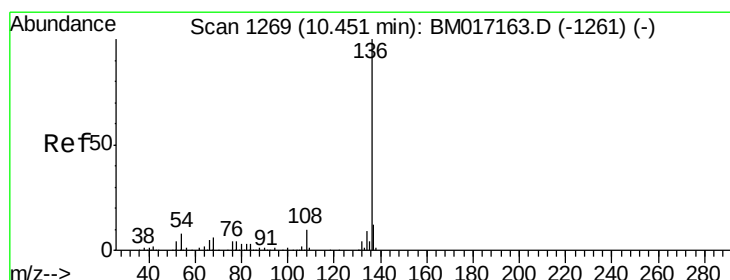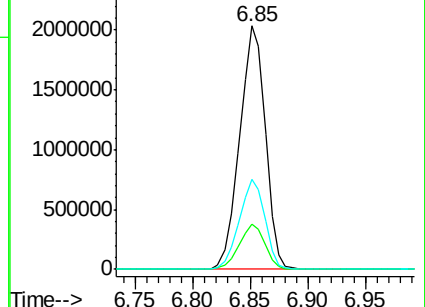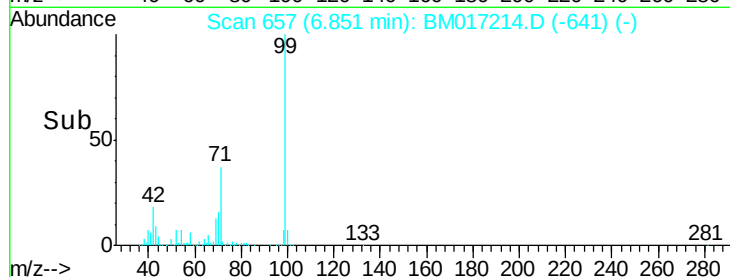

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.45 min Scan# 1268

Delta R.T. -0.01 min

Lab File: BM017214.D

Acq: 19 Oct 2018 03:58

Tgt Ion: 136 Resp: 1285636


Ion Ratio Lower Upper

136 100

137 10.5 9.2 13.8

54 7.7 6.7 10.1

68 5.3 4.7 7.1


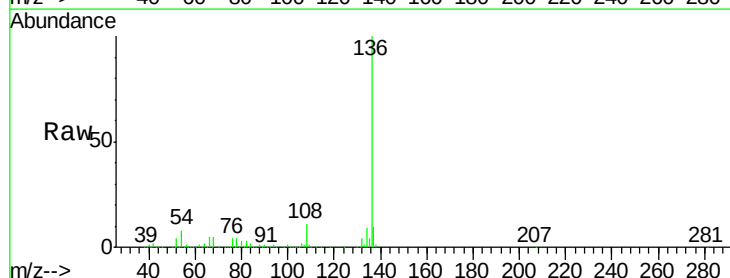



Abundance Ion 136.00 (135.70 to 136.70): BM017214.D (-1252) (-)

Ion 137.00 (136.70 to 137.70): BM017214.D (-1252) (-)

Ion 54.00 (53.70 to 54.70): BM017214.D (-1252) (-)

Ion 68.00 (67.70 to 68.70): BM017214.D (-1252) (-)



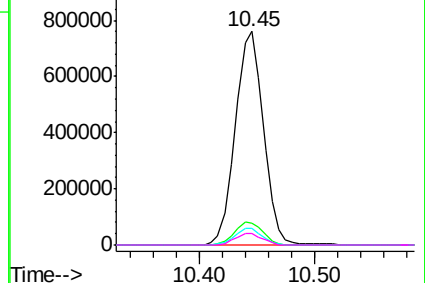
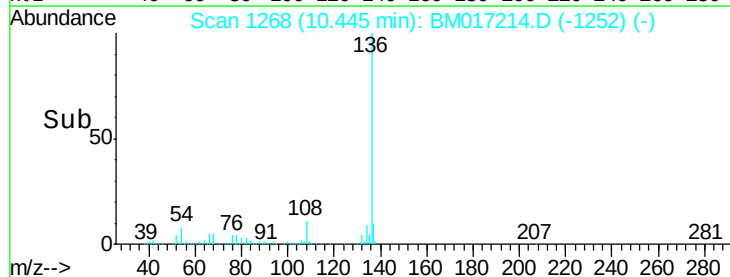


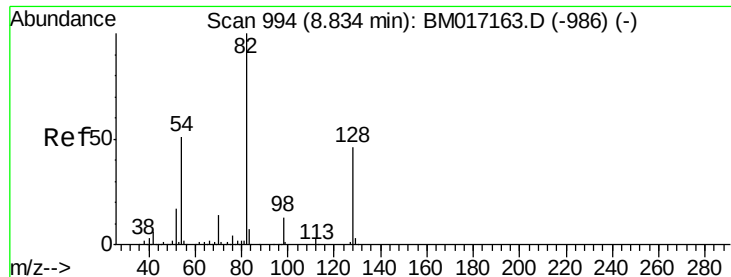

#23
 Nitrobenzene-d5
 Concen: 85.783 ng
 RT: 8.82 min Scan# 992
 Delta R.T. -0.01 min
 Lab File: BM017214.D
 Acq: 19 Oct 2018 03:58




Instrument :
 BNA_M
 ClientSampleId :
 PB113953BL


Tgt Ion: 82 Resp: 1885690
 Ion Ratio Lower Upper
 82 100
 128 42.8 37.0 55.6
 54 50.7 40.7 61.1

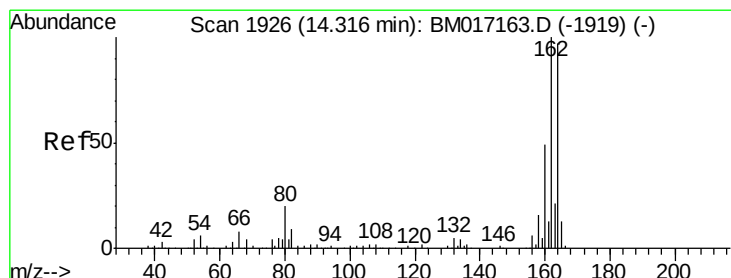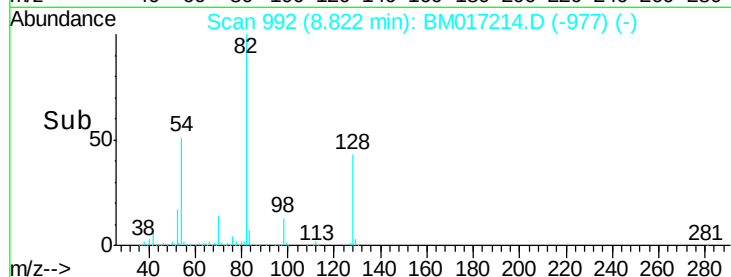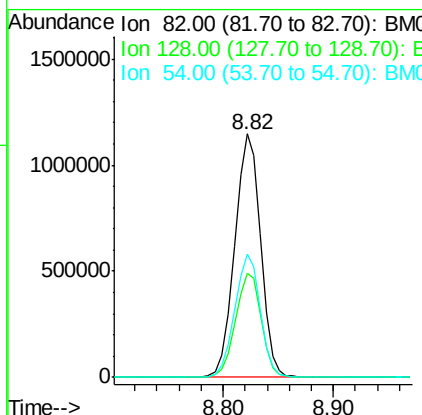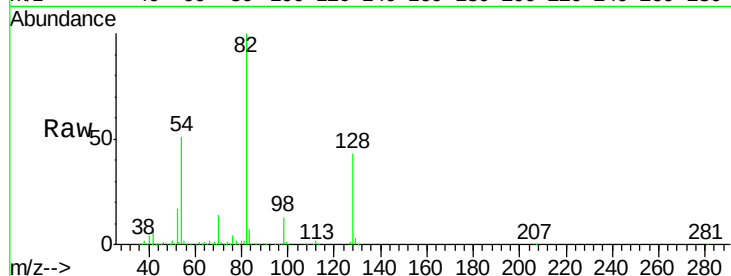

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.31 min Scan# 1925
 Delta R.T. -0.01 min
 Lab File: BM017214.D
 Acq: 19 Oct 2018 03:58

Tgt Ion: 164 Resp: 755060
 Ion Ratio Lower Upper
 164 100
 162 101.0 82.1 123.1
 160 45.0 40.2 60.2

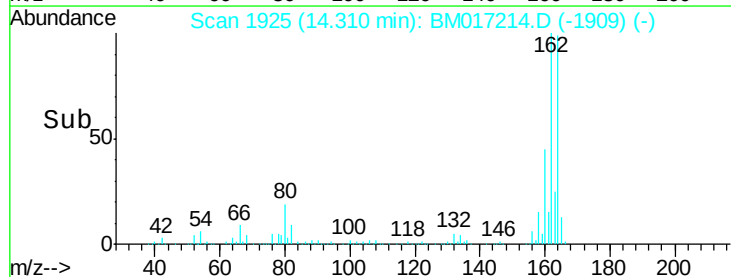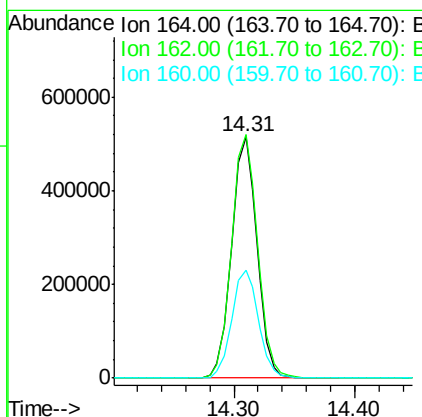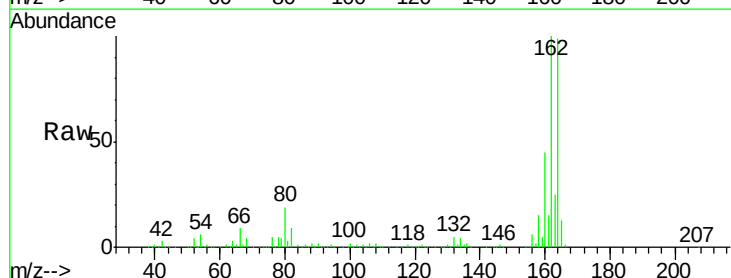


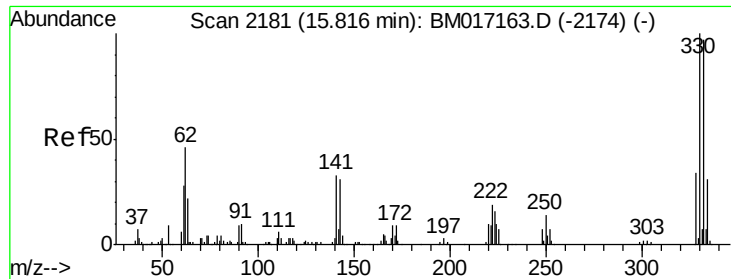




#42
 2,4,6-Tribromophenol
 Concen: 124.120 ng
 RT: 15.81 min Scan# 2180
 Delta R.T. -0.01 min
 Lab File: BM017214.D
 Acq: 19 Oct 2018 03:58

Instrument :
 BNA_M
 ClientSampleId :
 PB113953BL

Tgt Ion:330 Resp: 1267397
 Ion Ratio Lower Upper
 330 100
 332 96.3 77.3 115.9
 141 34.3 27.4 41.0

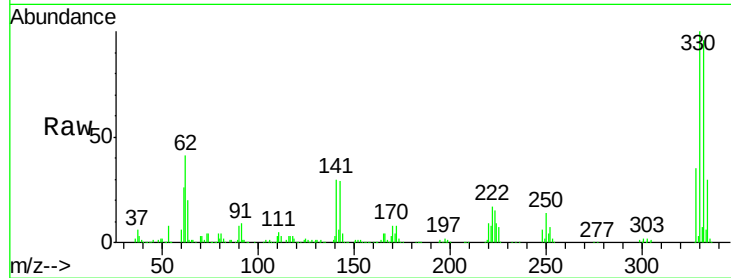


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

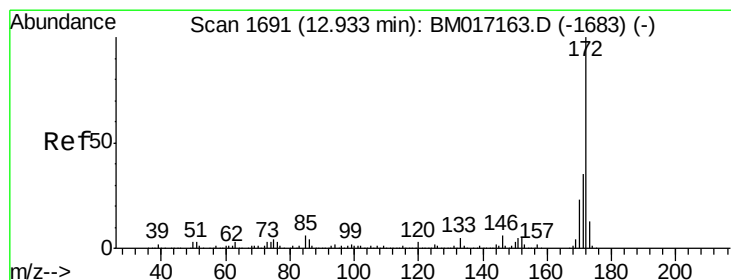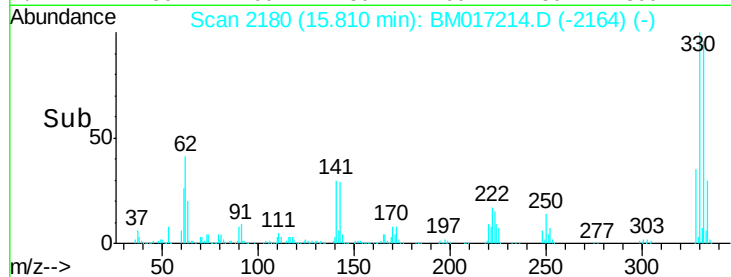
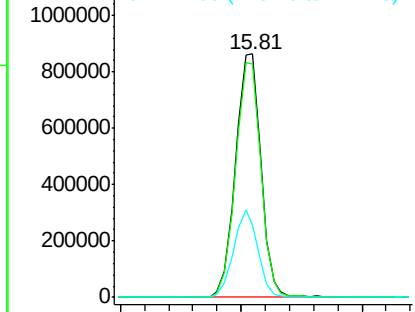



#45
 2-Fluorobiphenyl
 Concen: 80.202 ng
 RT: 12.93 min Scan# 1690
 Delta R.T. -0.01 min
 Lab File: BM017214.D
 Acq: 19 Oct 2018 03:58

Tgt Ion:172 Resp: 4551298
 Ion Ratio Lower Upper
 172 100
 171 34.6 28.3 42.5
 170 22.8 18.3 27.5

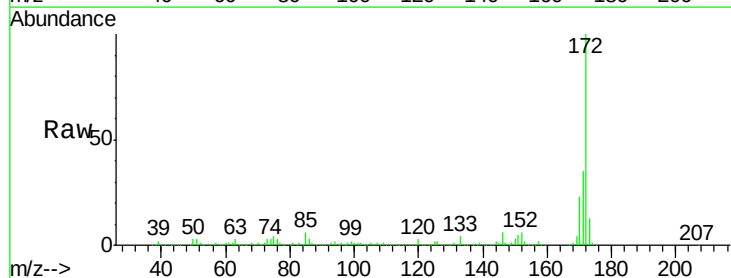

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

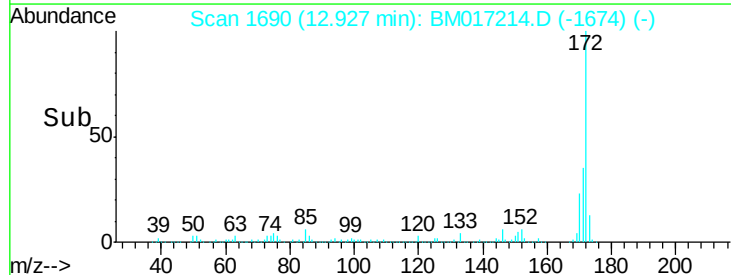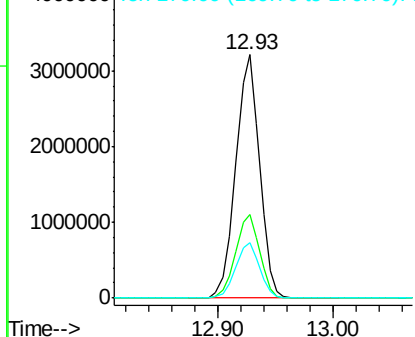

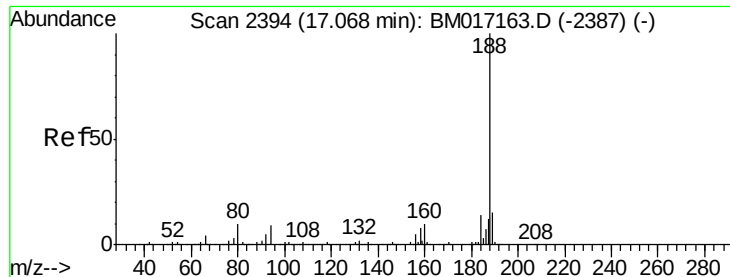

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.06 min Scan# 2392

Delta R.T. -0.01 min

Lab File: BM017214.D

Acq: 19 Oct 2018 03:58

Instrument :

BNA_M

ClientSampleId :

PB113953BL


Tgt Ion:188 Resp: 1695105

Ion Ratio Lower Upper

188 100

94 8.6 7.0 10.4




80 9.6 7.7 11.5

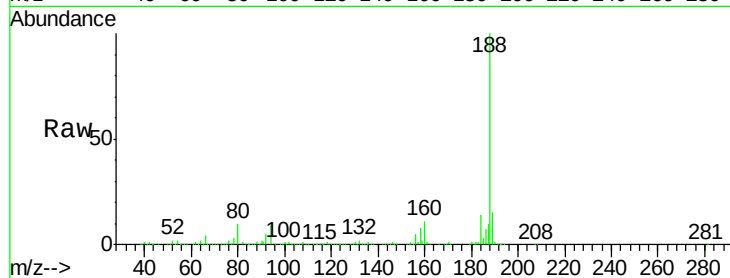

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM0

Ion 80.00 (79.70 to 80.70): BM0

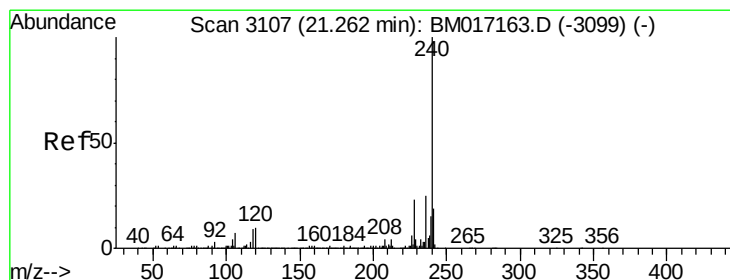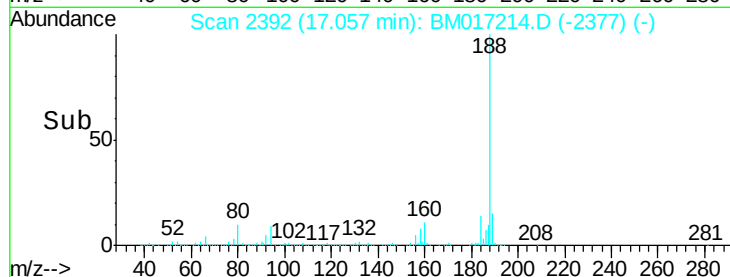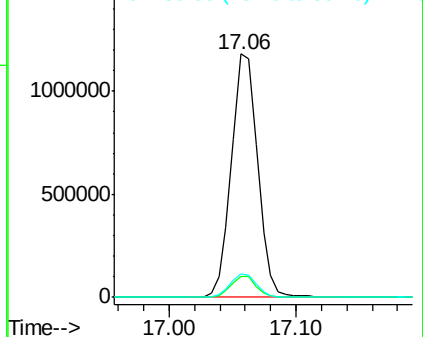

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.25 min Scan# 3105

Delta R.T. -0.01 min

Lab File: BM017214.D

Acq: 19 Oct 2018 03:58


Tgt Ion:240 Resp: 1525539

Ion Ratio Lower Upper

240 100

120 9.7 8.1 12.1



236 24.9 19.9 29.9

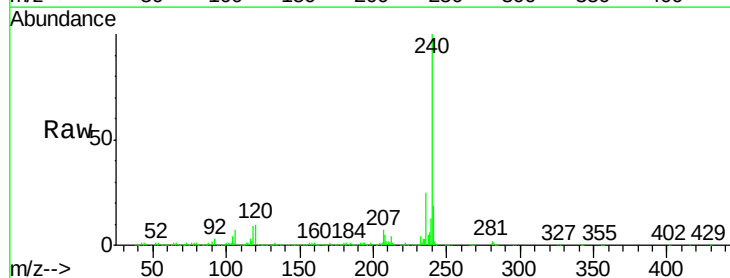


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

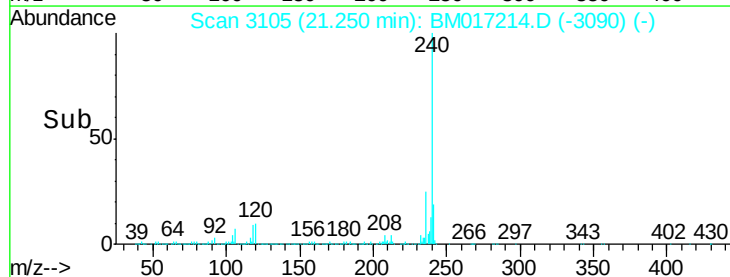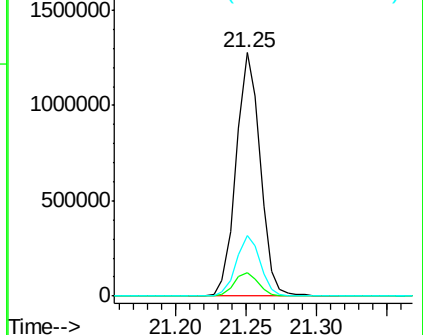

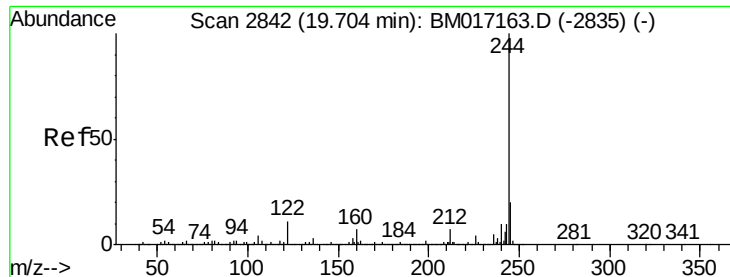

#79

Terphenyl-d14

Concen: 92.200 ng

RT: 19.70 min Scan# 2841

Delta R.T. -0.01 min

Lab File: BM017214.D

Acq: 19 Oct 2018 03:58

Instrument :

BNA_M

ClientSampleId :

PB113953BL


Tgt Ion:244 Resp: 6240229

Ion Ratio Lower Upper

244 100

212 7.4 5.5 8.3




122 10.0 8.4 12.6

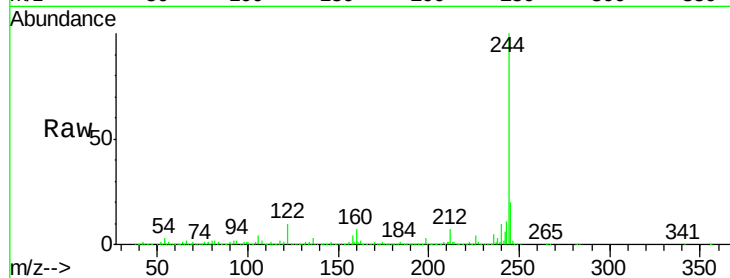

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

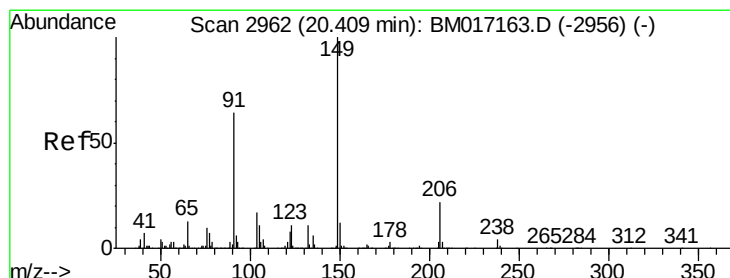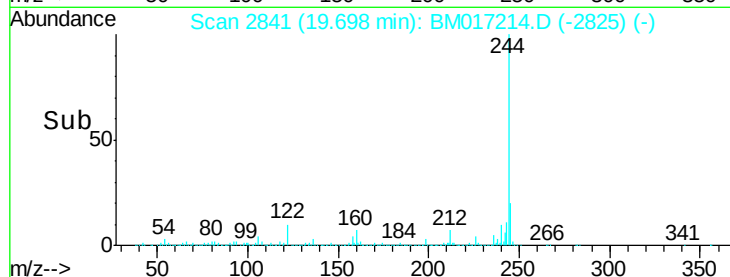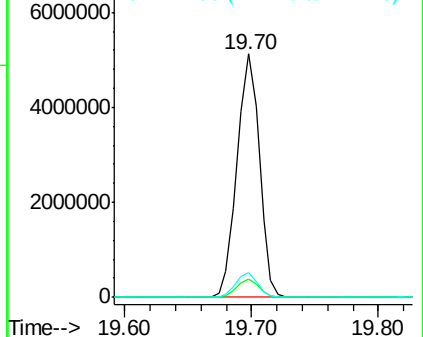

#80

Butylbenzylphthalate

Concen: 7.201 ng

RT: 20.40 min Scan# 2960

Delta R.T. -0.01 min

Lab File: BM017214.D

Acq: 19 Oct 2018 03:58


Tgt Ion:149 Resp: 956

Ion Ratio Lower Upper

149 100

91 0.0 51.3 76.9#



206 0.0 18.0 27.0#

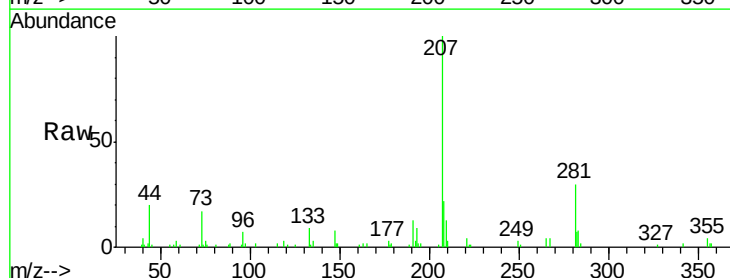


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 91.00 (90.70 to 91.70): BM0

Ion 206.00 (205.70 to 206.70): E

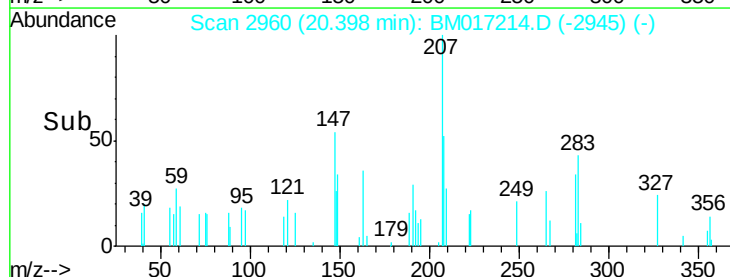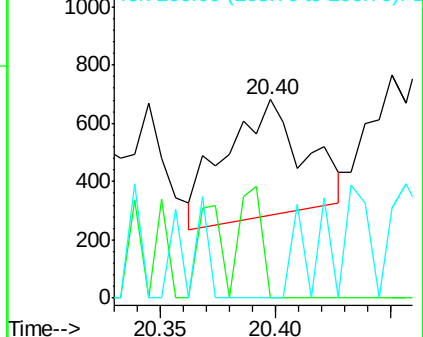


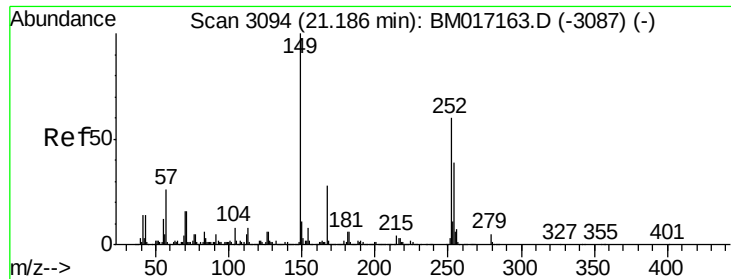




#84
 Bis(2-ethylhexyl)phthalate
 Concen: 5.318 ng
 RT: 21.17 min Scan# 3092
 Delta R.T. -0.01 min
 Lab File: BM017214.D
 Acq: 19 Oct 2018 03:58

Instrument :
 BNA_M
 ClientSampleId :
 PB113953BL

Tgt Ion:149 Resp: 563
 Ion Ratio Lower Upper
 149 100
 167 0.0 22.2 33.4#
 279 0.0 3.6 5.4#

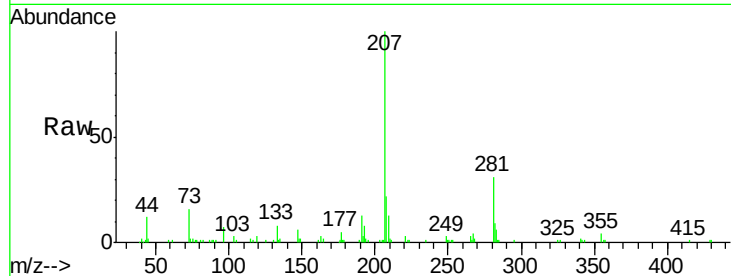


Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 167.00 (166.70 to 167.70): E
 Ion 279.00 (278.70 to 279.70): E

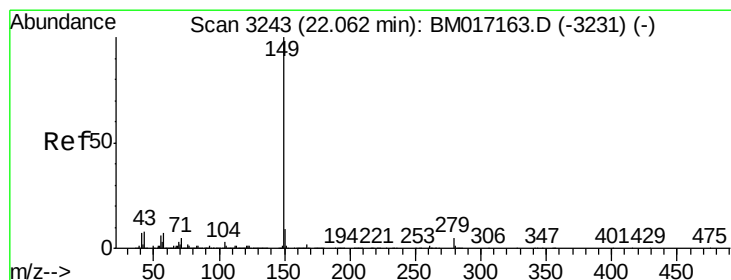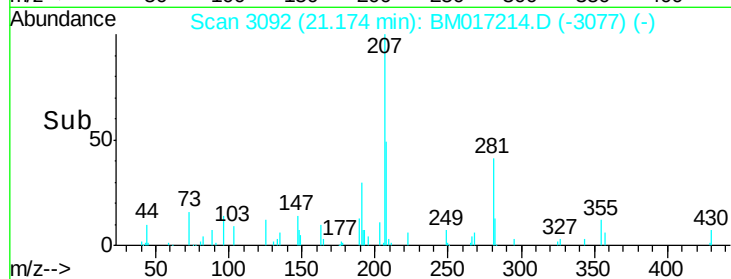
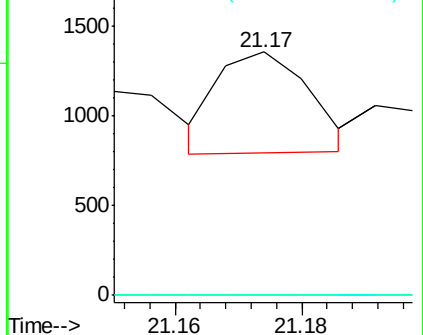





#85
 Di-n-octyl phthalate
 Concen: 5.592 ng
 RT: 22.07 min Scan# 3244
 Delta R.T. 0.01 min
 Lab File: BM017214.D
 Acq: 19 Oct 2018 03:58

Tgt Ion:149 Resp: 1978
 Ion Ratio Lower Upper
 149 100
 167 5.8 1.4 2.0#
 43 0.0 7.2 10.8#

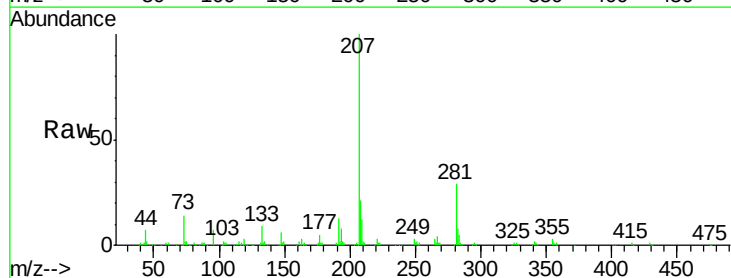

Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 167.00 (166.70 to 167.70): E
 Ion 43.00 (42.70 to 43.70): BM0

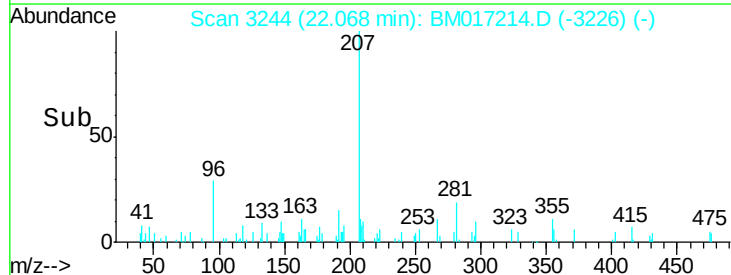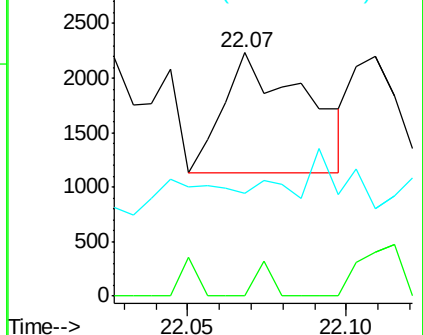

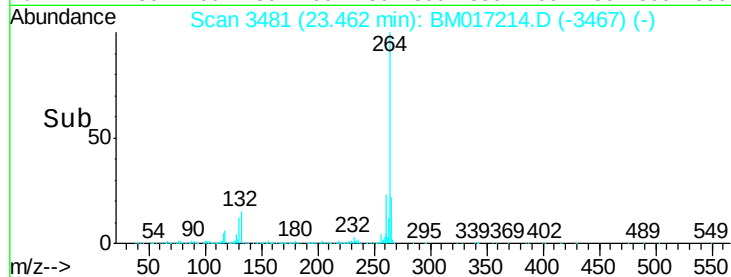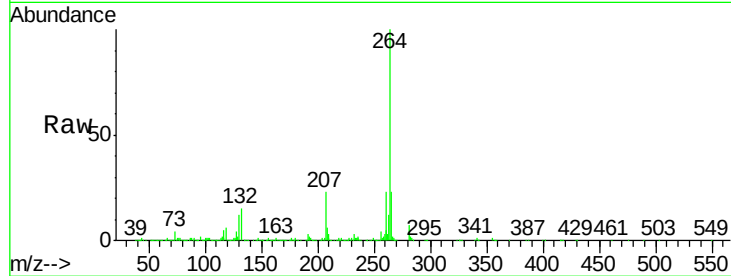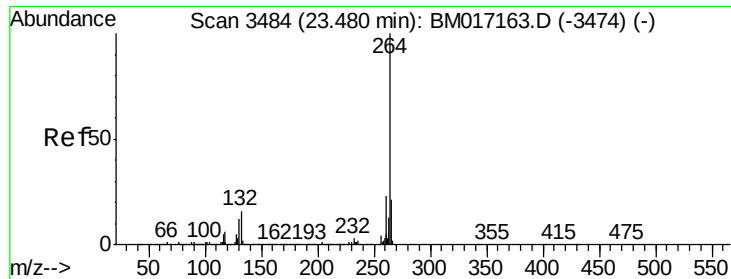

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.46 min Scan# 3481

Delta R.T. -0.02 min

Lab File: BM017214.D

Acq: 19 Oct 2018 03:58

Instrument :

BNA_M

ClientSampleId :

PB113953BL

Tgt Ion:264 Resp: 1264046

Ion Ratio Lower Upper

264 100

260 23.5 18.6 27.8

265 22.8 17.8 26.8

