

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM101818\
 Data File : BM017214.D
 Acq On : 19 Oct 2018 03:58
 Operator : MJ/SJ
 Sample : PB113953BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB113953BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.840	310	315	325	rBV	242925	343552	2.02%	0.347%
2	5.287	384	391	405	rBV	5982274	8398924	49.38%	8.476%
3	6.851	648	657	671	rBV	5723830	8946803	52.60%	9.029%
4	7.204	710	717	731	rBV	5835567	9135586	53.71%	9.220%
5	7.669	788	796	804	rBV	1248073	1950306	11.47%	1.968%
6	7.987	842	850	859	rBV	4437744	6965947	40.96%	7.030%
7	8.822	984	992	1003	rBV	3344964	5499665	32.34%	5.550%
8	10.445	1259	1268	1280	rBV	1534225	2616665	15.39%	2.641%
9	12.927	1682	1690	1699	rBV	9200759	13118872	77.13%	13.240%
10	14.310	1918	1925	1937	rBV2	2297425	3519285	20.69%	3.552%
11	15.804	2172	2179	2197	rBV	6954635	10004843	58.82%	10.097%
12	17.057	2386	2392	2405	rBV2	2878647	4176259	24.55%	4.215%
13	19.698	2835	2841	2849	rBV	14027436	17007816	100.00%	17.165%
14	21.250	3100	3105	3111	rBV	3443588	4131174	24.29%	4.169%
15	23.462	3475	3481	3495	rVB	1735922	3270037	19.23%	3.300%


Sum of corrected areas: 99085734

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM101818\
Data File : BM017214.D
Acq On : 19 Oct 2018 03:58
Operator : MJ/SJ
Sample : PB113953BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB113953BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

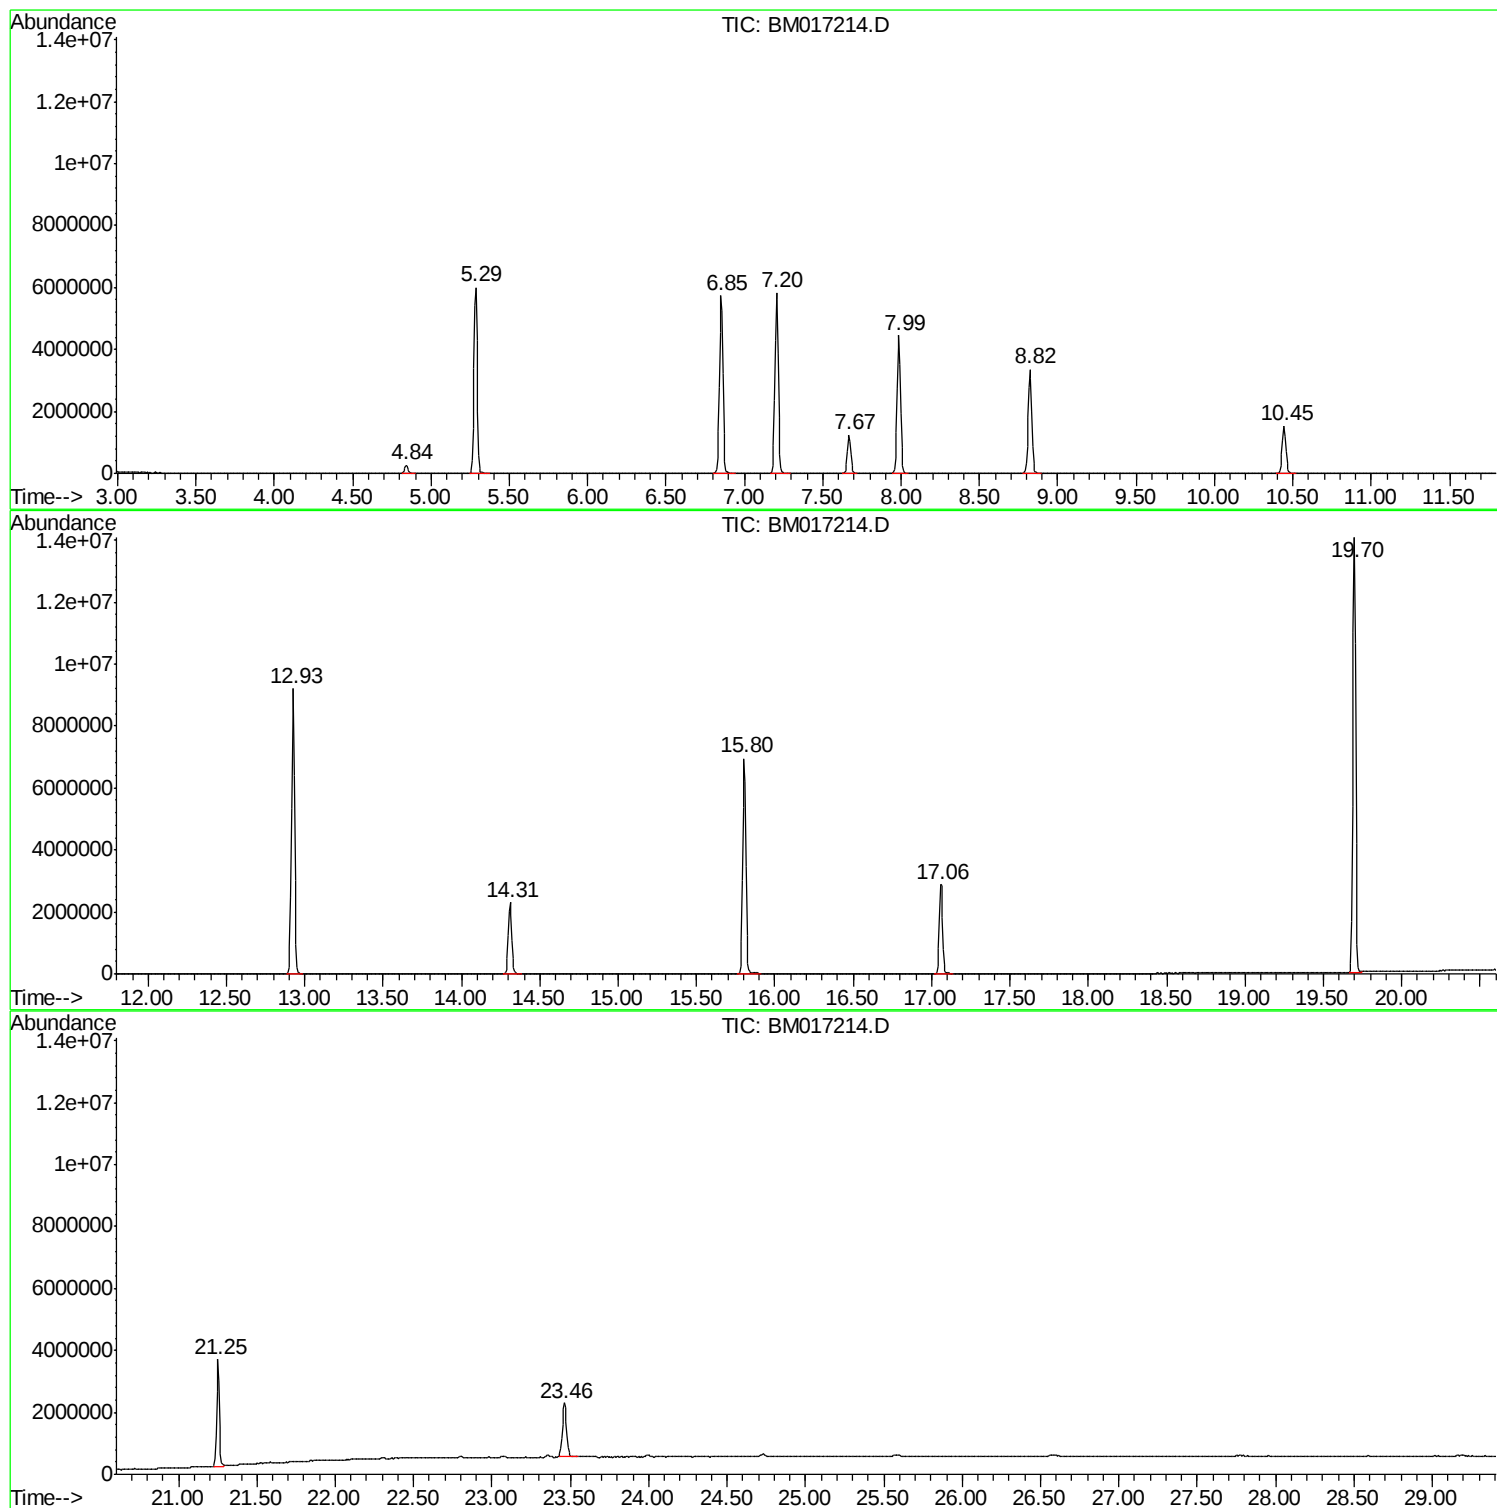

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM101818\
Data File : BM017214.D
Acq On : 19 Oct 2018 03:58
Operator : MJ/SJ
Sample : PB113953BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB113953BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.84	3.52 ng	343552	1,4-Dichlorobenzene-d4	7.67

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	40
2			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	35
3			Butyl aldoxime, 3-methyl-, syn-	101	C5H11NO	005780-40-5	25
4			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23
5			2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	23

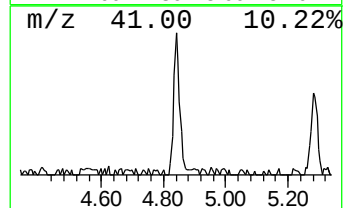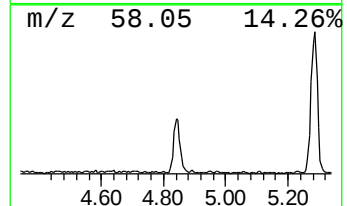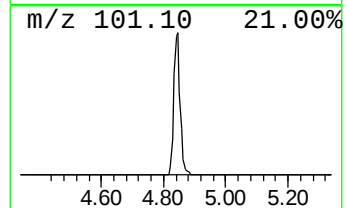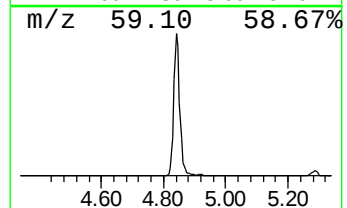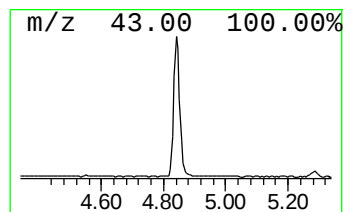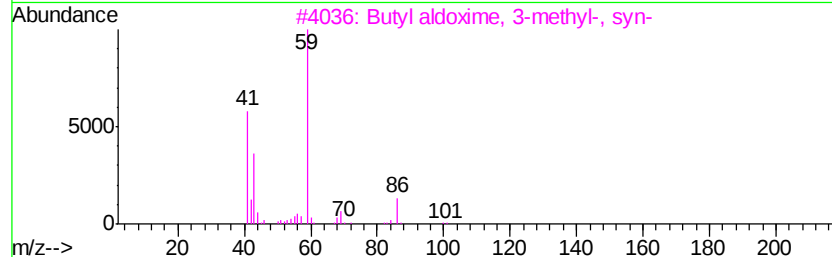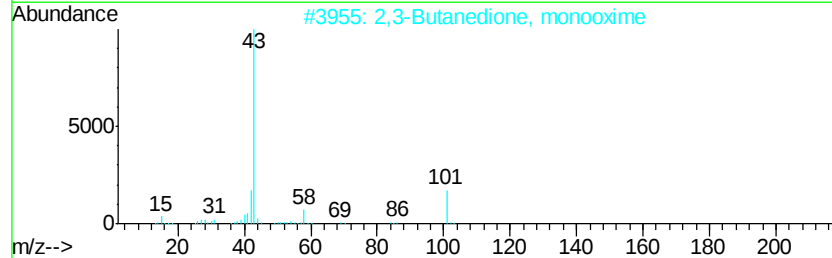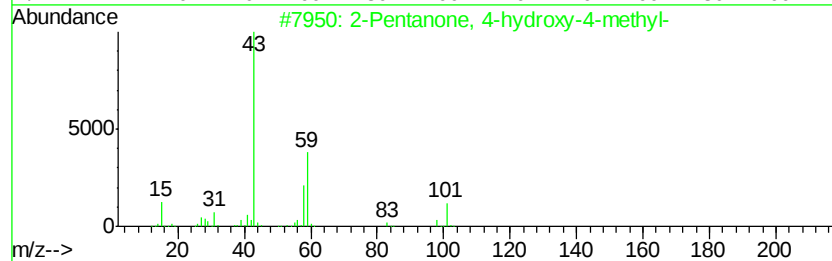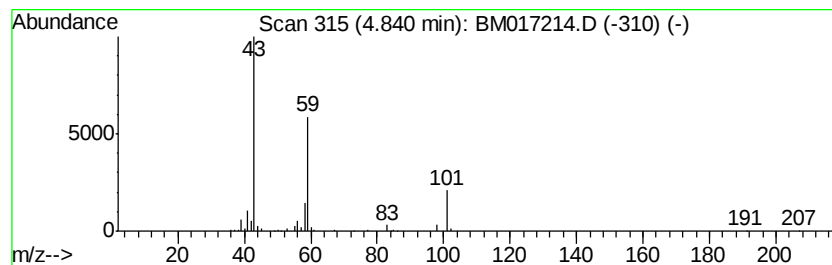

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM101818\
Data File : BM017214.D
Acq On : 19 Oct 2018 03:58
Operator : MJ/SJ
Sample : PB113953BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB113953BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.20 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.20	93.68 ng	9135590	1,4-Dichlorobenzene-d4	7.67

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3			5-Aminoindole	132	C8H8N2	005192-03-0	12
4			Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5			Benzene, 1-ethenyl-3,5-dimethyl-	132	C10H12	005379-20-4	9

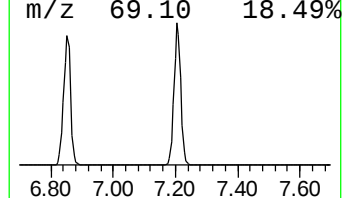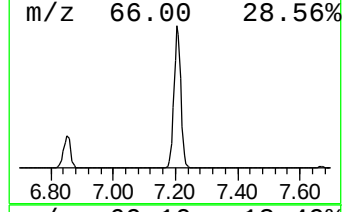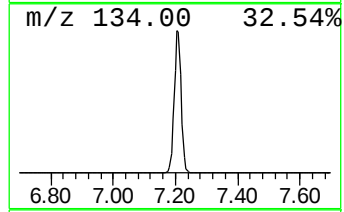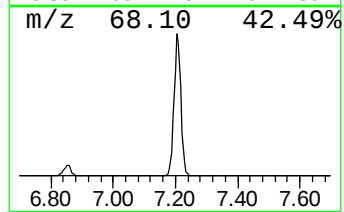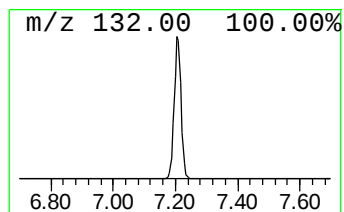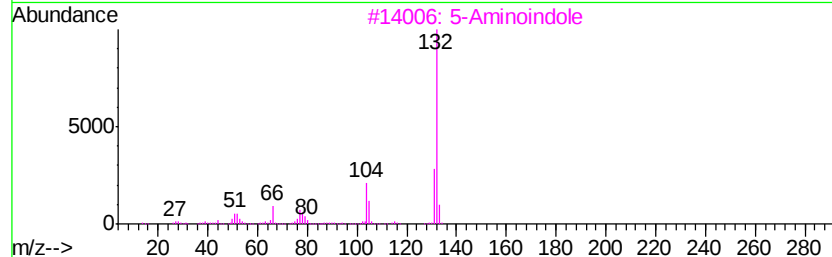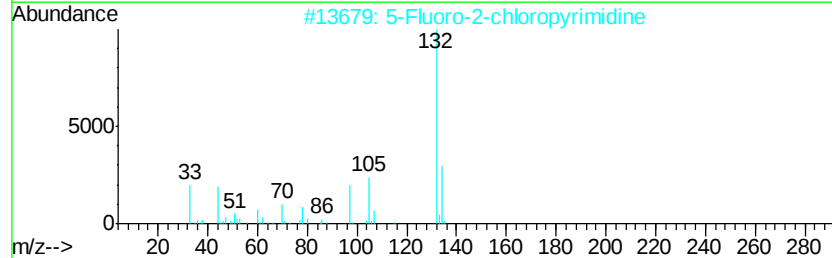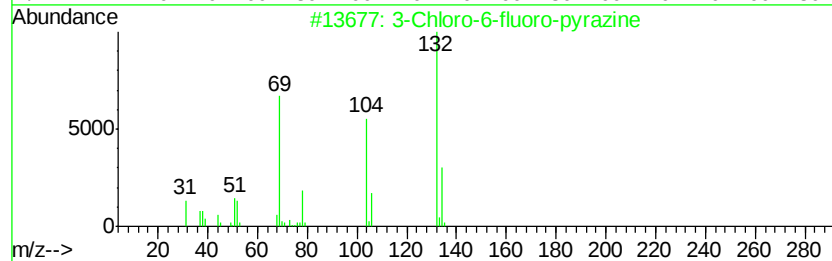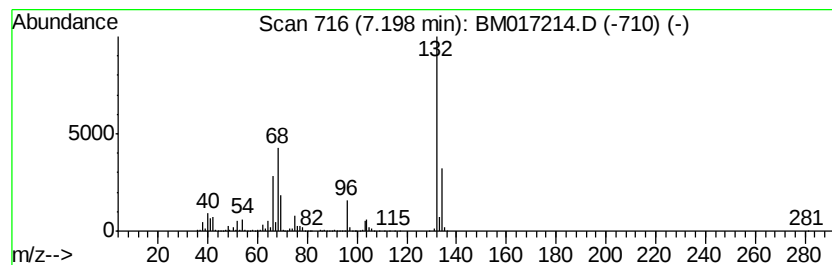

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM101818\
Data File : BM017214.D
Acq On : 19 Oct 2018 03:58
Operator : MJ/SJ
Sample : PB113953BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB113953BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.84	3.5	ng	343552	1	7.67	1950310	20.0
unknown7.20	7.20	93.7	ng	9135590	1	7.67	1950310	20.0