


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM101818\
 Data File : BM017189.D
 Acq On : 18 Oct 2018 12:50
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 17 14:23:17 2018

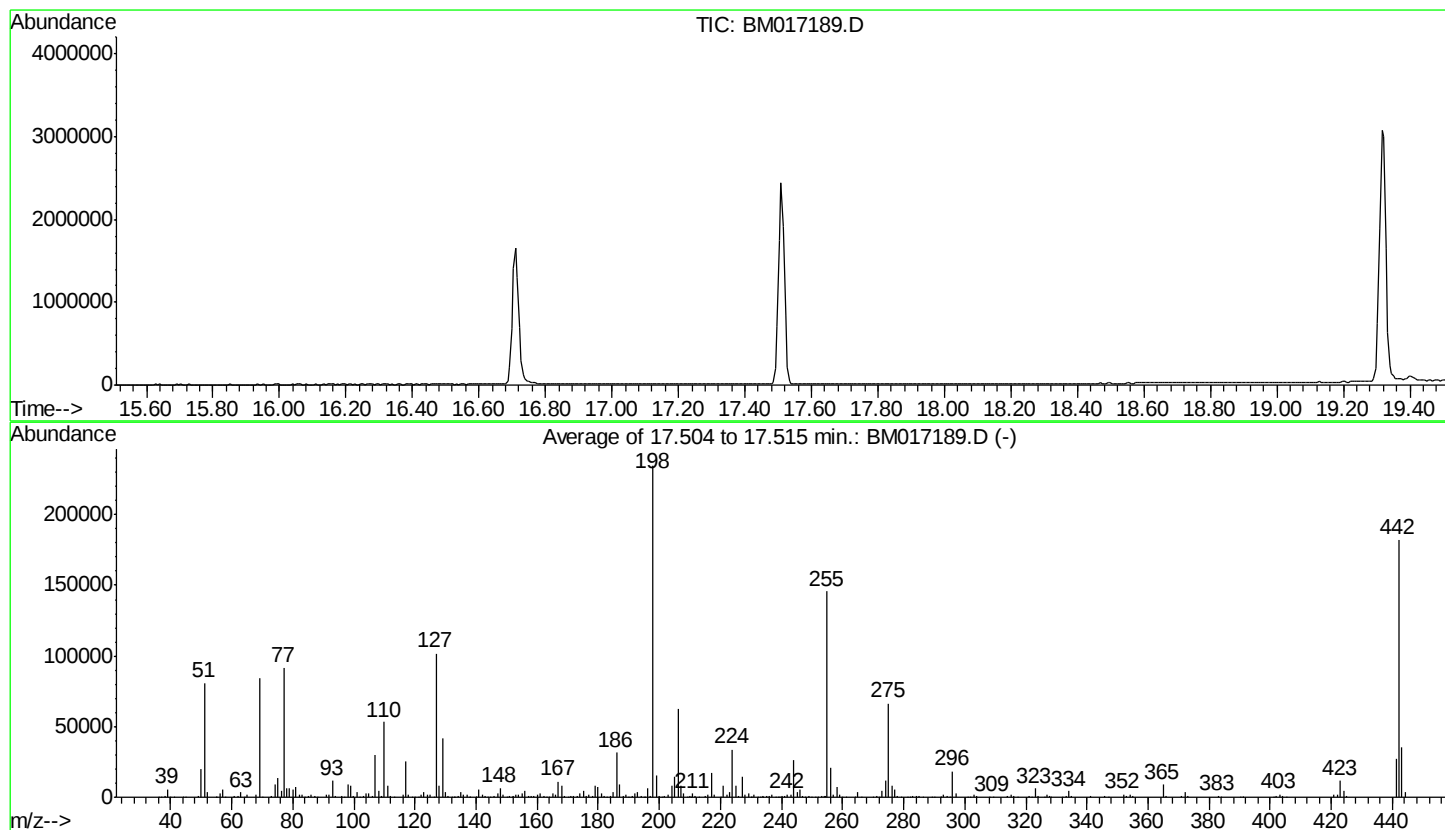

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	80762	PASS
68	69	0.00	2	1.9	1584	PASS
69	198	0.00	100	36.0	84448	PASS
70	69	0.00	2	0.5	393	PASS
127	198	10	80	43.4	101925	PASS
197	198	0.00	2	0.5	1245	PASS
198	198	100	100	100.0	234709	PASS
199	198	5	9	6.4	15003	PASS
275	198	10	60	28.2	66181	PASS
365	198	1	100	3.7	8686	PASS
441	198	0.01	100	11.5	27022	PASS
442	198	50	100	77.6	182160	PASS
443	442	15	24	19.3	35197	PASS