


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM101818\
 Data File : BM017197.D
 Acq On : 18 Oct 2018 17:45
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 17 14:23:17 2018

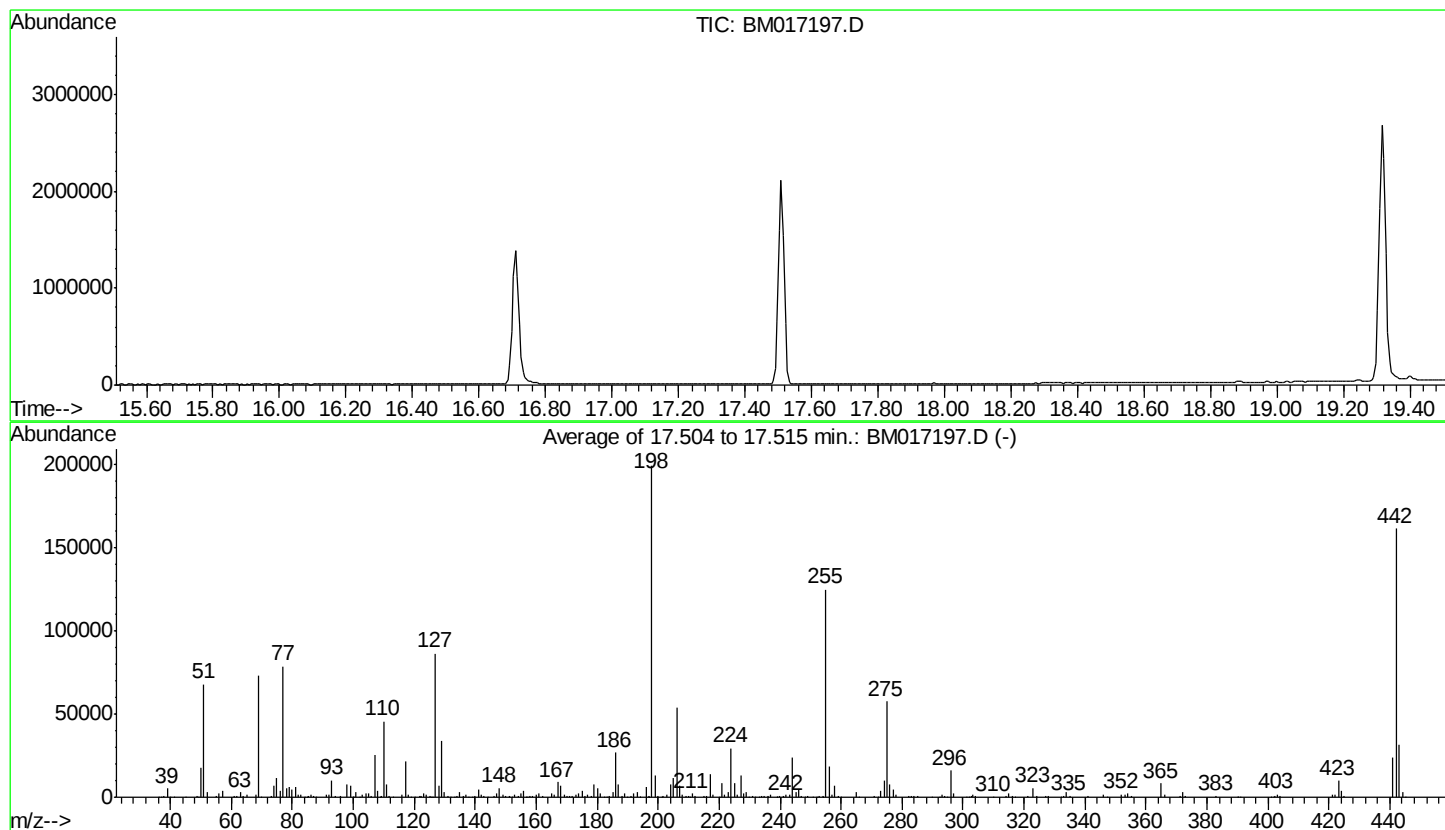

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	68048	PASS
68	69	0.00	2	1.8	1329	PASS
69	198	0.00	100	36.8	73386	PASS
70	69	0.00	2	0.5	338	PASS
127	198	10	80	43.4	86546	PASS
197	198	0.00	2	0.5	933	PASS
198	198	100	100	100.0	199488	PASS
199	198	5	9	6.6	13149	PASS
275	198	10	60	28.9	57669	PASS
365	198	1	100	4.2	8426	PASS
441	198	0.01	100	12.0	23963	PASS
442	198	50	100	80.9	161429	PASS
443	442	15	24	19.6	31600	PASS