

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101821\
 Data File : BM032567.D
 Acq On : 18 Oct 2021 11:17
 Operator : CG/JU
 Sample : M4029-20
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C00T1

Quant Time: Oct 18 11:53:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 18 10:38:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.553	152	3916	0.40	ng/ul	0.00
4) Naphthalene-d8	10.335	136	12051	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.209	164	5869	0.40	ng/ul	0.00
13) Phenanthrene-d10	16.946	188	10586	0.40	ng/ul	0.00
17) Chrysene-d12	21.125	240	6419	0.40	ng/ul	0.00
23) Perylene-d12	23.261	264	6205	0.40	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.920	96	8210	1.87	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.936	152	3150	0.20	ng/ul	0.00
18) Fluoranthene-d10	18.973	212	5097	0.25	ng/ul	0.00
Target Compounds						
						Qvalue
15) Phenanthrene	16.988	178	757	0.02	ng/ul#	76
19) Fluoranthene	19.000	202	985	0.03	ng/ul#	77
20) Pyrene	19.366	202	950	0.03	ng/ul#	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101821\
Data File : BM032567.D
Acq On : 18 Oct 2021 11:17
Operator : CG/JU
Sample : M4029-20
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C00T1


Quant Time: Oct 18 11:53:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 18 10:38:29 2021
Response via : Initial Calibration

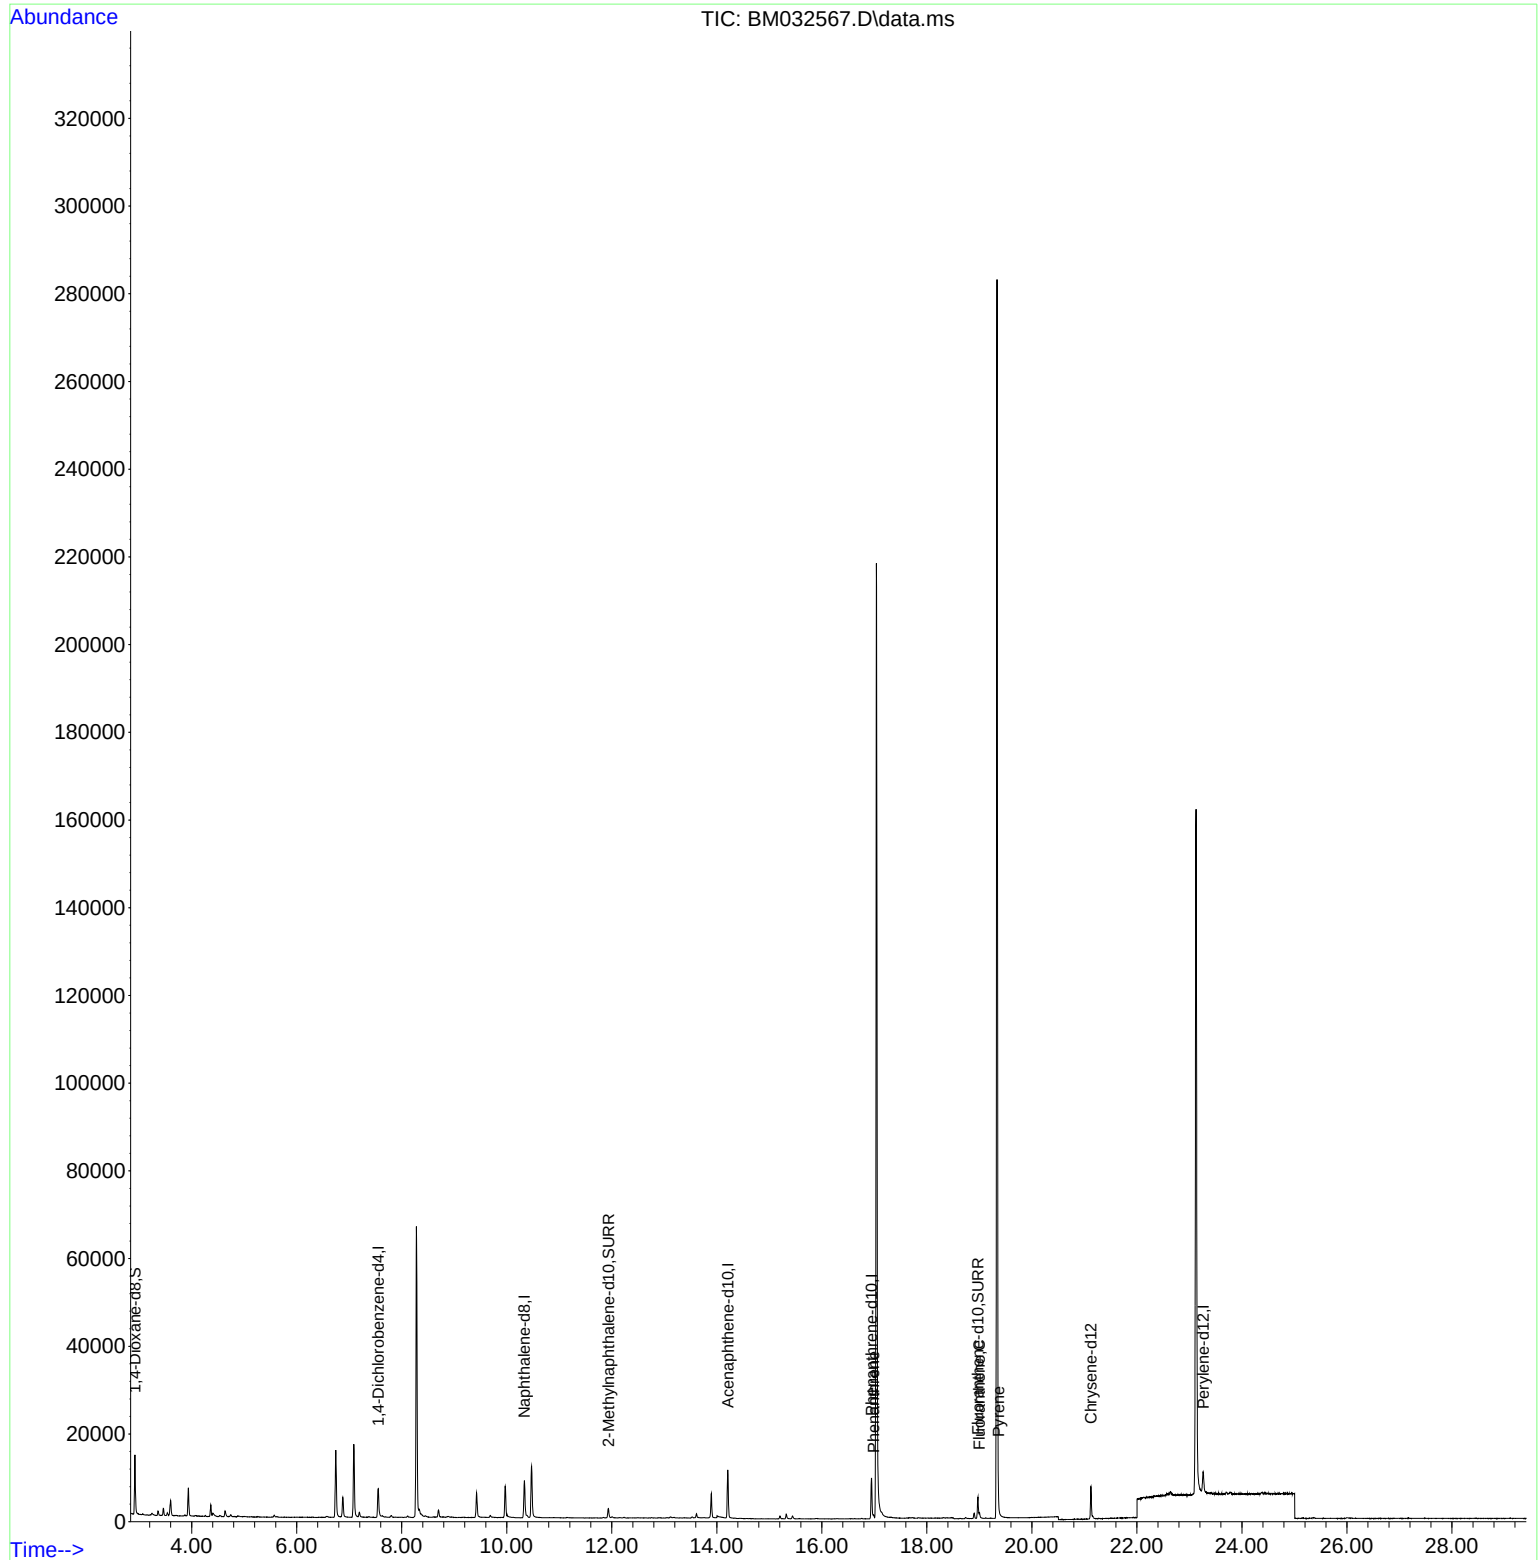



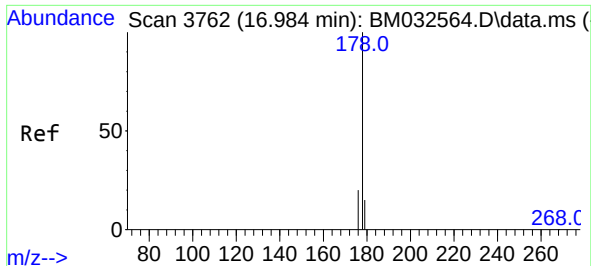


#15
Phenanthrene
Concen: 0.02 ng/ul
RT: 16.988 min Scan# 3763
Delta R.T. 0.003 min
Lab File: BM032567.D
Acq: 18 Oct 2021 11:17

Instrument :
BNA_M
ClientSampled :
C00T1



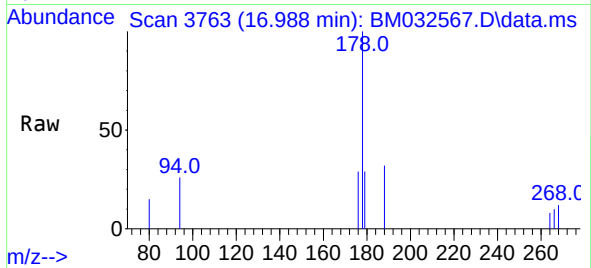



Tgt Ion:178 Resp: 757
Ion Ratio Lower Upper
178 100
179 28.9 12.9 19.3#
176 28.9 16.1 24.1#

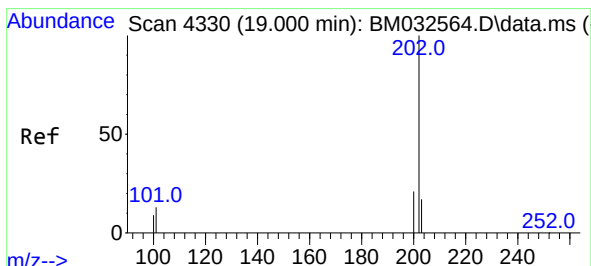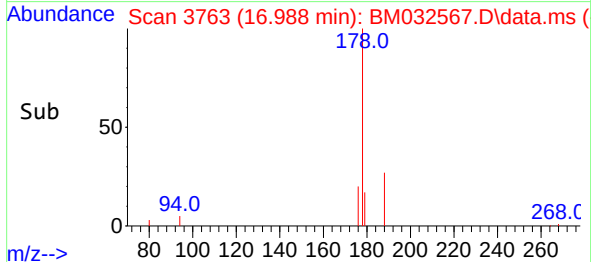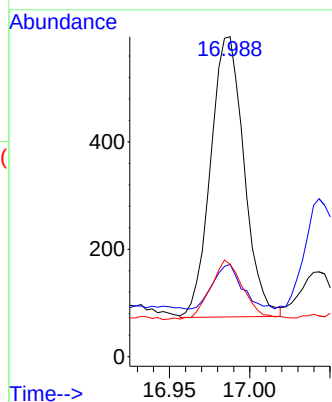

#19
Fluoranthene
Concen: 0.03 ng/ul
RT: 19.000 min Scan# 4330
Delta R.T. -0.000 min
Lab File: BM032567.D
Acq: 18 Oct 2021 11:17


Tgt Ion:202 Resp: 985
Ion Ratio Lower Upper
202 100
101 22.3 10.6 16.0#
100 18.6 7.8 11.8#

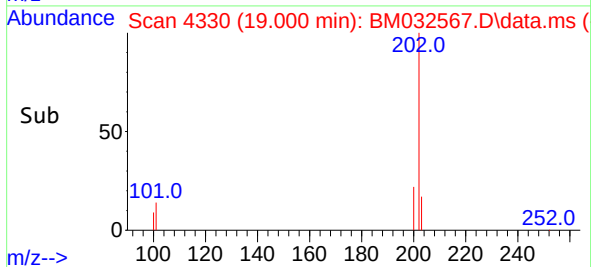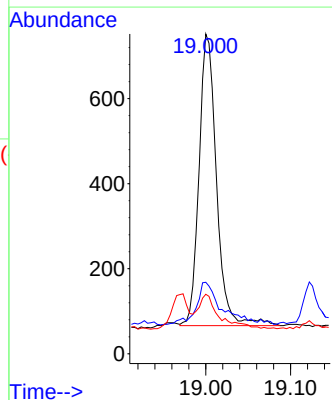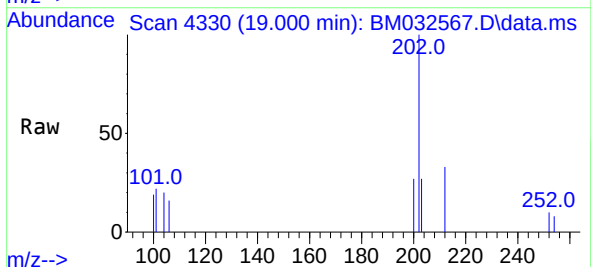

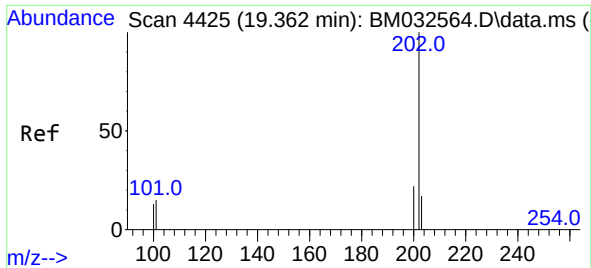

#20
Pyrene
Concen: 0.03 ng/ul
RT: 19.366 min Scan# 4426
Delta R.T. 0.004 min
Lab File: BM032567.D
Acq: 18 Oct 2021 11:17

Instrument :
BNA_M
ClientSampleId :
C00T1

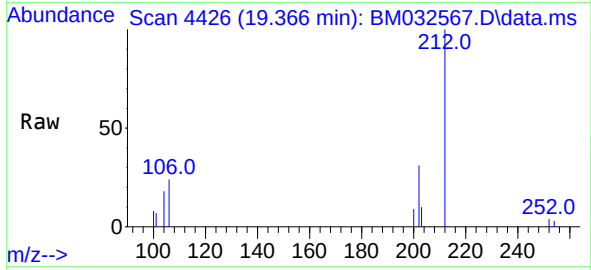

Tgt Ion:202 Resp: 950
Ion Ratio Lower Upper
202 100
101 22.9 12.3 18.5#
100 24.5 10.1 15.1#

