

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM101916\
 Data File : BM007691.D
 Acq On : 20 Oct 2016 03:39
 Operator : UM/SJ
 Sample : MDL-01-W
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MDL-01-W

Quant Time: Oct 20 07:04:59 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM101916-MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 20 03:26:07 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	232714	20.00	ng/ul	0.00
7) Naphthalene-d8	10.53	136	896151	20.00	ng/ul	0.00
13) Acenaphthene-d10	14.39	164	571859	20.00	ng/ul	0.00
18) Phenanthrene-d10	17.13	188	1110166	20.00	ng/ul	0.00
23) Chrysene-d12	21.31	240	1390965	20.00	ng/ul	0.00
25) Perylene-d12	23.57	264	1425188	20.00	ng/ul	0.00

System Monitoring Compounds

2) 1,4-Dioxane-d8	3.29	96	40474	7.42	ng/uL	0.00
3) Phenol-d5	6.93	99	596006	33.05	ng/ul	0.00
4) Bis-(2-Chloroethyl)ether-d	7.09	67	360347	33.72	ng/ul	0.00
5) 2-Chlorophenol-d4	7.29	132	474729	34.30	ng/ul	0.00
6) 4-Methylphenol-d8	8.46	113	464160	32.76	ng/ul	0.00
8) Nitrobenzene-d5	8.91	128	221705	35.02	ng/ul	0.00
9) 2-Nitrophenol-d4	9.63	143	242782	35.14	ng/ul	0.00
10) 2,4-Dichlorophenol-d3	10.16	165	439335	32.31	ng/ul	0.00
11) 4-Chloroaniline-d4	10.67	131	552473	35.81	ng/ul	0.00
14) Dimethylphthalate-d6	13.80	166	1299610	32.58	ng/ul	0.00
15) Acenaphthylene-d8	14.08	160	1584061	33.87	ng/ul	0.00
16) 4-Nitrophenol-d4	14.60	143	187628	28.60	ng/ul	0.00
17) Fluorene-d10	15.38	176	1133079	32.91	ng/ul	0.00
19) 4,6-Dinitro-2-methylphenol	15.51	200	197155	29.31	ng/ul	0.00
20) Anthracene-d10	17.23	188	1683126	33.35	ng/ul	0.00
24) Pyrene-d10	19.53	212	1953579	34.69	ng/ul	0.00
26) Benzo(a)pyrene-d12	23.43	264	2079559	33.50	ng/ul	0.00

Target Compounds


						Qvalue
12) 1-Methylnaphthalene	12.42	142	93476	3.03	ng/ul	96
21) 1,2,3,4-Tetrachlorobenzene	13.18	216	53855	3.33	ng/uL	93
22) Pentachlorobenzene	14.71	250	55612	3.29	ng/uL	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM101916\
Data File : BM007691.D
Acq On : 20 Oct 2016 03:39
Operator : UM/SJ
Sample : MDL-01-W
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MDL-01-W

Quant Time: Oct 20 07:04:59 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM101916-MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 20 03:26:07 2016
Response via : Initial Calibration

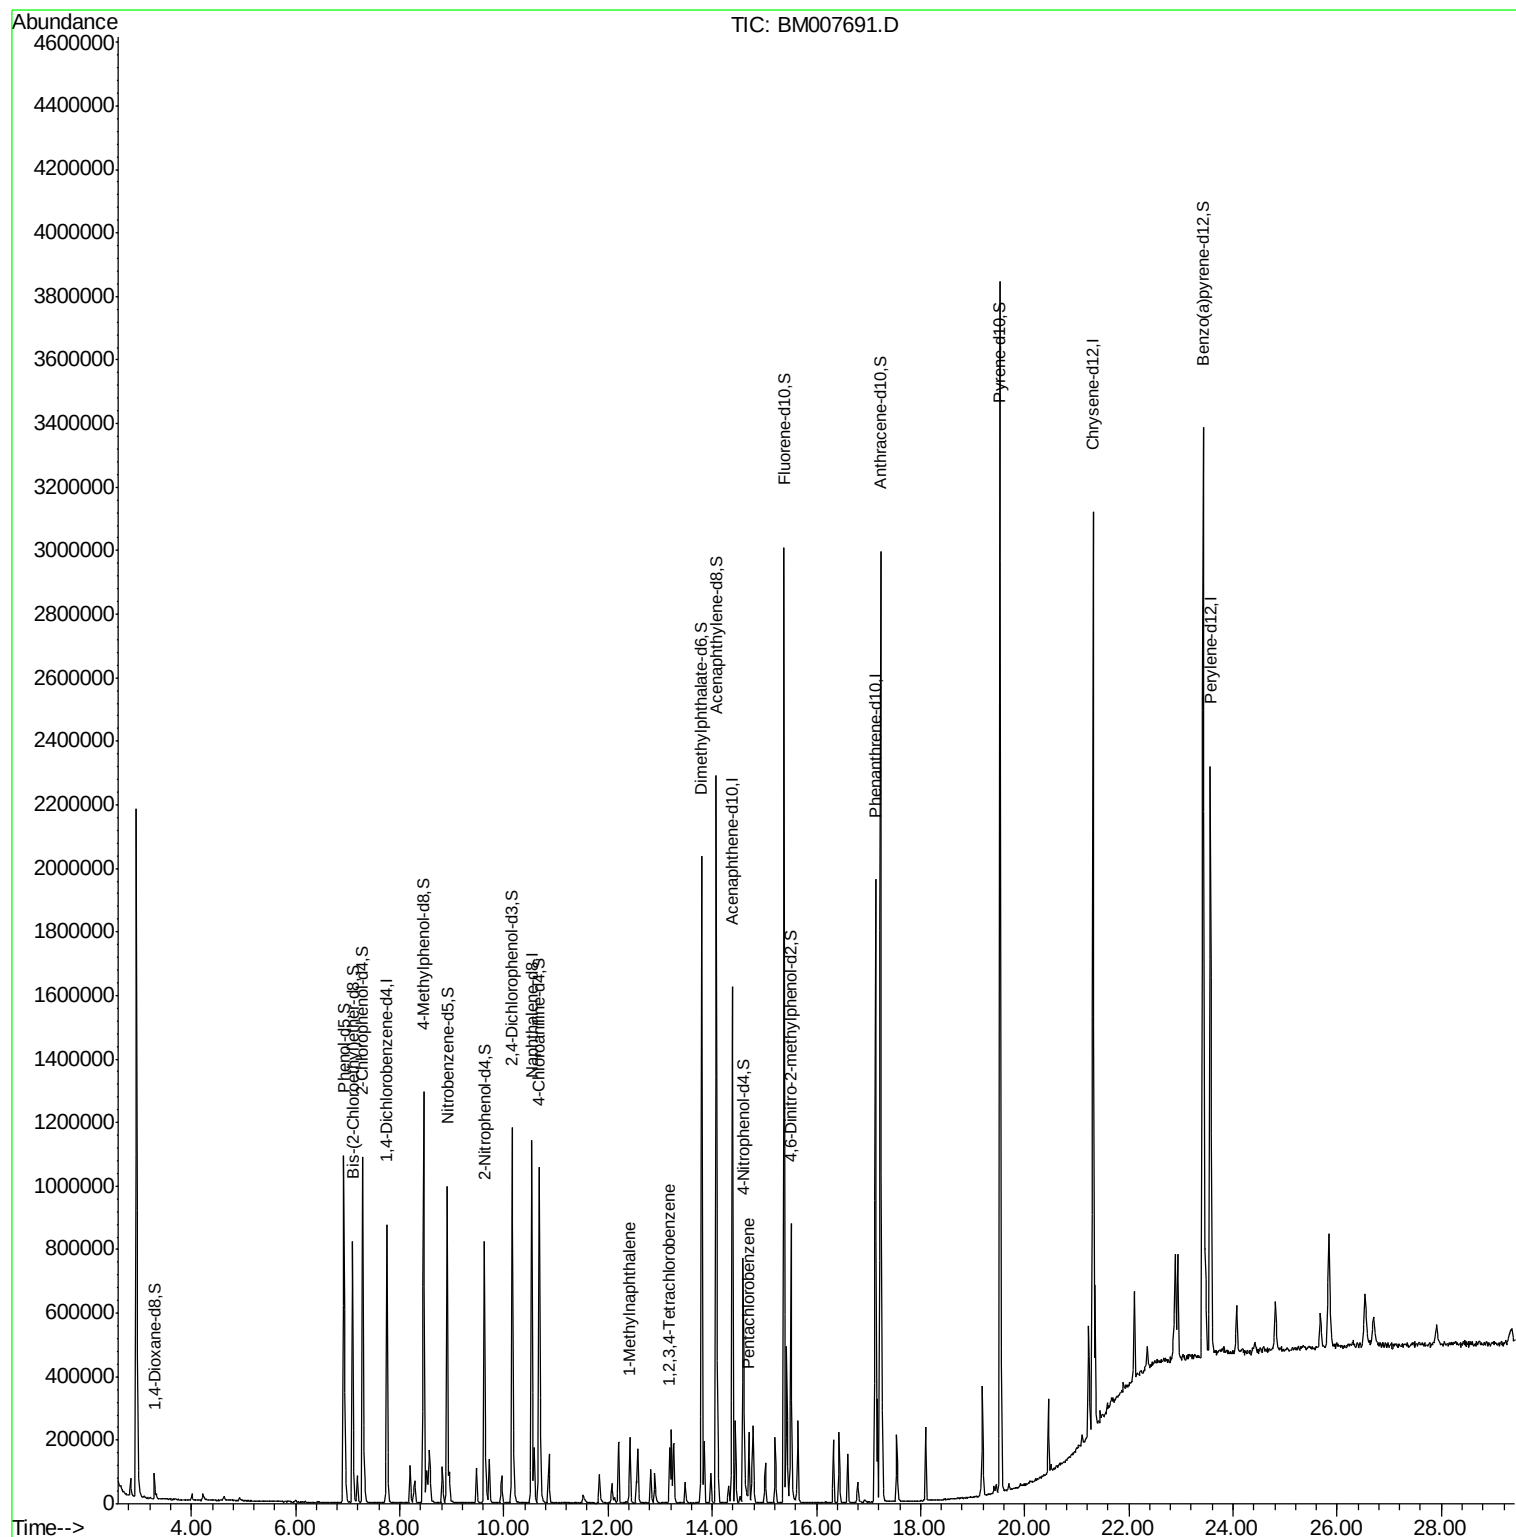

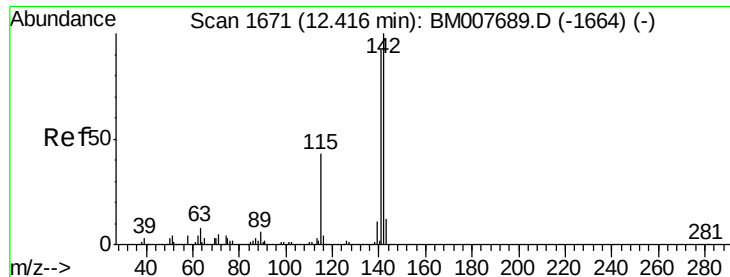

#12

1-Methylnaphthalene

Concen: 3.03 ng/uL

RT: 12.42 min Scan# 1672

Delta R.T. 0.01 min

Lab File: BM007691.D

Acq: 20 Oct 2016 03:39

Instrument :

BNA_M

ClientSampleId :

MDL-01-W


Tgt Ion:142 Resp: 93476

Ion Ratio Lower Upper

142 100

141 89.8 74.9 112.3




116 3.9 3.1 4.7

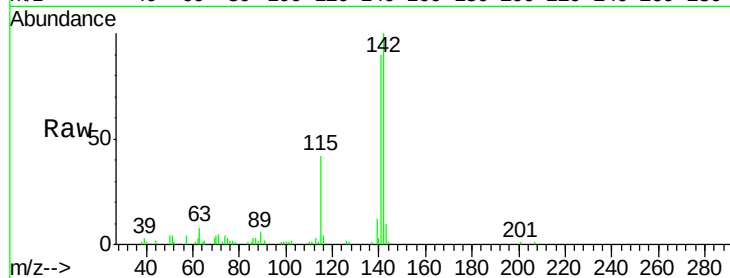

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 116.00 (115.70 to 116.70): E

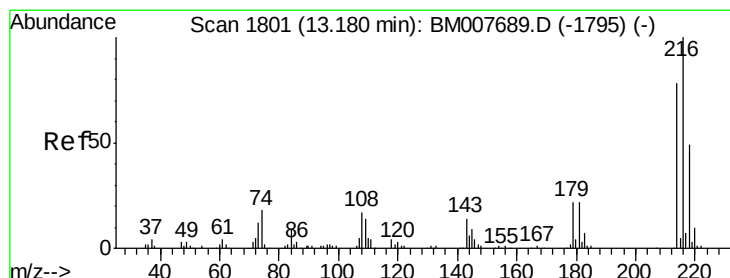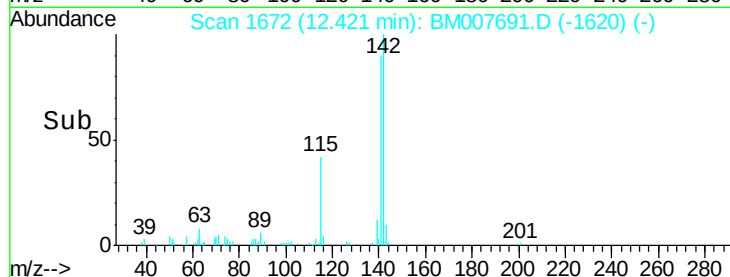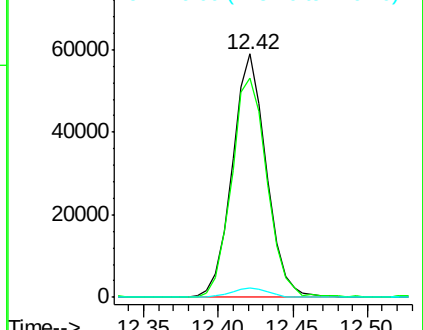

#21

1,2,3,4-Tetrachlorobenzene

Concen: 3.33 ng/uL

RT: 13.18 min Scan# 1801

Delta R.T. -0.00 min

Lab File: BM007691.D

Acq: 20 Oct 2016 03:39


Tgt Ion:216 Resp: 53855

Ion Ratio Lower Upper

216 100

214 70.6 62.5 93.7



218 45.7 38.4 57.6

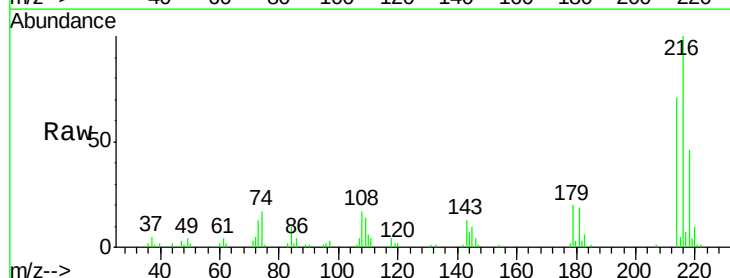


Abundance Ion 216.00 (215.70 to 216.70): E

Ion 214.00 (213.70 to 214.70): E

Ion 218.00 (217.70 to 218.70): E

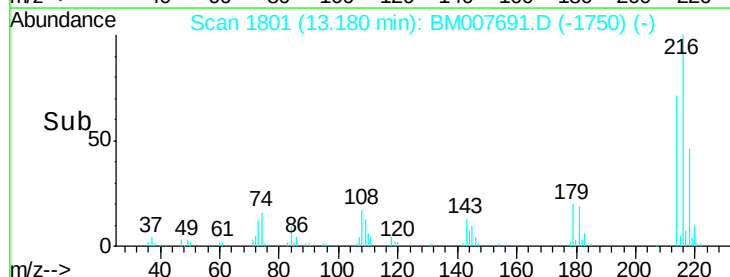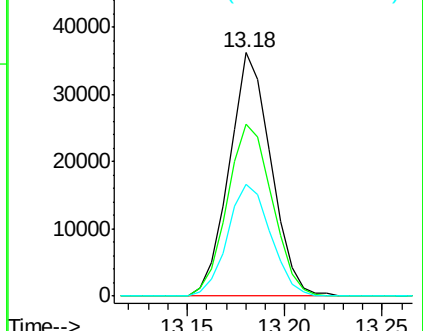

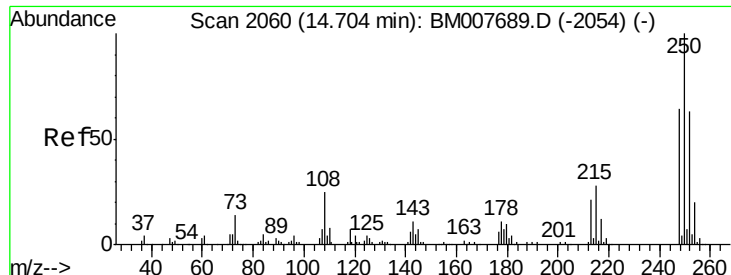

#22

Pentachlorobenzene

Concen: 3.29 ng/uL

RT: 14.71 min Scan# 2061

Delta R.T. 0.01 min

Lab File: BM007691.D


Acq: 20 Oct 2016 03:39

Instrument :

BNA_M

ClientSampleId :

MDL-01-W

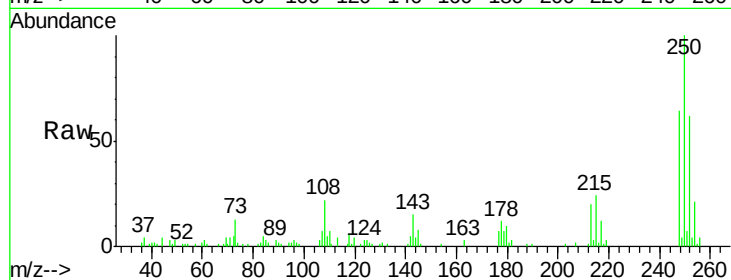


Tgt Ion:250 Resp: 55612

Ion Ratio Lower Upper

250 100

248 64.2 50.6 75.8

252 62.2 51.4 77.0

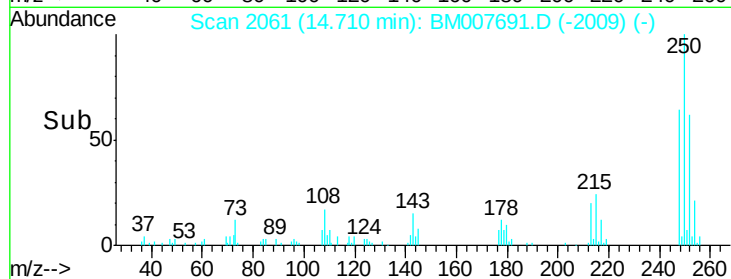

Abundance Ion 250.00 (249.70 to 250.70): E

Ion 248.00 (247.70 to 248.70): E

Ion 252.00 (251.70 to 252.70): E

