



Data Path : Z:\HPCHEM1\BNA_M\DATA\BM101916\
Data File : BM007693.D
Acq On : 20 Oct 2016 04:49
Operator : UM/SJ
Sample : MDL-03-W
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleID :
MDL-03-W

Quant Time: Oct 20 07:05:19 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM101916-MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 20 03:26:07 2016
Response via : Initial Calibration

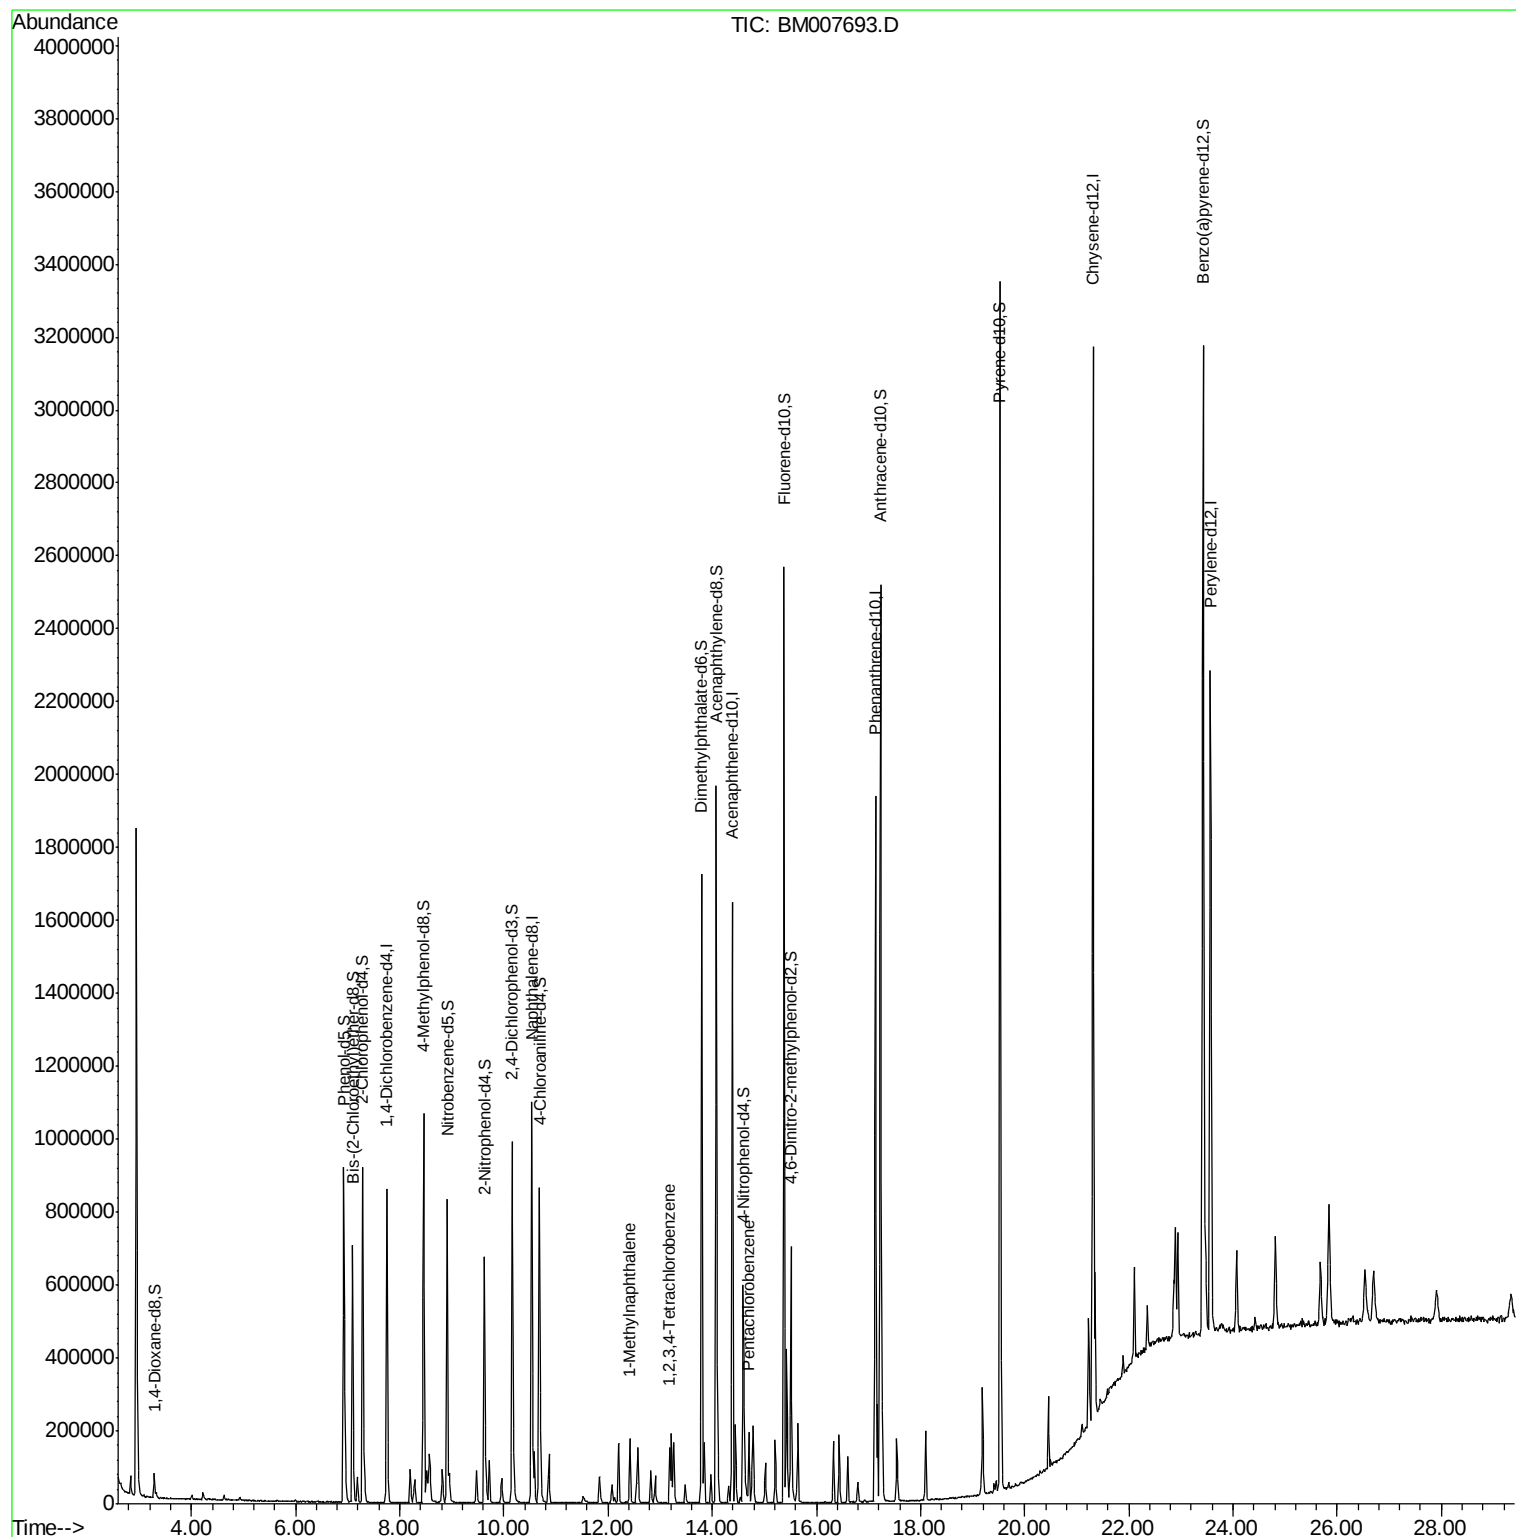

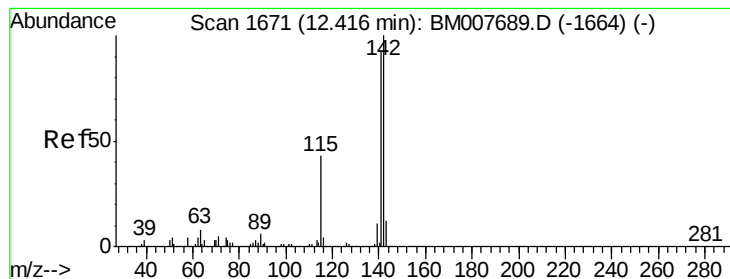

#12

1-Methylnaphthalene

Concen: 2.60 ng/uL

RT: 12.42 min Scan# 1672

Delta R.T. 0.01 min

Lab File: BM007693.D

Acq: 20 Oct 2016 04:49

Instrument :

BNA_M

ClientSampleId :

MDL-03-W


Tgt Ion:142 Resp: 79270

Ion Ratio Lower Upper

142 100

141 103.3 74.9 112.3




116 3.9 3.1 4.7

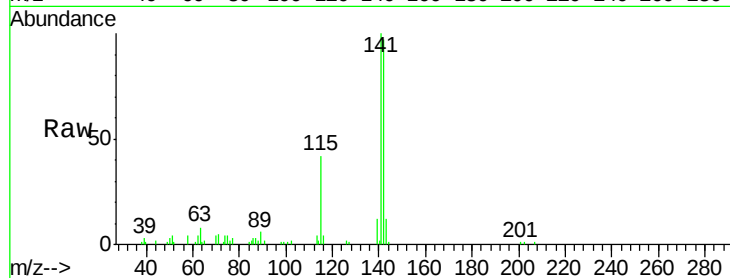

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 116.00 (115.70 to 116.70): E

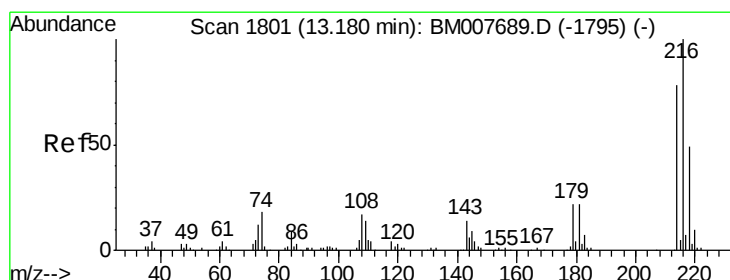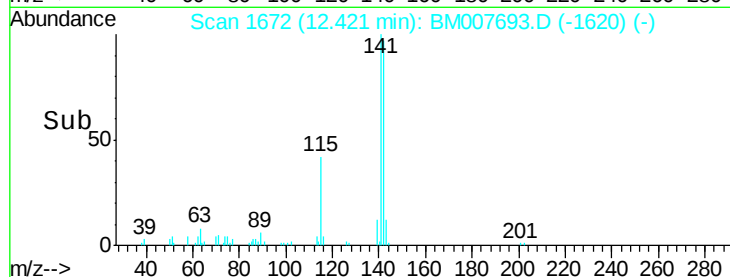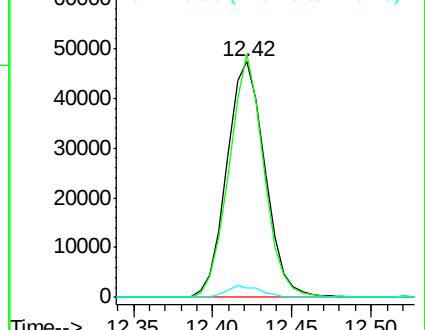

#21

1,2,3,4-Tetrachlorobenzene

Concen: 2.81 ng/uL

RT: 13.18 min Scan# 1801

Delta R.T. -0.00 min

Lab File: BM007693.D

Acq: 20 Oct 2016 04:49


Tgt Ion:216 Resp: 45533

Ion Ratio Lower Upper

216 100

214 81.6 62.5 93.7



218 46.8 38.4 57.6

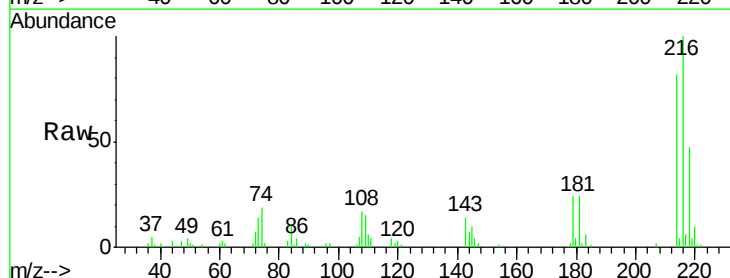


Abundance Ion 216.00 (215.70 to 216.70): E

Ion 214.00 (213.70 to 214.70): E

Ion 218.00 (217.70 to 218.70): E

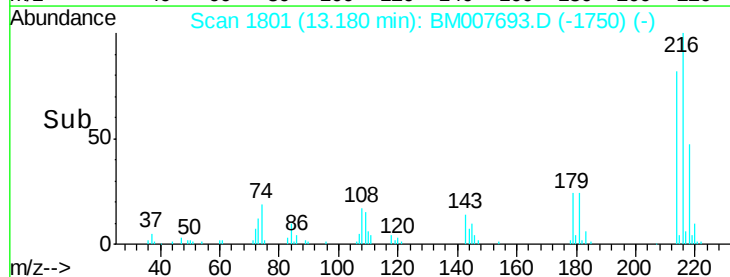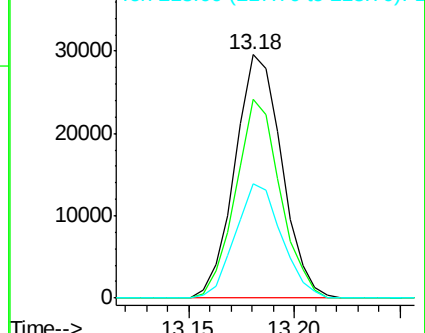


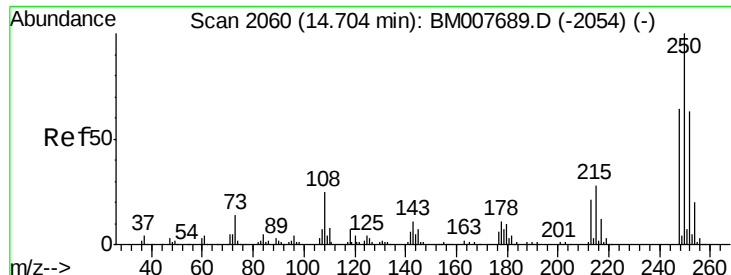



#22
 Pentachlorobenzene
 Concen: 2.76 ng/uL
 RT: 14.71 min Scan# 2061
 Delta R.T. 0.01 min
 Lab File: BM007693.D
 Acq: 20 Oct 2016 04:49

Instrument :
 BNA_M
 ClientSampleId :
 MDL-03-W

Tgt Ion	Ratio	Lower	Upper
250	100		
248	63.6	50.6	75.8
252	67.5	51.4	77.0

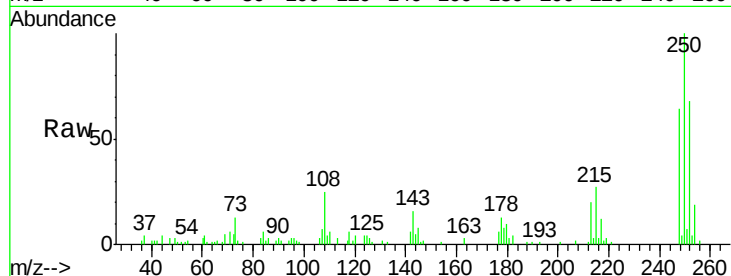

Abundance Ion 250.00 (249.70 to 250.70): E
 Ion 248.00 (247.70 to 248.70): E
 Ion 252.00 (251.70 to 252.70): E

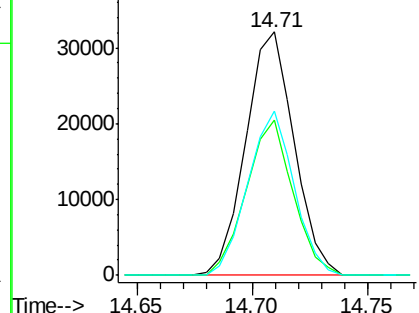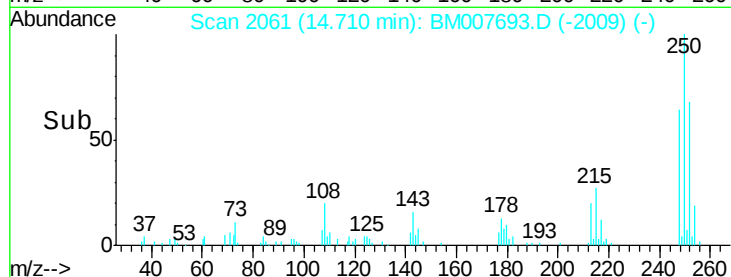

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM101916\
 Data File : BM007693.D
 Acq On : 20 Oct 2016 04:49
 Operator : UM/SJ
 Sample : MDL-03-W
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MDL-03-W

Quant Time: Oct 20 07:05:19 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM101916-MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 20 03:26:07 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	235130	20.00	ng/ul	0.00
7) Naphthalene-d8	10.53	136	887288	20.00	ng/ul	0.00
13) Acenaphthene-d10	14.39	164	563634	20.00	ng/ul	0.00
18) Phenanthrene-d10	17.13	188	1114170	20.00	ng/ul	0.00
23) Chrysene-d12	21.32	240	1412459	20.00	ng/ul	0.00
25) Perylene-d12	23.57	264	1447413	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
2) 1,4-Dioxane-d8	3.29	96	34272	6.22	ng/uL	0.00
3) Phenol-d5	6.93	99	497037	27.28	ng/ul	0.00
4) Bis-(2-Chloroethyl)ether-d	7.09	67	305563	28.30	ng/ul	0.00
5) 2-Chlorophenol-d4	7.29	132	401183	28.68	ng/ul	0.00
6) 4-Methylphenol-d8	8.46	113	387563	27.07	ng/ul	0.00
8) Nitrobenzene-d5	8.91	128	186216	29.71	ng/ul	0.00
9) 2-Nitrophenol-d4	9.63	143	202464	29.60	ng/ul	0.00
10) 2,4-Dichlorophenol-d3	10.16	165	375154	27.87	ng/ul	0.00
11) 4-Chloroaniline-d4	10.68	131	467837	30.63	ng/ul	0.00
14) Dimethylphthalate-d6	13.80	166	1109368	28.21	ng/ul	0.00
15) Acenaphthylene-d8	14.08	160	1327336	28.80	ng/ul	0.00
16) 4-Nitrophenol-d4	14.60	143	155674	24.08	ng/ul	0.00
17) Fluorene-d10	15.38	176	952179	28.06	ng/ul	0.00
19) 4,6-Dinitro-2-methylphenol	15.51	200	164264	24.33	ng/ul	0.00
20) Anthracene-d10	17.23	188	1438674	28.40	ng/ul	0.00
24) Pyrene-d10	19.53	212	1679027	29.37	ng/ul	0.00
26) Benzo(a)pyrene-d12	23.43	264	1821932	28.90	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
12) 1-Methylnaphthalene	12.42	142	79270	2.60	ng/ul	90
21) 1,2,3,4-Tetrachlorobenzene	13.18	216	45533	2.81	ng/uL	97
22) Pentachlorobenzene	14.71	250	46884	2.76	ng/uL	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed