

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101921\
 Data File : BM032602.D
 Acq On : 20 Oct 2021 02:36
 Operator : CG/JU
 Sample : M4204-07
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JDGH9

Quant Time: Oct 20 04:04:21 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 19 15:20:30 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.560	152	5161	0.40	ng/ul	0.00
4) Naphthalene-d8	10.344	136	15728	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.213	164	7876	0.40	ng/ul	0.00
13) Phenanthrene-d10	16.946	188	14727	0.40	ng/ul	# 0.00
17) Chrysene-d12	21.121	240	9709	0.40	ng/ul	# 0.00
23) Perylene-d12	23.259	264	10119	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.923	96	27002	4.67	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.940	152	6433	0.31	ng/ul	0.00
18) Fluoranthene-d10	18.973	212	14329	0.47	ng/ul	0.00
Target Compounds						
15) Phenanthrene	16.988	178	2461	0.05	ng/ul#	Qvalue 11


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101921\
Data File : BM032602.D
Acq On : 20 Oct 2021 02:36
Operator : CG/JU
Sample : M4204-07
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JDGH9


Quant Time: Oct 20 04:04:21 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 19 15:20:30 2021
Response via : Initial Calibration

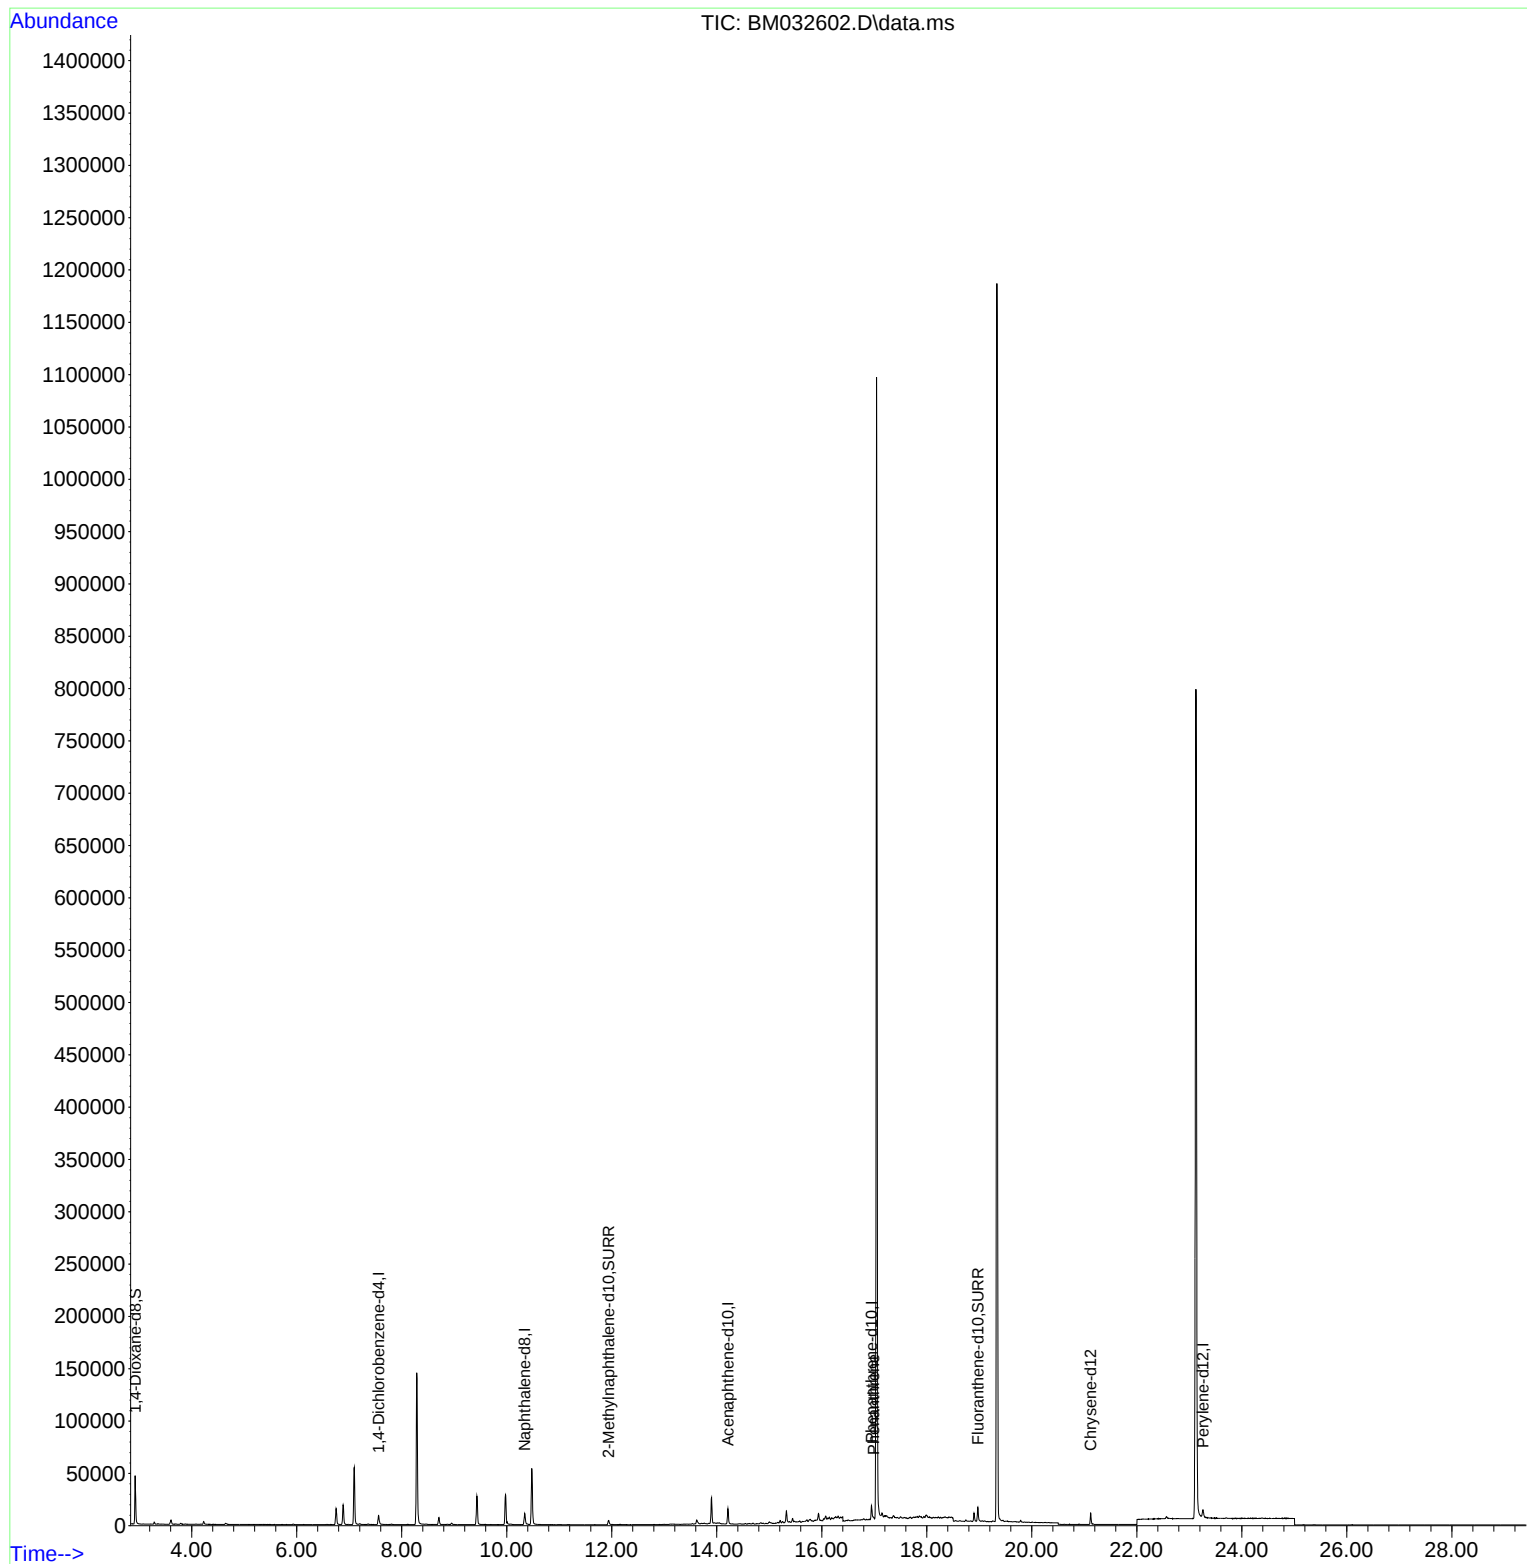

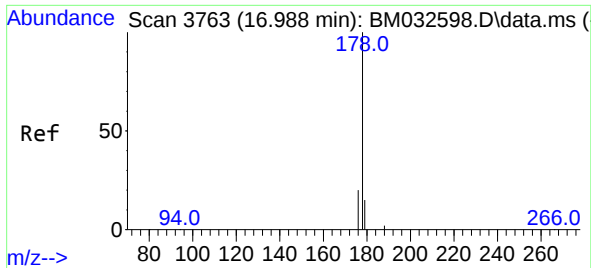

#15
Phenanthrene
Concen: 0.05 ng/u1
RT: 16.988 min Scan# 3763
Delta R.T. 0.000 min
Lab File: BM032602.D
Acq: 20 Oct 2021 02:36

Instrument :
BNA_M
ClientSampleId :
JDGH9

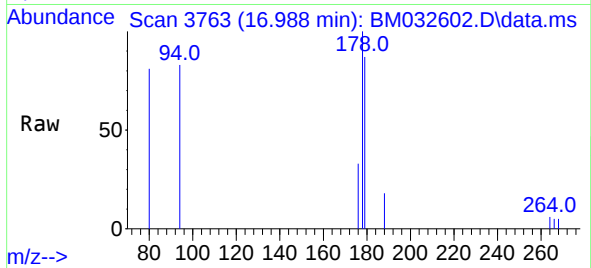

Tgt Ion:178 Resp: 2461
Ion Ratio Lower Upper
178 100
179 87.0 12.9 19.3#
176 32.8 16.1 24.1#

