

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101921\
 Data File : BM032603.D
 Acq On : 20 Oct 2021 03:12
 Operator : CG/JU
 Sample : M4204-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 J0AA3

Quant Time: Oct 20 04:04:36 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 19 15:20:30 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.560	152	5254	0.40	ng/ul	0.00
4) Naphthalene-d8	10.343	136	16016	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.213	164	7974	0.40	ng/ul	0.00
13) Phenanthrene-d10	16.946	188	14709	0.40	ng/ul	0.00
17) Chrysene-d12	21.120	240	10003	0.40	ng/ul	0.00
23) Perylene-d12	23.259	264	11196	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.923	96	29125	4.95	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.940	152	6788	0.32	ng/ul	0.00
18) Fluoranthene-d10	18.973	212	14896	0.47	ng/ul	0.00
Target Compounds						
15) Phenanthrene	16.988	178	1879	0.04	ng/ul#	Qvalue 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101921\
Data File : BM032603.D
Acq On : 20 Oct 2021 03:12
Operator : CG/JU
Sample : M4204-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
J0AA3


Quant Time: Oct 20 04:04:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 19 15:20:30 2021
Response via : Initial Calibration

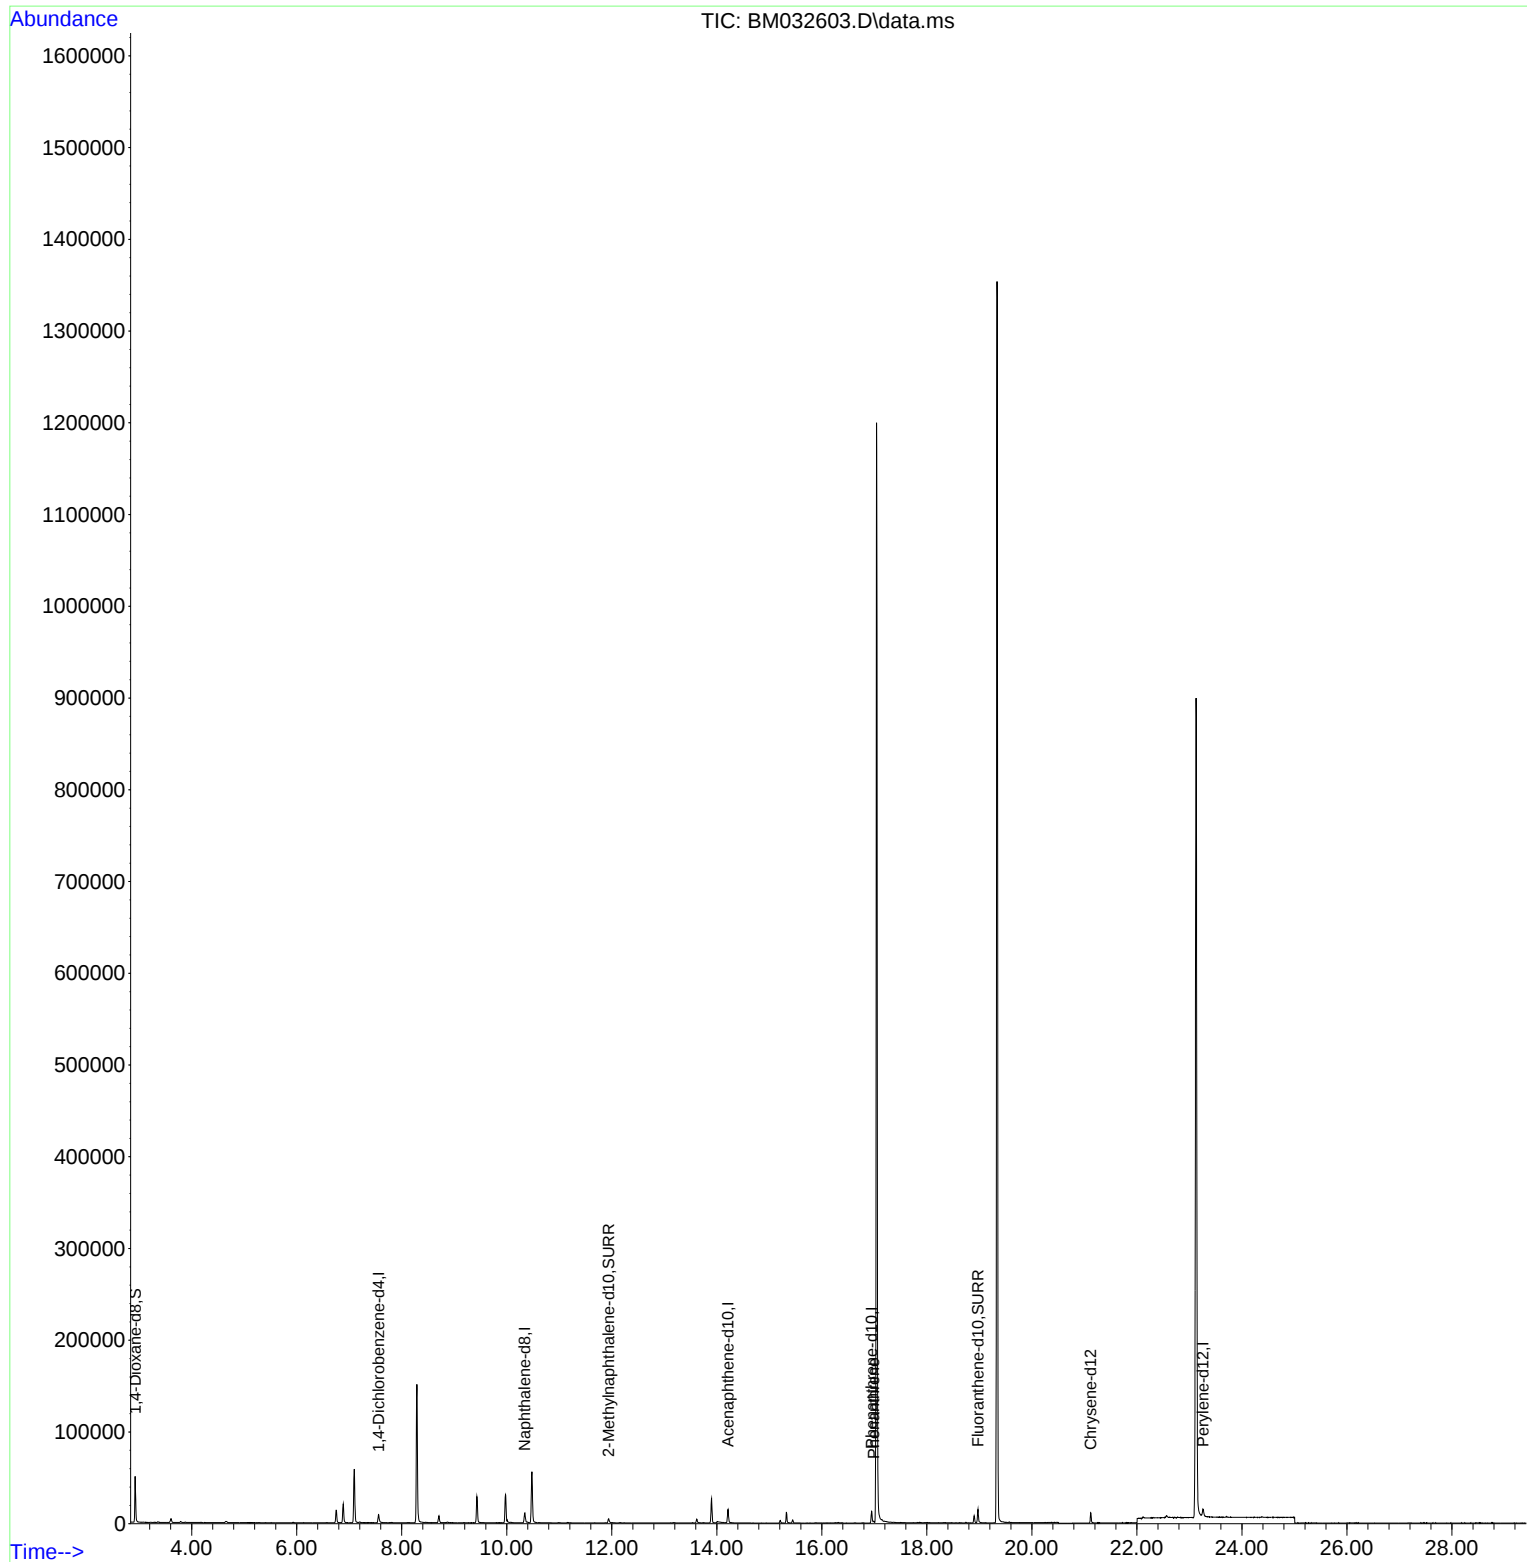

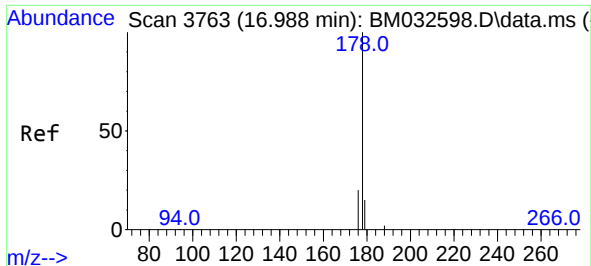

#15
Phenanthrene
Concen: 0.04 ng/ul
RT: 16.988 min Scan# 3763
Delta R.T. -0.000 min
Lab File: BM032603.D
Acq: 20 Oct 2021 03:12

Instrument :
BNA_M
ClientSampleId :
J0AA3

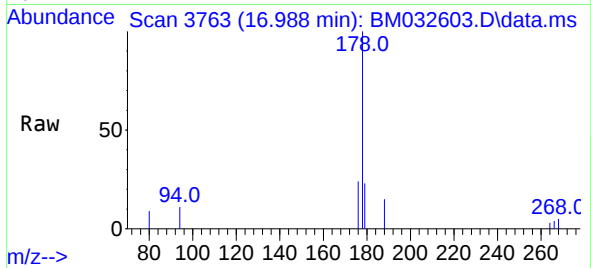

Tgt Ion:178 Resp: 1879
Ion Ratio Lower Upper
178 100
179 23.1 12.9 19.3#
176 23.7 16.1 24.1

