

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101921\
 Data File : BM032604.D
 Acq On : 20 Oct 2021 03:48
 Operator : CG/JU
 Sample : M4204-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JDGH2

Quant Time: Oct 20 04:44:57 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 19 15:20:30 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.560	152	5320	0.40	ng/ul	0.00
4) Naphthalene-d8	10.343	136	16240	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.213	164	8012	0.40	ng/ul	0.00
13) Phenanthrene-d10	16.949	188	13979	0.40	ng/ul	# 0.00
17) Chrysene-d12	21.121	240	9218	0.40	ng/ul	0.00
23) Perylene-d12	23.259	264	10277	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.923	96	28264	4.74	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.940	152	6892	0.32	ng/ul	0.00
18) Fluoranthene-d10	18.973	212	12273	0.42	ng/ul	0.00
Target Compounds						
						Qvalue
22) Chrysene	21.157	228	801	0.02	ng/ul#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101921\
Data File : BM032604.D
Acq On : 20 Oct 2021 03:48
Operator : CG/JU
Sample : M4204-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JDGH2


Quant Time: Oct 20 04:44:57 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 19 15:20:30 2021
Response via : Initial Calibration

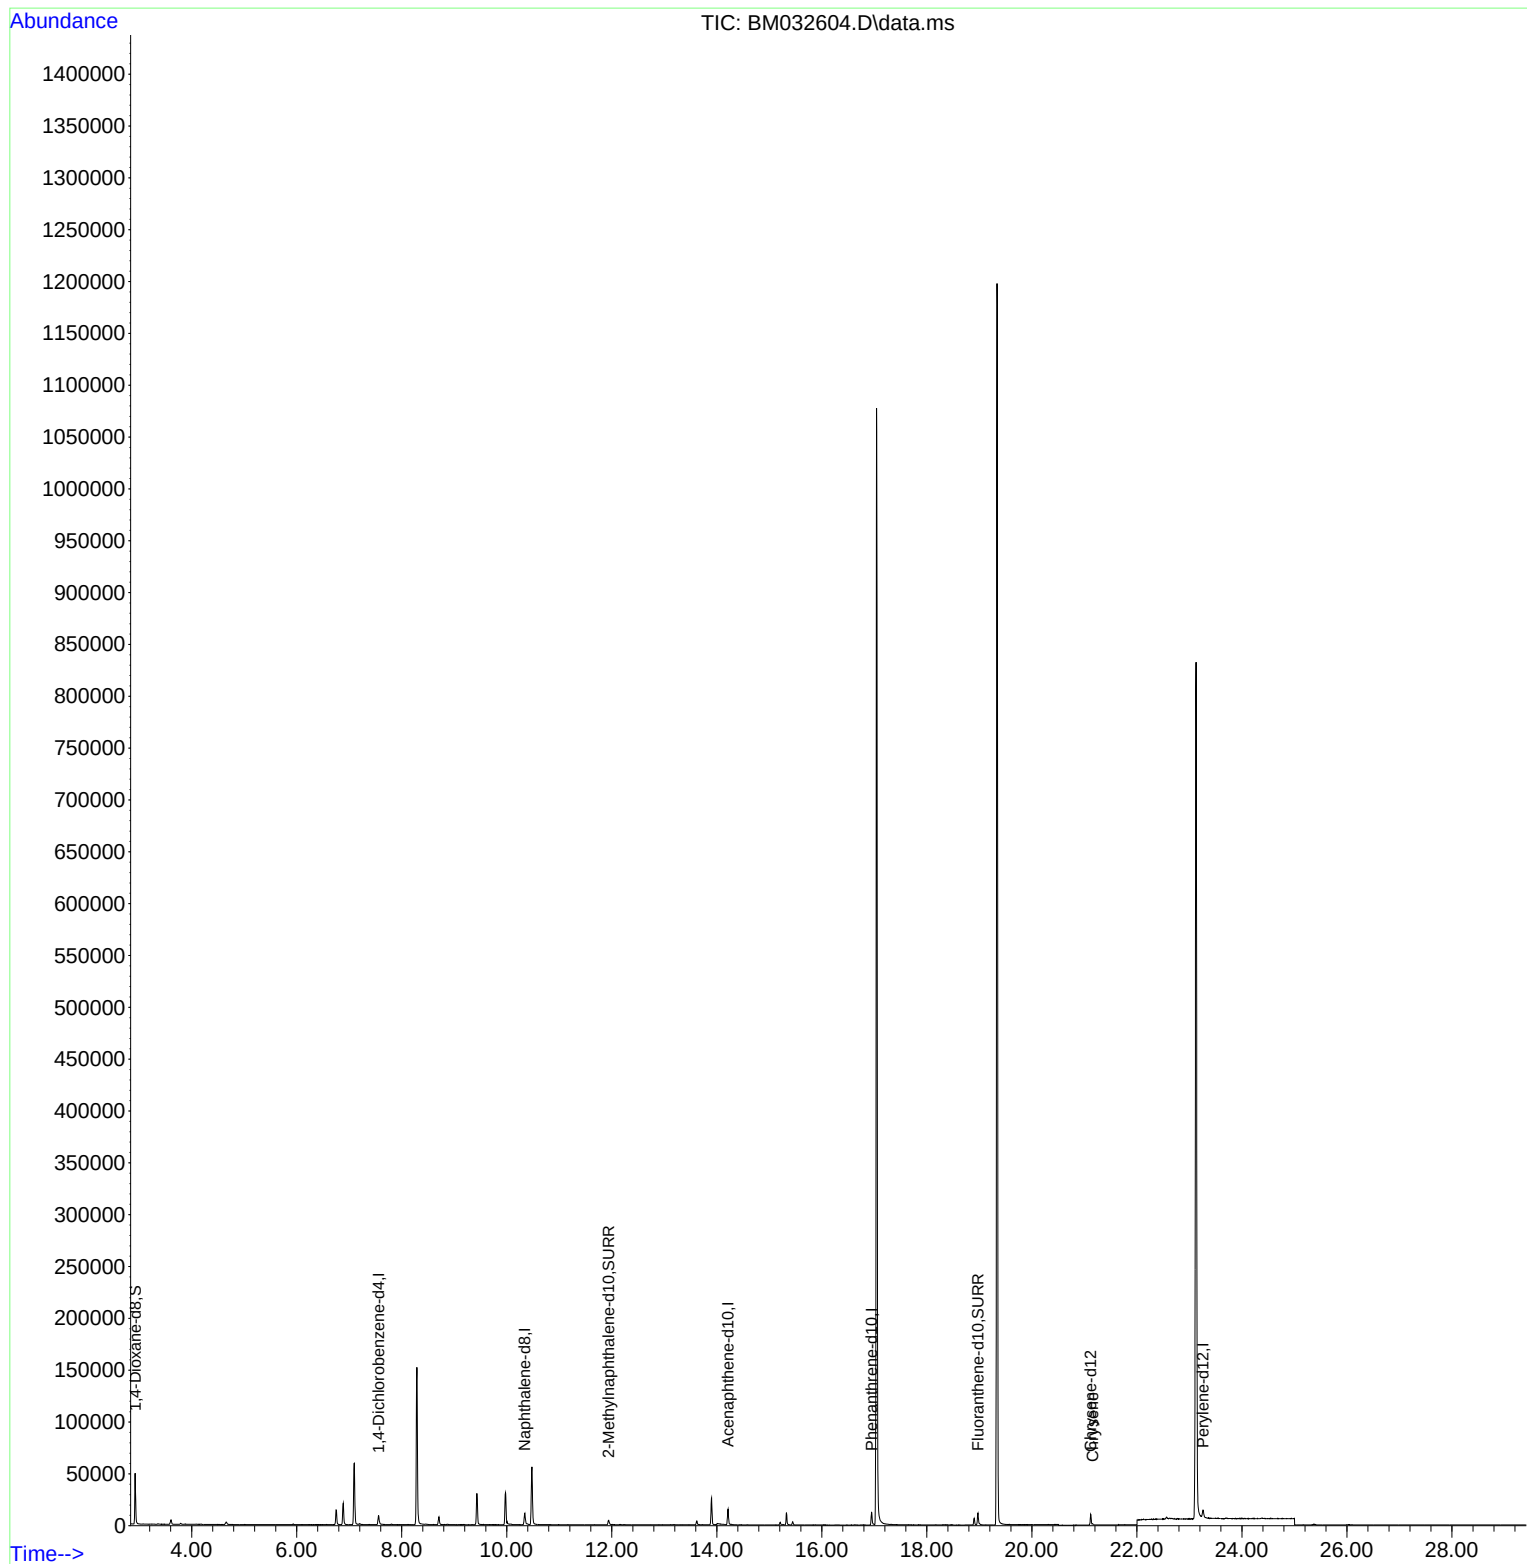

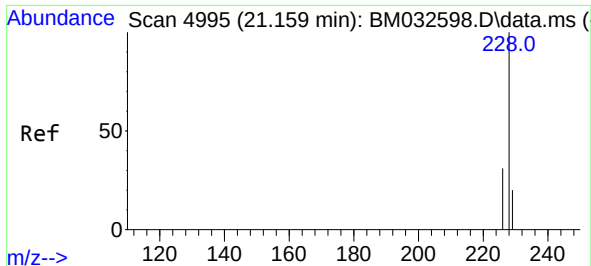

#22
Chrysene
Concen: 0.02 ng/u1
RT: 21.157 min Scan# 4994
Delta R.T. -0.002 min
Lab File: BM032604.D
Acq: 20 Oct 2021 03:48

Instrument :
BNA_M
ClientSampleId :
JDGH2

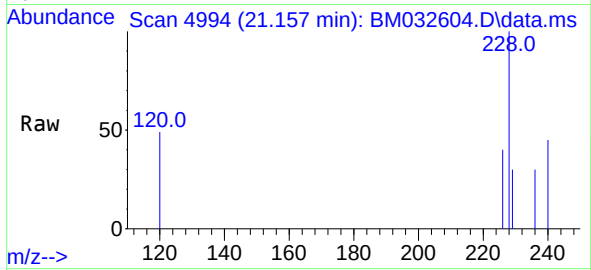

Tgt Ion:228 Resp: 801
Ion Ratio Lower Upper
228 100
226 39.6 25.1 37.7#
229 30.3 15.7 23.5#

