

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM101921\  
 Data File : BM032645.D  
 Acq On : 21 Oct 2021 07:34  
 Operator : CG/JU  
 Sample : M4196-16  
 Misc :  
 ALS Vial : 64 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 JDGD2

Quant Time: Oct 21 08:07:42 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-SIM-BM101421.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Oct 20 16:33:56 2021  
 Response via : Initial Calibration


| Compound                    | R.T.   | QIon | Response | Conc | Units  | Dev(Min) |
|-----------------------------|--------|------|----------|------|--------|----------|
| -----                       |        |      |          |      |        |          |
| Internal Standards          |        |      |          |      |        |          |
| 1) 1,4-Dichlorobenzene-d4   | 7.550  | 152  | 6420     | 0.40 | ng/ul  | 0.00     |
| 4) Naphthalene-d8           | 10.335 | 136  | 21078    | 0.40 | ng/ul  | 0.00     |
| 9) Acenaphthene-d10         | 14.209 | 164  | 10392    | 0.40 | ng/ul  | 0.00     |
| 13) Phenanthrene-d10        | 16.943 | 188  | 18692    | 0.40 | ng/ul  | # 0.00   |
| 17) Chrysene-d12            | 21.118 | 240  | 13163    | 0.40 | ng/ul  | 0.00     |
| 23) Perylene-d12            | 23.252 | 264  | 12793    | 0.40 | ng/ul  | 0.00     |
|                             |        |      |          |      |        |          |
| System Monitoring Compounds |        |      |          |      |        |          |
| 3) 1,4-Dioxane-d8           | 2.920  | 96   | 9315     | 1.29 | ng/ul  | 0.00     |
| 6) 2-Methylnaphthalene-d10  | 11.931 | 152  | 4140     | 0.15 | ng/ul  | 0.00     |
| 18) Fluoranthene-d10        | 18.966 | 212  | 6943     | 0.17 | ng/ul  | 0.00     |
|                             |        |      |          |      |        |          |
| Target Compounds            |        |      |          |      |        | Qvalue   |
| 5) Naphthalene              | 10.384 | 128  | 2124     | 0.03 | ng/ul# | 90       |
| -----                       |        |      |          |      |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM101921\  
Data File : BM032645.D  
Acq On : 21 Oct 2021 07:34  
Operator : CG/JU  
Sample : M4196-16  
Misc :  
ALS Vial : 64 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
JDGD2

Quant Time: Oct 21 08:07:42 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-SIM-BM101421.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Oct 20 16:33:56 2021  
Response via : Initial Calibration

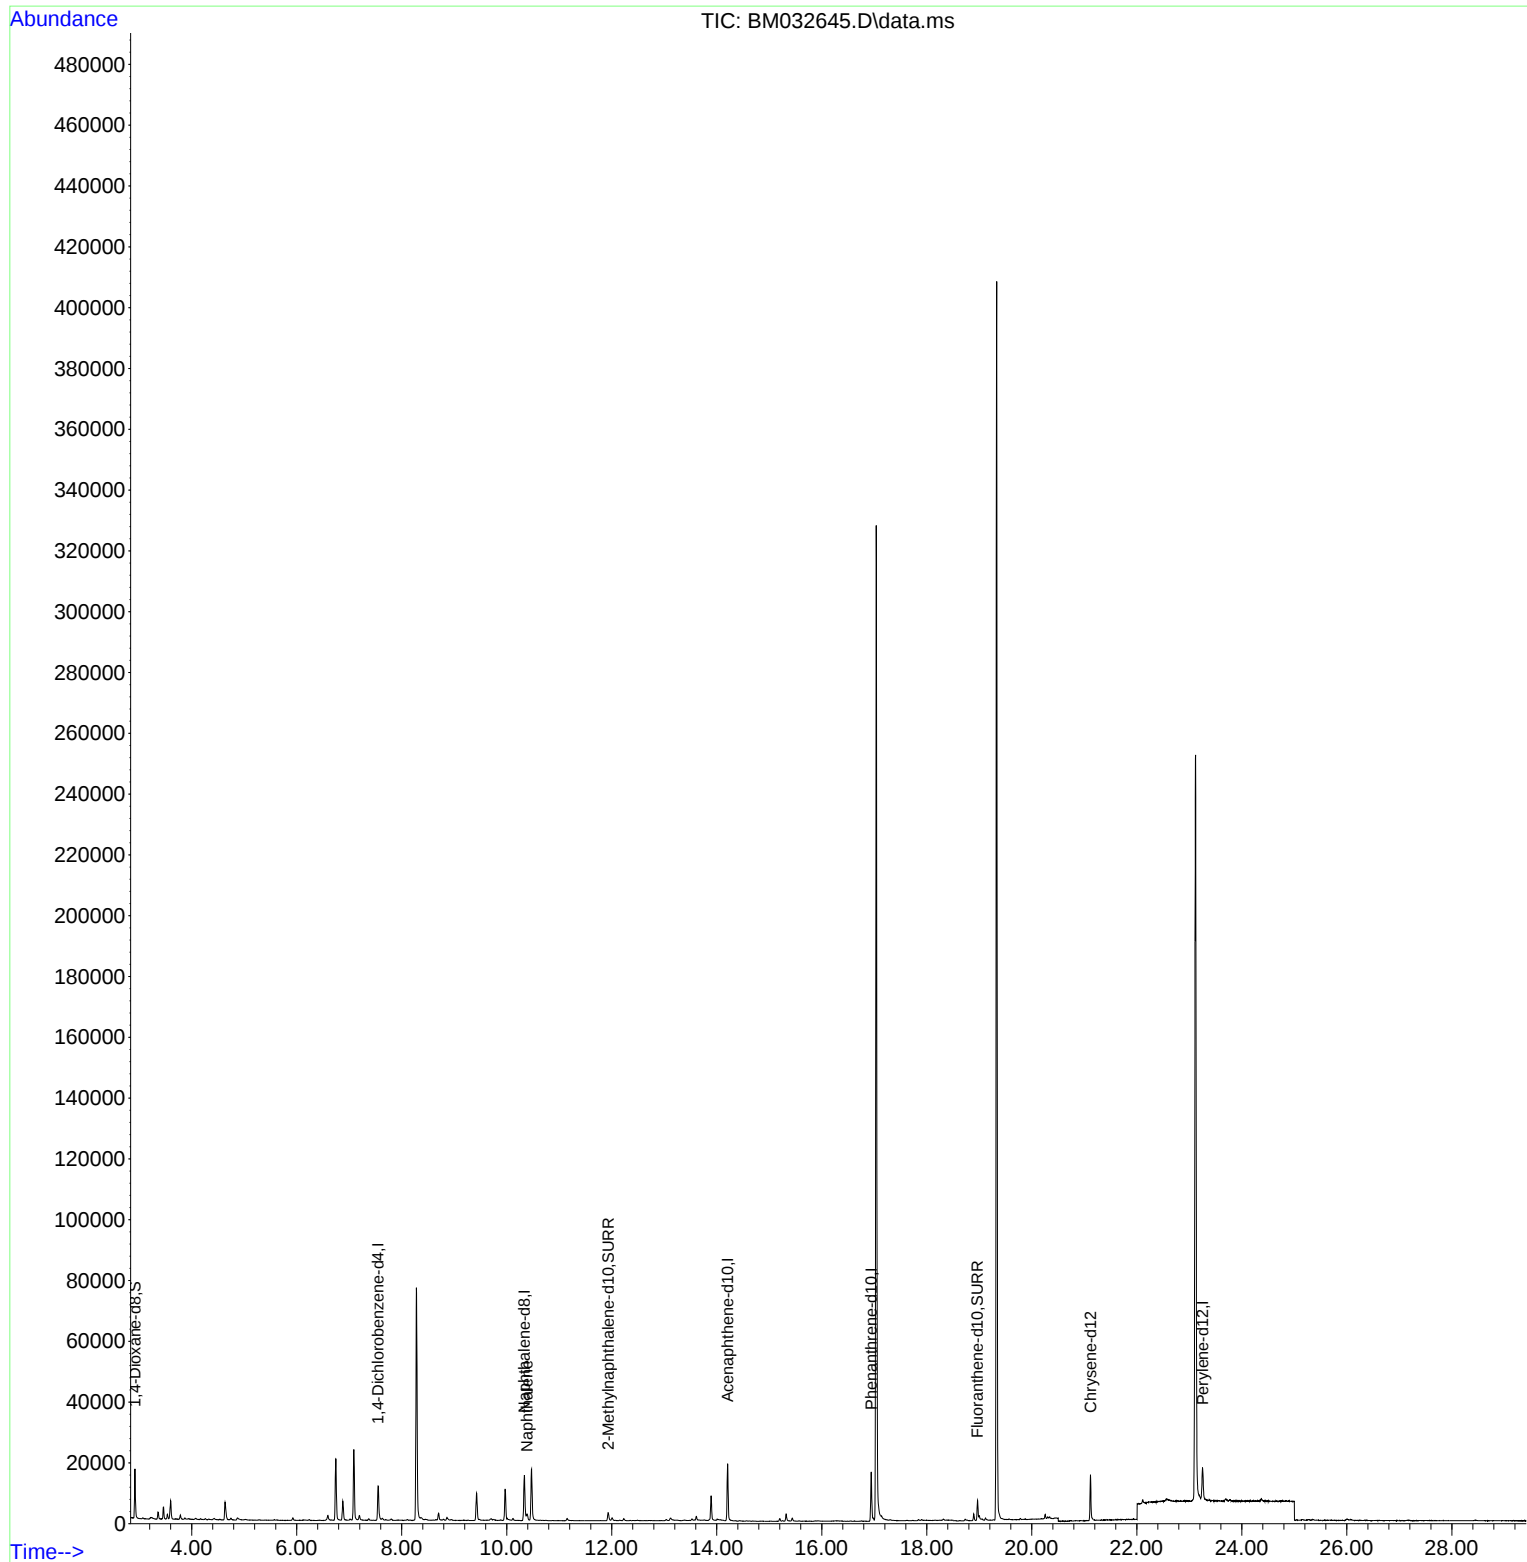

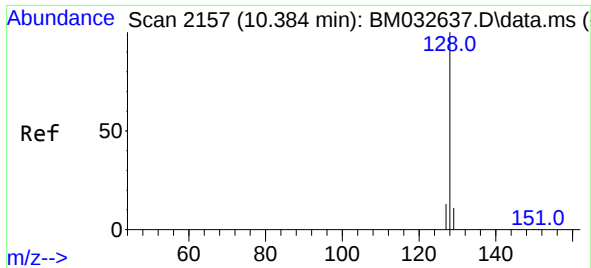

#5  
Naphthalene  
Concen: 0.03 ng/ul  
RT: 10.384 min Scan# 2157  
Delta R.T. -0.005 min  
Lab File: BM032645.D  
Acq: 21 Oct 2021 07:34

Instrument :  
BNA\_M  
ClientSampleId :  
JDGD2

Tgt Ion:128 Resp: 2124  
Ion Ratio Lower Upper  
128 100  
129 17.0 9.1 13.7#  
127 16.4 11.1 16.7

