

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101921\
 Data File : BM032652.D
 Acq On : 21 Oct 2021 11:47
 Operator : CG/JU
 Sample : M4196-15
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JDGD1

Quant Time: Oct 21 14:24:53 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 20 16:33:56 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.553	152	6199	0.40	ng/ul	0.00
4) Naphthalene-d8	10.335	136	20920	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.206	164	10261	0.40	ng/ul	0.00
13) Phenanthrene-d10	16.943	188	18069	0.40	ng/ul	# 0.00
17) Chrysene-d12	21.118	240	12594	0.40	ng/ul	0.00
23) Perylene-d12	23.254	264	12042	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.920	96	9550	1.37	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.931	152	4416	0.16	ng/ul	0.00
18) Fluoranthene-d10	18.966	212	7329	0.18	ng/ul	0.00
Target Compounds						
						Qvalue
5) Naphthalene	10.384	128	1285	0.02	ng/ul#	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101921\
Data File : BM032652.D
Acq On : 21 Oct 2021 11:47
Operator : CG/JU
Sample : M4196-15
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JDGD1


Quant Time: Oct 21 14:24:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 20 16:33:56 2021
Response via : Initial Calibration

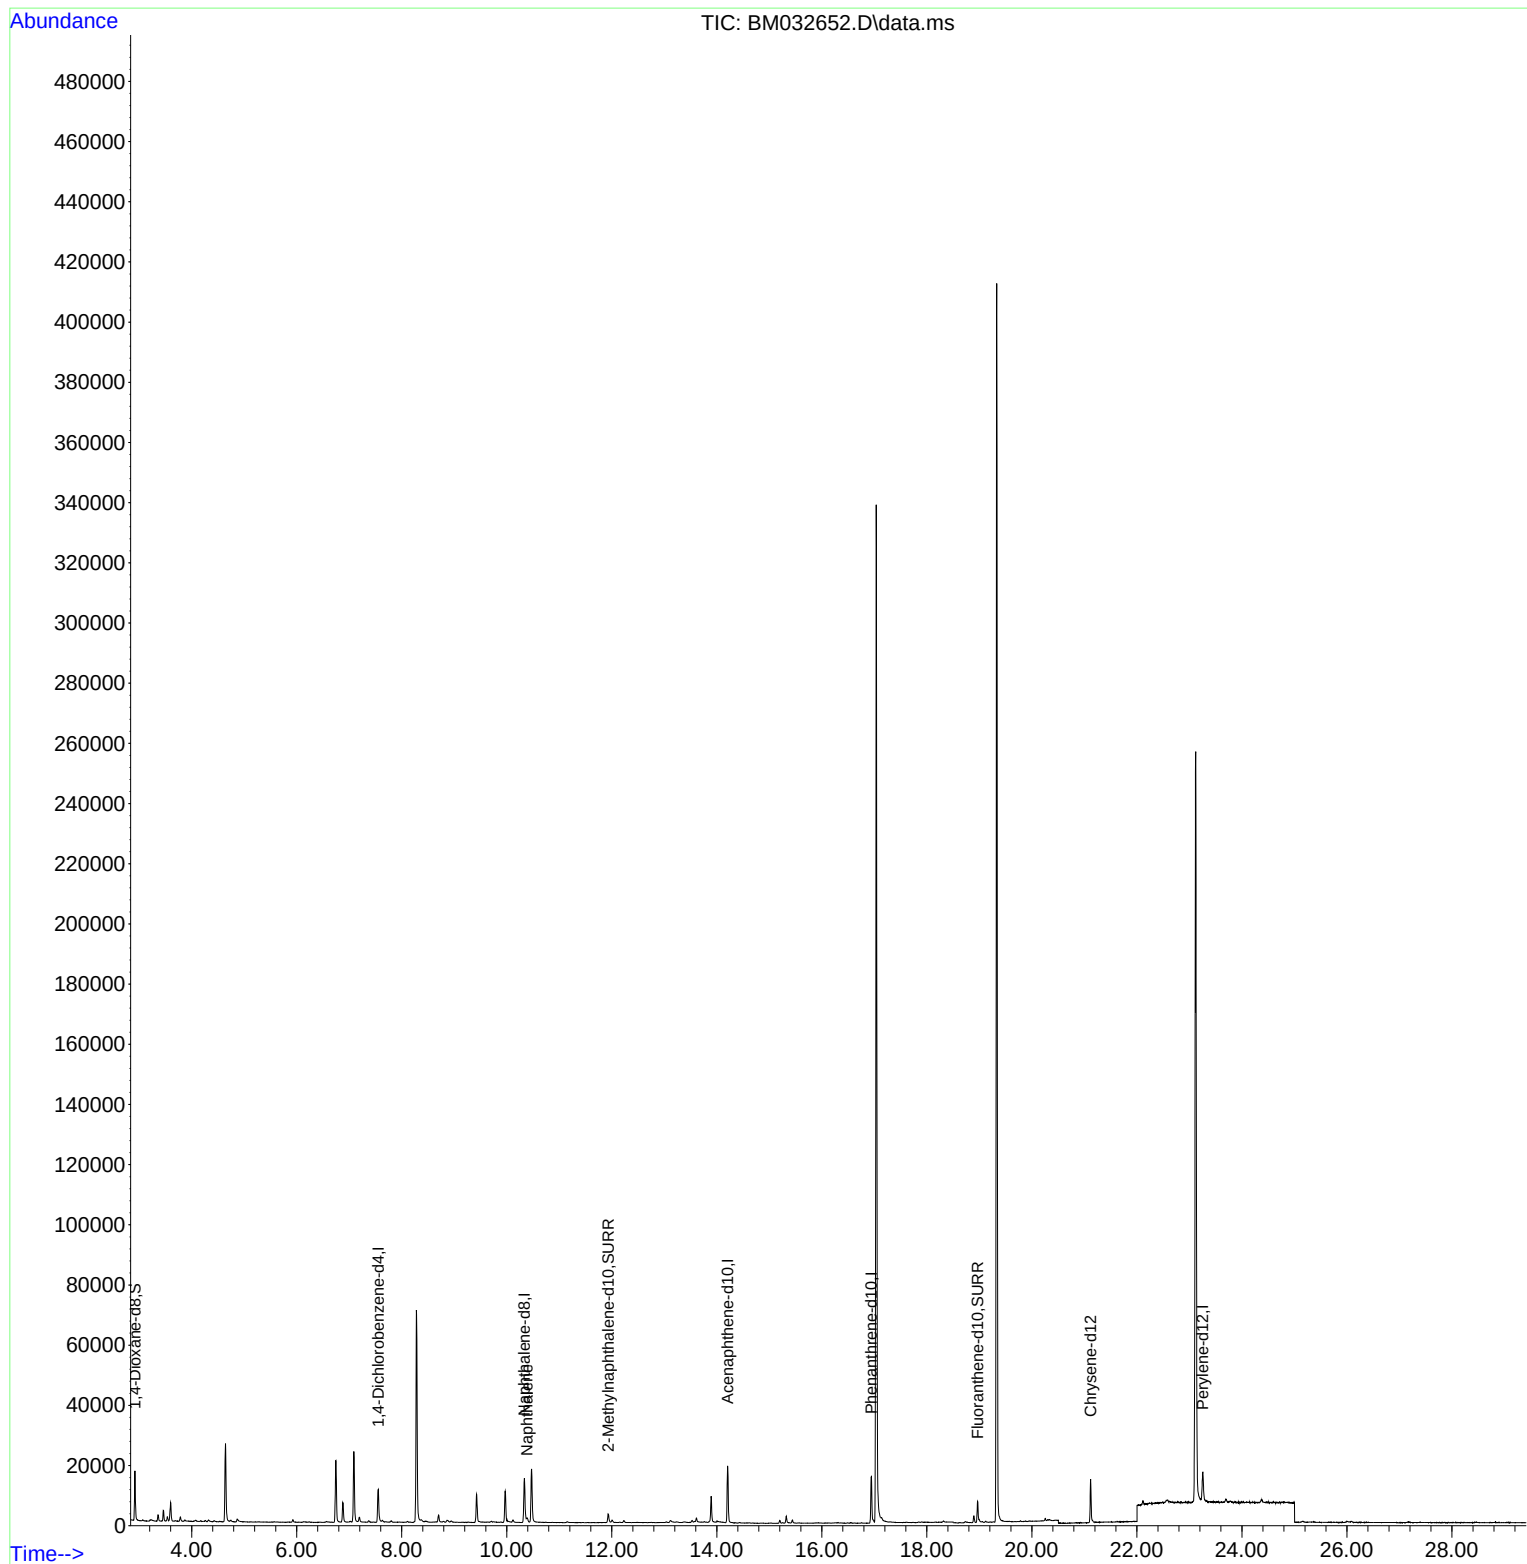

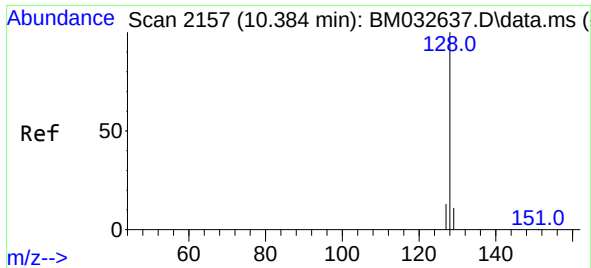

#5
Naphthalene
Concen: 0.02 ng/ul
RT: 10.384 min Scan# 2157
Delta R.T. -0.005 min
Lab File: BM032652.D
Acq: 21 Oct 2021 11:47

Instrument :
BNA_M
ClientSampleId :
JDGD1

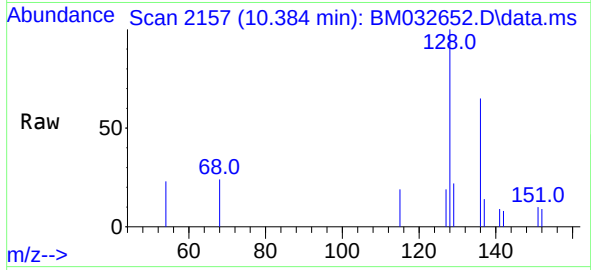

Tgt Ion:128 Resp: 1285

Ion	Ratio	Lower	Upper
128	100		
129	21.6	9.1	13.7#
127	19.2	11.1	16.7#

