

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101921\
 Data File : BM032653.D
 Acq On : 21 Oct 2021 12:23
 Operator : CG/JU
 Sample : M4196-06
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JDGA5

Quant Time: Oct 21 13:34:00 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 20 16:33:56 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.553	152	6066	0.40	ng/ul	0.00
4) Naphthalene-d8	10.335	136	18207	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.206	164	8779	0.40	ng/ul	0.00
13) Phenanthrene-d10	16.943	188	15352	0.40	ng/ul	# 0.00
17) Chrysene-d12	21.118	240	12048	0.40	ng/ul	0.00
23) Perylene-d12	23.254	264	13051	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.920	96	33955	4.99	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.931	152	8724	0.36	ng/ul	0.00
18) Fluoranthene-d10	18.966	212	14012	0.37	ng/ul	0.00
Target Compounds						
						Qvalue
7) 2-Methylnaphthalene	12.008	142	1839	0.05	ng/ul	99
8) 1-Methylnaphthalene	12.228	142	947	0.03	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM101921\
Data File : BM032653.D
Acq On : 21 Oct 2021 12:23
Operator : CG/JU
Sample : M4196-06
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JDGA5

Quant Time: Oct 21 13:34:00 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 20 16:33:56 2021
Response via : Initial Calibration




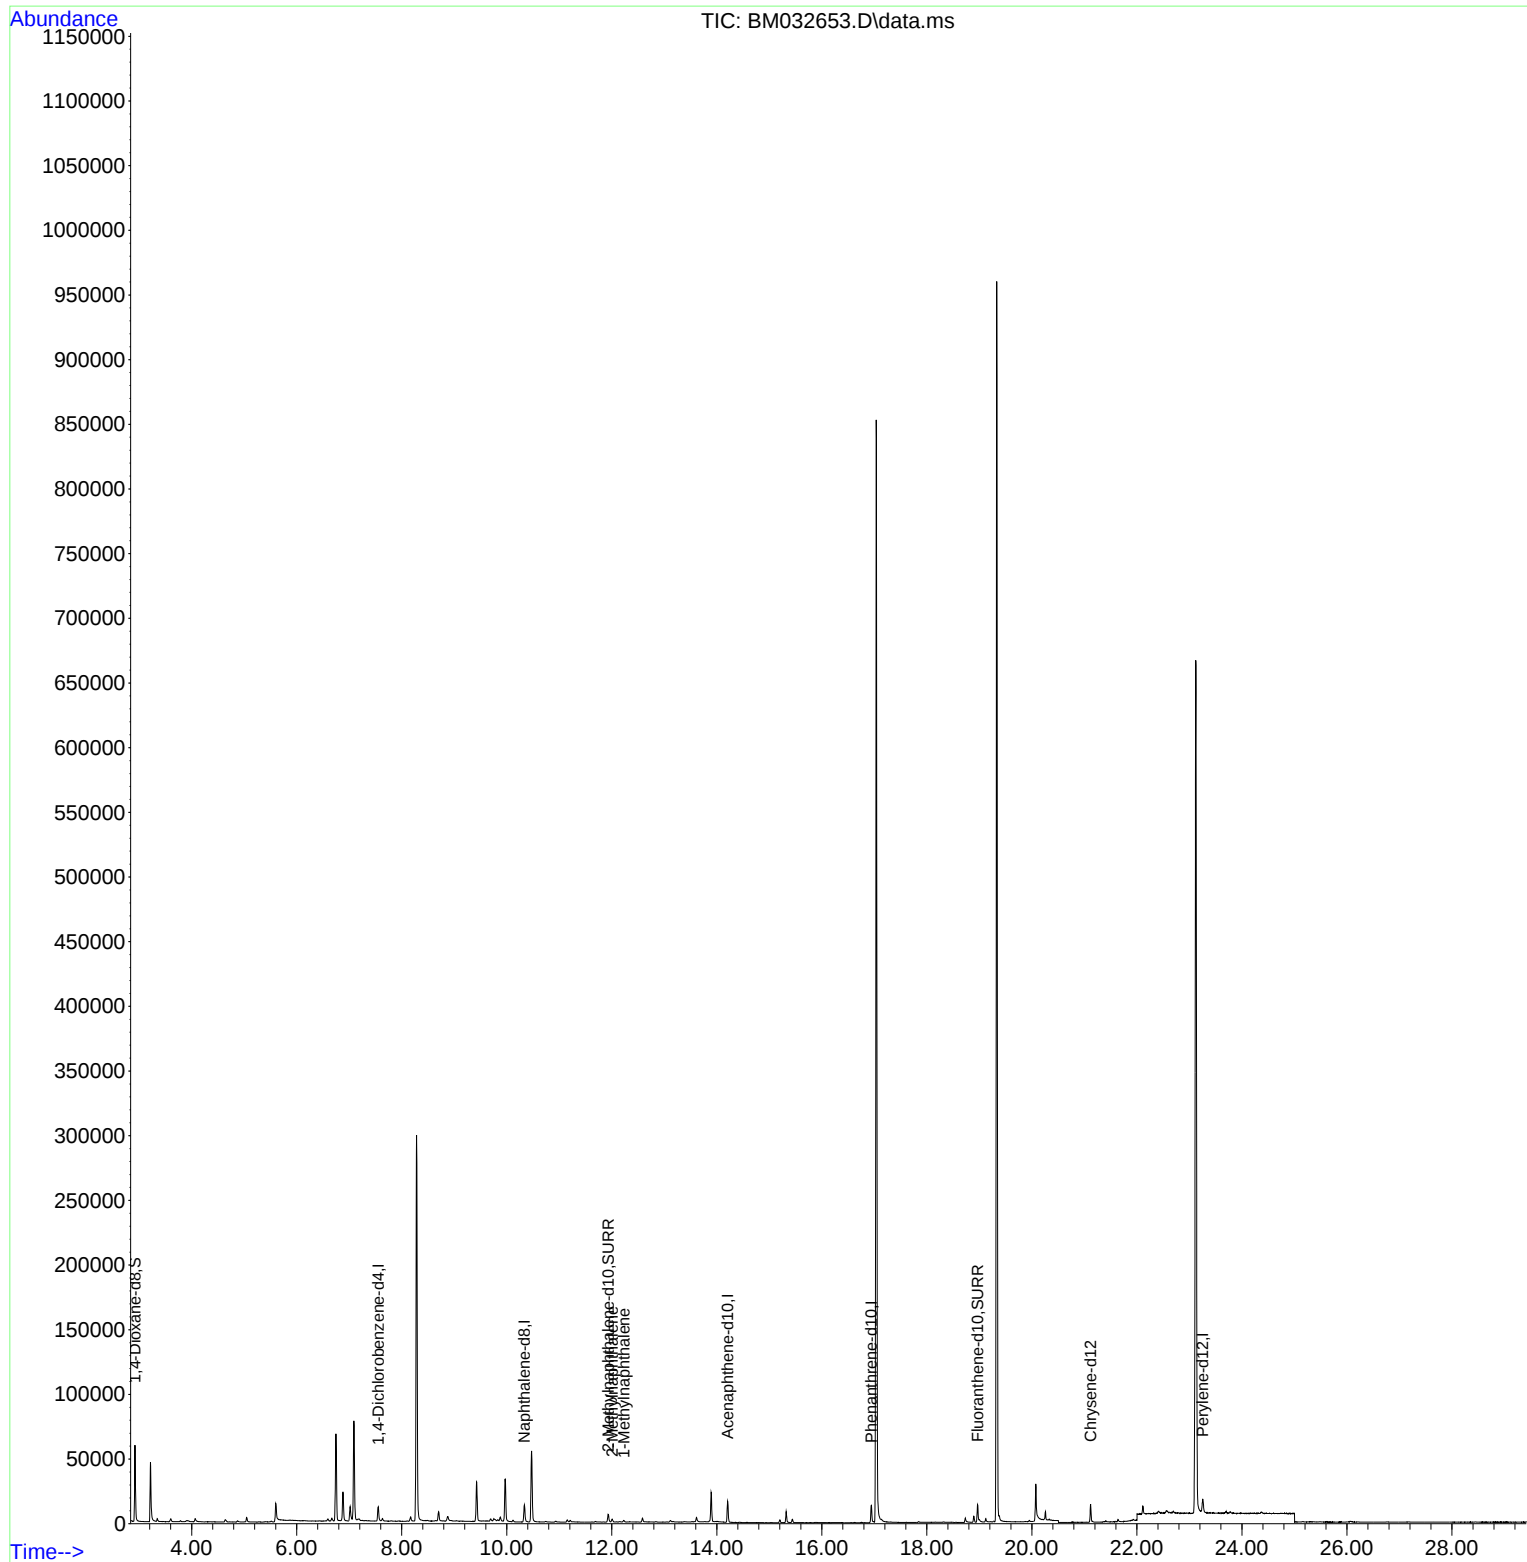


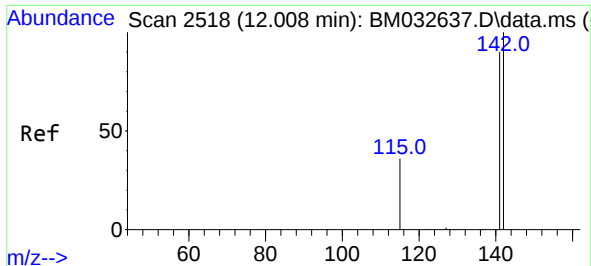

#7
2-Methylnaphthalene
Concen: 0.05 ng/ul
RT: 12.008 min Scan# 2518
Delta R.T. -0.004 min
Lab File: BM032653.D
Acq: 21 Oct 2021 12:23

Instrument :
BNA_M
ClientSampleId :
JDGA5

Tgt Ion:142 Resp: 1839
Ion Ratio Lower Upper
142 100
141 89.6 72.2 108.2

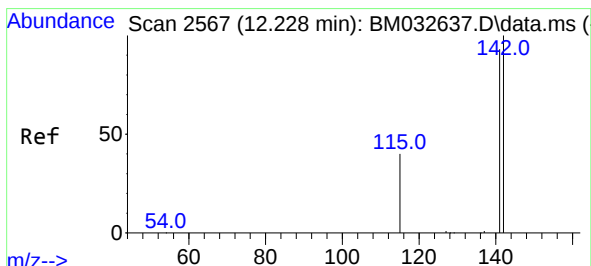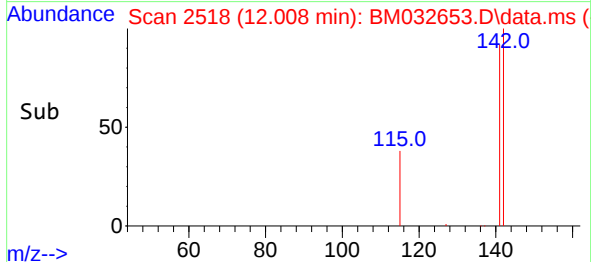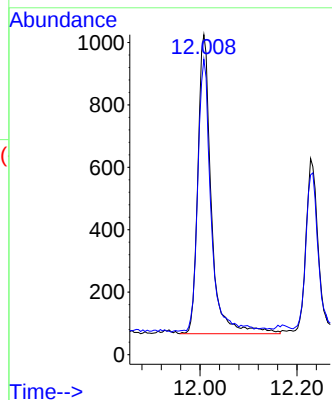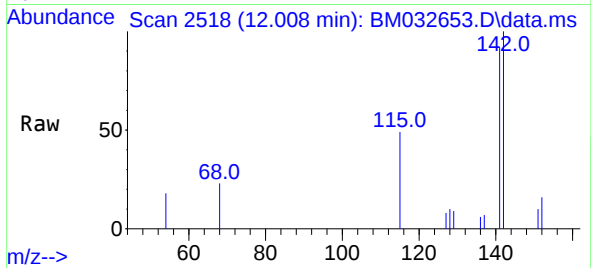

#8
1-Methylnaphthalene
Concen: 0.03 ng/ul
RT: 12.228 min Scan# 2567
Delta R.T. -0.004 min
Lab File: BM032653.D
Acq: 21 Oct 2021 12:23

Tgt Ion:142 Resp: 947
Ion Ratio Lower Upper
142 100
141 91.9 74.9 112.3

