

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102016\
 Data File : BM007710.D
 Acq On : 20 Oct 2016 19:15
 Operator : UM/SJ
 Sample : H5330-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B84

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM102016.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.646	7	10	21	rVB2	49991	110480	2.54%	0.287%
2	4.004	236	241	248	rVB	101154	137229	3.16%	0.356%
3	5.422	476	482	495	rBV2	64829	138618	3.19%	0.360%
4	6.928	733	738	749	rBV	135807	235841	5.43%	0.612%
5	7.092	759	766	774	rBV	588133	910040	20.93%	2.362%
6	7.287	793	799	810	rBV	617945	1018387	23.43%	2.643%
7	7.751	872	878	891	rVB	621868	992050	22.82%	2.575%
8	8.457	992	998	1009	rBV	447405	731400	16.82%	1.898%
9	8.910	1067	1075	1085	rBV	703887	1197510	27.55%	3.108%
10	9.628	1190	1197	1212	rBV	556096	977953	22.50%	2.538%
11	10.163	1281	1288	1304	rBV	735634	1403695	32.29%	3.643%
12	10.533	1343	1351	1361	rBV	763292	1294868	29.79%	3.361%
13	13.798	1900	1906	1918	rBV	1546048	2167063	49.85%	5.624%
14	14.080	1945	1954	1962	rBV	1657117	2527342	58.14%	6.559%
15	14.386	1998	2006	2016	rBV	1149947	1653742	38.04%	4.292%
16	14.621	2040	2046	2058	rBV2	38046	104814	2.41%	0.272%
17	15.380	2168	2175	2183	rBV	2207863	3246385	74.68%	8.425%
18	15.510	2192	2197	2208	rBV	546208	863770	19.87%	2.242%
19	17.133	2467	2473	2483	rBV	1344618	1883063	43.32%	4.887%
20	17.233	2483	2490	2505	rVV	2298124	3428496	78.87%	8.898%
21	19.527	2874	2880	2891	rBV	2953053	4085254	93.97%	10.602%
22	21.315	3179	3184	3191	rBV	1927623	2550970	58.68%	6.621%
23	23.427	3536	3543	3551	rBV2	2277565	4347235	100.00%	11.282%
24	23.568	3561	3567	3577	rVB	1307474	2524958	58.08%	6.553%


Sum of corrected areas: 38531163

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102016\
Data File : BM007710.D
Acq On : 20 Oct 2016 19:15
Operator : UM/SJ
Sample : H5330-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B84

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM102016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

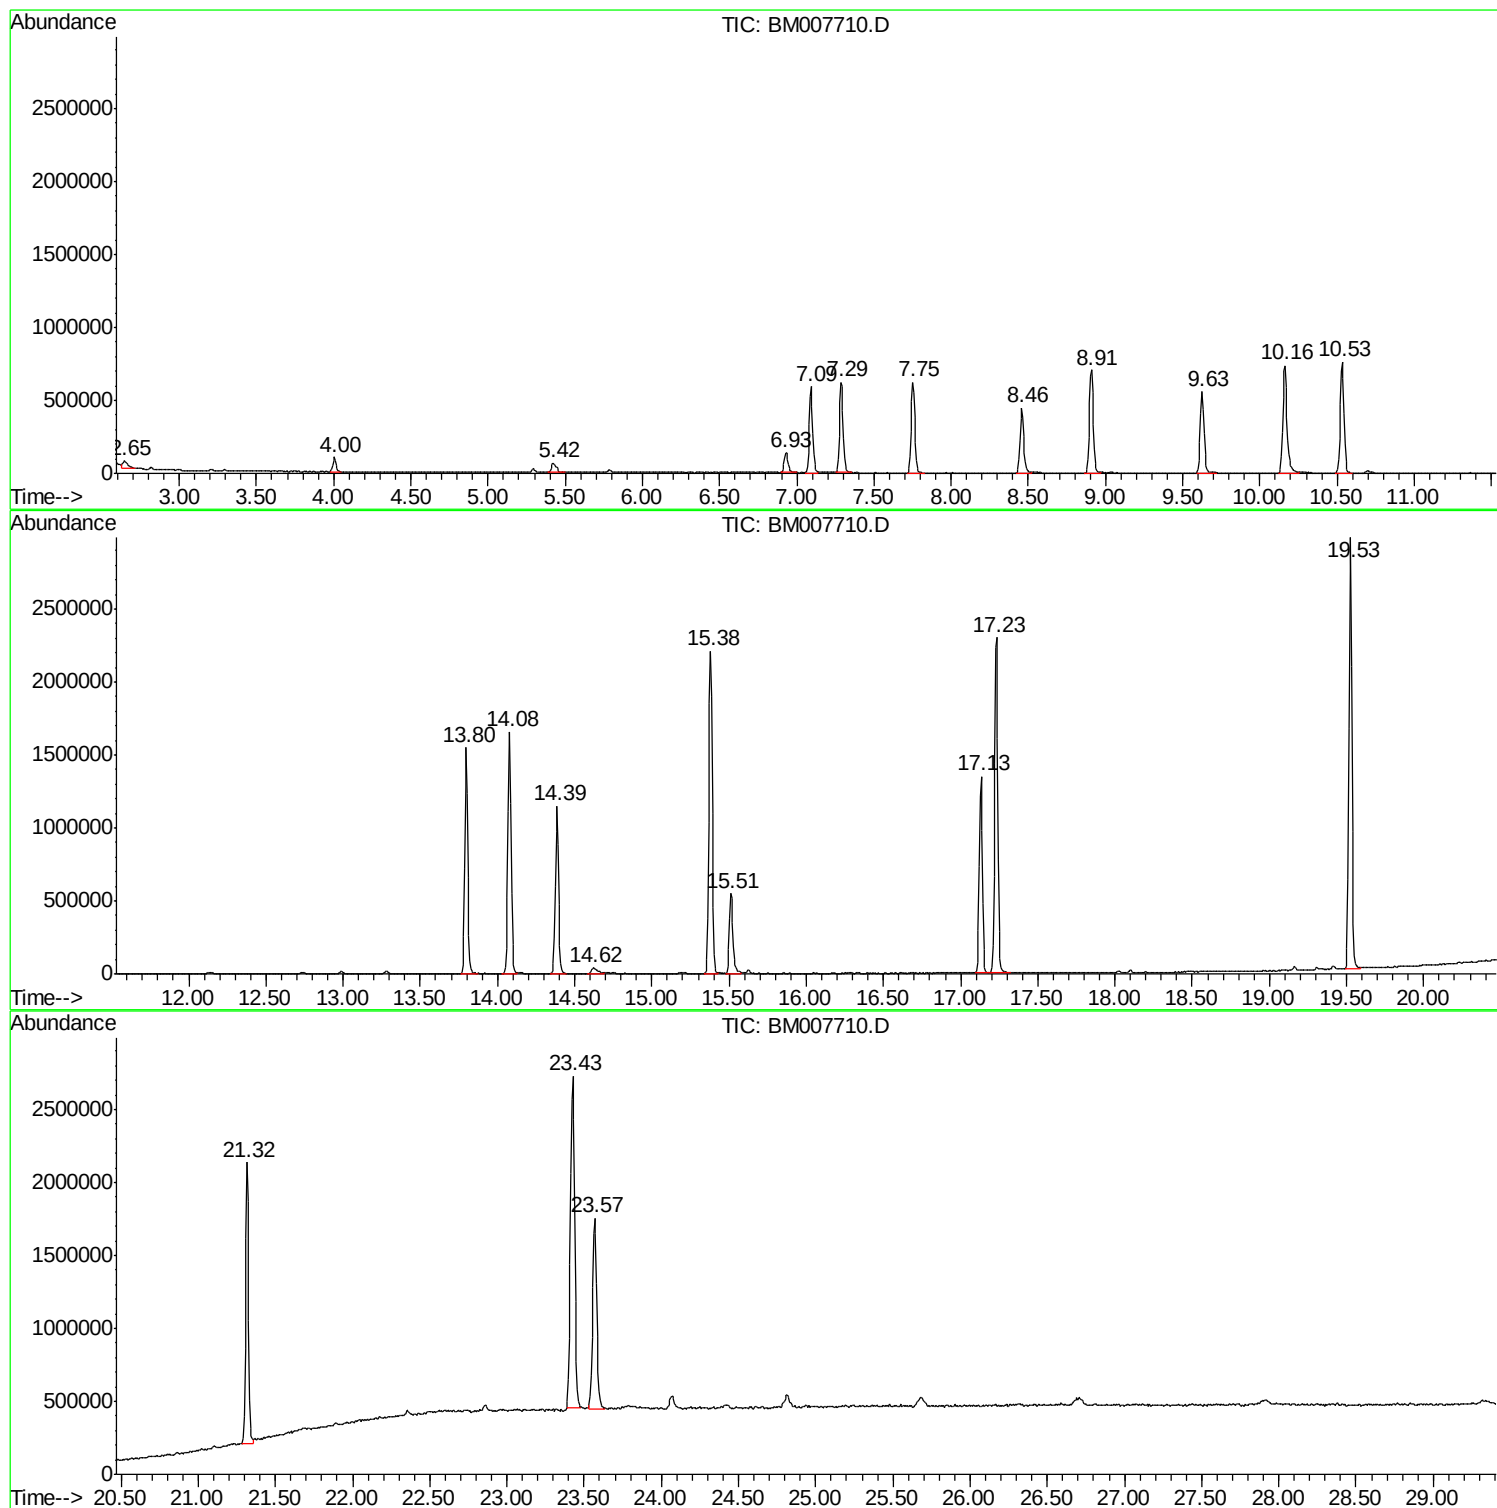

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM102016\
Data File : BM007710.D
Acq On : 20 Oct 2016 19:15
Operator : UM/SJ
Sample : H5330-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B84

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM102016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM102016\
Data File : BM007710.D
Acq On : 20 Oct 2016 19:15
Operator : UM/SJ
Sample : H5330-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B84

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM102016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc