

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102017\
 Data File : BM012318.D
 Acq On : 20 Oct 2017 14:17
 Operator : SJ/JU
 Sample : PB103431BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK31

Quant Time: Oct 23 01:20:18 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 23 01:17:35 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	188010	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	862458	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	578936	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.18	188	1393504	20.00	ng/ul	0.00
75) Chrysene-d12	21.37	240	1608468	20.00	ng/ul	0.00
83) Perylene-d12	23.66	264	1656581	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.19	96	28868	7.30	ng/uL	0.00
5) Phenol-d5	6.95	99	524367	34.37	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.11	67	351239	38.39	ng/ul	0.00
9) 2-Chlorophenol-d4	7.31	132	462659	35.76	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	486453	37.04	ng/ul	0.00
19) Nitrobenzene-d5	8.94	128	239364	36.37	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	289257	37.61	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.21	165	477741	32.54	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	693801	50.49	ng/ul	0.00
43) Dimethylphthalate-d6	13.84	166	2050456	40.07	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	2287604	36.93	ng/ul	0.00
51) 4-Nitrophenol-d4	14.68	143	223311	29.03	ng/ul	0.00
57) Fluorene-d10	15.42	176	1621139	38.60	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.58	200	232604	24.32	ng/ul	0.00
70) Anthracene-d10	17.28	188	2649276	38.45	ng/ul	0.00
76) Pyrene-d10	19.58	212	3049417	37.35	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.52	264	3098367	38.80	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	8.50	70	14481	1.354	ng/ul# 1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102017\
Data File : BM012318.D
Acq On : 20 Oct 2017 14:17
Operator : SJ/JU
Sample : PB103431BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK31

Quant Time: Oct 23 01:20:18 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 23 01:17:35 2017
Response via : Initial Calibration

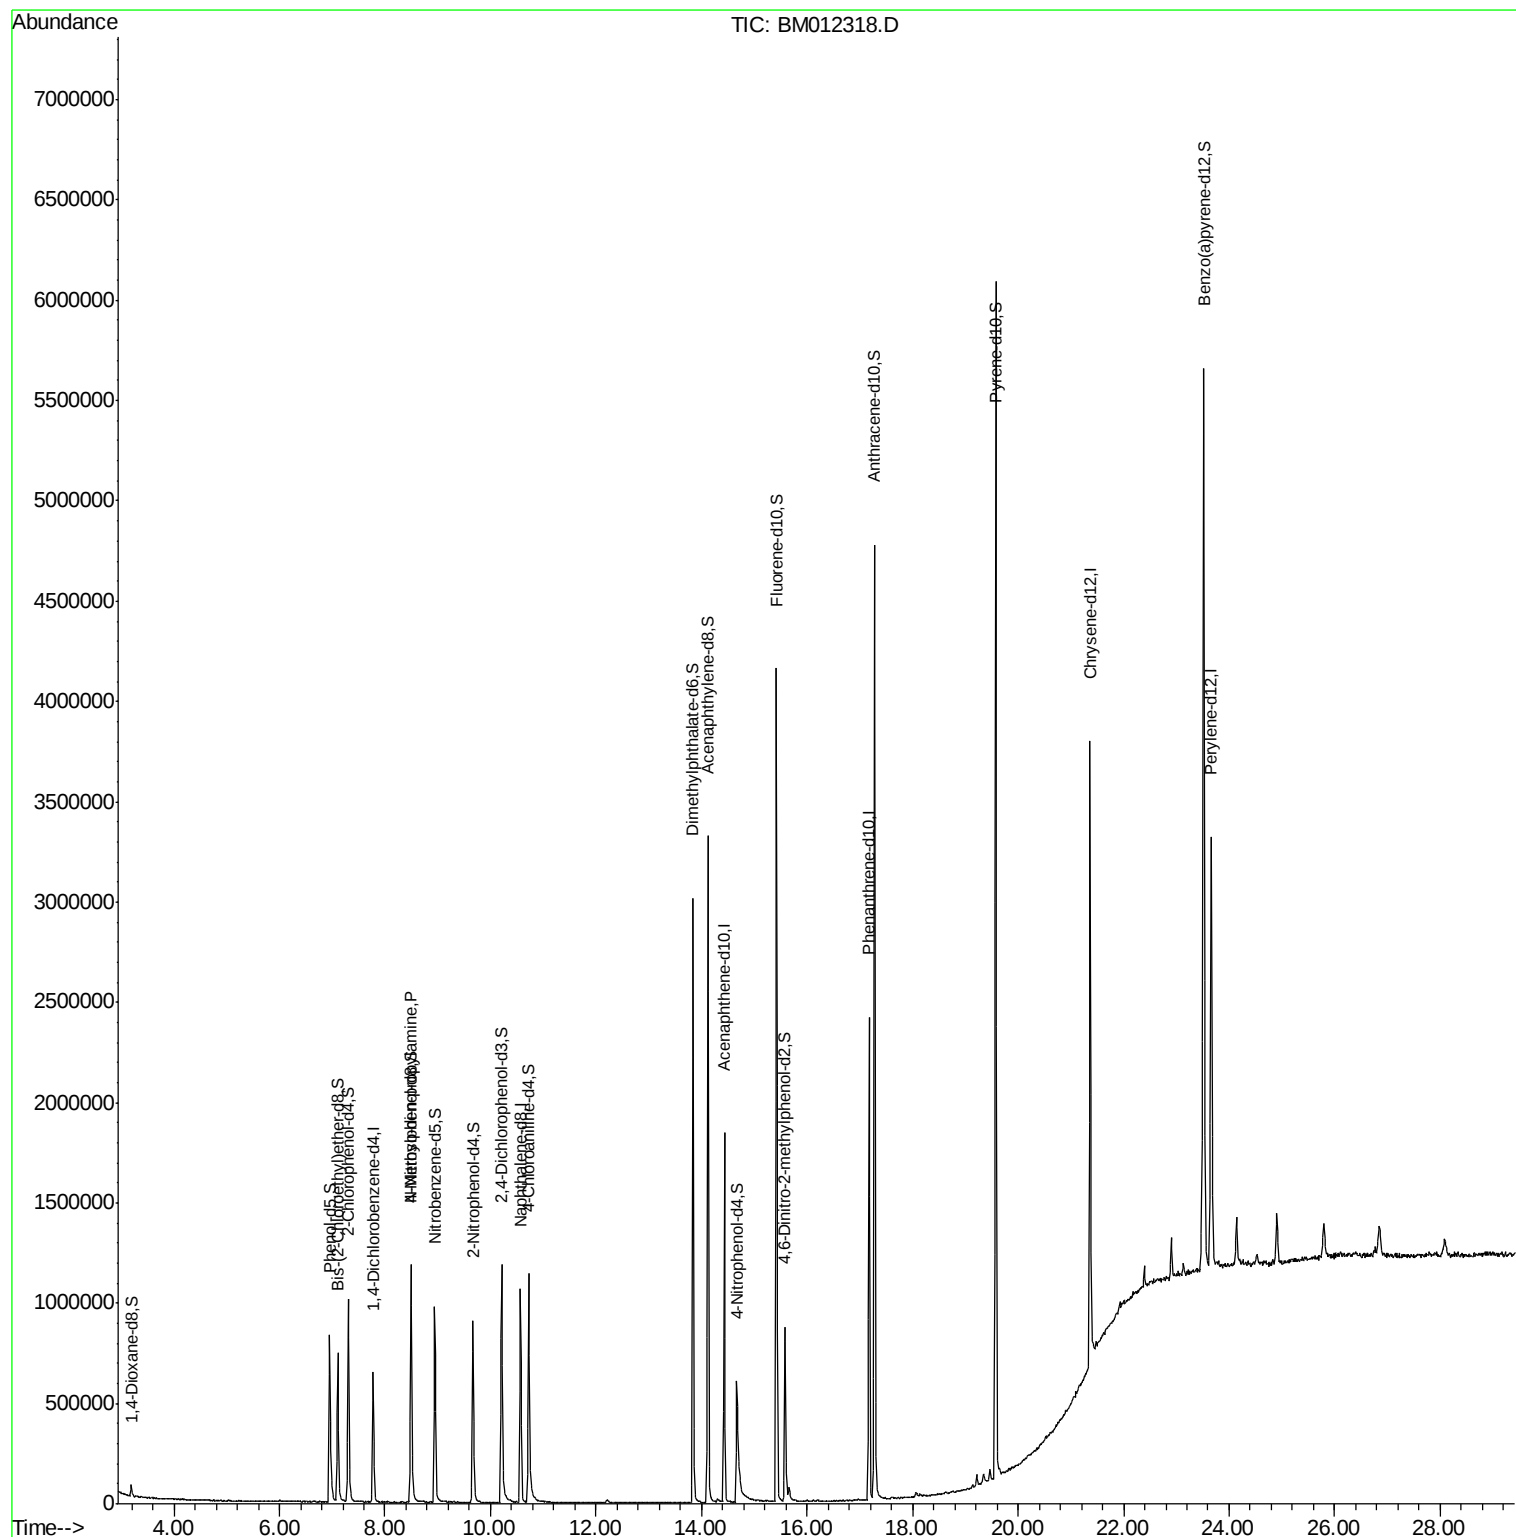

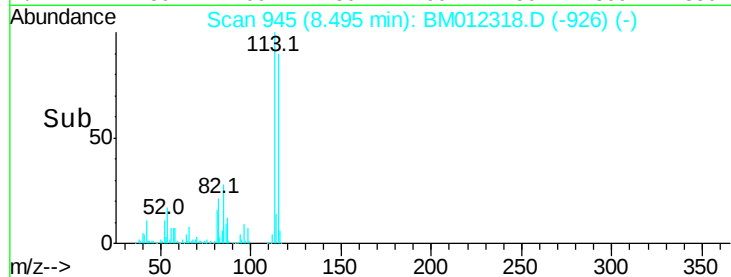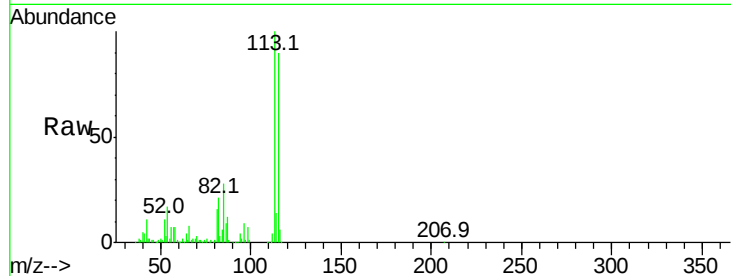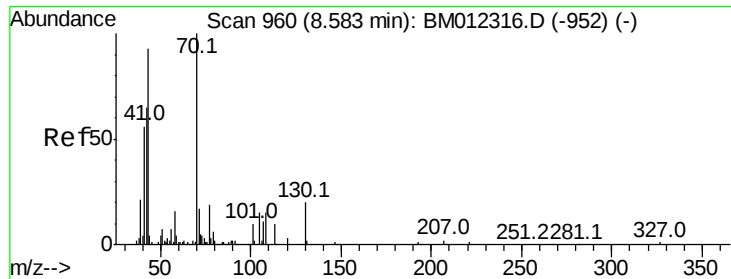

#15
N-Nitroso-di-n-propylamine
Concen: 1.354 ng/ul
RT: 8.50 min Scan# 945
Delta R.T. -0.09 min
Lab File: BM012318.D
Acq: 20 Oct 2017 14:17

Instrument :
BNA_M
ClientSampleId :
SBLK31

Tot Ion: 70 Resp: 14481
Ion Ratio Lower Upper
70 100
42 363.9 43.0 64.4#
101 0.0 8.2 12.2#
130 0.0 18.6 28.0#

