

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102017\
 Data File : BM012344.D
 Acq On : 21 Oct 2017 06:01
 Operator : SJ/JU
 Sample : I5656-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 B0C94

Quant Time: Oct 23 02:46:37 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 23 02:34:17 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	310090	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	1344958	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.42	164	824221	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	1887519	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	1634836	20.00	ng/ul	0.00
83) Perylene-d12	23.65	264	1373002	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.19	96	24773	3.80	ng/uL	0.00
5) Phenol-d5	6.94	99	571476	22.71	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	352238	23.34	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	507231	23.77	ng/ul	0.00
13) 4-Methylphenol-d8	8.48	113	517621	23.90	ng/ul	0.00
19) Nitrobenzene-d5	8.94	128	245355	23.90	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	293766	24.49	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	557361	24.34	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	595040	27.77	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	1840797	25.27	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	2259112	25.62	ng/ul	0.00
51) 4-Nitrophenol-d4	14.67	143	159183	14.53	ng/ul	0.00
57) Fluorene-d10	15.42	176	1581673	26.45	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.57	200	194380	15.01	ng/ul	0.00
70) Anthracene-d10	17.27	188	2367326	25.36	ng/ul	0.00
76) Pyrene-d10	19.57	212	2646290	31.89	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.51	264	1782196	26.92	ng/ul	0.00
Target Compounds						
6) Phenol	6.97	94	108510	4.172	ng/ul	91
44) Dimethylphthalate	13.88	163	754429	10.337	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102017\
Data File : BM012344.D
Acq On : 21 Oct 2017 06:01
Operator : SJ/JU
Sample : I5656-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B0C94

Quant Time: Oct 23 02:46:37 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 23 02:34:17 2017
Response via : Initial Calibration

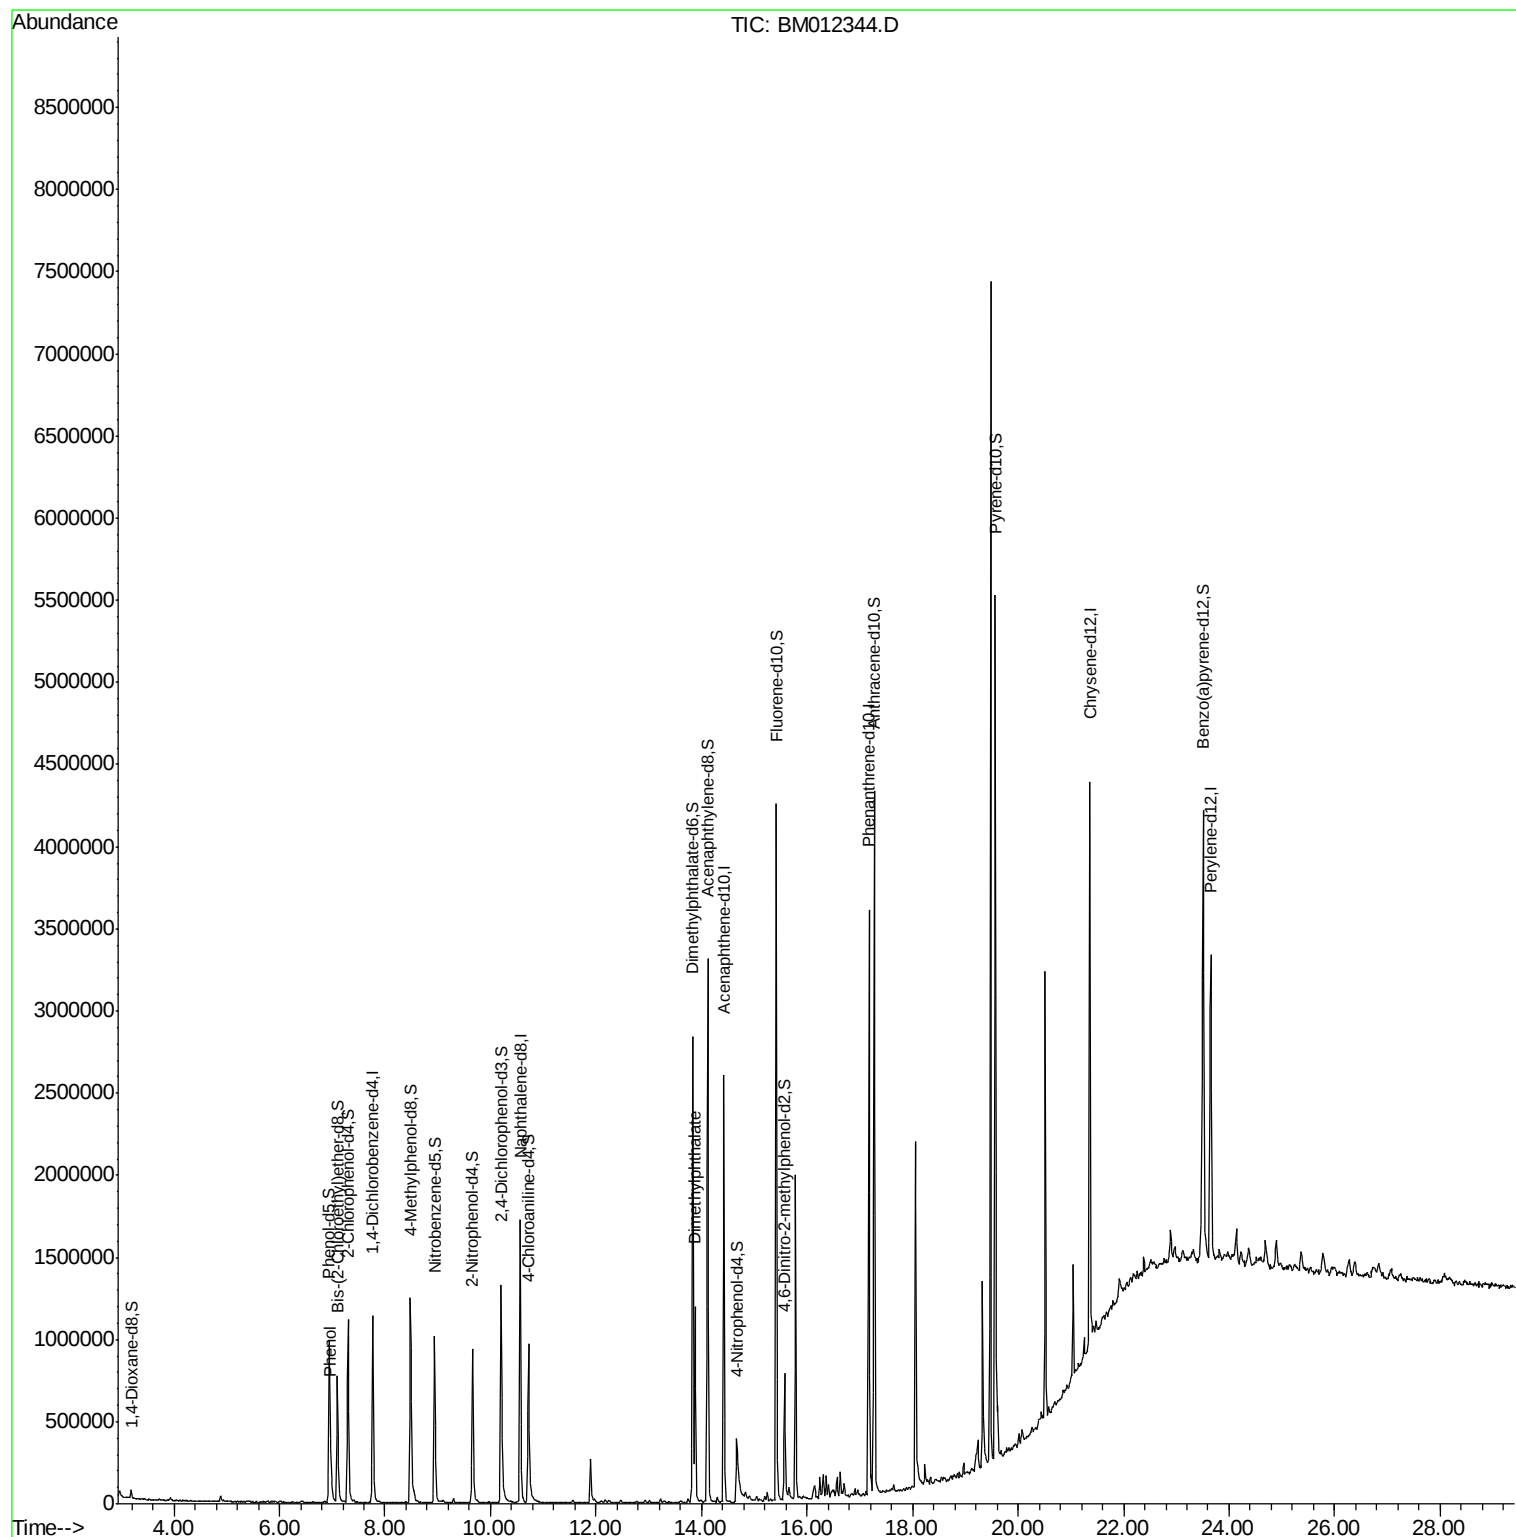

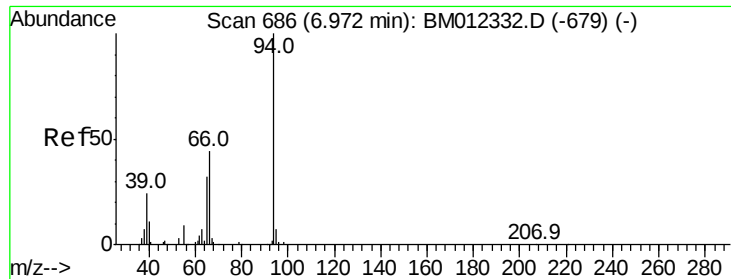

#6

Phenol

Concen: 4.172 ng/ul

RT: 6.97 min Scan# 686

Delta R.T. 0.00 min

Lab File: BM012344.D

Acq: 21 Oct 2017 06:01

Instrument :


BNA_M

ClientSampleId :

B0C94

Tot Ion: 94 Resp: 108510


Ion	Ratio	Lower	Upper
94	100		
65	34.3	24.4	36.6
66	50.1	35.0	52.4

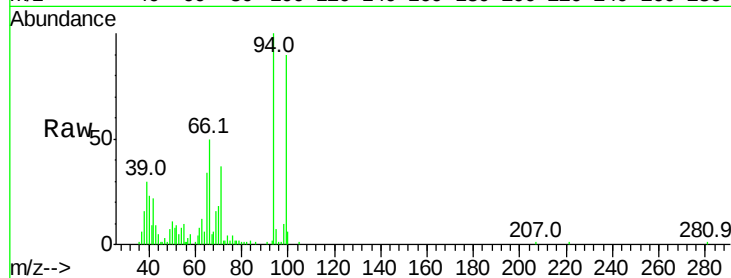



Abundance Ion 94.00 (93.70 to 94.70): BM012332.D (-679) (-)

Ion 65.00 (64.70 to 65.70): BM012332.D (-679) (-)

Ion 66.00 (65.70 to 66.70): BM012332.D (-679) (-)

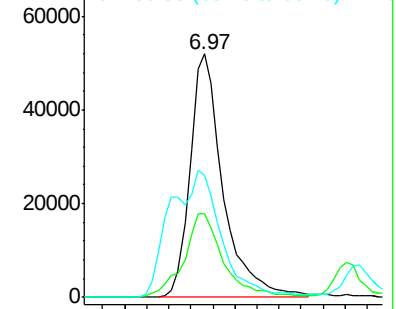

Time-->

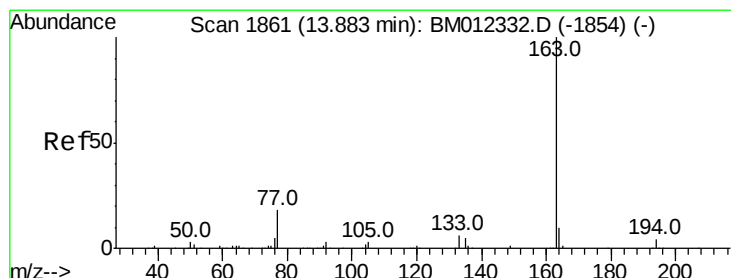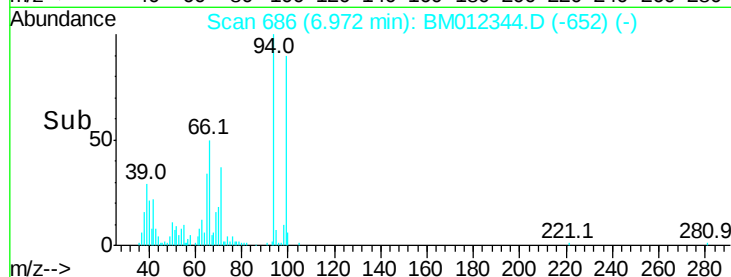

#44

Dimethylphthalate

Concen: 10.337 ng/ul

RT: 13.88 min Scan# 1860


Delta R.T. -0.01 min

Lab File: BM012344.D

Acq: 21 Oct 2017 06:01

Tgt Ion:163 Resp: 754429


Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.7	5.5
164	10.2	8.1	12.1

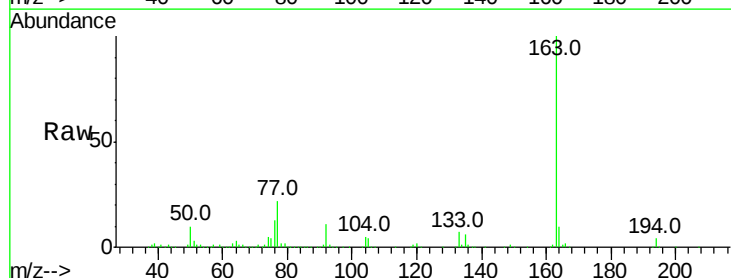

Abundance Ion 163.00 (162.70 to 163.70): BM012332.D (-1854) (-)

Ion 194.00 (193.70 to 194.70): BM012332.D (-1854) (-)

Ion 164.00 (163.70 to 164.70): BM012332.D (-1854) (-)

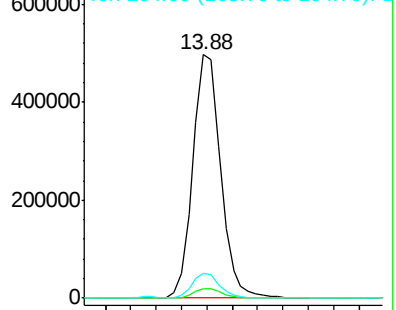

Time-->

