

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102017\
 Data File : BM012317.D
 Acq On : 20 Oct 2017 13:40
 Operator : SJ/JU
 Sample : PB103432BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK32

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101217.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.190	39	43	50	rBV	42487	62537	1.01%	0.104%
2	6.954	677	683	701	rBV	566651	1197669	19.28%	1.996%
3	7.107	703	709	723	rVB	515919	886506	14.27%	1.477%
4	7.307	736	743	762	rBV	721941	1302422	20.96%	2.170%
5	7.772	816	822	840	rBV	651941	1240697	19.97%	2.067%
6	8.495	938	945	963	rBV	830204	1634797	26.31%	2.724%
7	8.948	1015	1022	1034	rBV	674700	1309869	21.08%	2.183%
8	9.672	1138	1145	1160	rBV	599989	1225787	19.73%	2.042%
9	10.213	1230	1237	1263	rBV	787003	1699449	27.35%	2.832%
10	10.572	1290	1298	1313	rBV	1092696	1876572	30.20%	3.127%
11	10.725	1317	1324	1343	rBV	699766	1697174	27.32%	2.828%
12	13.836	1847	1853	1870	rBV	2001564	3137298	50.50%	5.228%
13	14.124	1895	1902	1918	rBV	2161017	3440435	55.37%	5.733%
14	14.430	1947	1954	1969	rBV2	1788573	2810372	45.23%	4.683%
15	14.683	1990	1997	2013	rBV	333303	1063857	17.12%	1.773%
16	15.424	2117	2123	2130	rBV	2809200	4257932	68.53%	7.095%
17	15.583	2144	2150	2161	rBV	527921	1073255	17.27%	1.788%
18	15.665	2161	2164	2172	rVB3	43150	83421	1.34%	0.139%
19	17.177	2415	2421	2432	rBV2	2426887	3636465	58.53%	6.059%
20	17.277	2432	2438	2450	rVV2	3151210	4809347	77.41%	8.014%
21	19.218	2764	2768	2776	rBV2	38468	70583	1.14%	0.118%
22	19.342	2785	2789	2800	rBV10	74121	184781	2.97%	0.308%
23	19.577	2823	2829	2838	rBV	4073988	5756660	92.65%	9.592%
24	21.365	3128	3133	3150	rBV	3251090	4820424	77.59%	8.032%
25	23.518	3492	3499	3509	rVB2	3035203	6213054	100.00%	10.353%
26	23.665	3518	3524	3537	rVB2	2176416	4522916	72.80%	7.536%


Sum of corrected areas: 60014279

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102017\
Data File : BM012317.D
Acq On : 20 Oct 2017 13:40
Operator : SJ/JU
Sample : PB103432BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK32

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

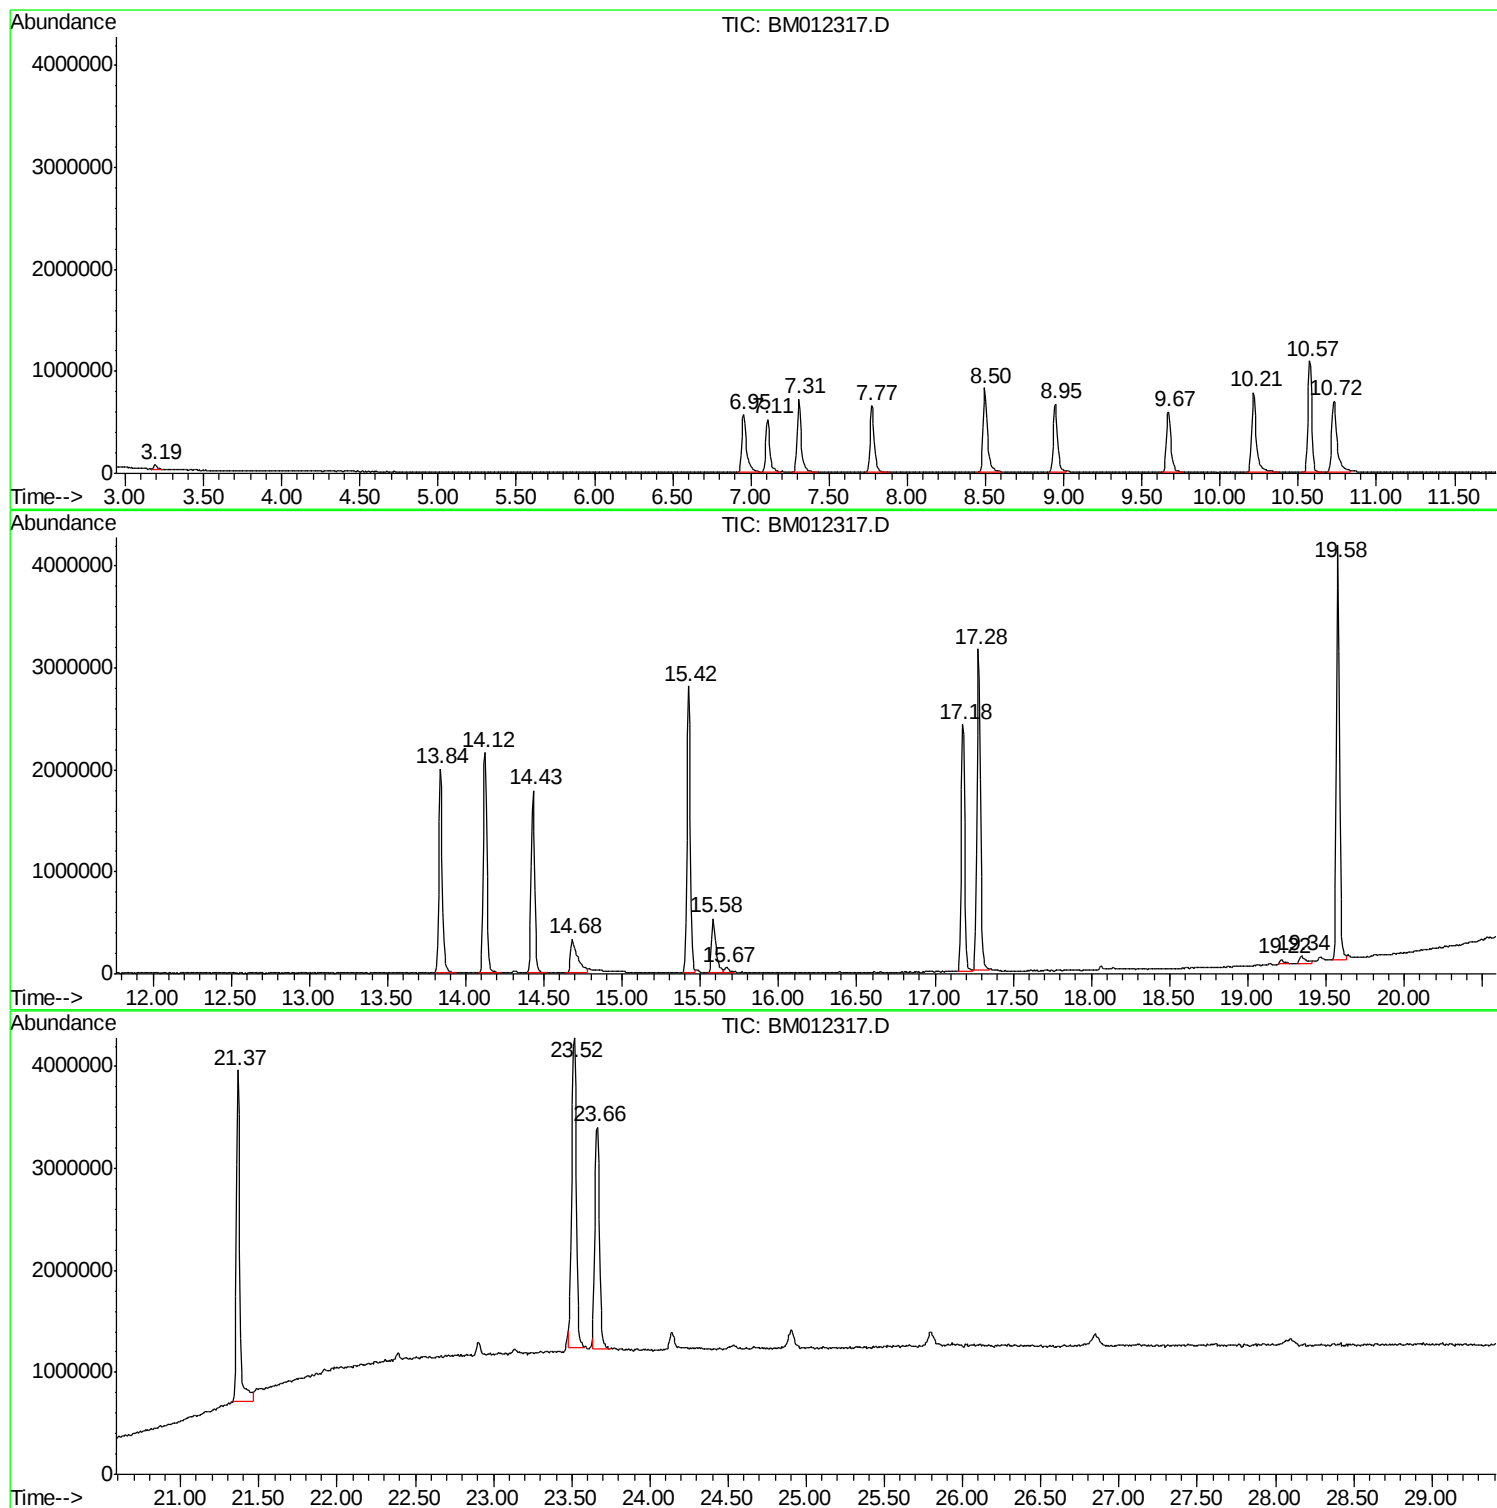

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM102017\
Data File : BM012317.D
Acq On : 20 Oct 2017 13:40
Operator : SJ/JU
Sample : PB103432BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK32

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM102017\
Data File : BM012317.D
Acq On : 20 Oct 2017 13:40
Operator : SJ/JU
Sample : PB103432BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK32

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc