

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102017\
 Data File : BM012319.D
 Acq On : 20 Oct 2017 14:53
 Operator : SJ/JU
 Sample : I5846-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD9T0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101217.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.954	676	683	697	rBV	191759	459588	5.59%	0.640%
2	7.107	703	709	723	rBV	718497	1220421	14.85%	1.700%
3	7.307	736	743	761	rBV	831408	1545238	18.81%	2.152%
4	7.772	816	822	833	rBV	703714	1336225	16.26%	1.861%
5	8.496	939	945	960	rBV	657511	1335142	16.25%	1.860%
6	8.943	1014	1021	1040	rBV	986172	1886230	22.96%	2.627%
7	9.666	1137	1144	1165	rBV	907932	1781563	21.68%	2.482%
8	10.213	1229	1237	1262	rBV	924983	2430034	29.58%	3.385%
9	10.572	1291	1298	1311	rBV	1166453	2019522	24.58%	2.813%
10	13.836	1845	1853	1869	rBV	2932434	4473893	54.45%	6.232%
11	14.125	1895	1902	1920	rBV	3330801	5076198	61.79%	7.071%
12	14.430	1947	1954	1965	rBV2	1920580	3044958	37.06%	4.241%
13	14.707	1995	2001	2015	rBV4	83745	334687	4.07%	0.466%
14	15.425	2116	2123	2140	rBV	4427071	6271055	76.33%	8.735%
15	15.577	2143	2149	2161	rVV	1007590	1887710	22.98%	2.629%
16	15.672	2161	2165	2172	rVB2	55319	101521	1.24%	0.141%
17	17.177	2415	2421	2431	rBV2	2695959	3870718	47.11%	5.392%
18	17.277	2432	2438	2458	rVB2	4584583	6977692	84.93%	9.719%
19	17.830	2528	2532	2537	rVB	165356	209970	2.56%	0.292%
20	18.060	2566	2571	2581	rBV4	81256	164116	2.00%	0.229%
21	19.218	2764	2768	2775	rBV2	57766	88783	1.08%	0.124%
22	19.336	2784	2788	2798	rBV	188874	382960	4.66%	0.533%
23	19.465	2807	2810	2816	rVB2	58175	99733	1.21%	0.139%
24	19.577	2823	2829	2838	rBV	5867844	8215853	100.00%	11.444%
25	21.365	3128	3133	3142	rBV	3317254	4581827	55.77%	6.382%
26	23.512	3492	3498	3513	rVB2	3882606	7880715	95.92%	10.977%
27	23.659	3517	3523	3533	rVB	2020978	4114859	50.08%	5.732%


Sum of corrected areas: 71791211

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102017\
Data File : BM012319.D
Acq On : 20 Oct 2017 14:53
Operator : SJ/JU
Sample : I5846-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD9T0

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

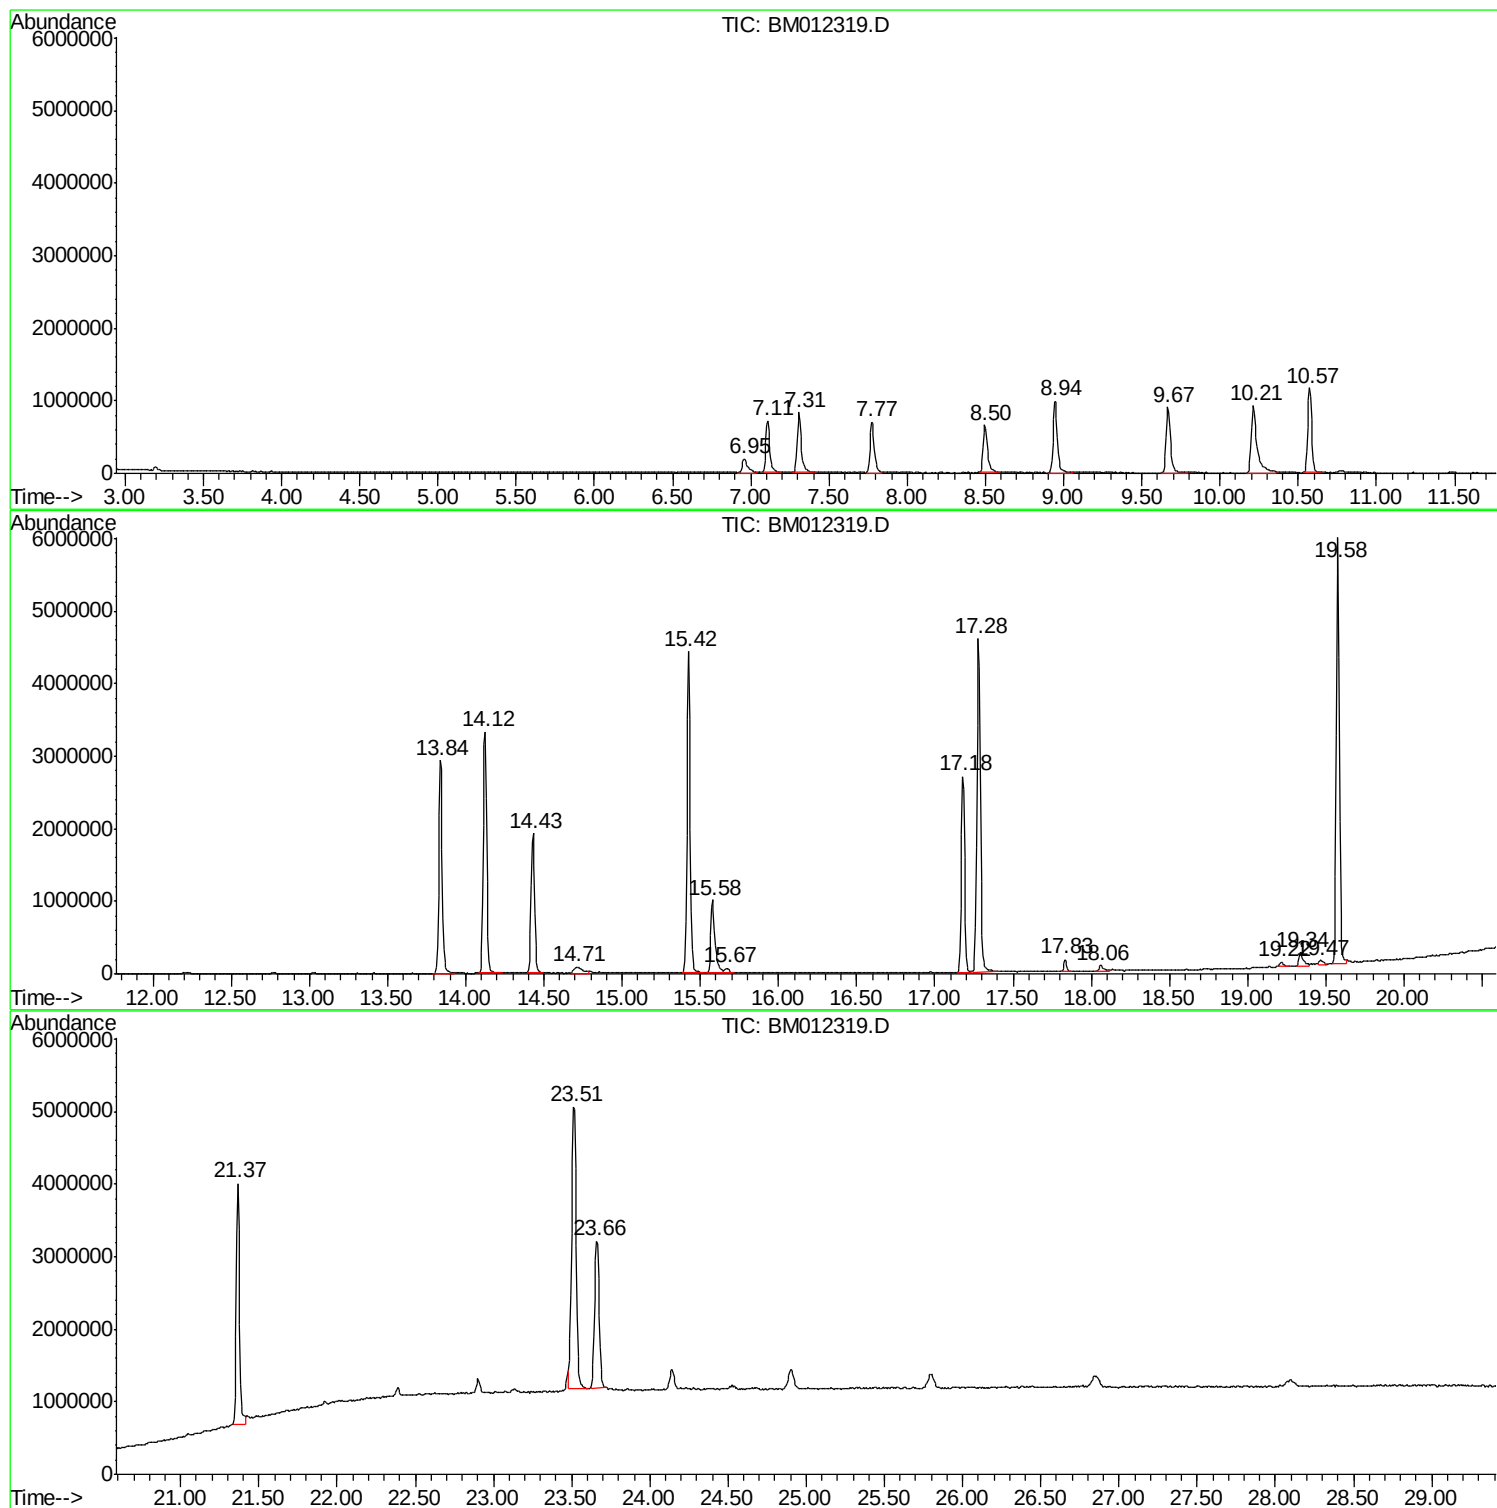

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM102017\
Data File : BM012319.D
Acq On : 20 Oct 2017 14:53
Operator : SJ/JU
Sample : I5846-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD9T0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM102017\
Data File : BM012319.D
Acq On : 20 Oct 2017 14:53
Operator : SJ/JU
Sample : I5846-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD9T0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc