

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102017\
 Data File : BM012331.D
 Acq On : 20 Oct 2017 22:11
 Operator : SJ/JU
 Sample : I5846-13
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BE2P6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101217.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.954	677	683	702	rBV	184862	466381	4.87%	0.611%
2	7.101	702	708	723	rBV	712071	1283591	13.40%	1.681%
3	7.307	736	743	761	rBV	818697	1627912	17.00%	2.132%
4	7.772	814	822	839	rBV	704040	1353713	14.14%	1.772%
5	8.495	938	945	962	rBV	650035	1367357	14.28%	1.790%
6	8.943	1014	1021	1040	rBV	1034827	1933212	20.19%	2.531%
7	9.666	1137	1144	1160	rBV	913648	1801317	18.81%	2.359%
8	10.207	1229	1236	1260	rBV	854681	2416066	25.23%	3.163%
9	10.572	1290	1298	1318	rVB	1122491	2020085	21.10%	2.645%
10	13.836	1846	1853	1871	rBV	3012572	4668794	48.76%	6.113%
11	14.119	1894	1901	1919	rBV	3538238	5229266	54.61%	6.847%
12	14.425	1946	1953	1967	rVB2	1877960	3037151	31.72%	3.977%
13	14.719	1993	2003	2017	rBV5	73157	312785	3.27%	0.410%
14	15.424	2116	2123	2139	rBV	4338485	6610157	69.03%	8.655%
15	15.572	2142	2148	2161	rVV	1061266	2061336	21.53%	2.699%
16	15.666	2161	2164	2174	rVB2	62813	108985	1.14%	0.143%
17	17.177	2414	2421	2431	rBV	2800437	3917049	40.90%	5.129%
18	17.277	2431	2438	2458	rVB	4802539	7391776	77.19%	9.678%
19	19.212	2762	2767	2776	rBV	67034	121493	1.27%	0.159%
20	19.336	2784	2788	2799	rBV9	60334	139636	1.46%	0.183%
21	19.571	2822	2828	2851	rBV	6310390	9036905	94.37%	11.833%
22	21.359	3127	3132	3141	rBV	3271417	4925936	51.44%	6.450%
23	23.512	3490	3498	3513	rVB2	4795327	9575971	100.00%	12.538%
24	23.653	3516	3522	3540	rVB2	2280366	4966656	51.87%	6.503%


Sum of corrected areas: 76373530

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102017\
Data File : BM012331.D
Acq On : 20 Oct 2017 22:11
Operator : SJ/JU
Sample : I5846-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE2P6

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

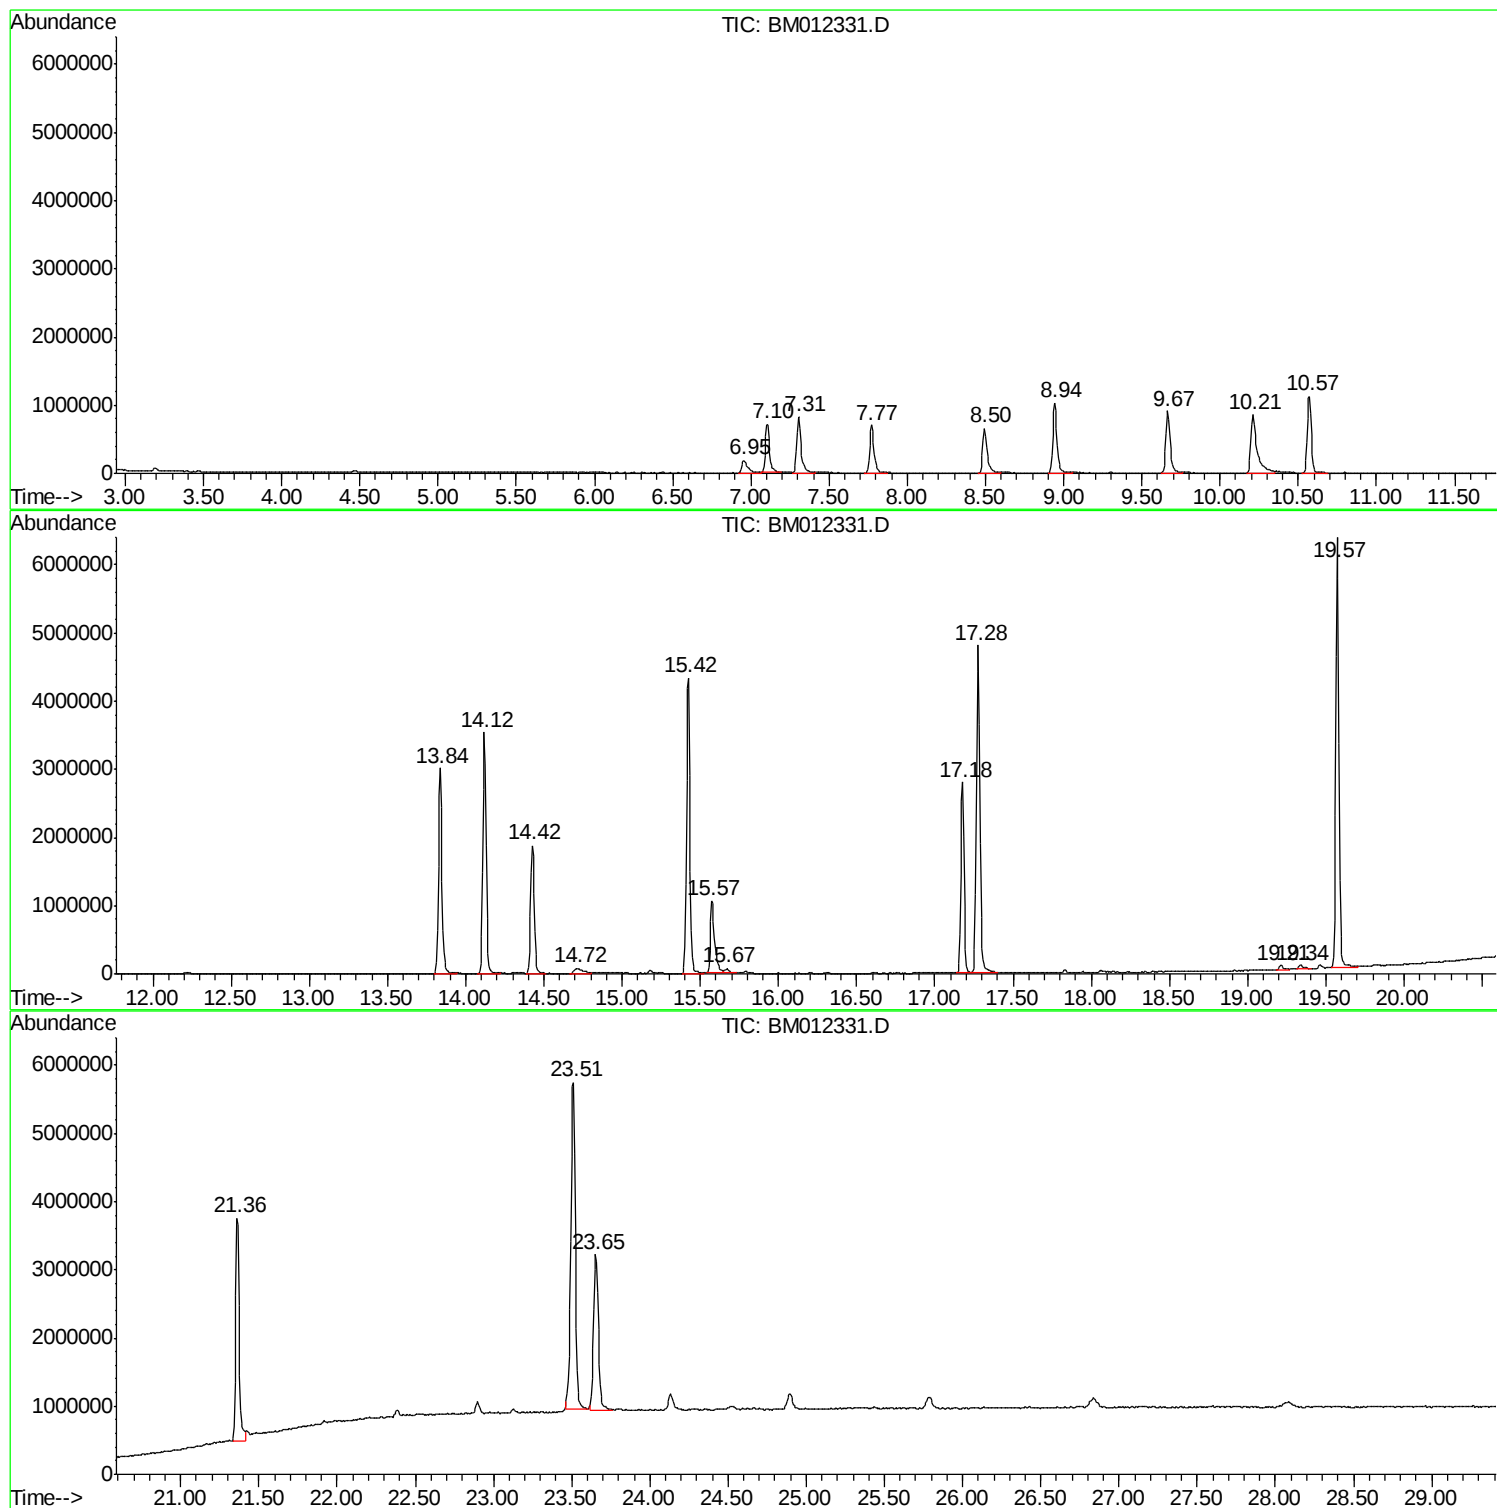

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM102017\
Data File : BM012331.D
Acq On : 20 Oct 2017 22:11
Operator : SJ/JU
Sample : I5846-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE2P6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM102017\
Data File : BM012331.D
Acq On : 20 Oct 2017 22:11
Operator : SJ/JU
Sample : I5846-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE2P6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc