

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102117\
 Data File : BM012352.D
 Acq On : 21 Oct 2017 10:58
 Operator : SJ/JU
 Sample : PB103266
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 23 05:02:29 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 23 05:01:01 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	149380	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	694310	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.42	164	449060	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	1090501	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	1319777	20.00	ng/ul	0.00
83) Perylene-d12	23.65	264	1209739	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.19	96	22945	7.30	ng/uL	0.00
5) Phenol-d5	6.94	99	407711	33.64	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	264420	36.38	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	374596	36.44	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	382622	36.67	ng/ul	0.00
19) Nitrobenzene-d5	8.94	128	182010	34.35	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	220866	35.67	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	383248	32.42	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	513853	46.45	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	1412390	35.59	ng/ul	0.00
46) Acenaphthylene-d8	14.11	160	1729950	36.01	ng/ul	0.00
51) 4-Nitrophenol-d4	14.67	143	137720	23.08	ng/ul	0.00
57) Fluorene-d10	15.42	176	1223235	37.55	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.57	200	175887	23.50	ng/ul	0.00
70) Anthracene-d10	17.27	188	1971371	36.56	ng/ul	0.00
76) Pyrene-d10	19.57	212	2332482	34.82	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.51	264	2136419	36.63	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	8.49	70	10781	1.268	ng/ul# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102117\
Data File : BM012352.D
Acq On : 21 Oct 2017 10:58
Operator : SJ/JU
Sample : PB103266
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 23 05:02:29 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 23 05:01:01 2017
Response via : Initial Calibration

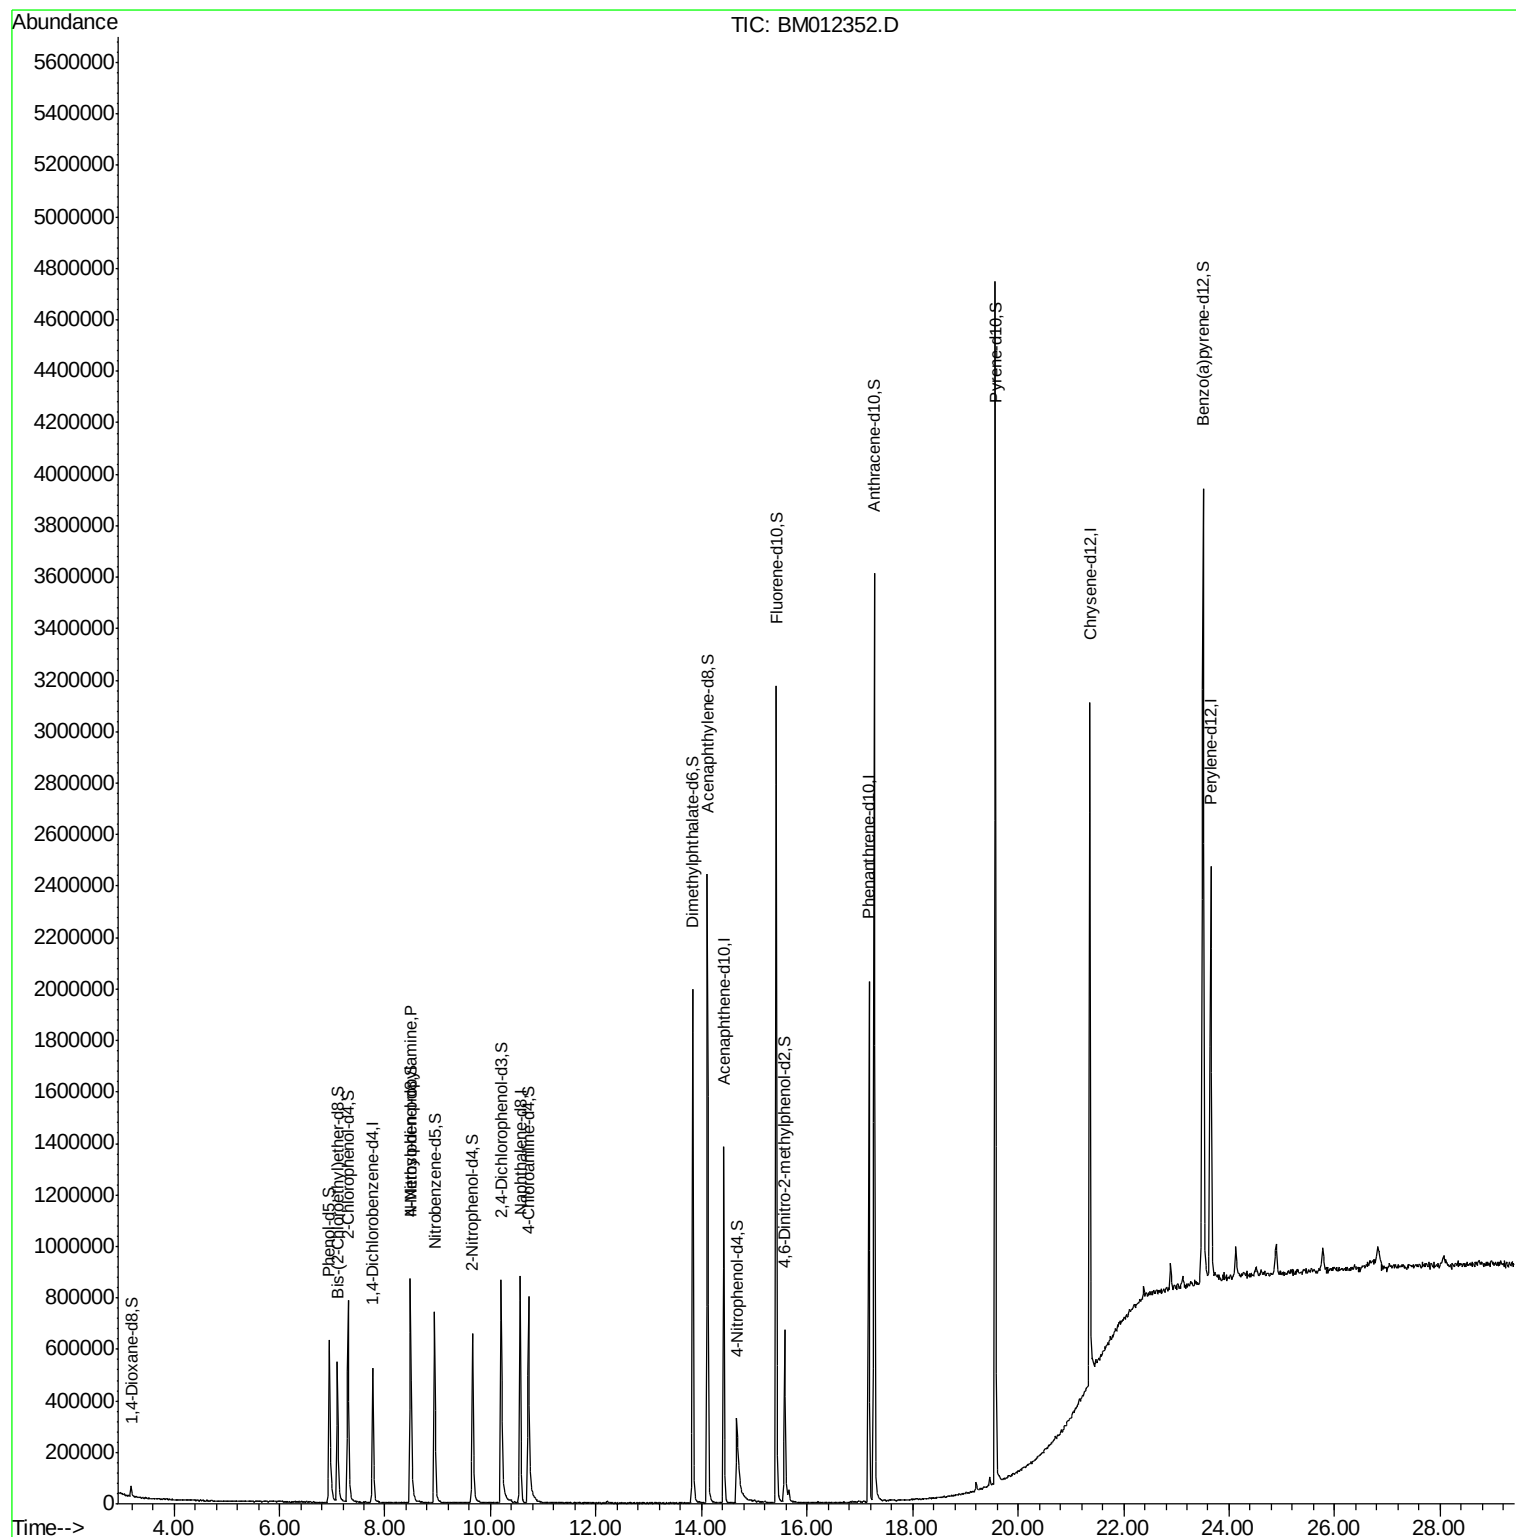

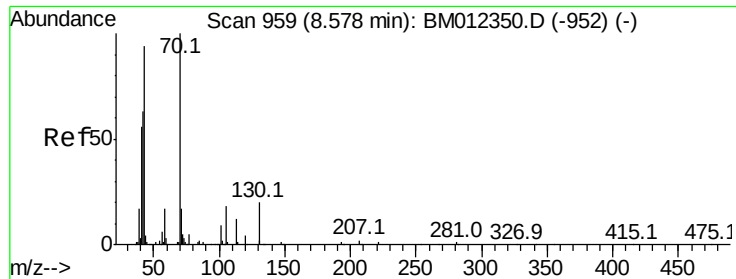

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.268 ng/ul
 RT: 8.49 min Scan# 944
 Delta R.T. -0.09 min
 Lab File: BM012352.D
 Acq: 21 Oct 2017 10:58

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
70	100		
42	371.5	43.0	64.4#
101	0.0	8.2	12.2#
130	0.0	18.6	28.0#

