

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102117\
 Data File : BM012377.D
 Acq On : 22 Oct 2017 02:06
 Operator : SJ/JU
 Sample : I5771-17
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 23 07:40:55 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 23 07:28:58 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	231138	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	1018356	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.42	164	652828	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	1494863	20.00	ng/ul	0.00
75) Chrysene-d12	21.35	240	1195660	20.00	ng/ul	0.00
83) Perylene-d12	23.64	264	992850	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.19	96	24294	4.99	ng/uL	0.00
5) Phenol-d5	6.94	99	535167	28.54	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	340171	30.25	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	482217	30.31	ng/ul	0.00
13) 4-Methylphenol-d8	8.48	113	502577	31.13	ng/ul	0.00
19) Nitrobenzene-d5	8.94	128	235715	30.33	ng/ul	0.00
22) 2-Nitrophenol-d4	9.65	143	288526	31.77	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	521817	30.10	ng/ul	0.00
29) 4-Chloroaniline-d4	10.71	131	626899	38.64	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	1947157	33.75	ng/ul	0.00
46) Acenaphthylene-d8	14.11	160	2288530	32.77	ng/ul	0.00
51) 4-Nitrophenol-d4	14.67	143	186588	21.51	ng/ul	0.00
57) Fluorene-d10	15.41	176	1612707	34.05	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.57	200	241070	23.50	ng/ul	0.00
70) Anthracene-d10	17.27	188	2551106	34.51	ng/ul	0.00
76) Pyrene-d10	19.57	212	2696062	44.42	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.50	264	1690434	35.32	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.88	163	76272	1.319	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102117\
Data File : BM012377.D
Acq On : 22 Oct 2017 02:06
Operator : SJ/JU
Sample : I5771-17
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 23 07:40:55 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 23 07:28:58 2017
Response via : Initial Calibration

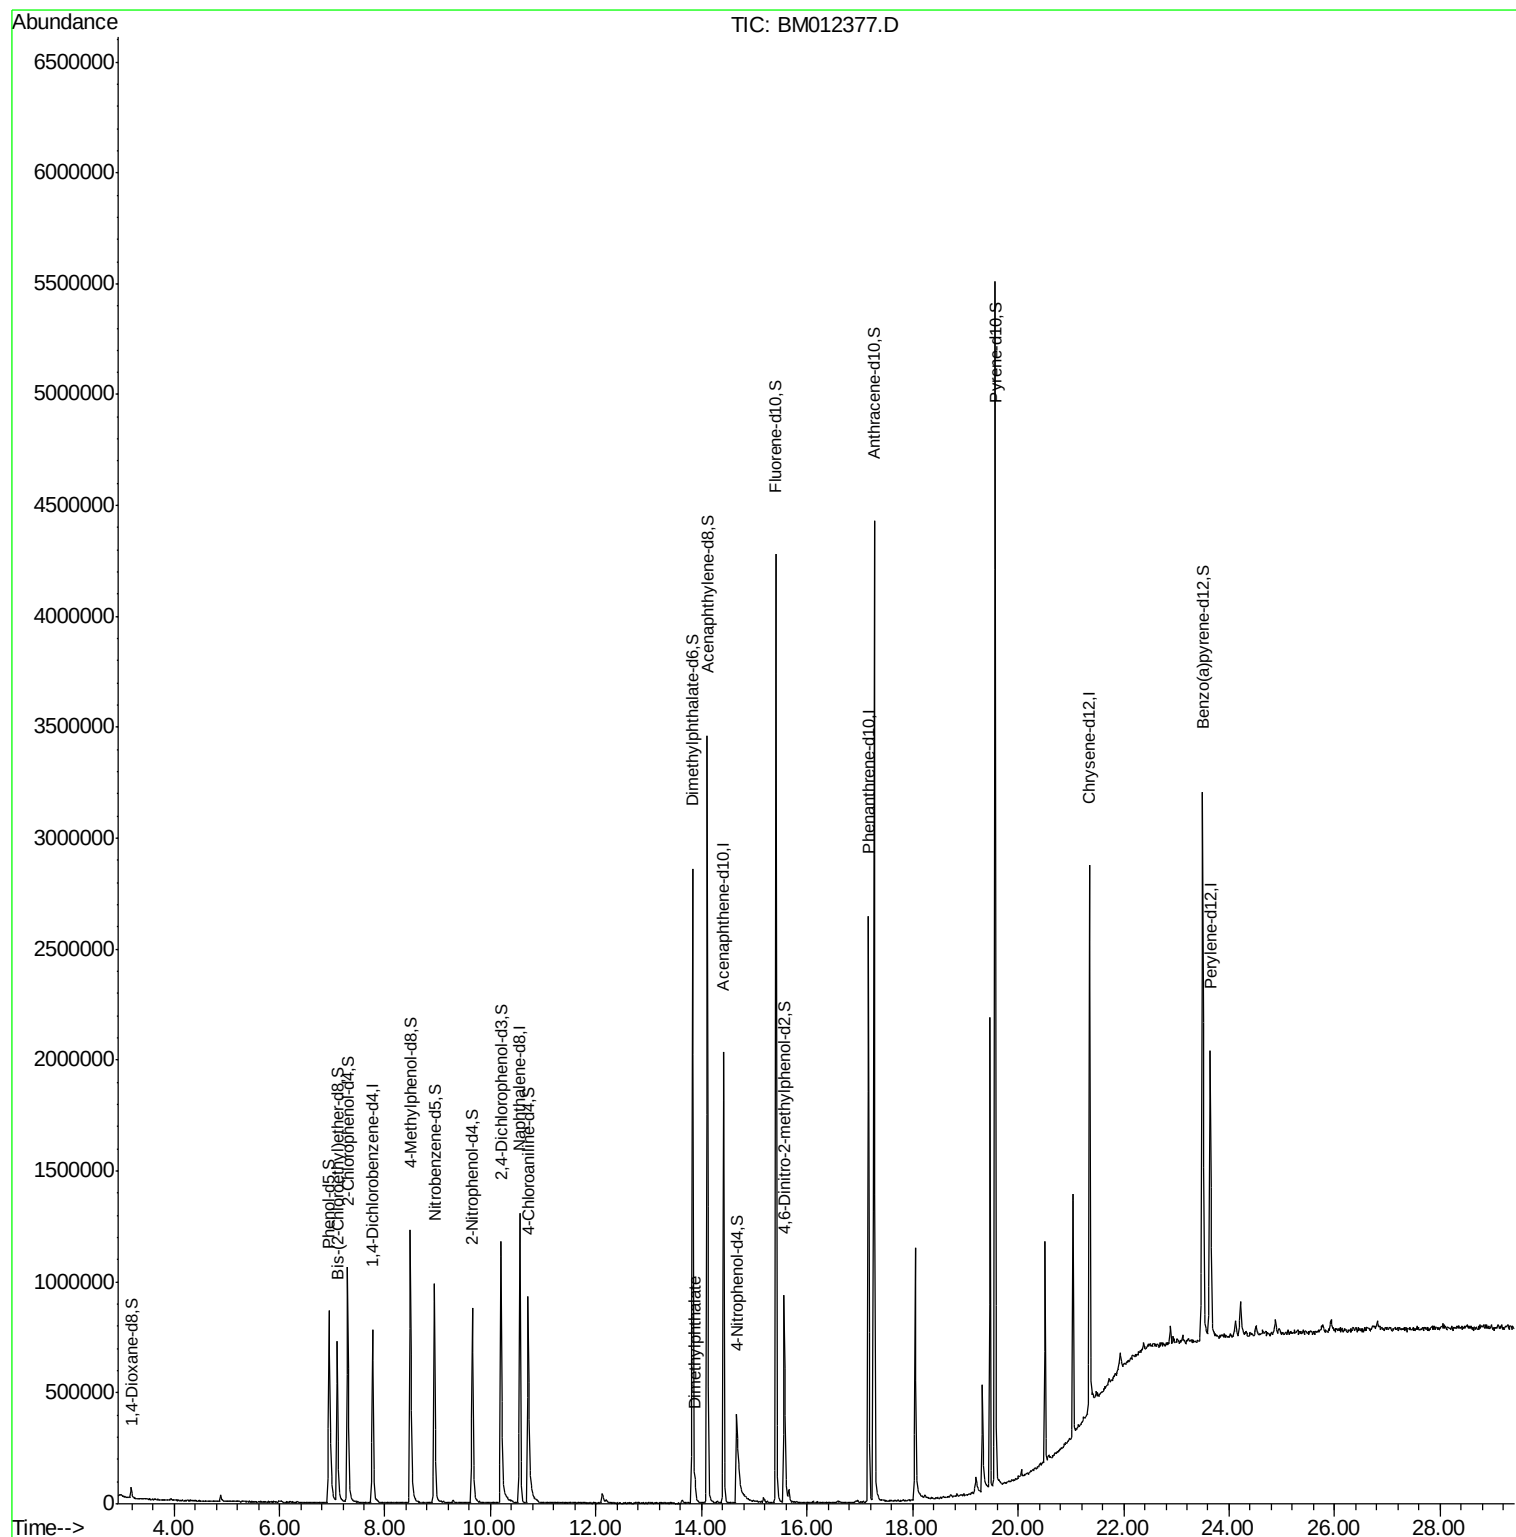

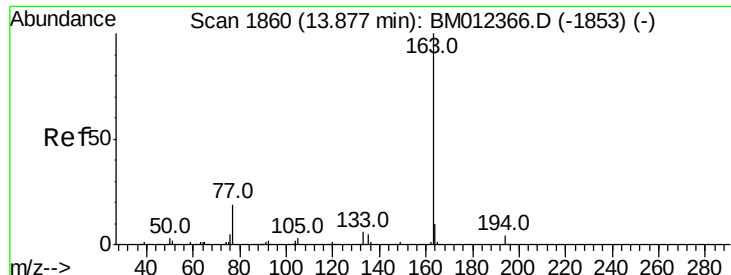

#44

Dimethylphthalate

Concen: 1.319 ng/ul

RT: 13.88 min Scan# 1860

Delta R.T. 0.00 min

Lab File: BM012377.D

Acq: 22 Oct 2017 02:06

Instrument :

BNA_M

ClientSampleId :


Tot Ion:163 Resp: 76272

Ion Ratio Lower Upper

163 100

194 4.0 3.7 5.5

164 11.0 8.1 12.1

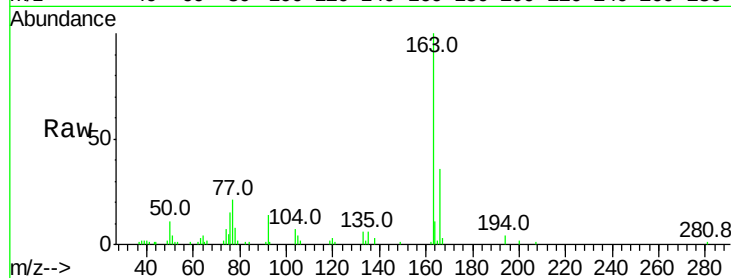

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

