

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102117\
 Data File : BM012374.D
 Acq On : 22 Oct 2017 00:17
 Operator : SJ/JU
 Sample : I5771-14
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 B0CX1

Manual Integrations
 APPROVED

Sohil
 10/23/2017 4:00:23 PM

Quant Time: Oct 23 08:00:50 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 23 07:28:58 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	211325	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	952888	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.42	164	616315	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	1436461	20.00	ng/ul	0.00
75) Chrysene-d12	21.35	240	1365986	20.00	ng/ul	0.00
83) Perylene-d12	23.64	264	1075423	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.19	96	19860	4.47	ng/uL	0.00
5) Phenol-d5	6.94	99	392894	22.91	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	258428	25.13	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	357200	24.56	ng/ul	0.00
13) 4-Methylphenol-d8	8.48	113	335082	22.70	ng/ul	0.00
19) Nitrobenzene-d5	8.94	128	174751	24.03	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	212659	25.03	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	377730	23.29	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	420437	27.69	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	1515618	27.82	ng/ul	0.00
46) Acenaphthylene-d8	14.11	160	1724532	26.15	ng/ul	0.00
51) 4-Nitrophenol-d4	14.68	143	119227m	14.56	ng/ul	0.01
57) Fluorene-d10	15.41	176	1270948	28.43	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.57	200	170434	17.29	ng/ul	0.00
70) Anthracene-d10	17.27	188	2037413	28.68	ng/ul	0.00
76) Pyrene-d10	19.57	212	2246701	32.40	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.50	264	1492542	28.79	ng/ul	0.00
Target Compounds						
6) Phenol	6.97	94	72838	4.109	ng/ul#	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM102117\
Data File : BM012374.D
Acq On : 22 Oct 2017 00:17
Operator : SJ/JU
Sample : I5771-14
Misc :
ALS Vial : 26 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
B0CX1

Manual Integrations
APPROVED

Sohil
10/23/2017 4:00:23 PM

Quant Time: Oct 23 08:00:50 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM101217.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 23 07:28:58 2017
Response via : Initial Calibration

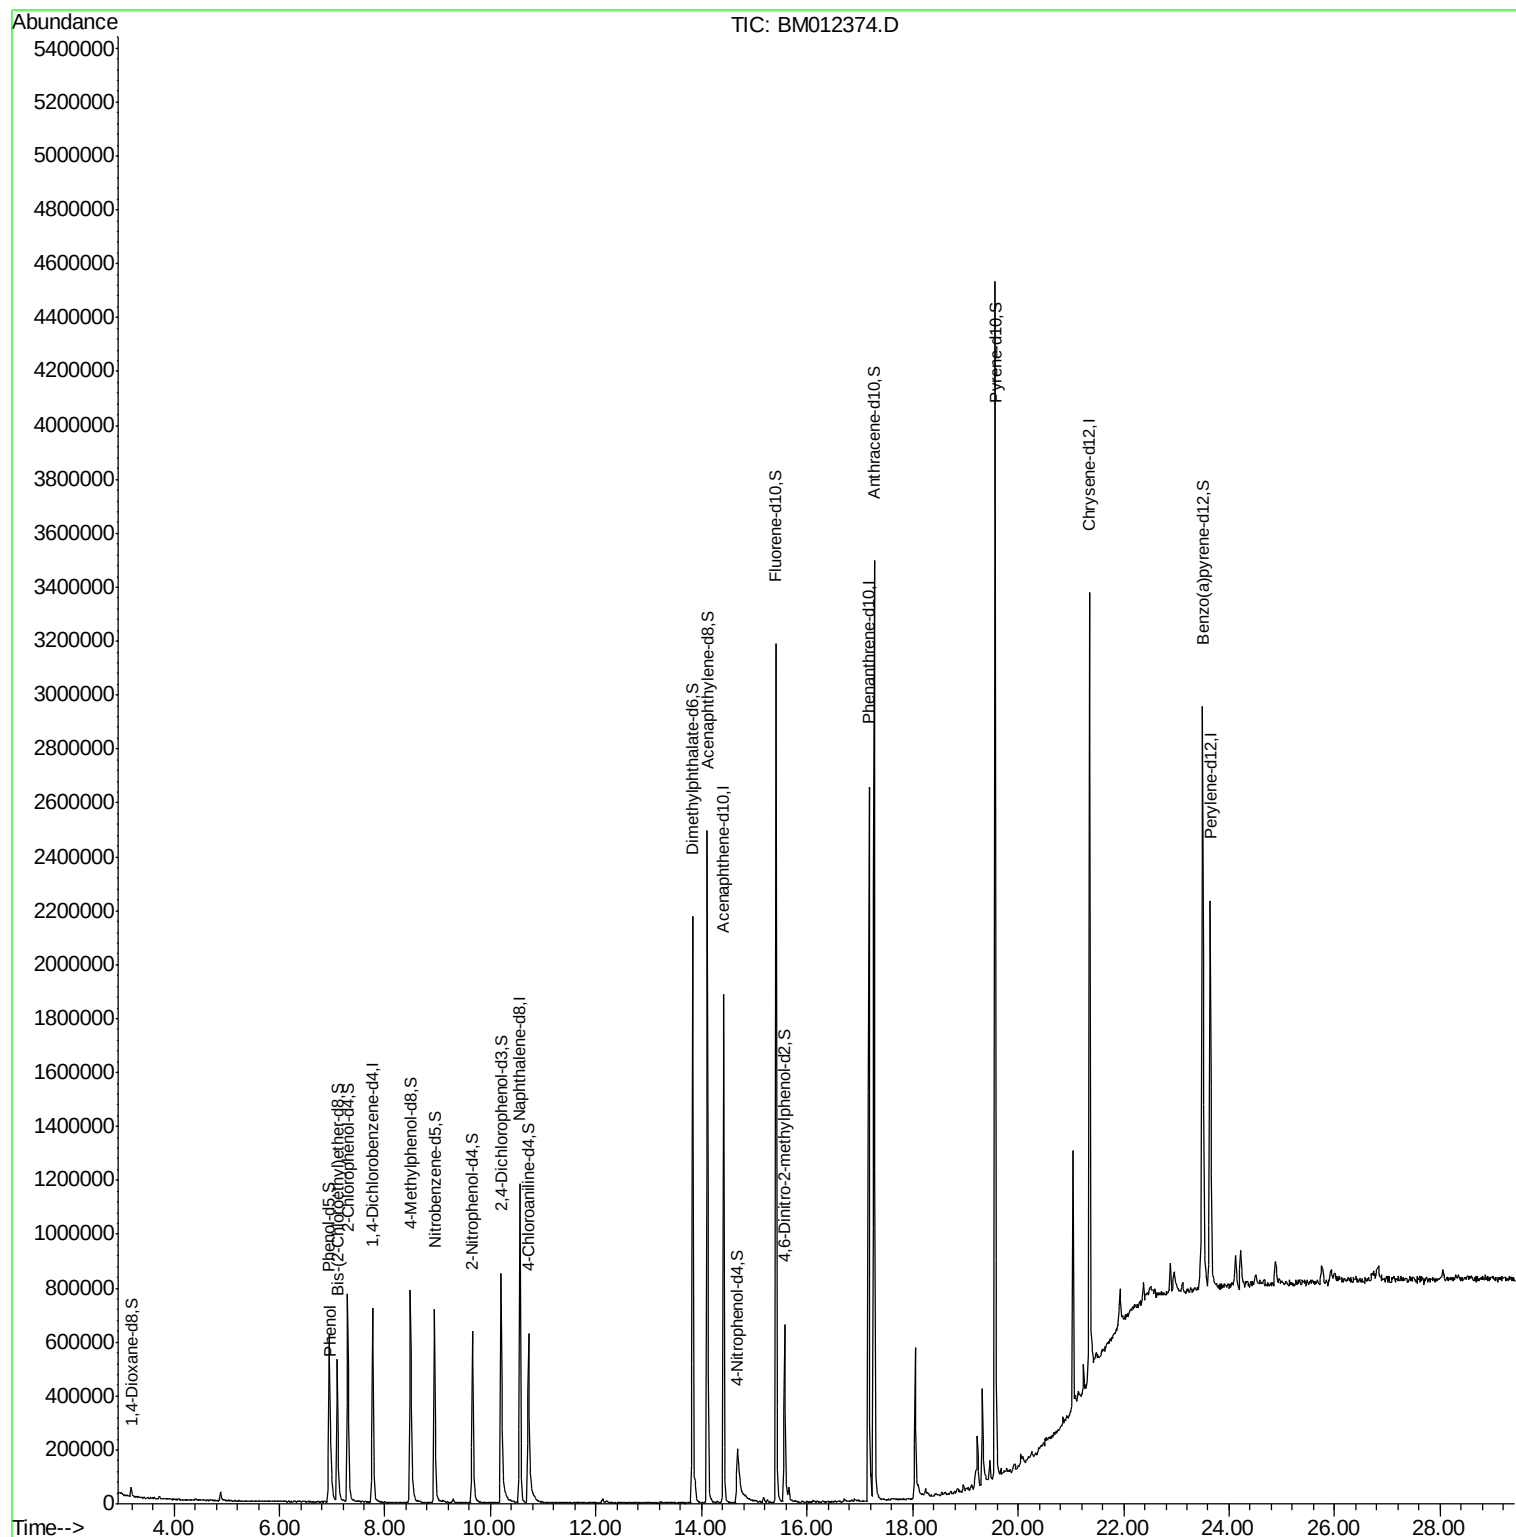

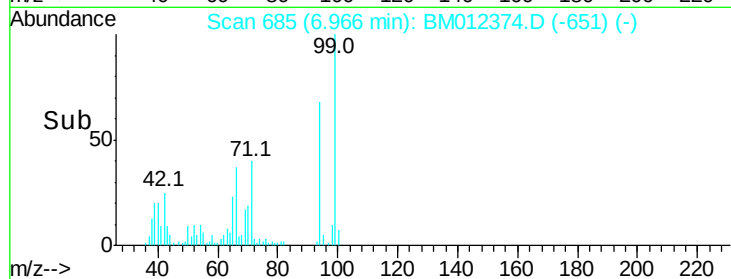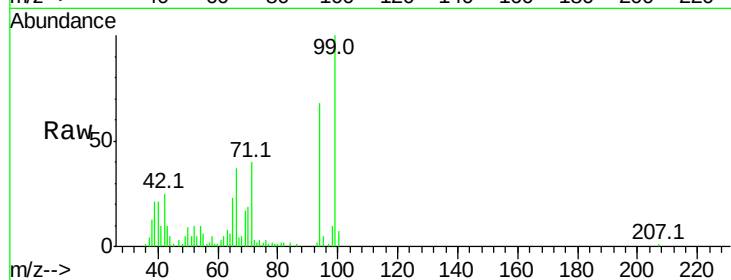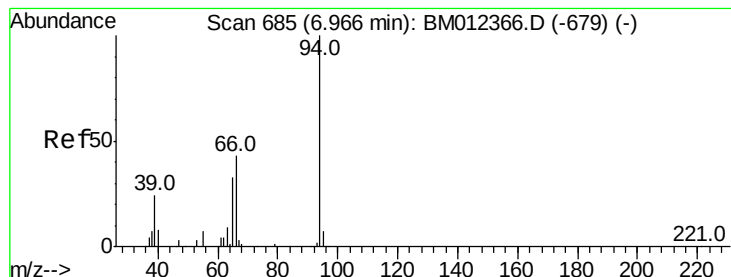

#6

Phenol

Concen: 4.109 ng/ul

RT: 6.97 min Scan# 685

Delta R.T. 0.00 min

Lab File: BM012374.D

Acq: 22 Oct 2017 00:17

Tot Ion	Ratio	Lower	Upper
94	100		
65	33.4	24.4	36.6
66	54.6	35.0	52.4

Instrument :

BNA_M

ClientSampleId :

B0CX1

Manual Integrations
APPROVED

Sohil
10/23/2017 4:00:23 PM

