




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048153.D
Acq On : 21 Oct 2024 13:59
Operator : RC/JU
Sample : P4380-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27G7

Manual IntegrationsAPPROVED

Quant Time: Oct 21 14:34:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 19 00:48:23 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

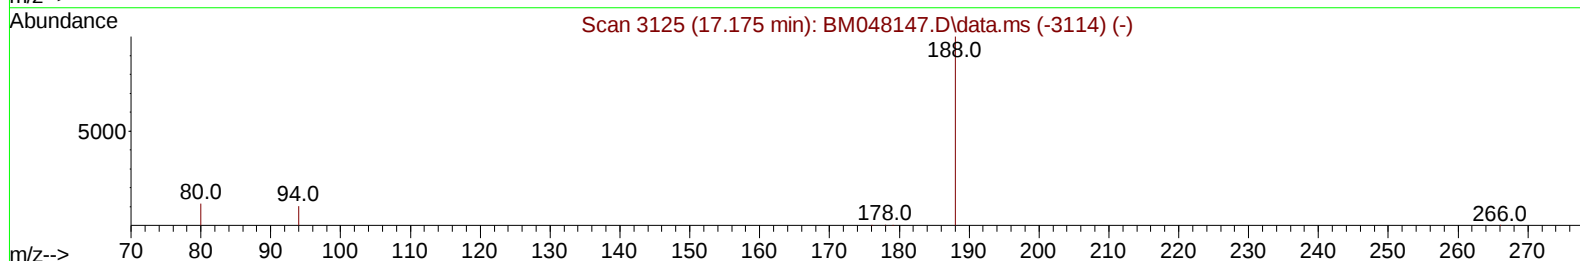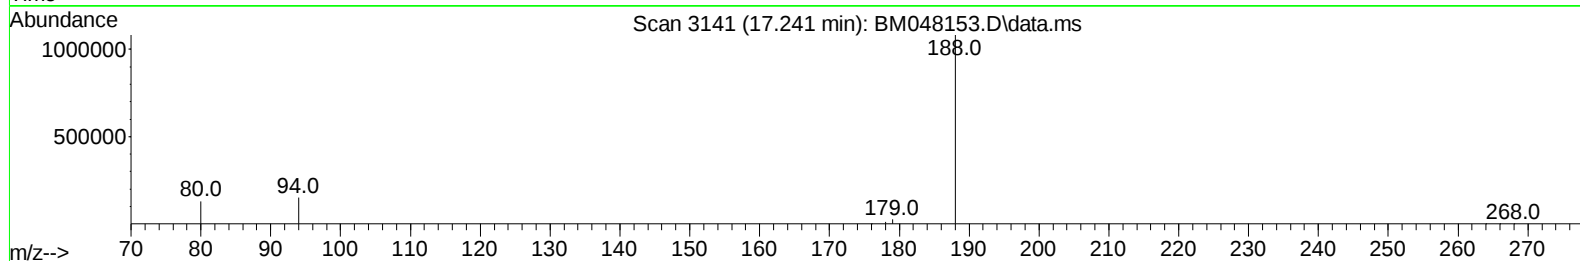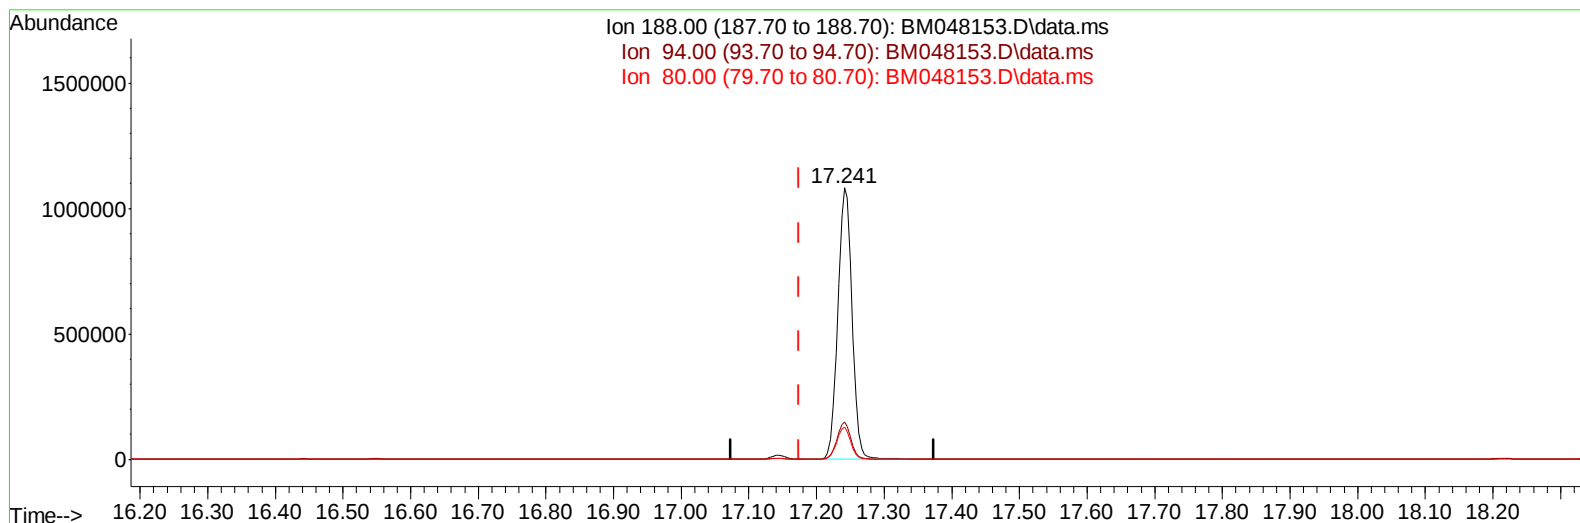

TIC: BM048153.D\data.ms

(13) Phenanthrene-d10 (I)

17.241min (+ 0.068) 0.40 ng/u1

response 1589157

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.80	13.84
80.00	12.40	11.95
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048153.D
Acq On : 21 Oct 2024 13:59
Operator : RC/JU
Sample : P4380-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27G7

Manual IntegrationsAPPROVED

Quant Time: Oct 21 14:34:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 19 00:48:23 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

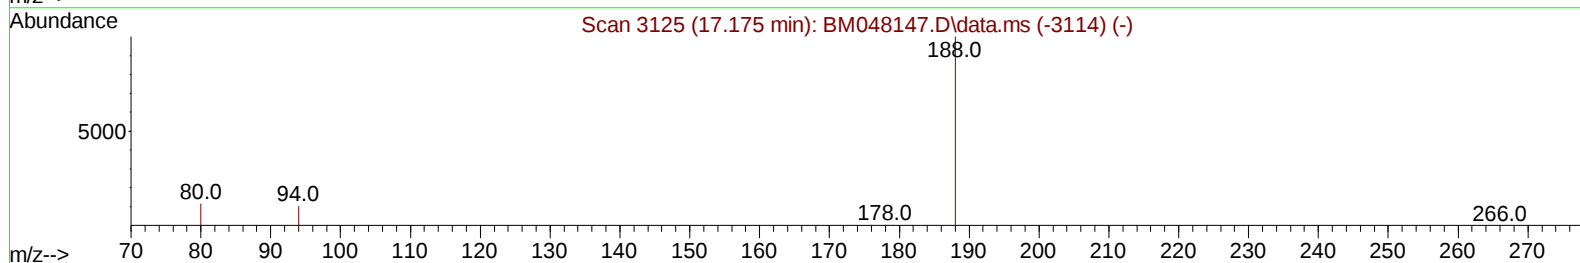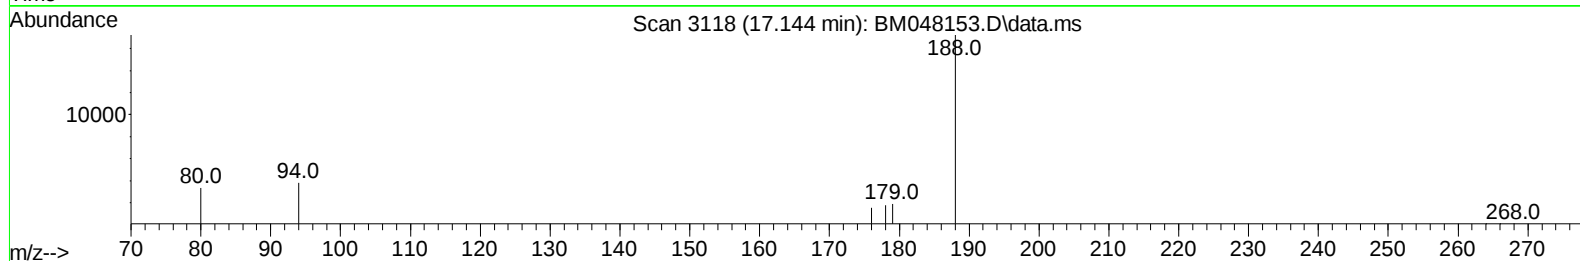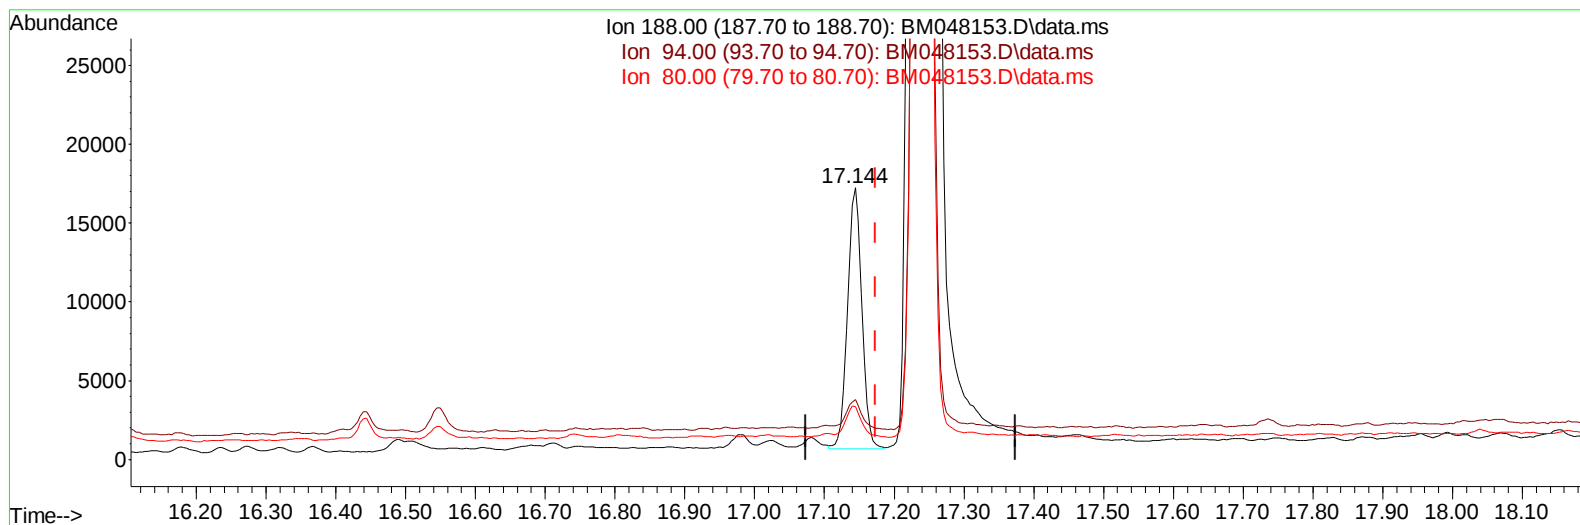

TIC: BM048153.D\data.ms

(13) Phenanthrene-d10 (I)

17.144min (-0.030) 0.40 ng/ul m

response 23539

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.80	22.09#
80.00	12.40	19.42#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048153.D
Acq On : 21 Oct 2024 13:59
Operator : RC/JU
Sample : P4380-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27G7

Manual IntegrationsAPPROVED

Quant Time: Oct 21 14:34:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 19 00:48:23 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

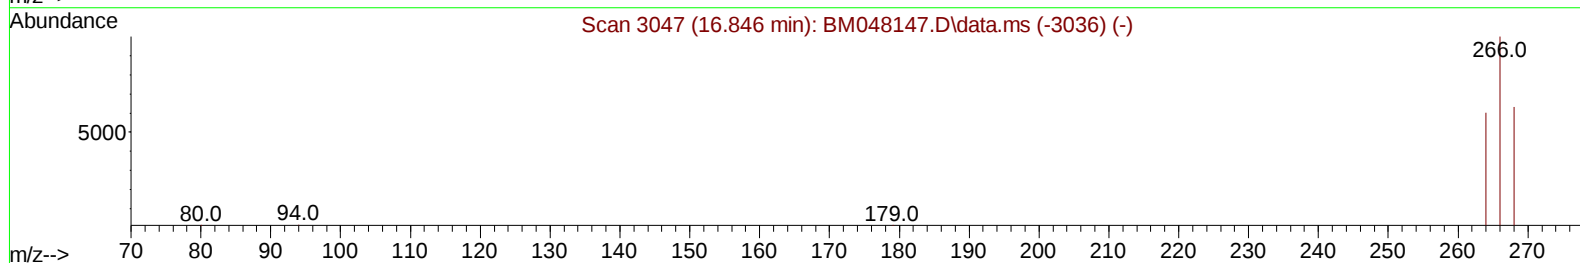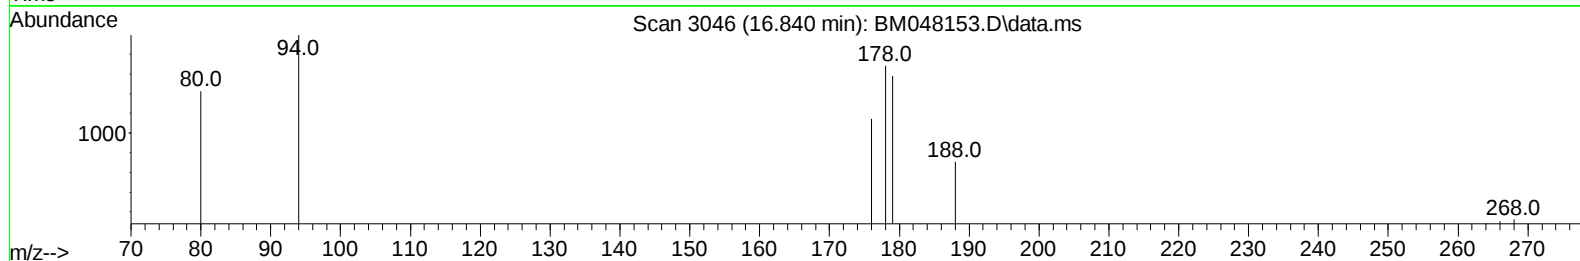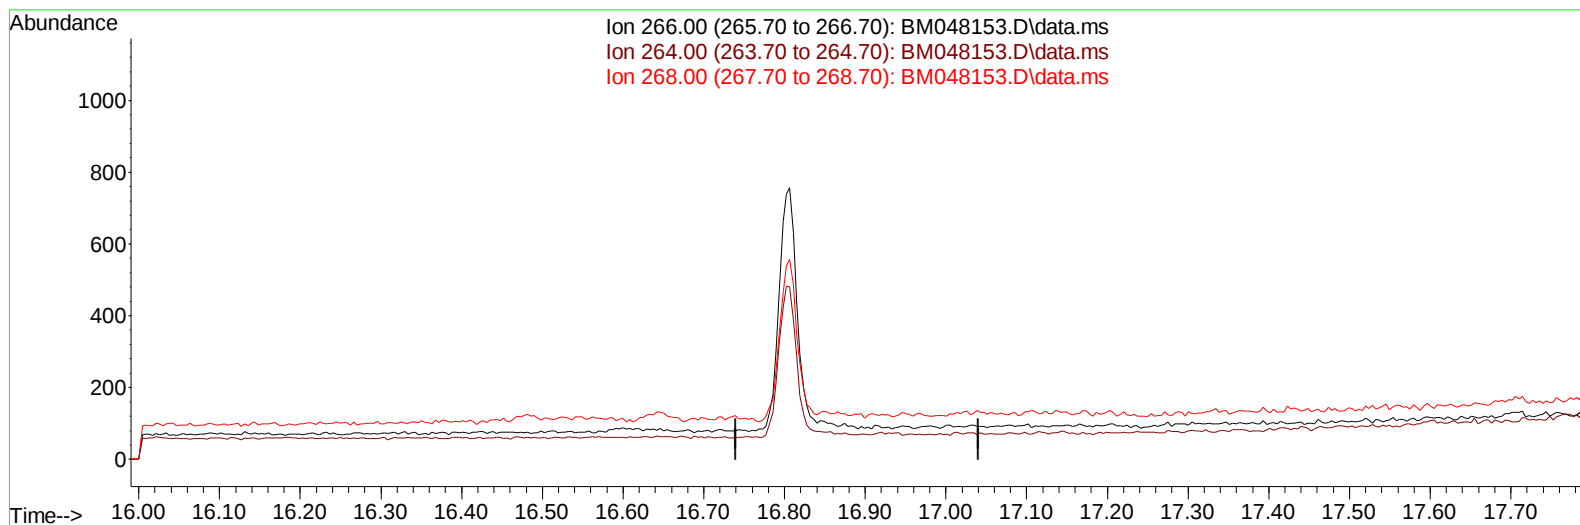

TIC: BM048153.D\data.ms

(14) Pentachlorophenol

16.840min (-16.840) 0.00 ng/ul

response 0

Ion	Exp%	Act%
266.00	100.00	0.00
264.00	62.70	0.00#
268.00	64.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048153.D
Acq On : 21 Oct 2024 13:59
Operator : RC/JU
Sample : P4380-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27G7

Manual IntegrationsAPPROVED

Quant Time: Oct 21 14:34:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 19 00:48:23 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

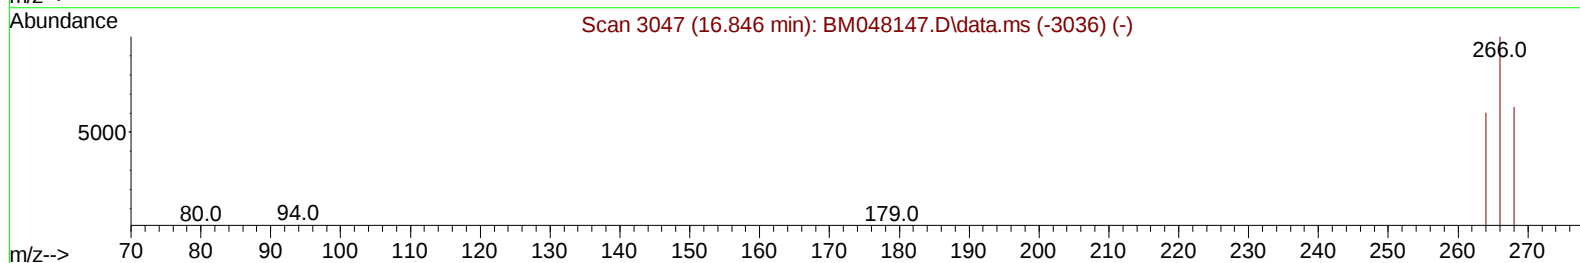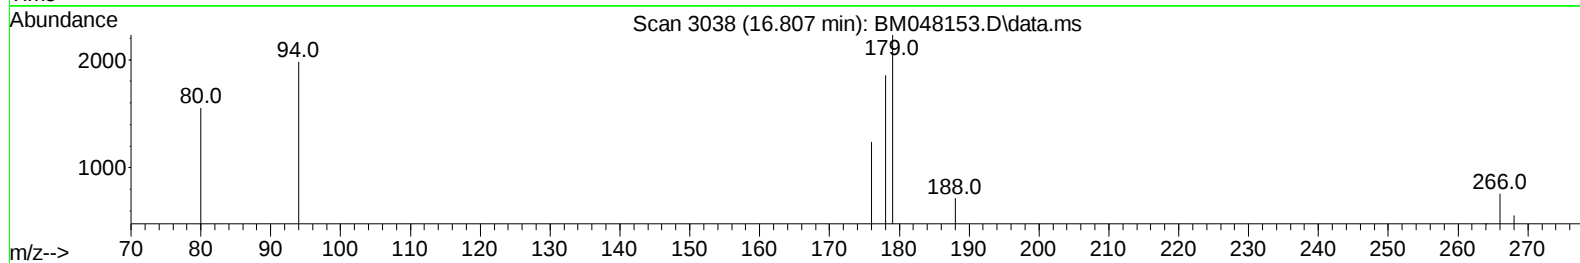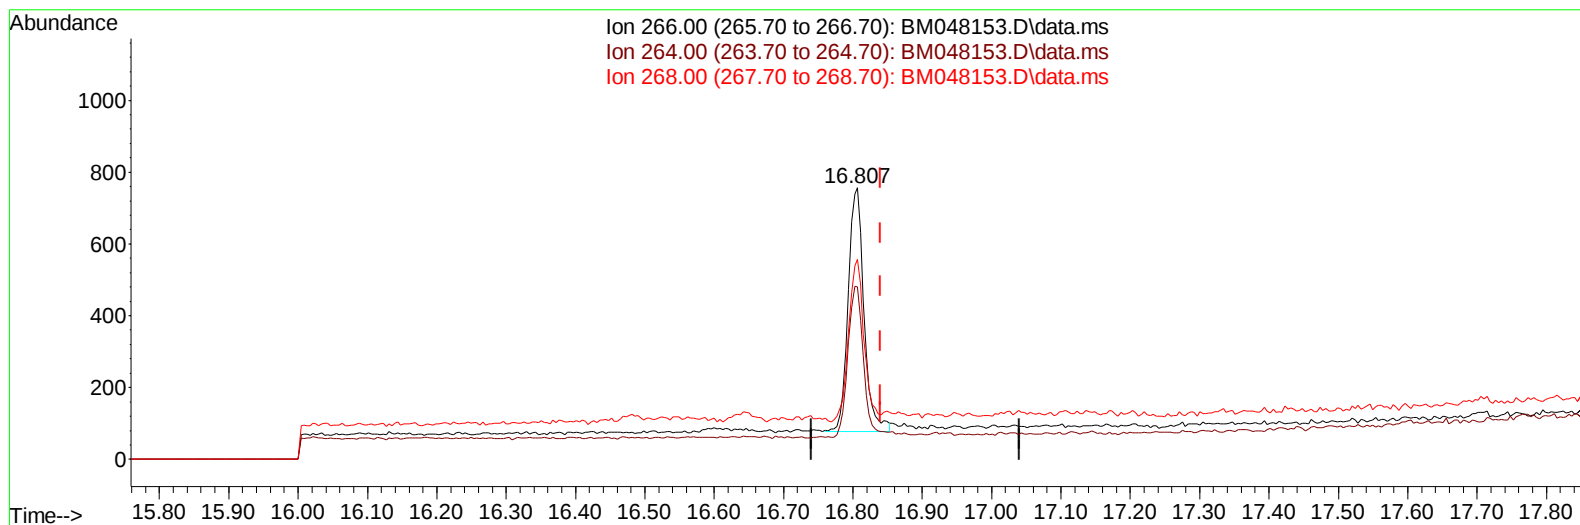

TIC: BM048153.D\data.ms

(14) Pentachlorophenol

16.807min (-0.034) 0.14 ng/ul m

response 1076

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	62.70	0.00#
268.00	64.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048153.D
Acq On : 21 Oct 2024 13:59
Operator : RC/JU
Sample : P4380-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27G7

Manual IntegrationsAPPROVED

Quant Time: Oct 21 14:34:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 19 00:48:23 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

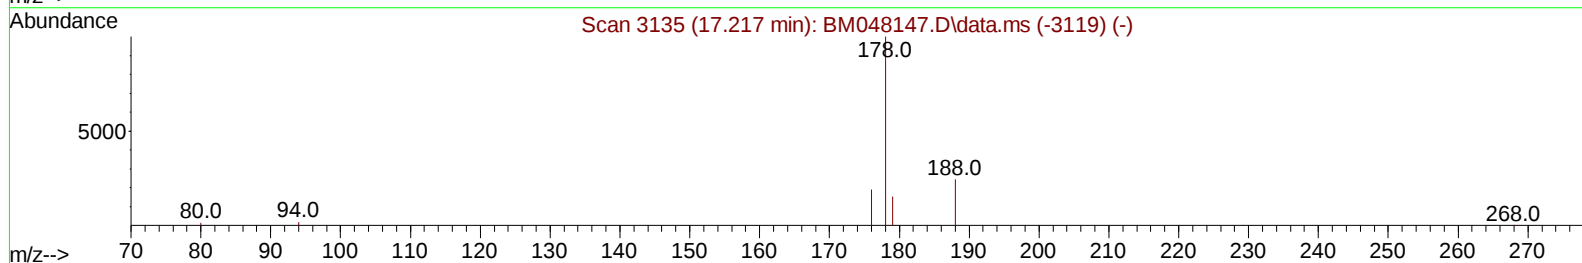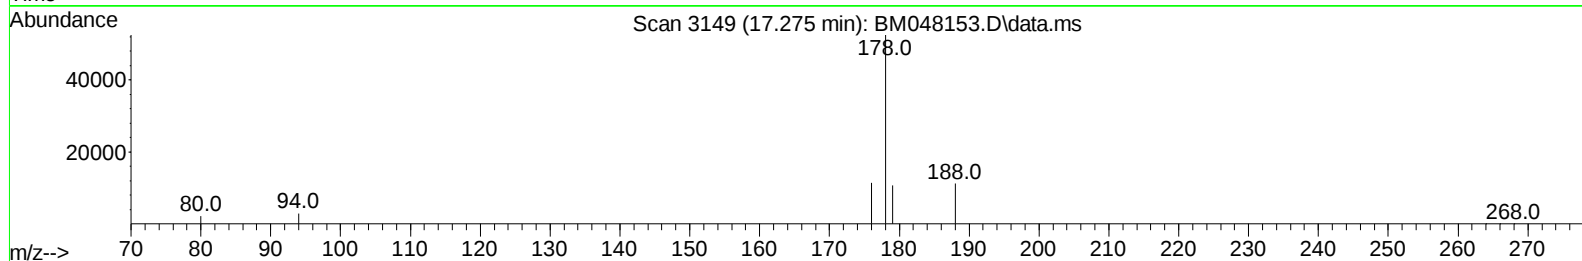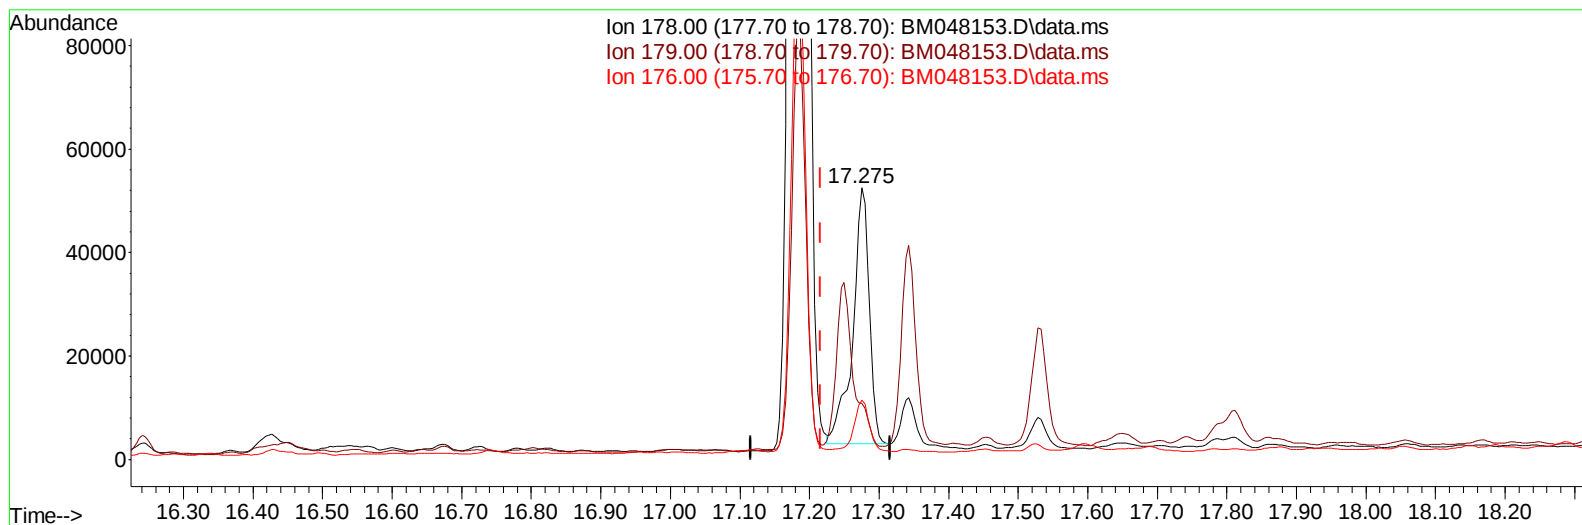

TIC: BM048153.D\data.ms

(15) Phenanthrene

17.275min (+ 0.059) 1.37 ng/u1

response 81395

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.50	20.57#
176.00	20.00	21.81
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
 Data File : BM048153.D
 Acq On : 21 Oct 2024 13:59
 Operator : RC/JU
 Sample : P4380-22
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E27G7

Manual IntegrationsAPPROVED

Quant Time: Oct 21 14:34:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 19 00:48:23 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
 Supervised By :mohammad ahmed 10/23/2024

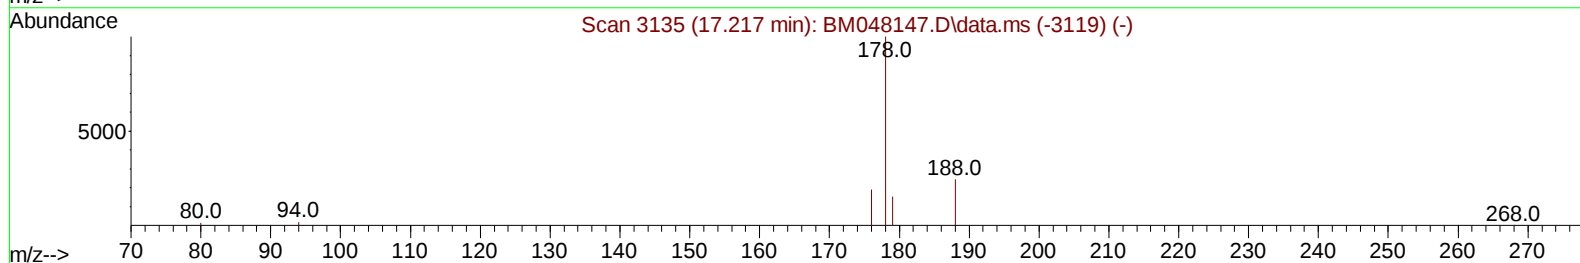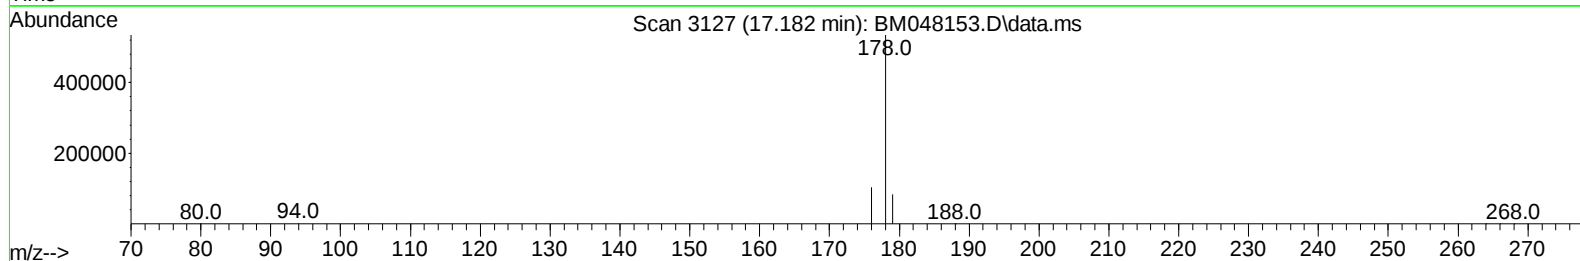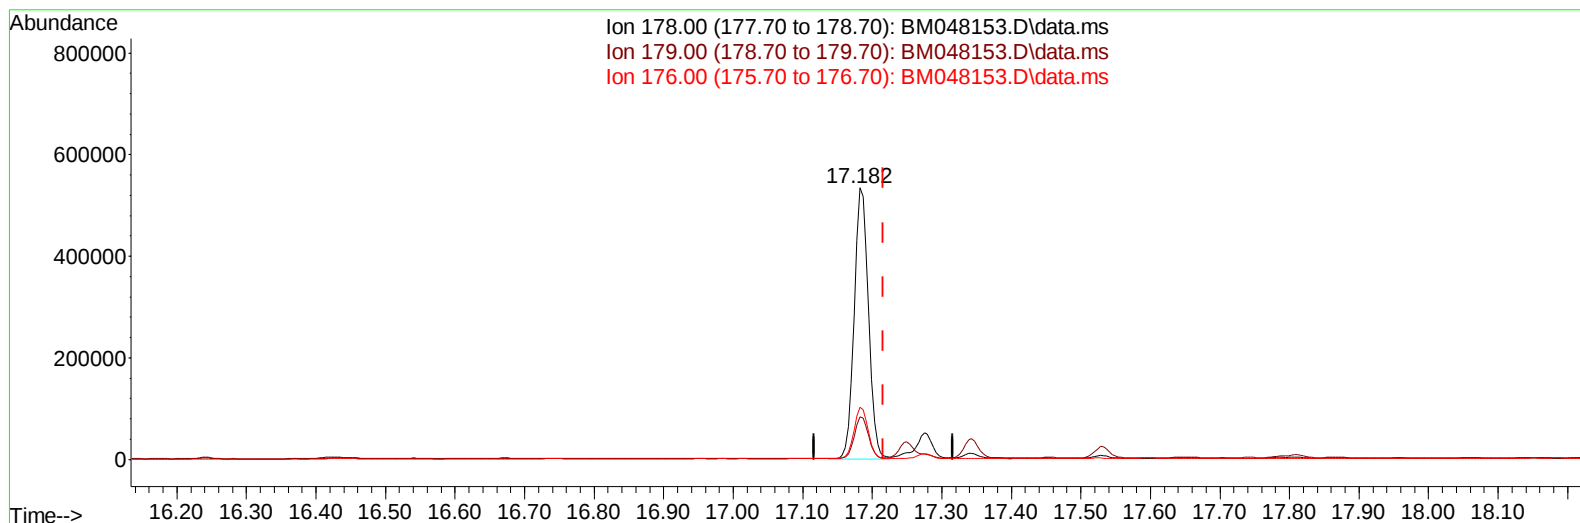

TIC: BM048153.D\data.ms

(15) Phenanthrene

17.182min (-0.034) 12.72 ng/ul m

response 756615

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.50	15.66
176.00	20.00	19.30
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048153.D
Acq On : 21 Oct 2024 13:59
Operator : RC/JU
Sample : P4380-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27G7

Manual IntegrationsAPPROVED

Quant Time: Oct 21 14:34:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 19 00:48:23 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

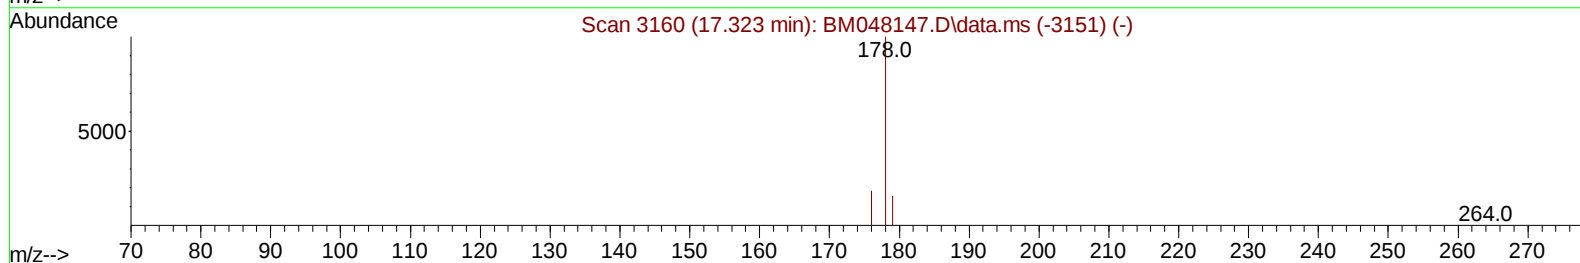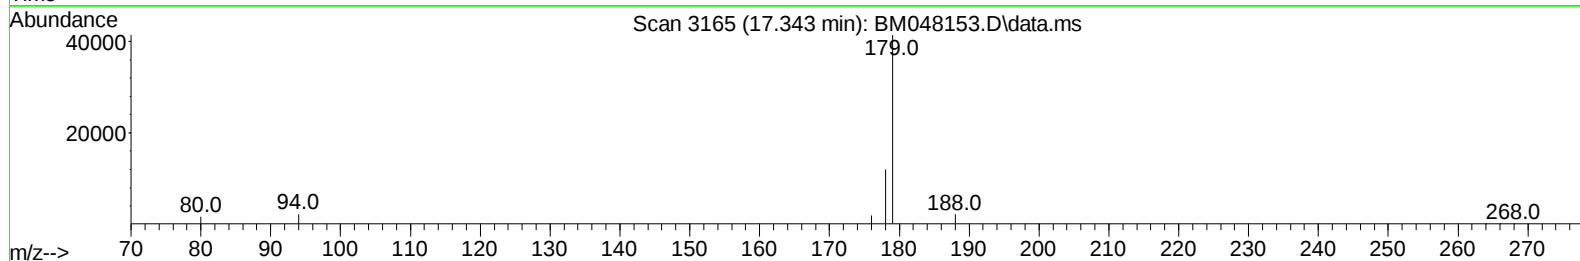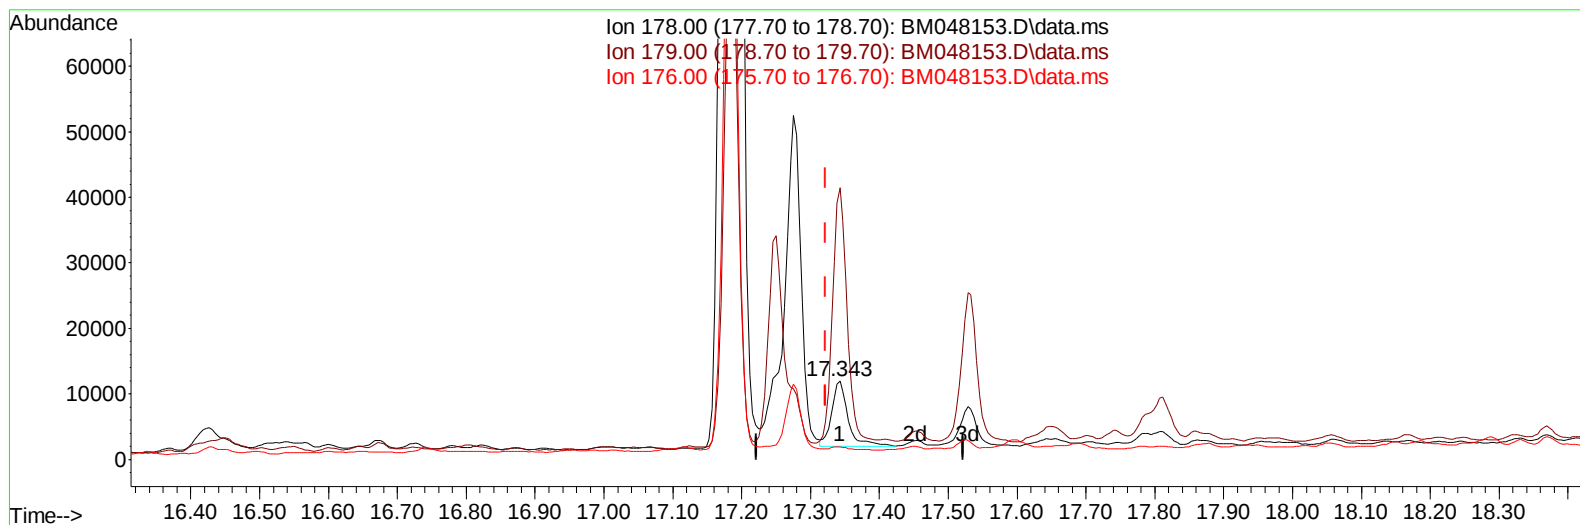

TIC: BM048153.D\data.ms

(16) Anthracene

17.343min (+ 0.021) 0.29 ng/u1

response 16304

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	18.10	345.25#
176.00	20.00	16.23
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048153.D
Acq On : 21 Oct 2024 13:59
Operator : RC/JU
Sample : P4380-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27G7

Manual IntegrationsAPPROVED

Quant Time: Oct 21 14:34:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 19 00:48:23 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

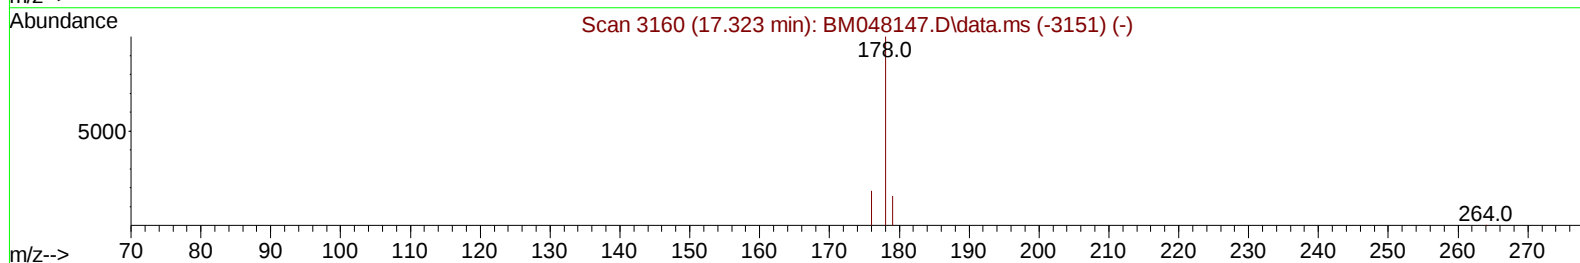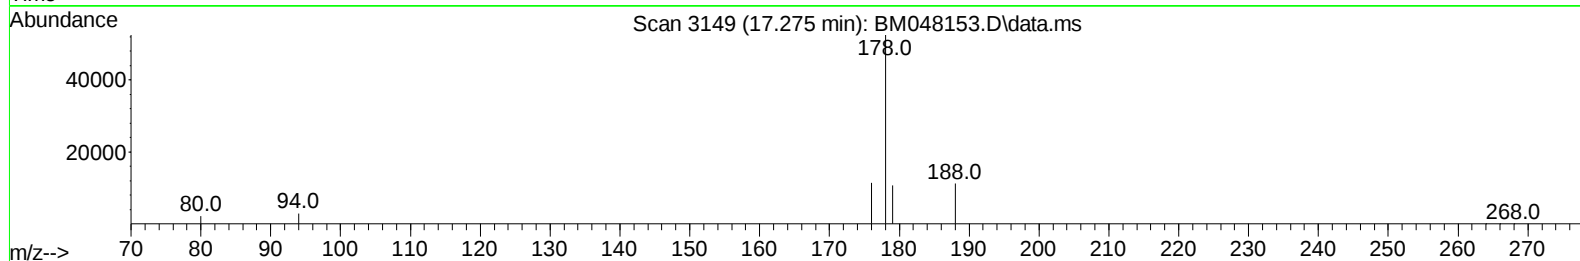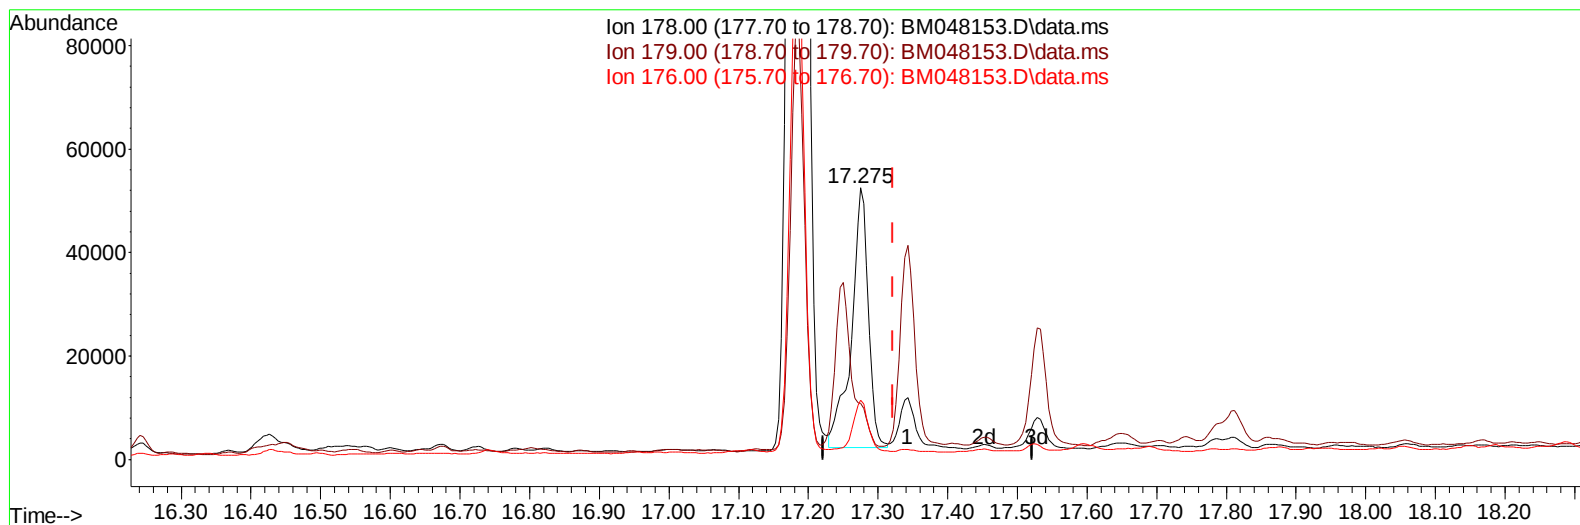

TIC: BM048153.D\data.ms

(16) Anthracene

17.275min (-0.046) 1.50 ng/ul m

response 84427

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	18.10	20.57
176.00	20.00	21.81
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048153.D
Acq On : 21 Oct 2024 13:59
Operator : RC/JU
Sample : P4380-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27G7

Manual IntegrationsAPPROVED

Quant Time: Oct 21 14:34:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 19 00:48:23 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

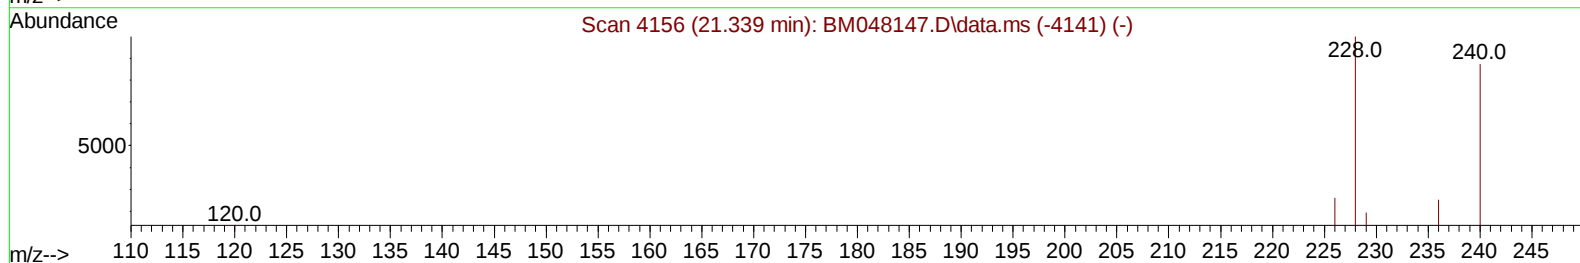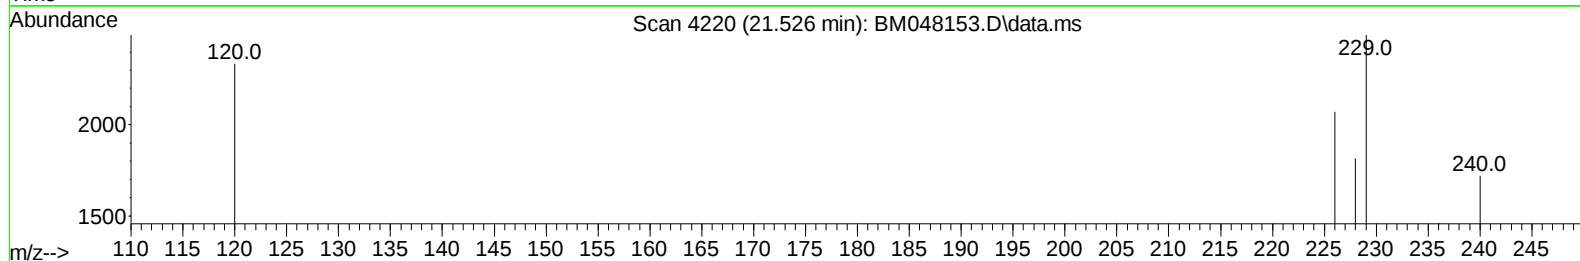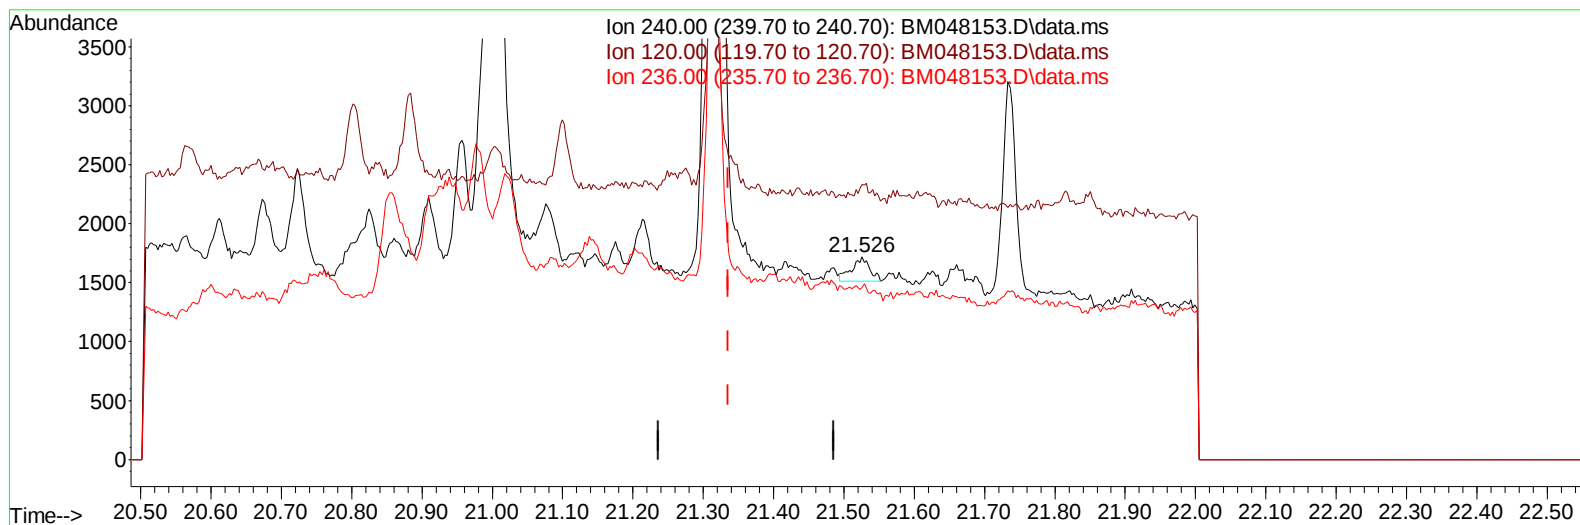

TIC: BM048153.D\data.ms

(17) Chrysene-d12

21.526min (+ 0.190) 0.40 ng/u1

response 356

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	22.80	135.76#
236.00	30.60	84.71#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048153.D
Acq On : 21 Oct 2024 13:59
Operator : RC/JU
Sample : P4380-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27G7

Manual IntegrationsAPPROVED

Quant Time: Oct 21 14:34:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 19 00:48:23 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

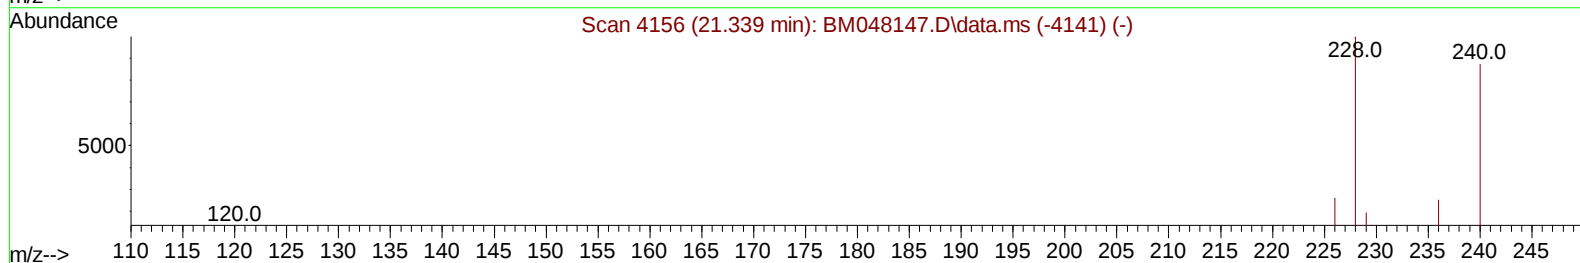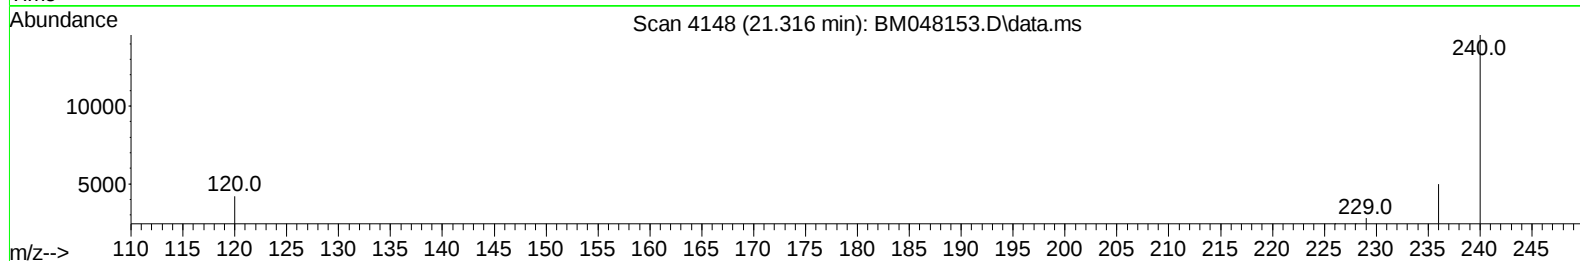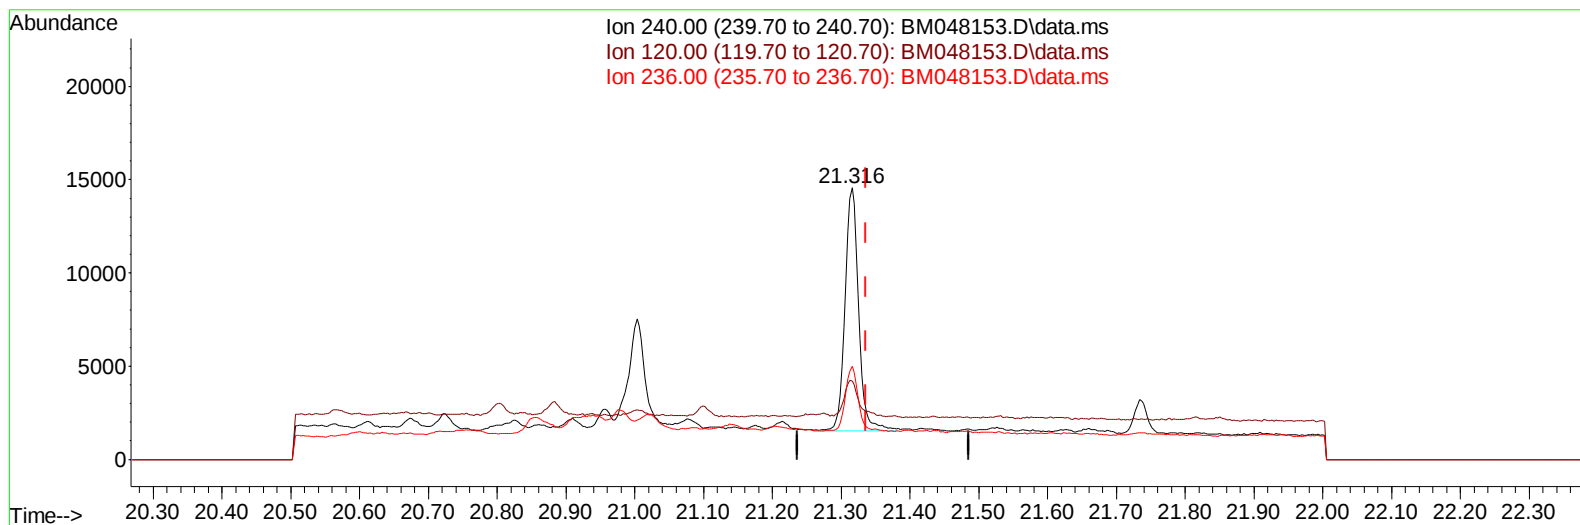

TIC: BM048153.D\data.ms

(17) Chrysene-d12

21.316min (-0.020) 0.40 ng/u1 m

response 17749

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	22.80	29.01#
236.00	30.60	34.30
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048153.D
Acq On : 21 Oct 2024 13:59
Operator : RC/JU
Sample : P4380-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27G7

Manual IntegrationsAPPROVED

Quant Time: Oct 21 14:34:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 19 00:48:23 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

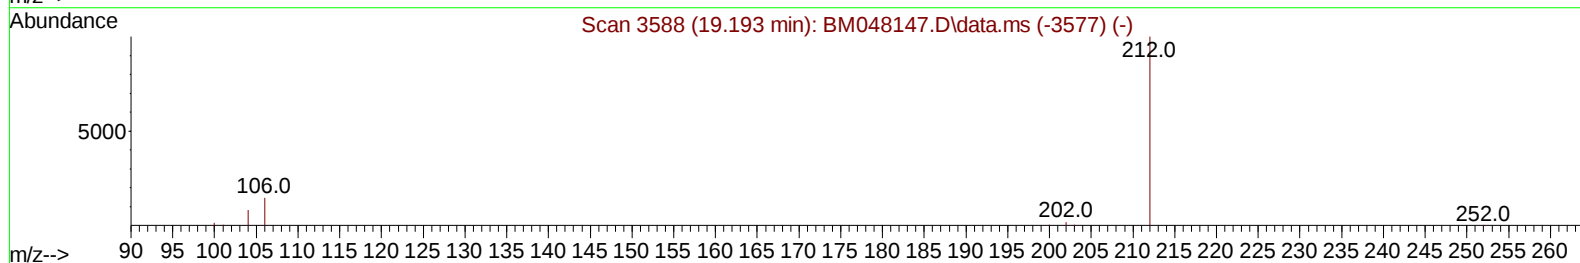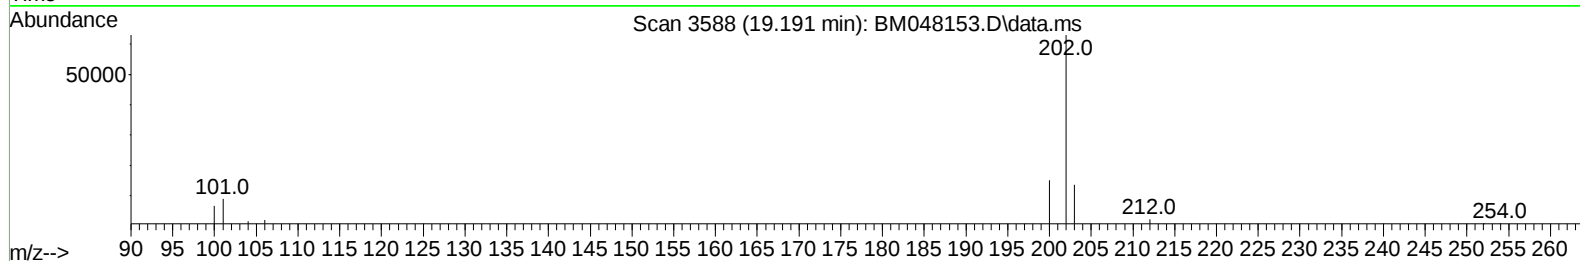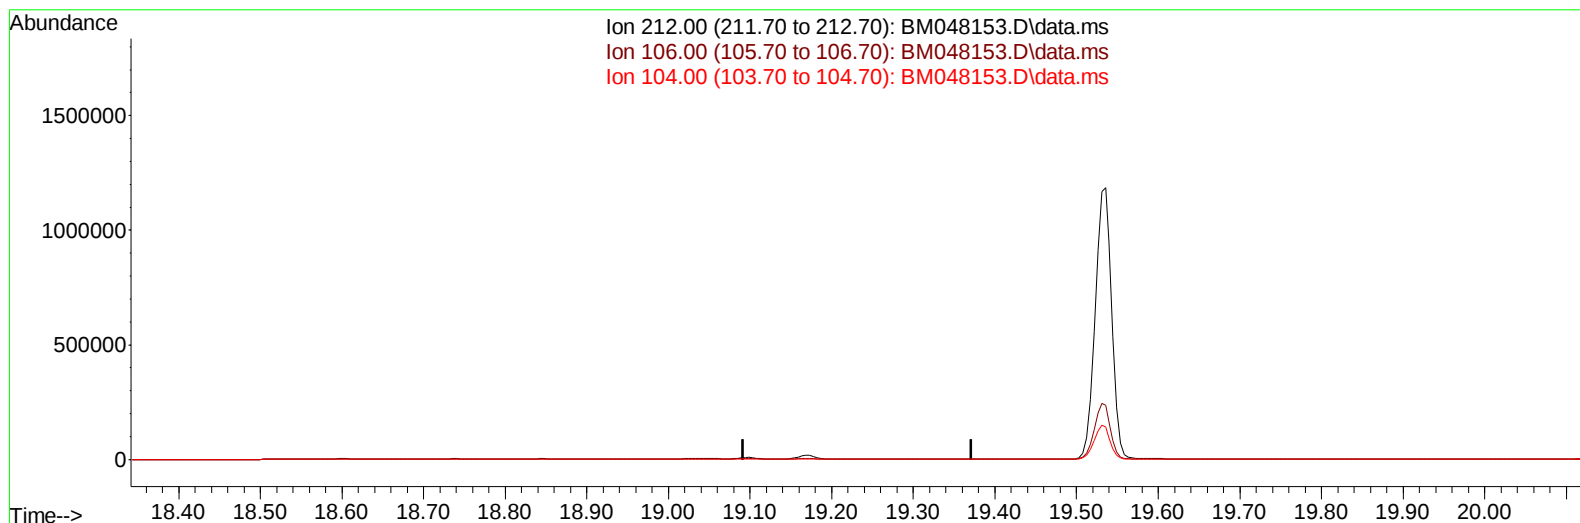

TIC: BM048153.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.191min (-19.191) 0.00 ng/u1

response 0

Ion	Exp%	Act%
212.00	100.00	0.00
106.00	15.00	0.00#
104.00	8.80	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048153.D
Acq On : 21 Oct 2024 13:59
Operator : RC/JU
Sample : P4380-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27G7

Manual IntegrationsAPPROVED

Quant Time: Oct 21 14:34:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 19 00:48:23 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

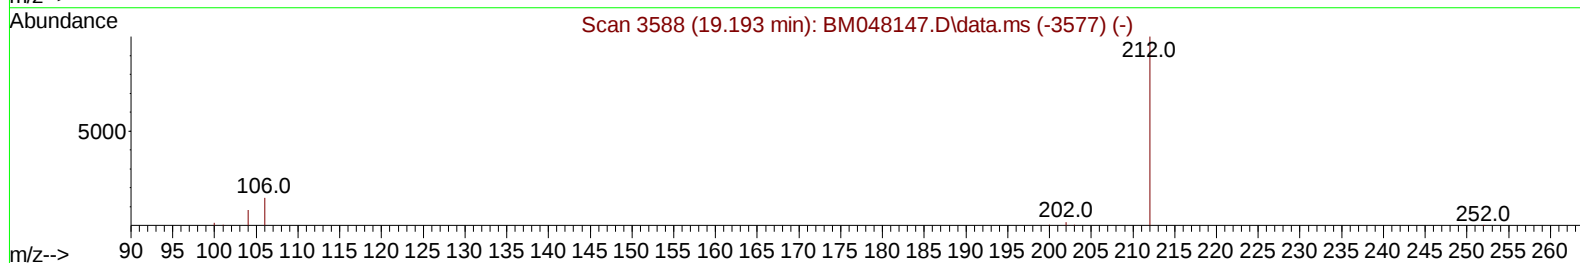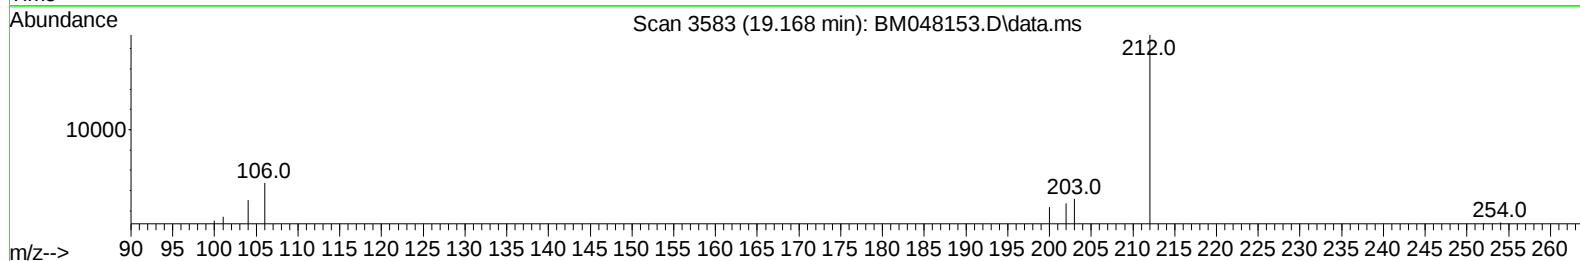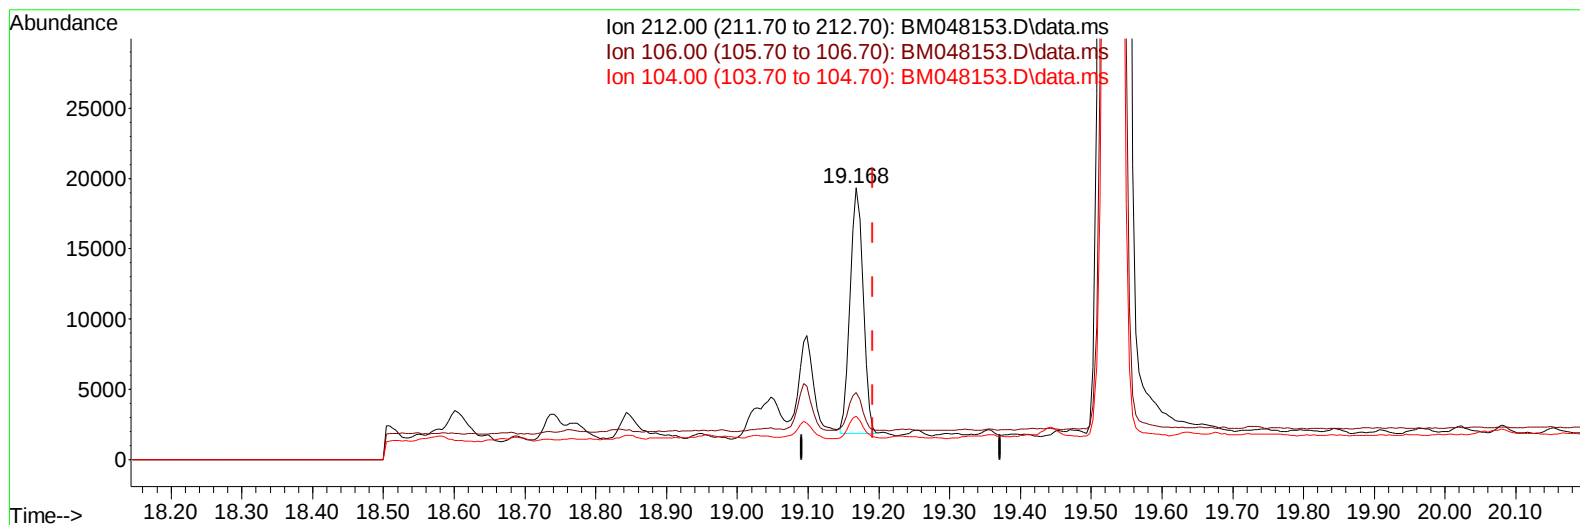

TIC: BM048153.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.168min (-0.023) 0.43 ng/u1 m

response 22230

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	15.00	0.00#
104.00	8.80	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048153.D
Acq On : 21 Oct 2024 13:59
Operator : RC/JU
Sample : P4380-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27G7

Manual IntegrationsAPPROVED

Quant Time: Oct 21 14:34:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 19 00:48:23 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

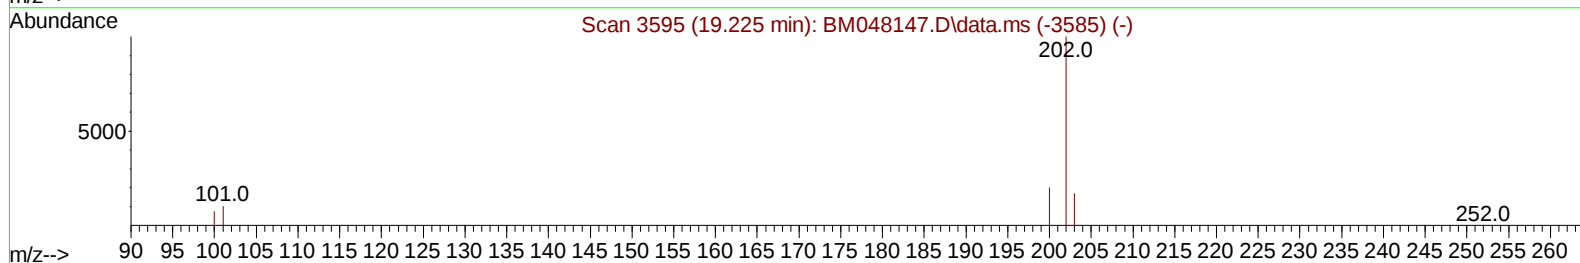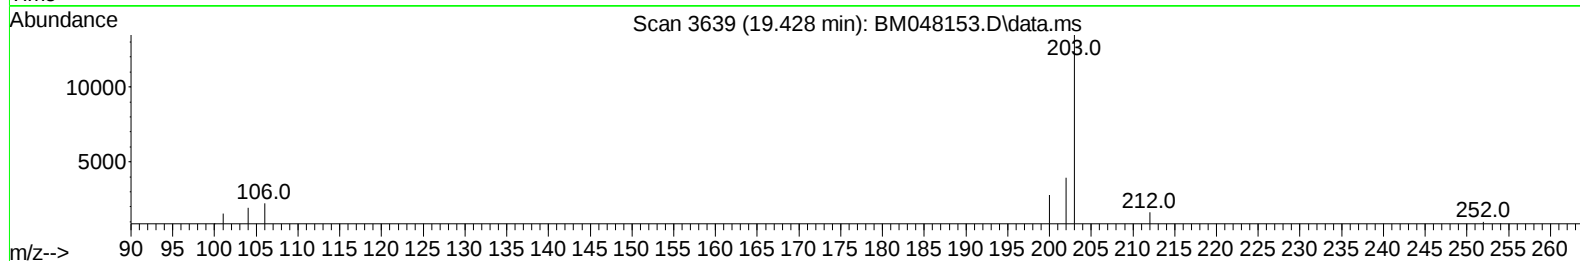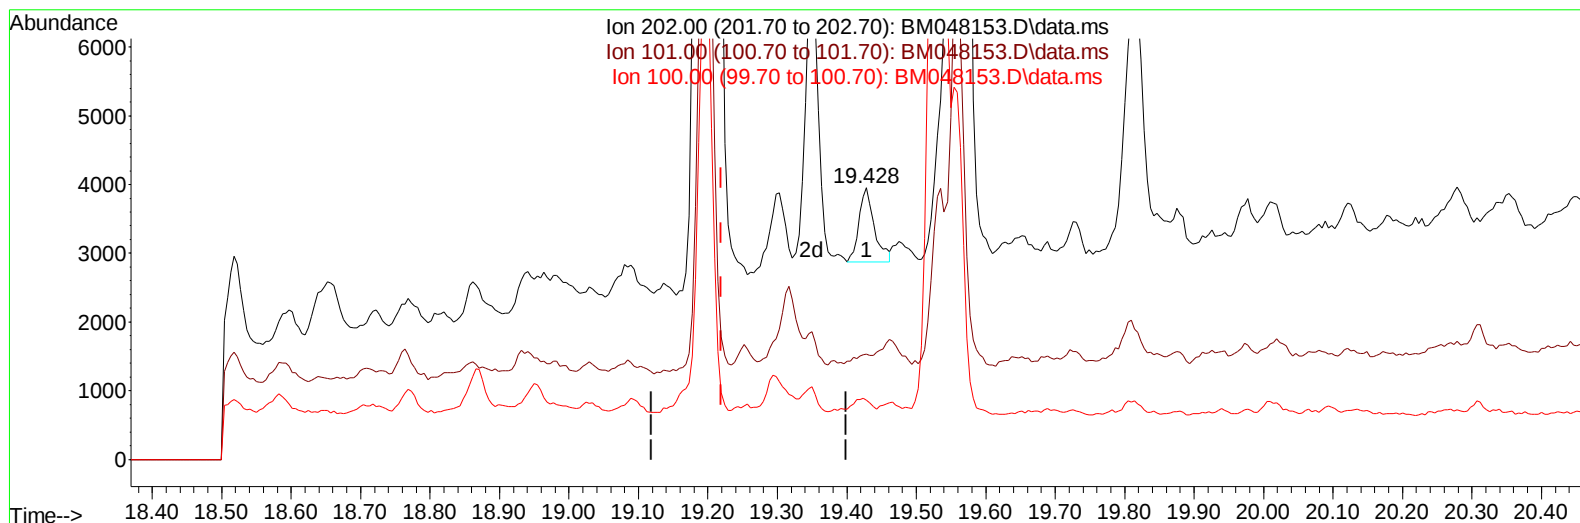

TIC: BM048153.D\data.ms

(19) Fluoranthene (C)

19.428min (+ 0.209) 0.02 ng/u1

response 1649

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	11.60	38.91#
100.00	8.90	21.92#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048153.D
Acq On : 21 Oct 2024 13:59
Operator : RC/JU
Sample : P4380-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27G7

Manual IntegrationsAPPROVED

Quant Time: Oct 21 14:34:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 19 00:48:23 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

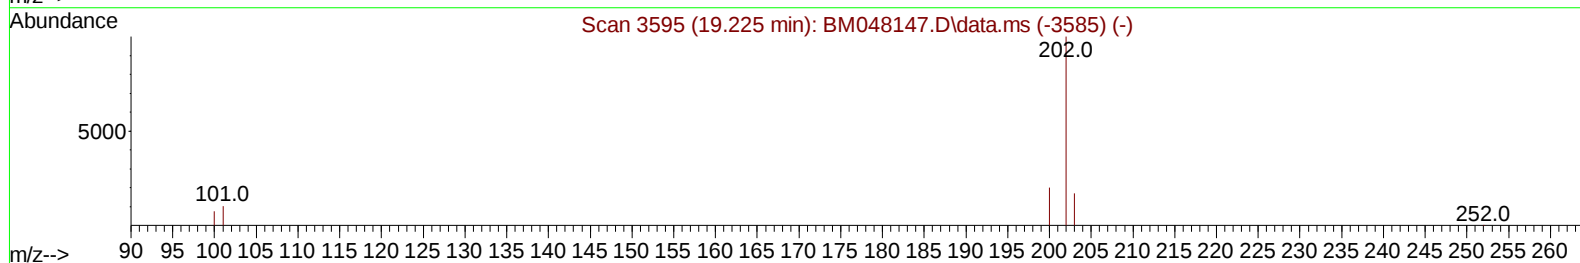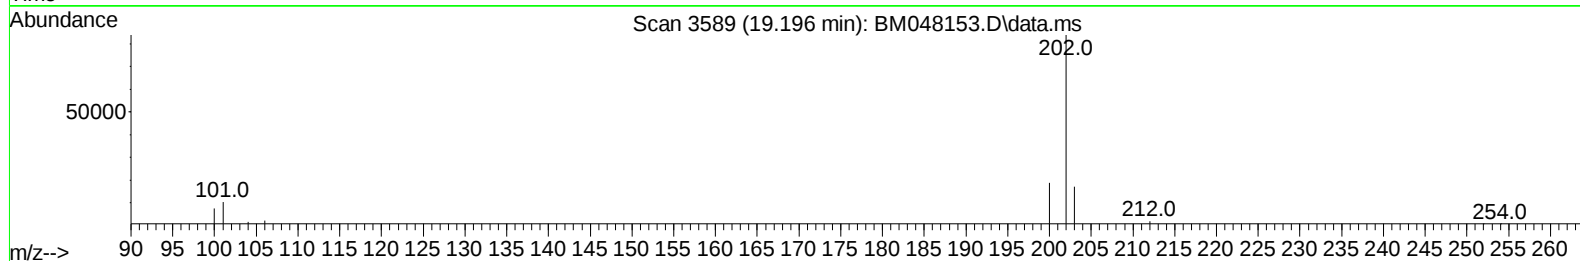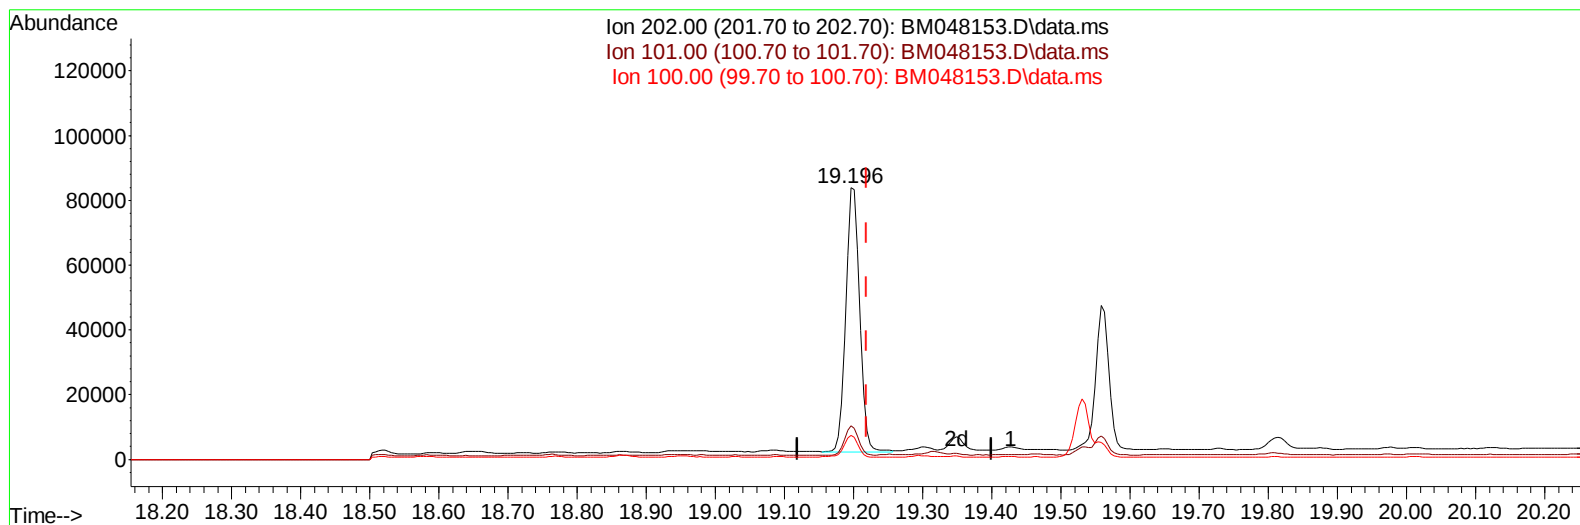

TIC: BM048153.D\data.ms

(19) Fluoranthene (C)

19.196min (-0.023) 1.64 ng/ul m

response 113973

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	11.60	12.47
100.00	8.90	8.95
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048153.D
Acq On : 21 Oct 2024 13:59
Operator : RC/JU
Sample : P4380-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27G7

Manual IntegrationsAPPROVED

Quant Time: Oct 21 14:34:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 19 00:48:23 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

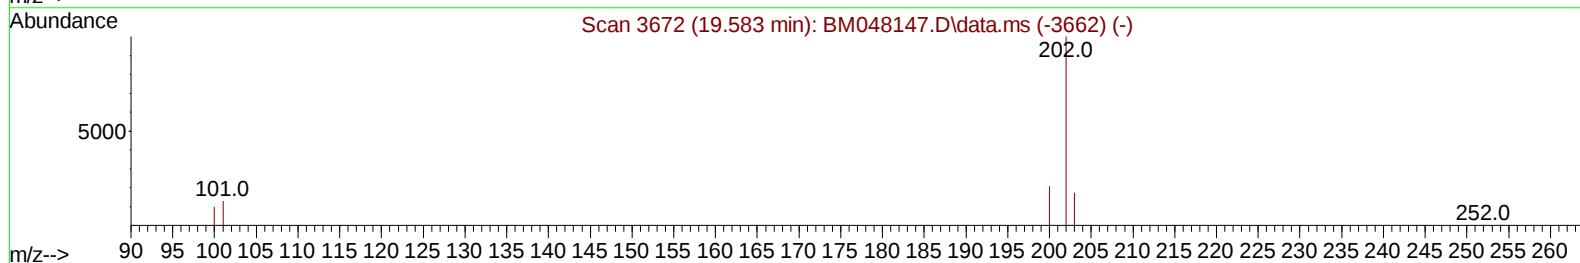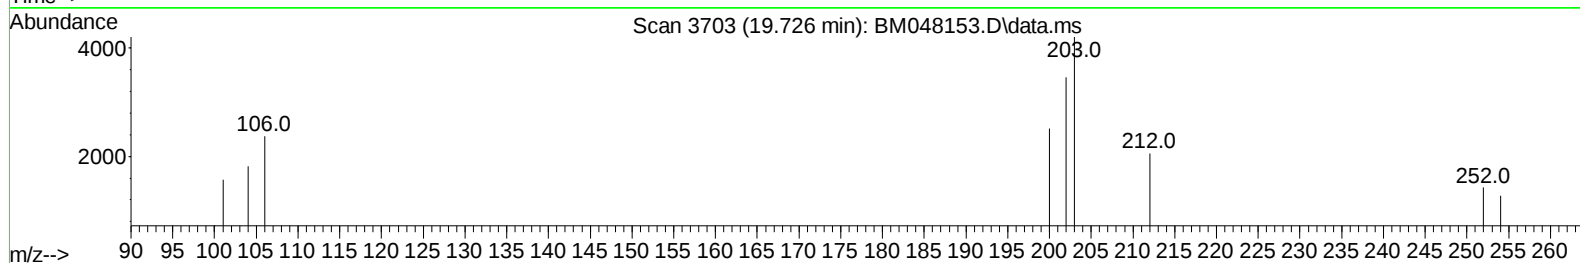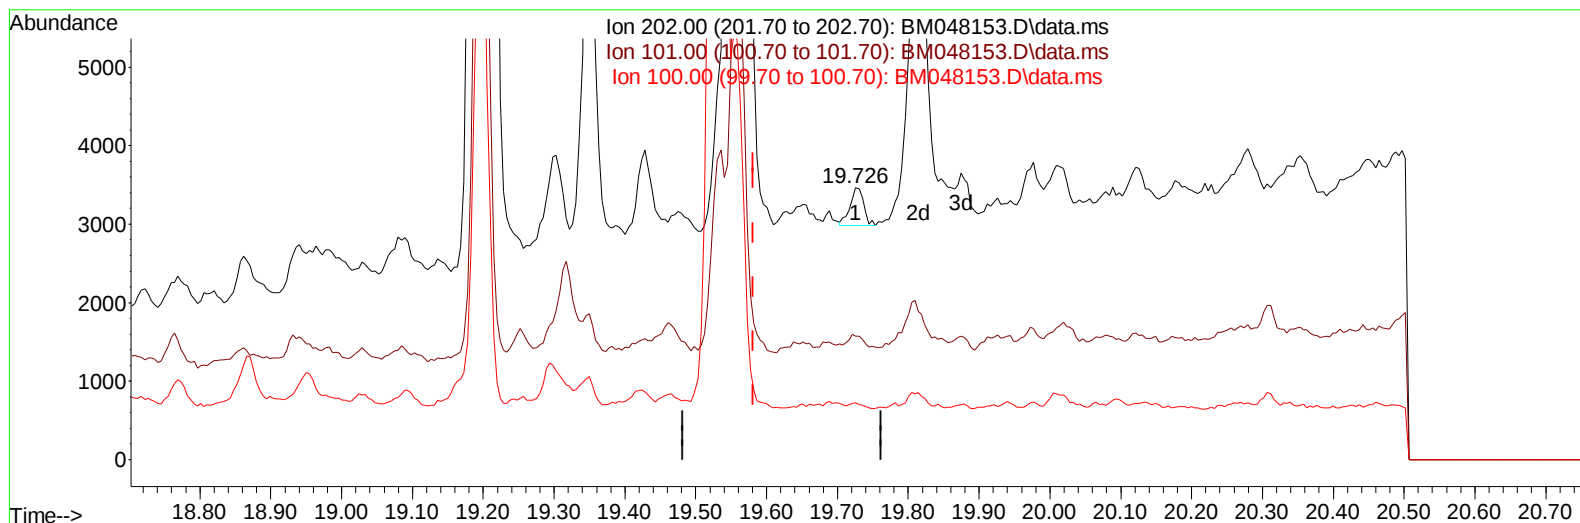

TIC: BM048153.D\data.ms

(20) Pyrene

19.726min (+ 0.144) 0.01 ng/u1

response 624

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	13.30	45.41#
100.00	10.10	20.85#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048153.D
Acq On : 21 Oct 2024 13:59
Operator : RC/JU
Sample : P4380-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27G7

Manual IntegrationsAPPROVED

Quant Time: Oct 21 14:34:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 19 00:48:23 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

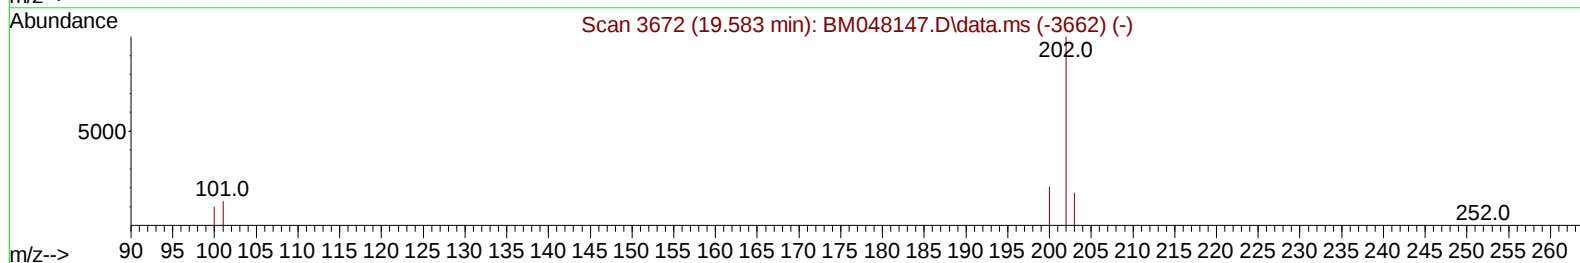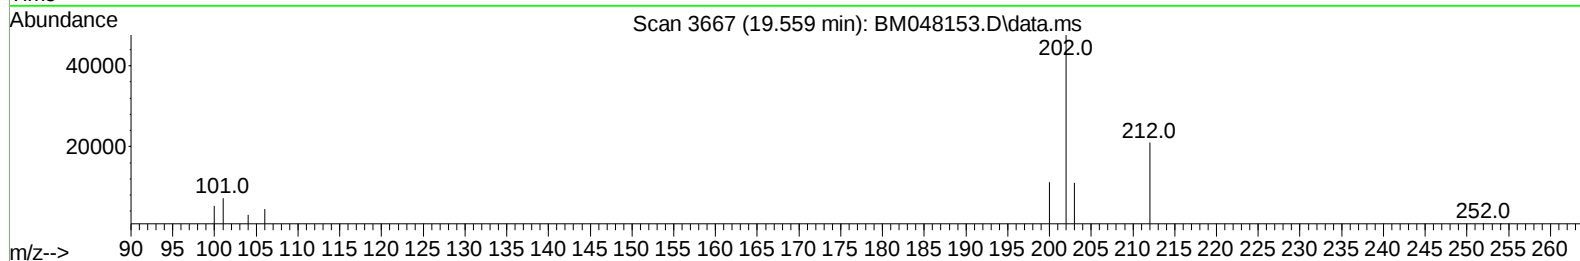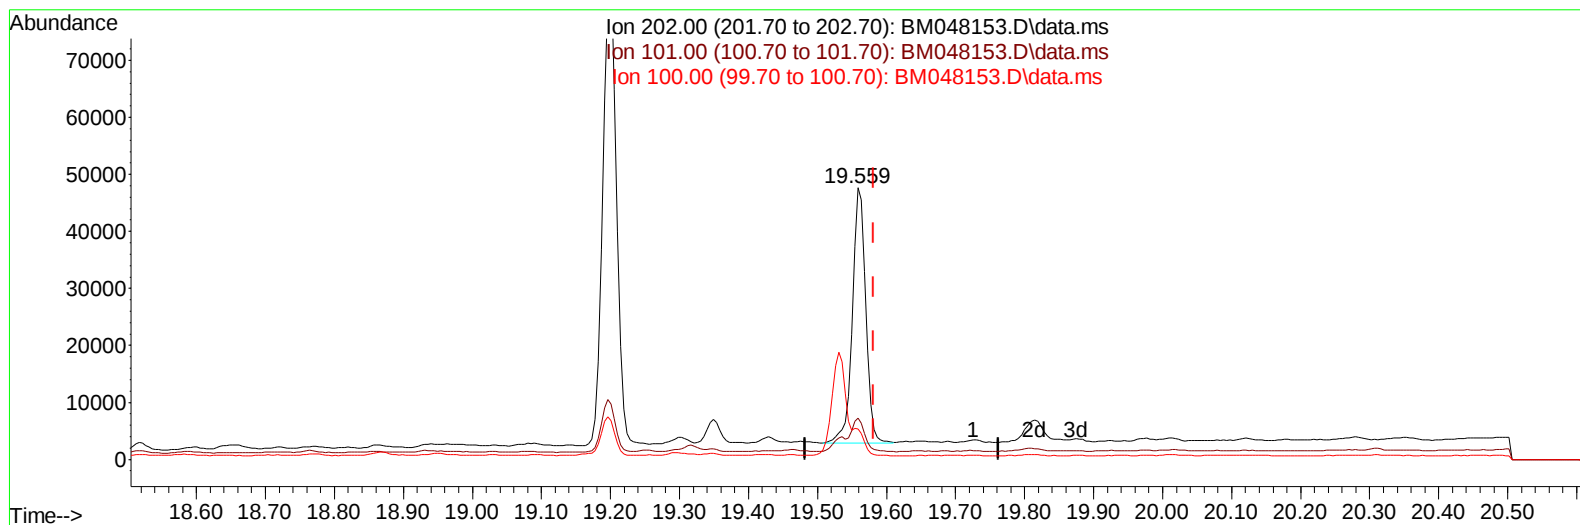

TIC: BM048153.D\data.ms

(20) Pyrene

19.559min (-0.023) 0.81 ng/u1 m

response 60495

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	13.30	15.21
100.00	10.10	11.22
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048153.D
Acq On : 21 Oct 2024 13:59
Operator : RC/JU
Sample : P4380-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27G7

Manual IntegrationsAPPROVED

Quant Time: Oct 21 14:34:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 19 00:48:23 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

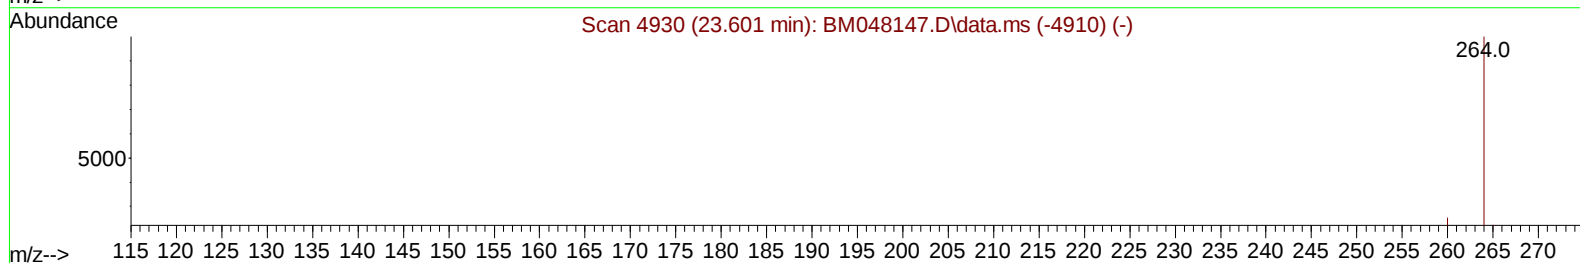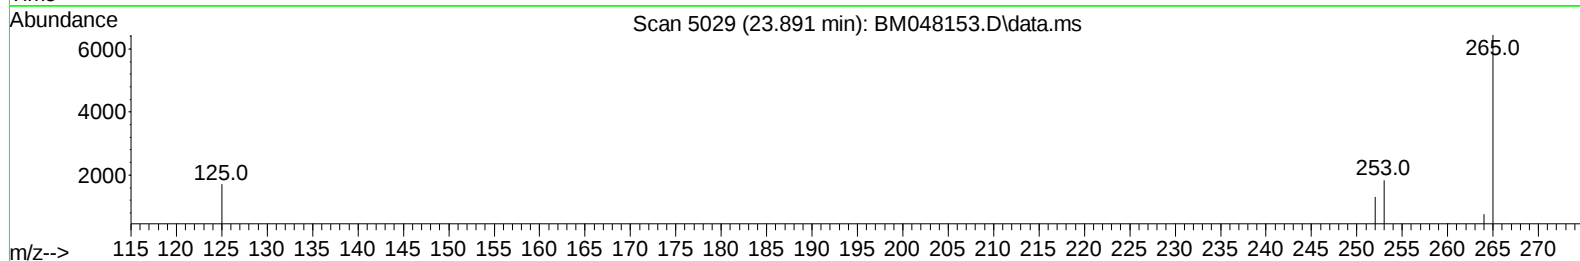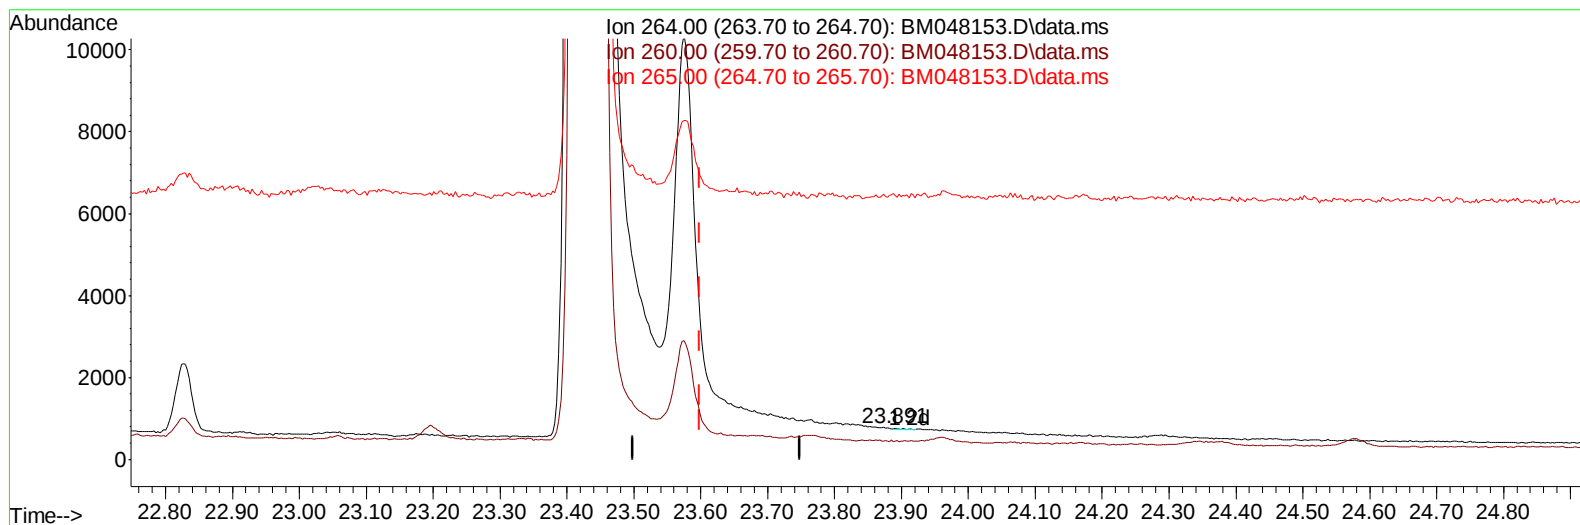

TIC: BM048153.D\data.ms

(23) Perylene-d12 (I)

23.891min (+ 0.292) 0.40 ng/u1

response 39

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	59.45#
265.00	128.10	845.41#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048153.D
Acq On : 21 Oct 2024 13:59
Operator : RC/JU
Sample : P4380-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27G7

Manual IntegrationsAPPROVED

Quant Time: Oct 21 14:34:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 19 00:48:23 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

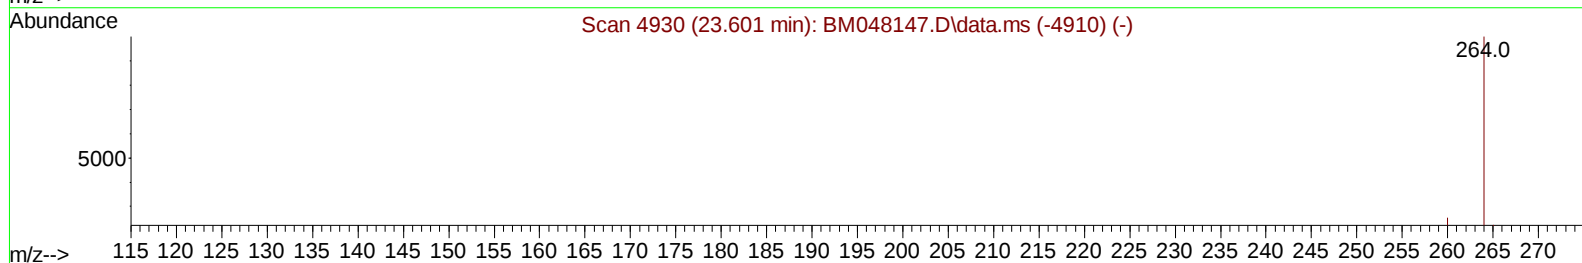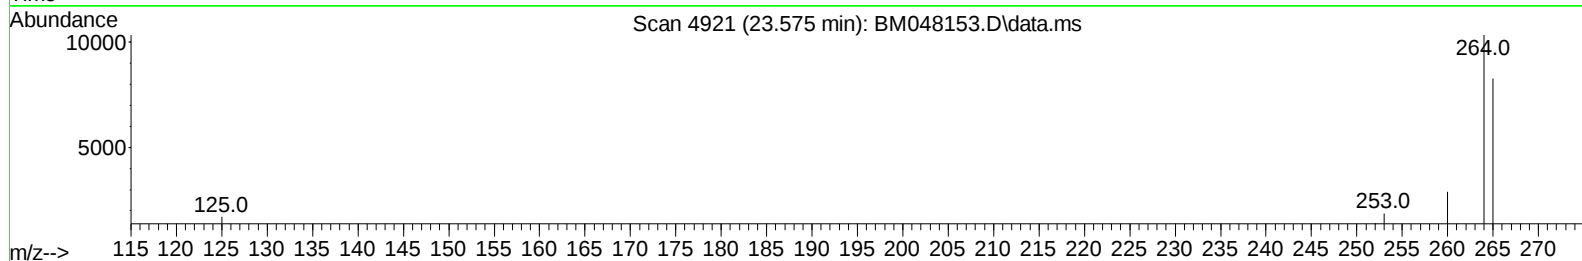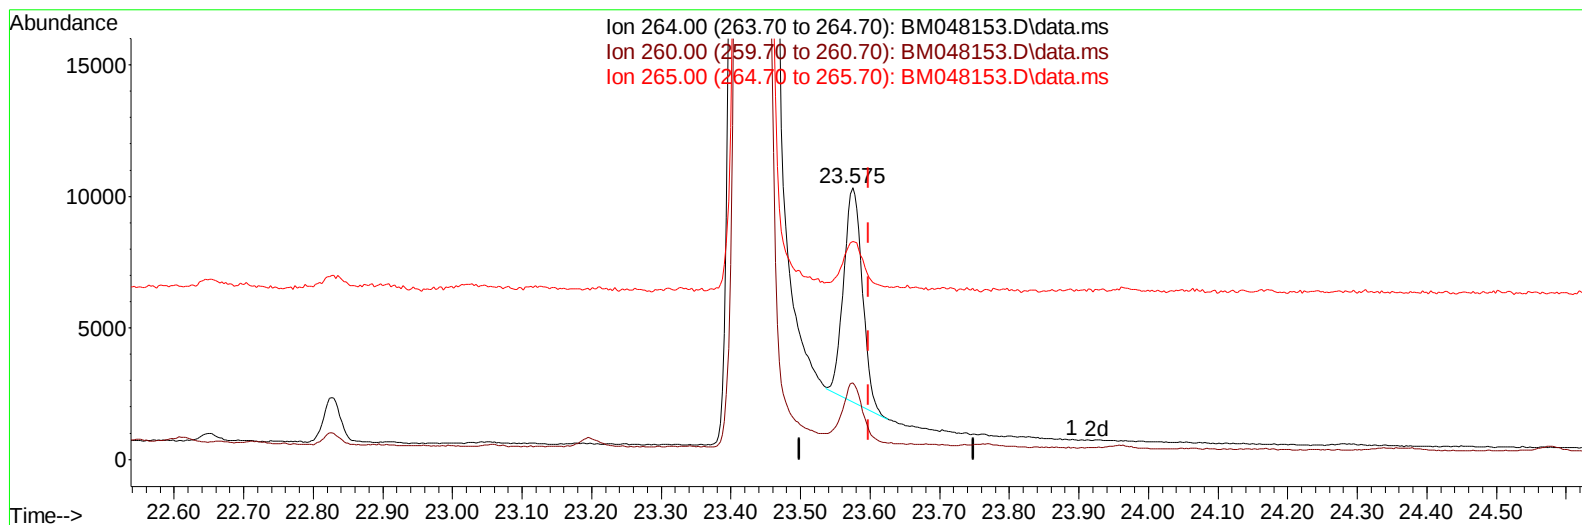

TIC: BM048153.D\data.ms

(23) Perylene-d12 (I)

23.575min (-0.023) 0.40 ng/ul m

response 15165

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	28.14
265.00	128.10	80.17#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
 Data File : BM048153.D
 Acq On : 21 Oct 2024 13:59
 Operator : RC/JU
 Sample : P4380-22
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E27G7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/22/2024
 Supervised By :mohammad ahmed 10/23/2024

Quant Time: Oct 21 14:34:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 19 00:48:23 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.771	152		6629	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.556	136		20548	0.400	ng/ul	-0.03
9) Acenaphthene-d10	14.399	164		15743	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.144	188		23539m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.316	240		17749m	0.400	ng/ul	-0.02
23) Perylene-d12	23.575	264		15165m	0.400	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.240	96		36948	4.100	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.151	152		11458	0.400	ng/ul	-0.05
18) Fluoranthene-d10	19.168	212		22230m	0.430	ng/ul	-0.02
Target Compounds							
							Qvalue
5) Naphthalene	10.611	128		9690747	173.533	ng/ul	98
7) 2-Methylnaphthalene	12.222	142		489231	15.312	ng/ul	97
8) 1-Methylnaphthalene	12.442	142		244836	6.659	ng/ul	98
10) Acenaphthylene	14.122	152		585410	8.050	ng/ul	98
11) Acenaphthene	14.464	153		256172	4.929	ng/ul	98
12) Fluorene	15.449	166		315975	5.675	ng/ul	99
14) Pentachlorophenol	16.807	266		1076m	0.136	ng/ul	
15) Phenanthrene	17.182	178		756615m	12.719	ng/ul	
16) Anthracene	17.275	178		84427m	1.500	ng/ul	
19) Fluoranthene	19.196	202		113973m	1.636	ng/ul	
20) Pyrene	19.559	202		60495m	0.808	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048153.D
Acq On : 21 Oct 2024 13:59
Operator : RC/JU
Sample : P4380-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27G7

Manual IntegrationsAPPROVED

Quant Time: Oct 21 14:34:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 19 00:48:23 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

